
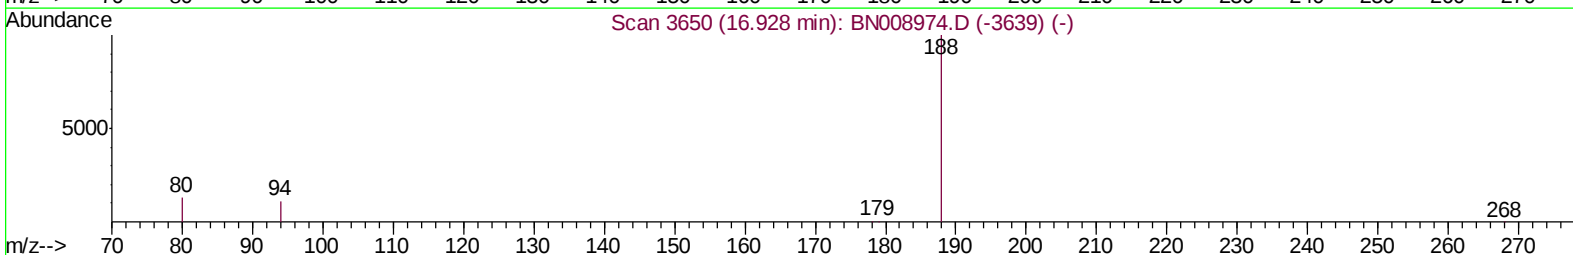
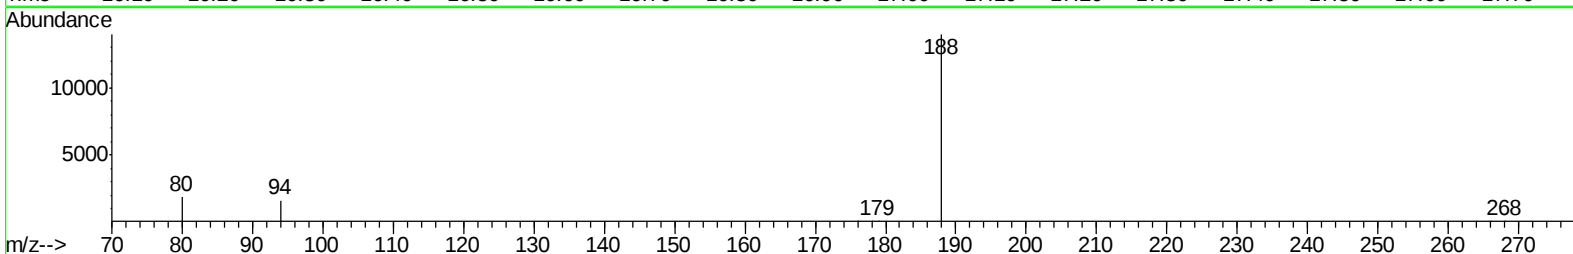


Data File : BN008985.D
Acq On : 14 Dec 2019 02:10
Operator : JU
Sample : PB-BL WATER
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 16 00:51:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

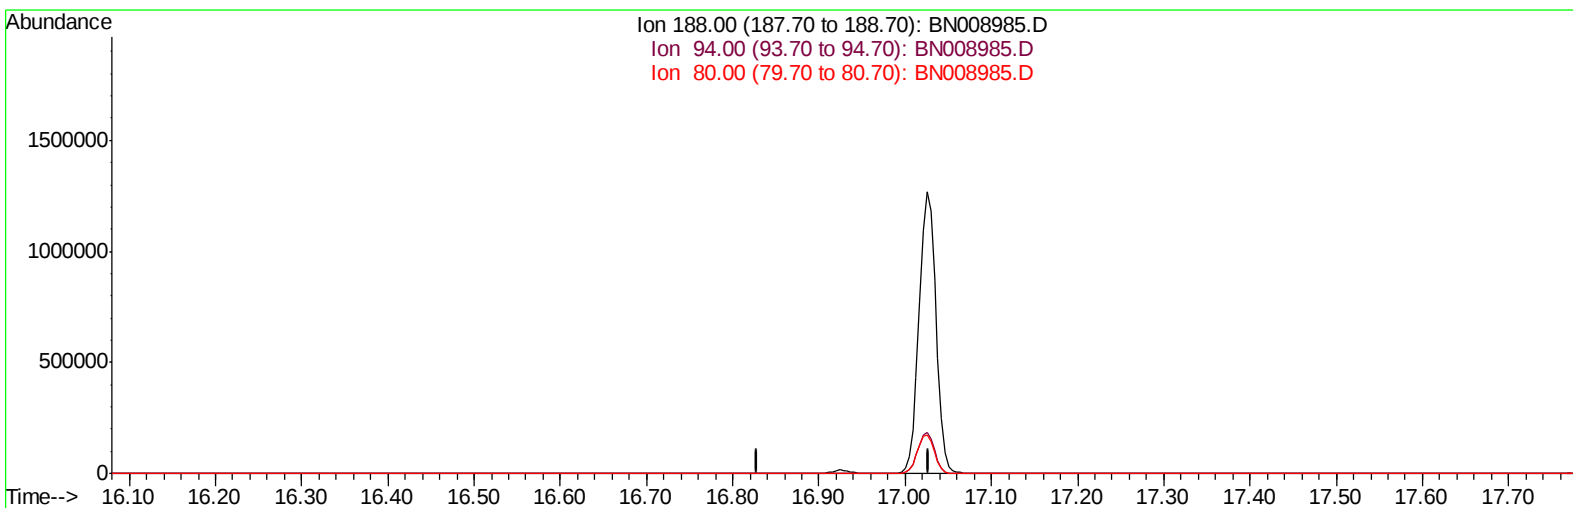

TIC: BN008985.D

(10) Phenanthrene-d10 (I)

16.928min (-16.928) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	12.20	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00