
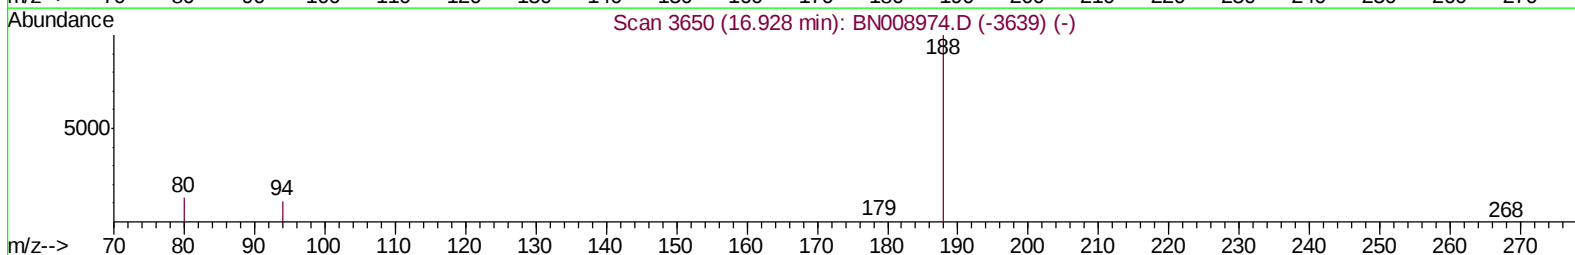
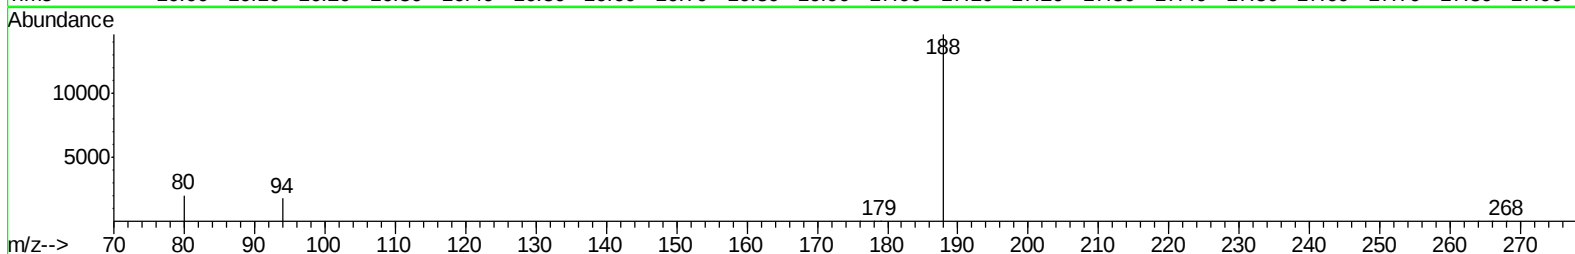


Data File : BN008985.D
Acq On : 14 Dec 2019 02:10
Operator : JU
Sample : PB-BL WATER
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 16 00:51:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

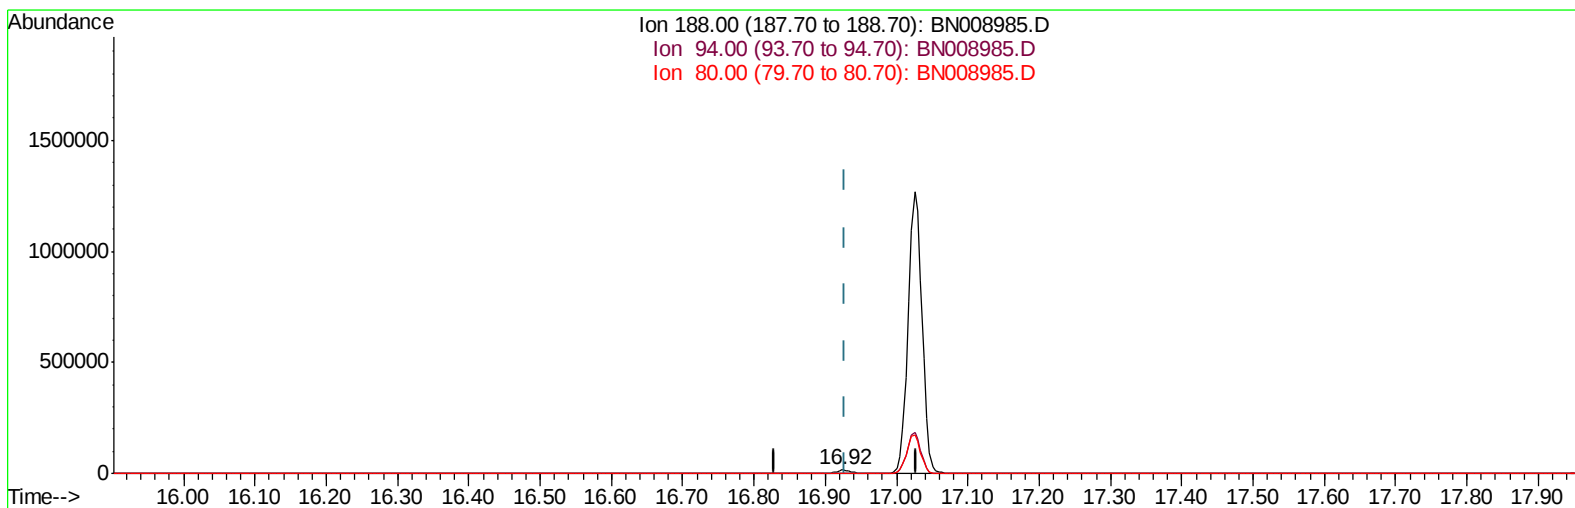

TIC: BN008985.D

(10) Phenanthrene-d10 (I)

16.924min (-0.004) 0.40ng/ul m

response 20070

Ion	Exp%	Act%
188.00	100	100
94.00	12.20	12.59
80.00	14.40	14.19
0.00	0.00	0.00