
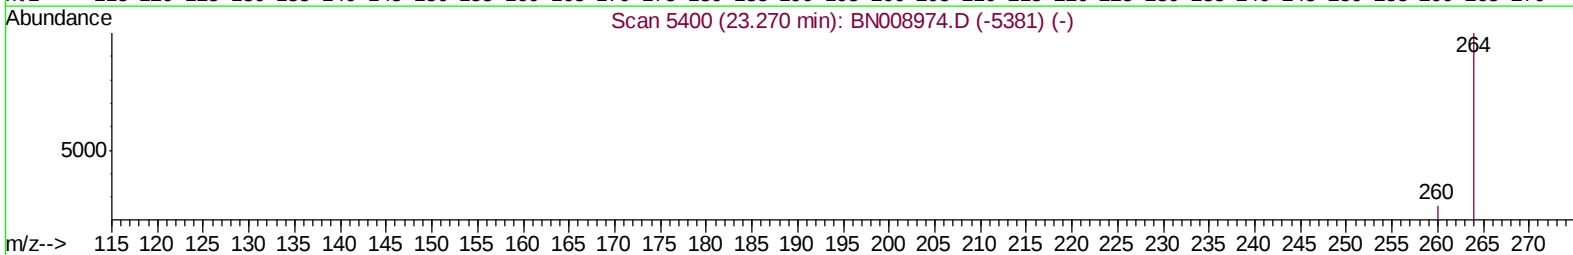
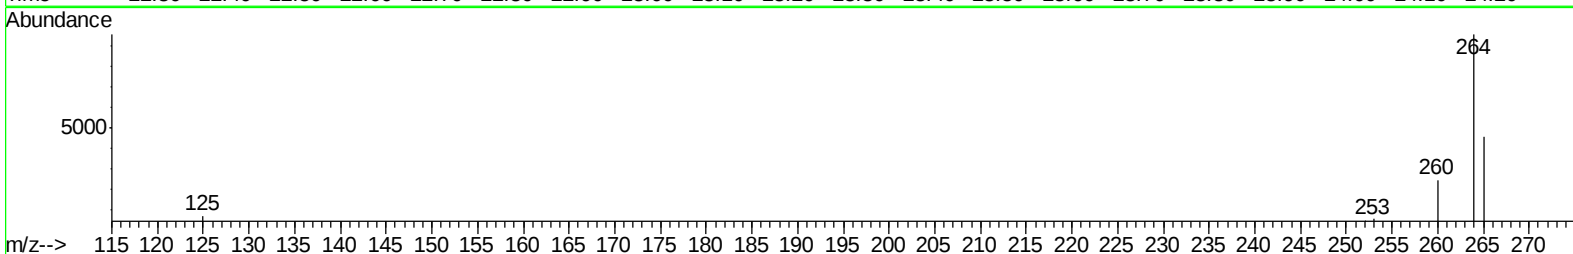


Data File : BN008985.D
Acq On : 14 Dec 2019 02:10
Operator : JU
Sample : PB-BL WATER
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Dec 16 00:57:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

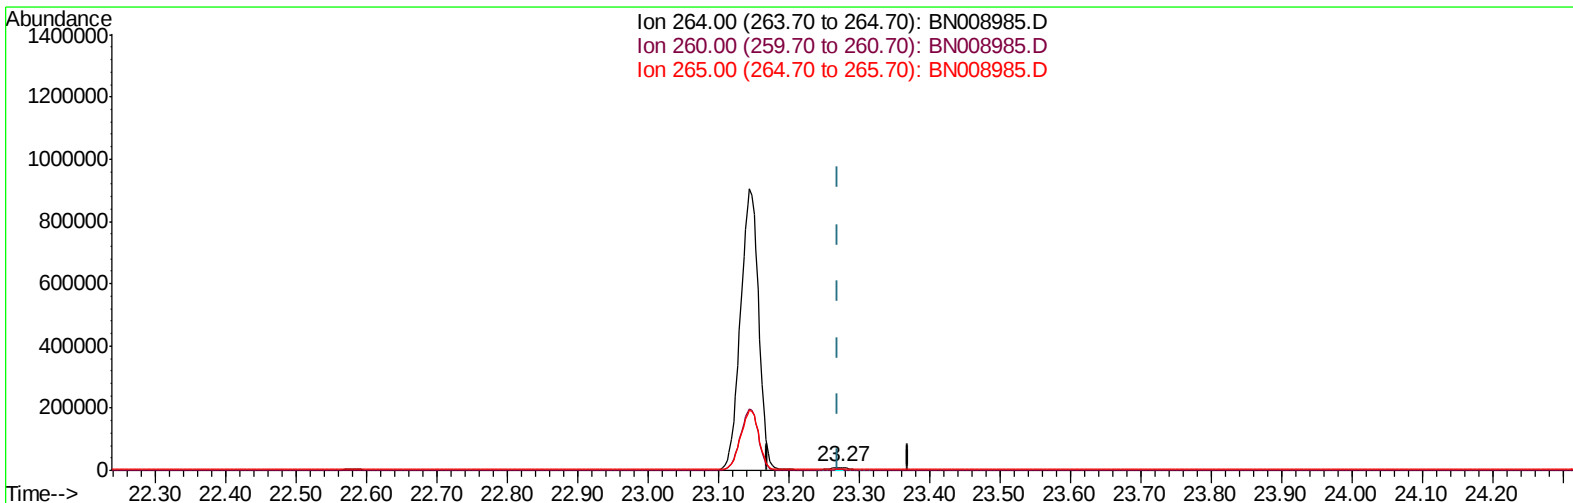

TIC: BN008985.D

(20) Perylene-d12 (I)

23.273min (+0.003) 0.40ng/ul m

response 14704

Ion	Exp%	Act%
264.00	100	100
260.00	26.80	25.60
265.00	59.90	47.26#
0.00	0.00	0.00