
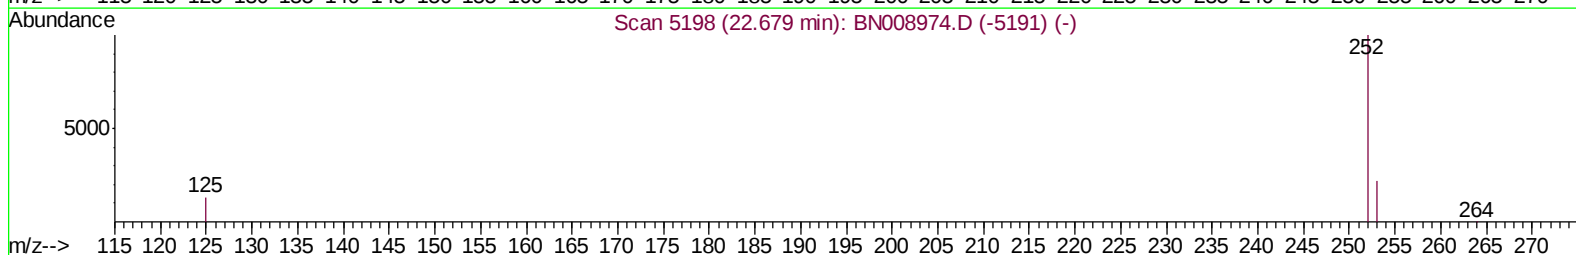
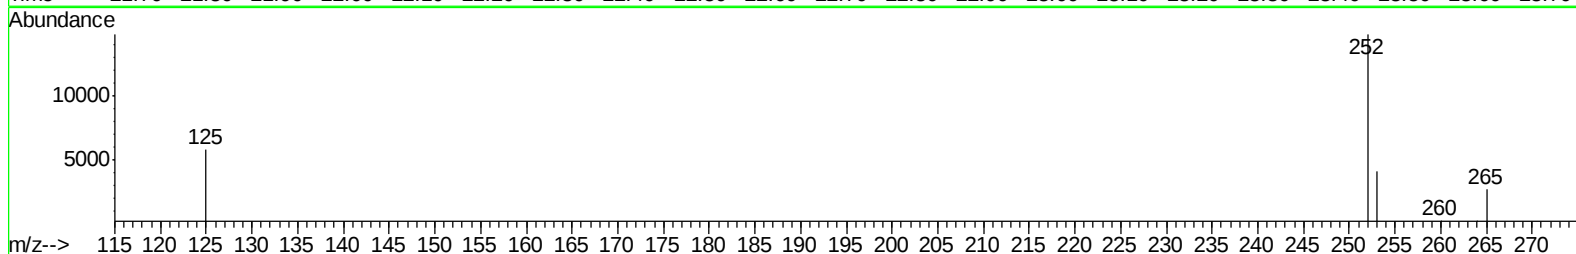


Data File : BN008987.D
Acq On : 14 Dec 2019 03:22
Operator : JU
Sample : K4649-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 16 01:06:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

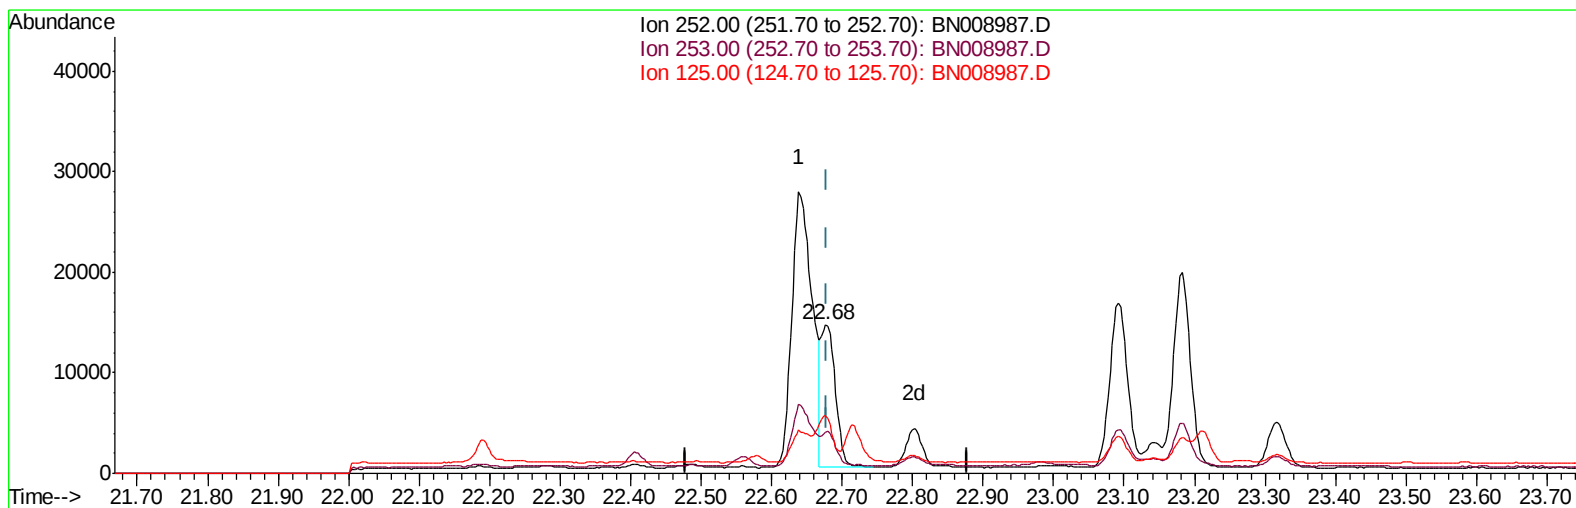

TIC: BN008987.D

(22) Benzo(k)fluoranthene

22.677min (-0.003) 0.26ng/ul m

response 19610

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	27.52
125.00	17.20	38.93#
0.00	0.00	0.00