
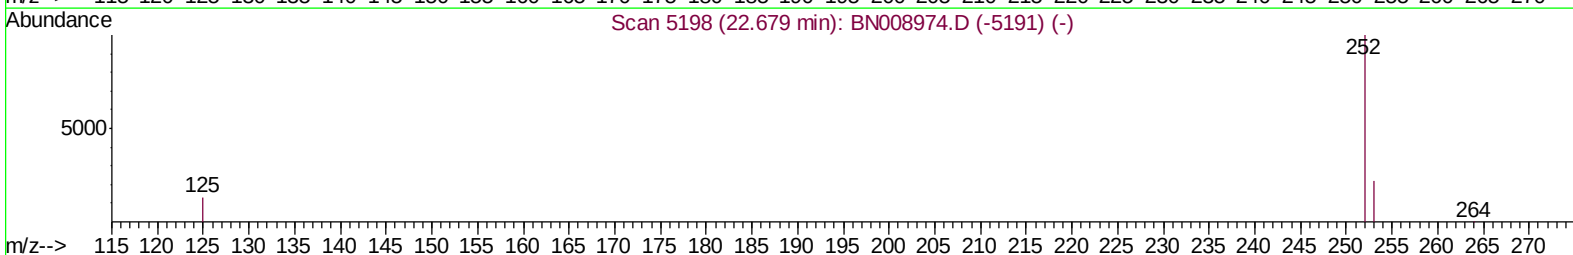
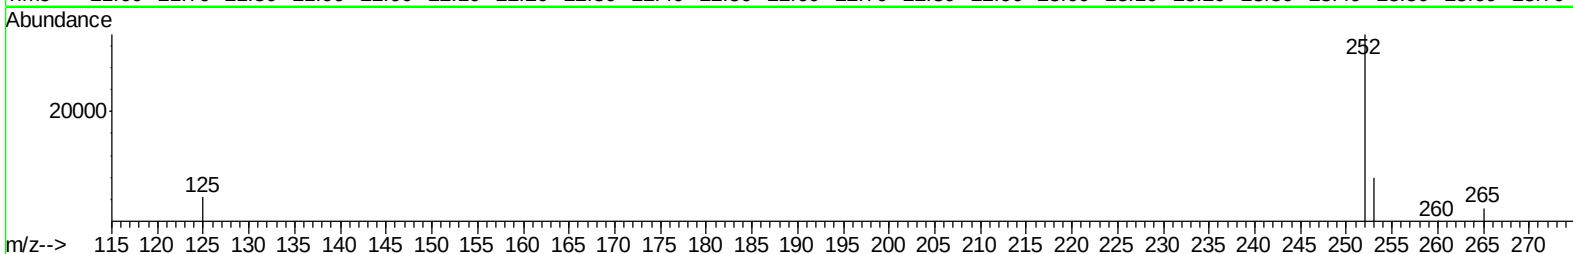


Data File : BN008990.D  
Acq On : 14 Dec 2019 05:10  
Operator : JU  
Sample : K4649-06DL 5X  
Misc :  
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Dec 16 00:52:13 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Dec 16 00:48:46 2019  
Response via : Initial Calibration

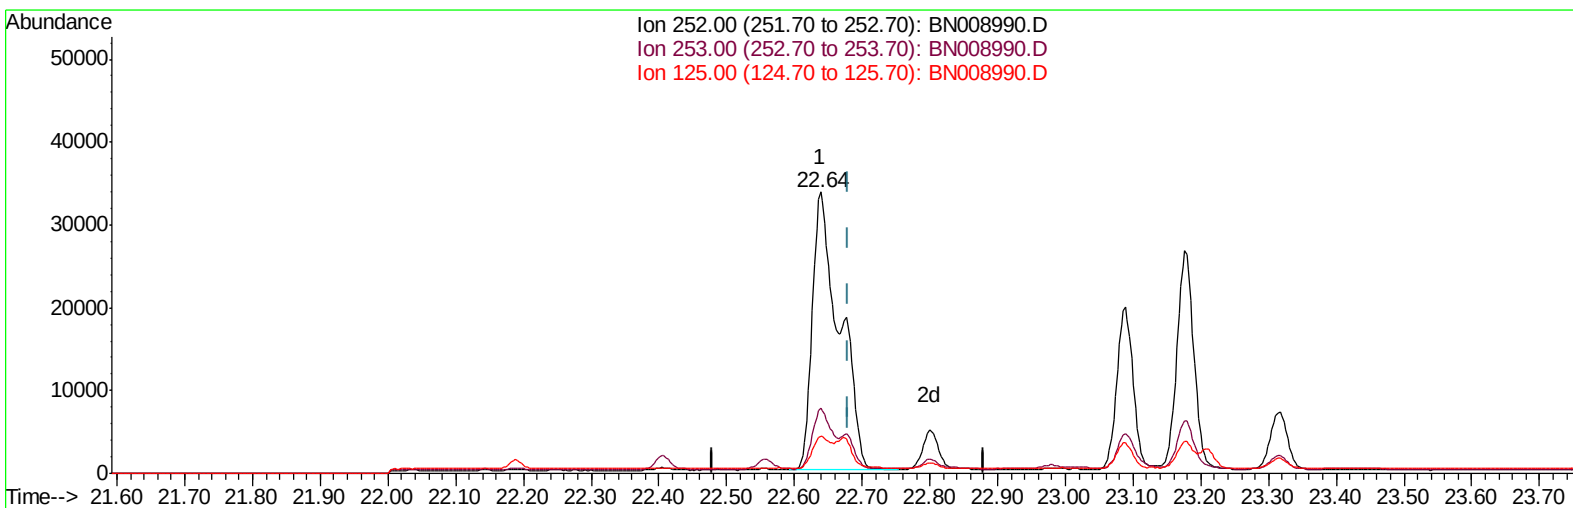

TIC: BN008990.D

(22) Benzo(k)fluoranthene  
22.638min (-0.041) 1.38ng/ul  
response 93242

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 24.50 | 23.29  |
| 125.00 | 17.20 | 13.10# |
| 0.00   | 0.00  | 0.00   |