
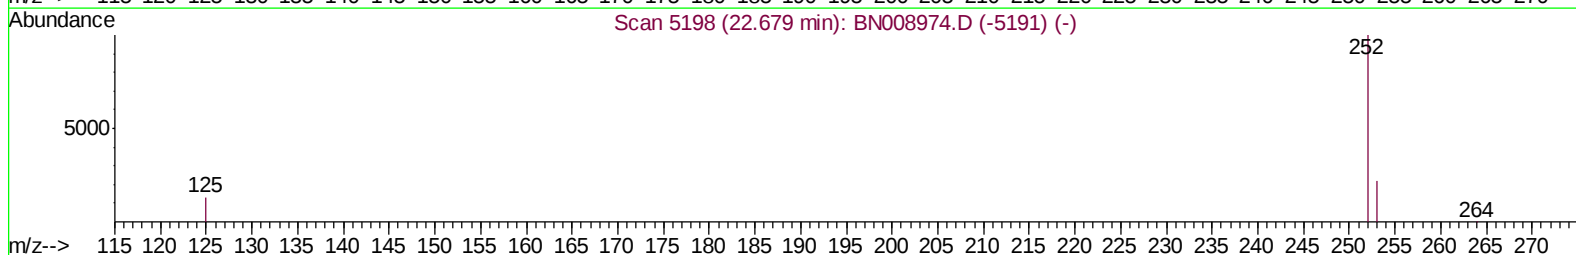
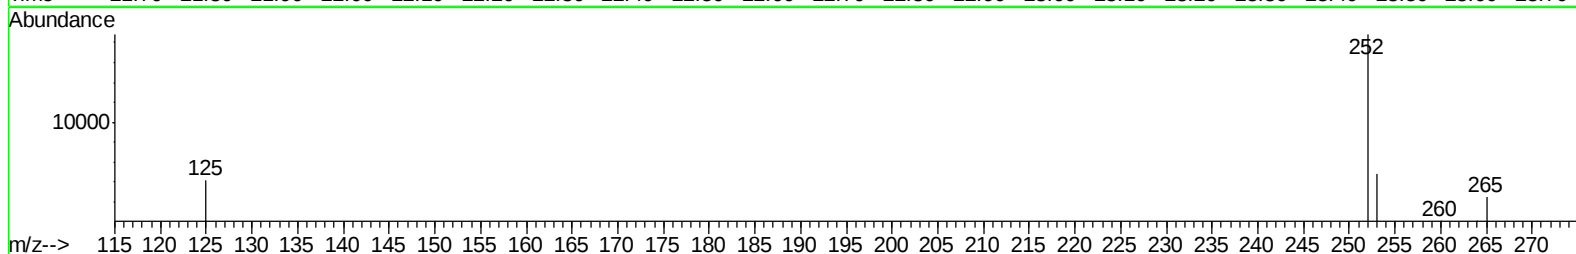


Data File : BN008990.D
Acq On : 14 Dec 2019 05:10
Operator : JU
Sample : K4649-06DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Dec 16 00:52:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

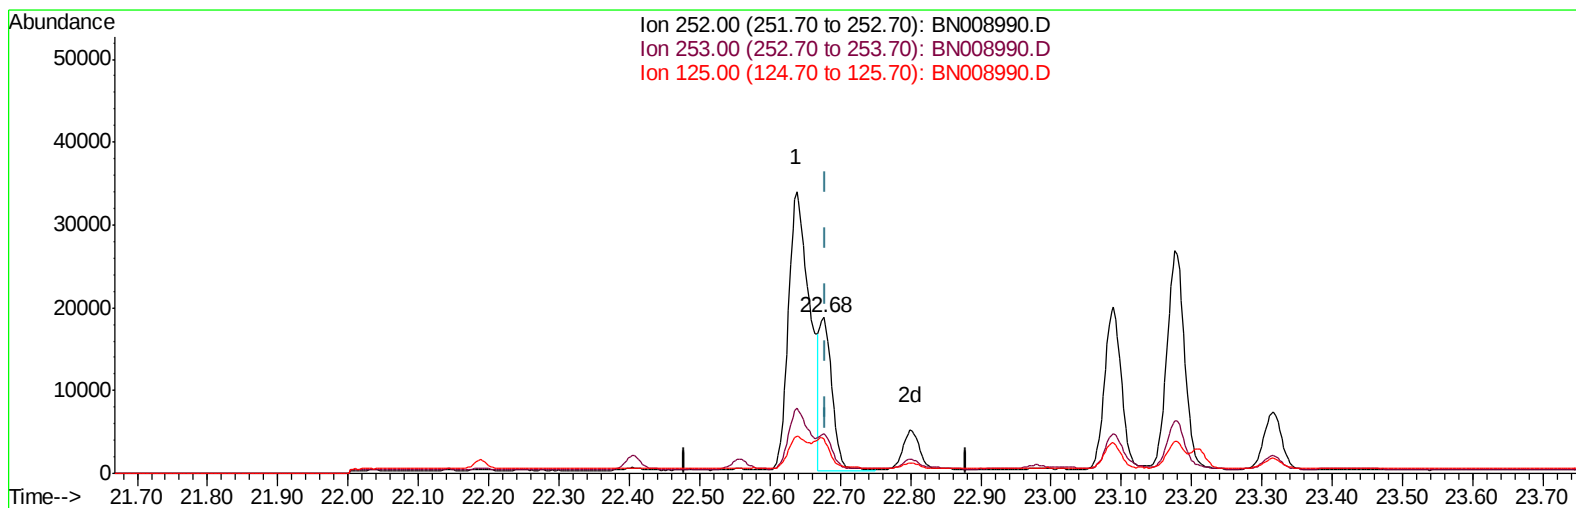

TIC: BN008990.D

(22) Benzo(k)fluoranthene

22.676min (-0.003) 0.35ng/ul m

response 23610

Ion	Exp%	Act%
252.00	100	100
253.00	24.50	25.47
125.00	17.20	21.97#
0.00	0.00	0.00