

Data File : BN008985.D
Acq On : 14 Dec 2019 02:10
Operator : JU
Sample : PB-BL WATER
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK046

Quant Time: Dec 16 00:51:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	2973	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	13839	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	8893	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.93
16) Chrysene-d12	21.13	240	18722	0.40	ng/ul	0.00
20) Perylene-d12	23.27	264	17204	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.90	152	9020	0.40	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	25811	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.18	166	3164	0.074	ng/ul#	13
17) Pyrene	19.33	202	3177	0.042	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN008985.D
Acq On : 14 Dec 2019 02:10
Operator : JU
Sample : PB-BL WATER
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK046

Quant Time: Dec 16 00:51:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 16 00:48:46 2019
Response via : Initial Calibration

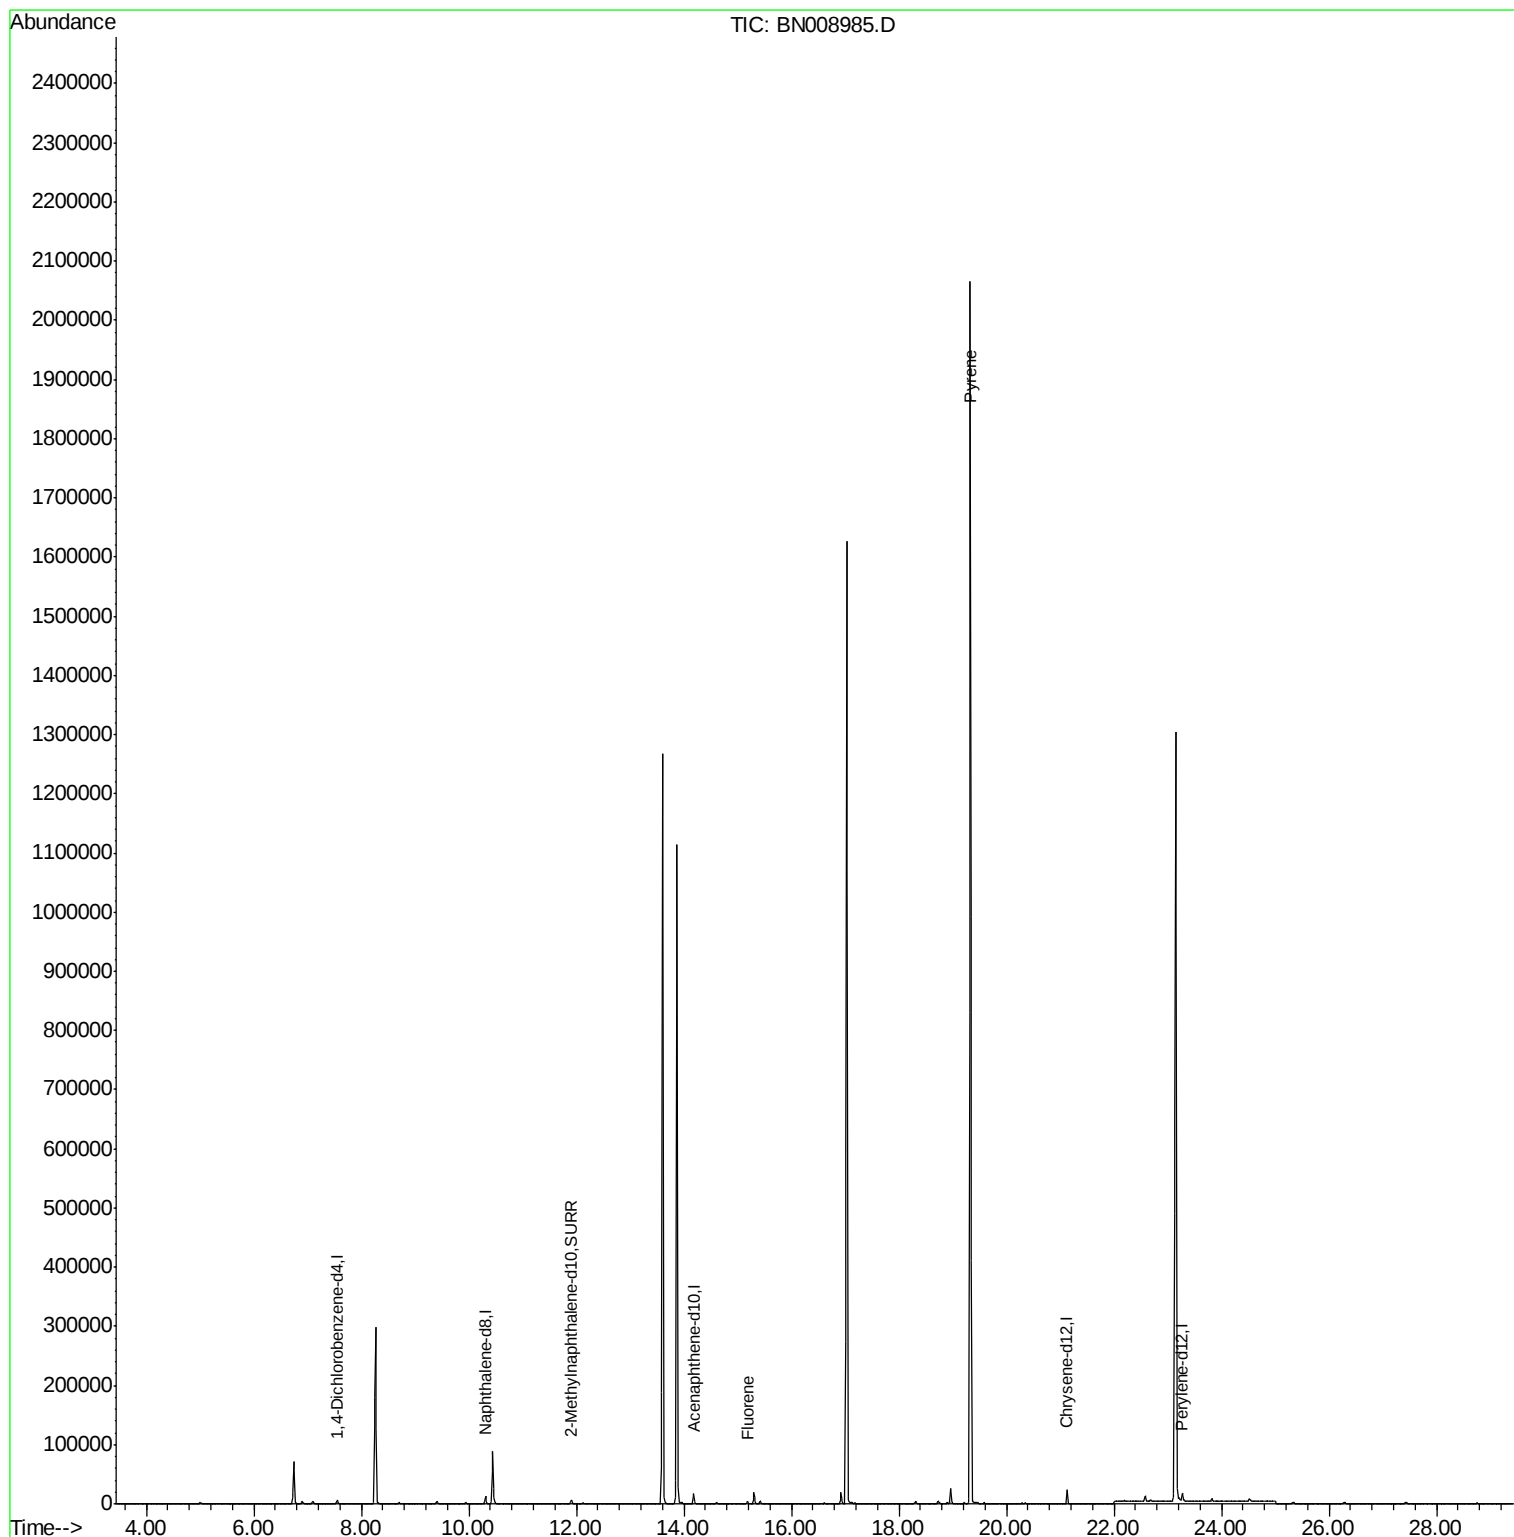

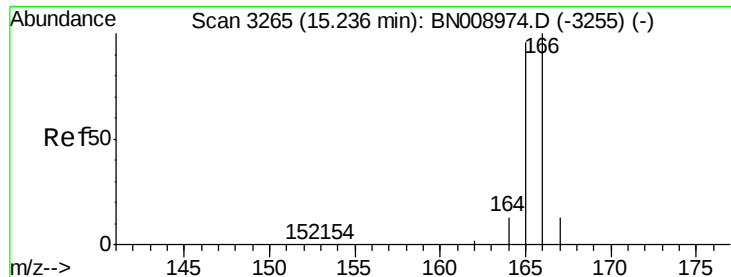

#9

Fluorene

Concen: 0.074 ng/ul

RT: 15.18 min Scan# 3253

Delta R.T. -0.06 min

Lab File: BN008985.D

Acq: 14 Dec 2019 02:10

Instrument :

BNA_N

ClientSampleId :

SBLK046


Tgt Ion:166 Resp: 3164

Ion Ratio Lower Upper

166 100

165 6.3 77.7 116.5#




167 33.5 11.1 16.7#

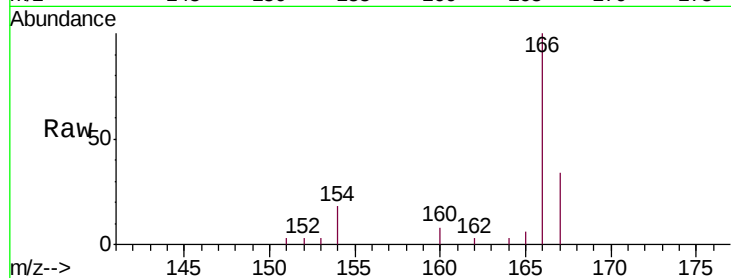

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

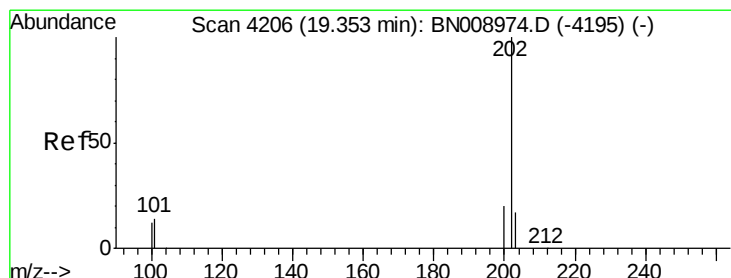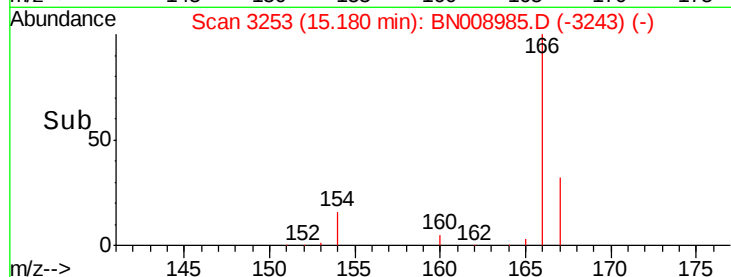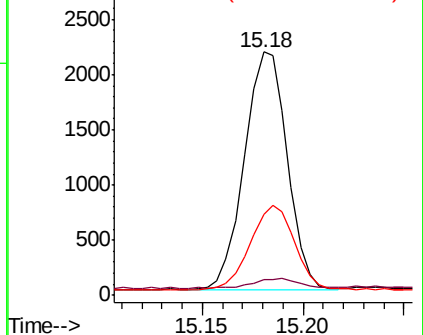

#17

Pyrene

Concen: 0.042 ng/ul

RT: 19.33 min Scan# 4201

Delta R.T. -0.02 min

Lab File: BN008985.D

Acq: 14 Dec 2019 02:10


Tgt Ion:202 Resp: 3177

Ion Ratio Lower Upper

202 100

101 168.5 12.2 18.4#

100 1102.4 9.5 14.3#

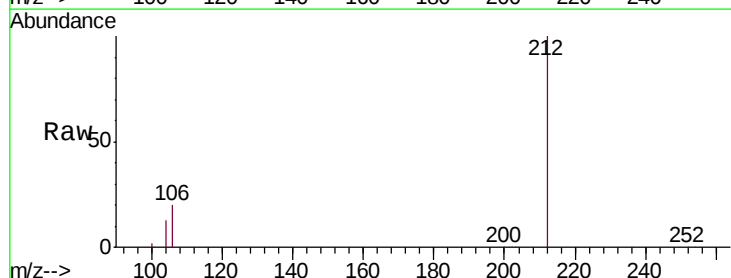

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

