


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121319\
Data File : BN008966.D
Acq On : 13 Dec 2019 14:02
Operator : JU
Sample : K6089-14DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1




Quant Time: Dec 13 14:38:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

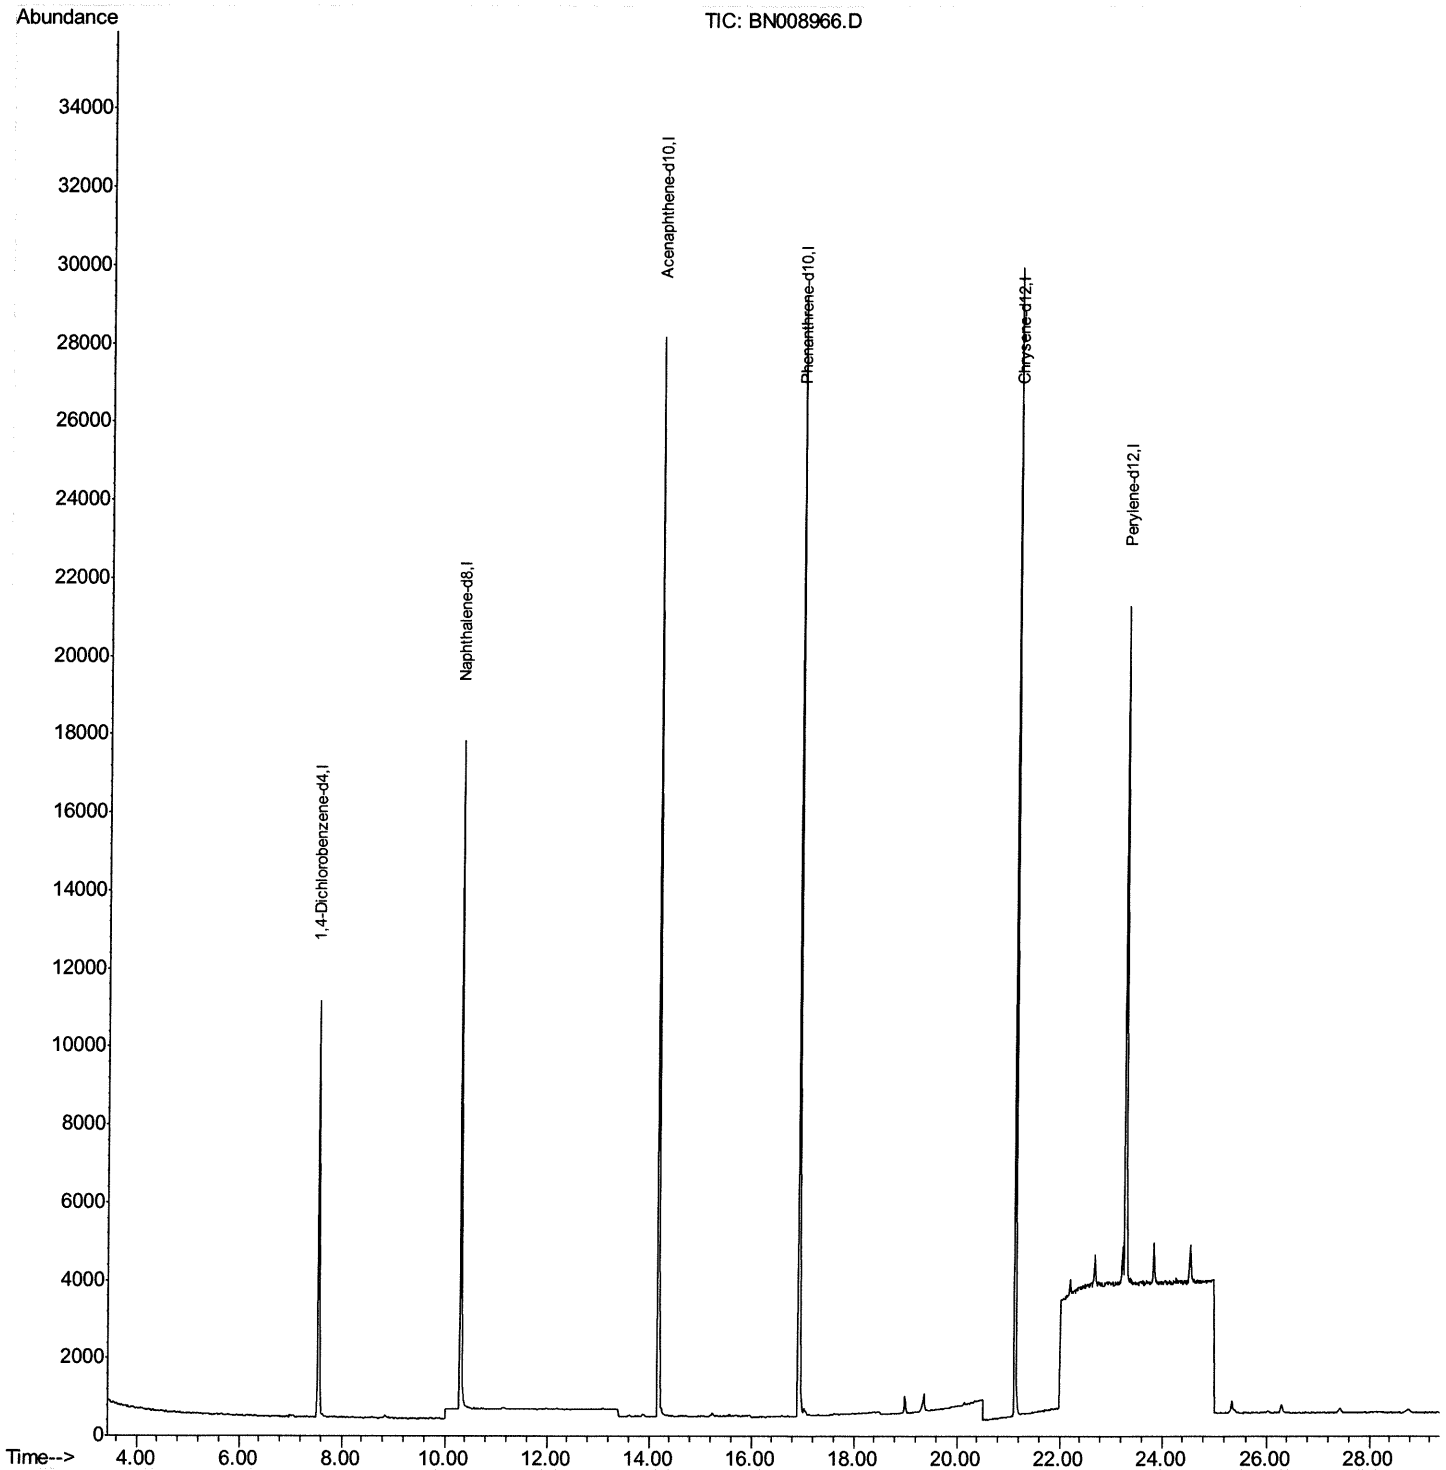

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121319\
 Data File : BN008965.D
 Acq On : 13 Dec 2019 13:26
 Operator : JU
 Sample : K6089-07DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 14:15:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 12 00:49:42 2019
 Response via : Initial Calibration

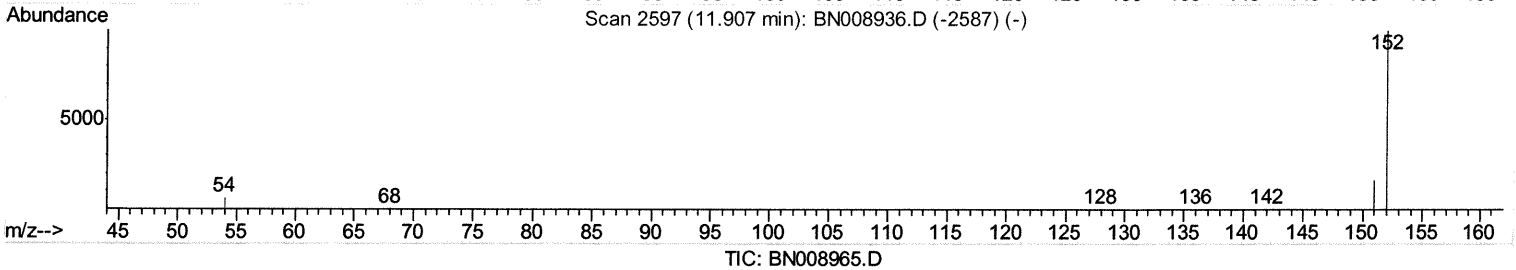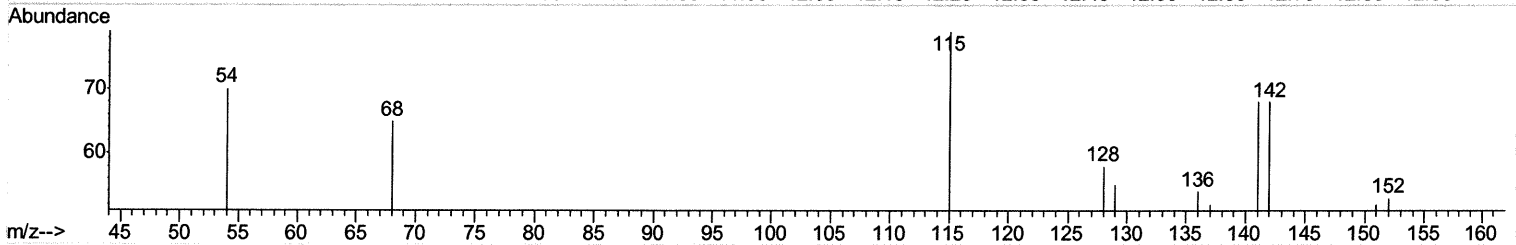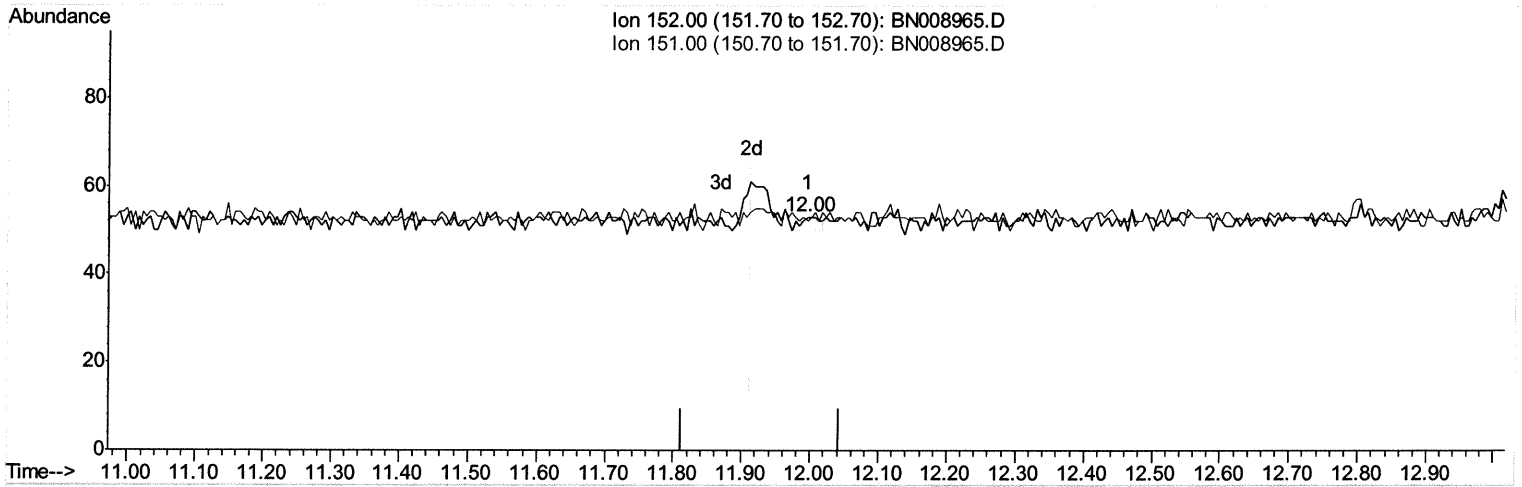

(4) 2-Methylnaphthalene-d10 (SURR)

11.995min (+0.082) 0.00ng/ul




response 6

Ion	Exp%	Act%
152.00	100	100
151.00	19.50	16.67
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121319\
Data File : BN008965.D
Acq On : 13 Dec 2019 13:26
Operator : JU
Sample : K6089-07DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 14:15:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

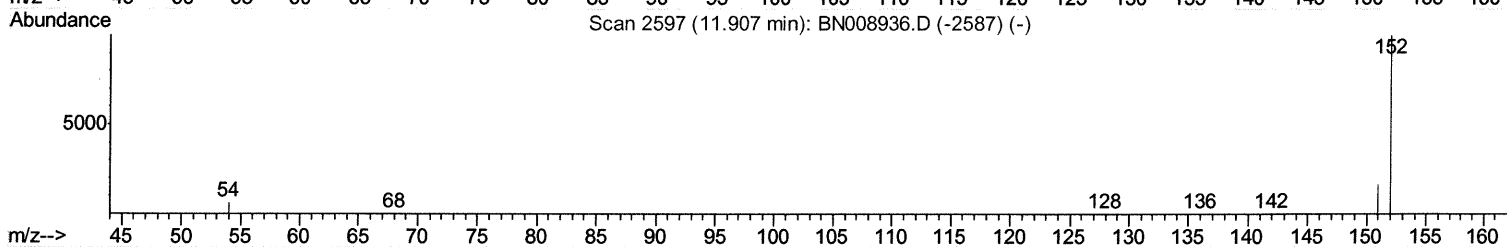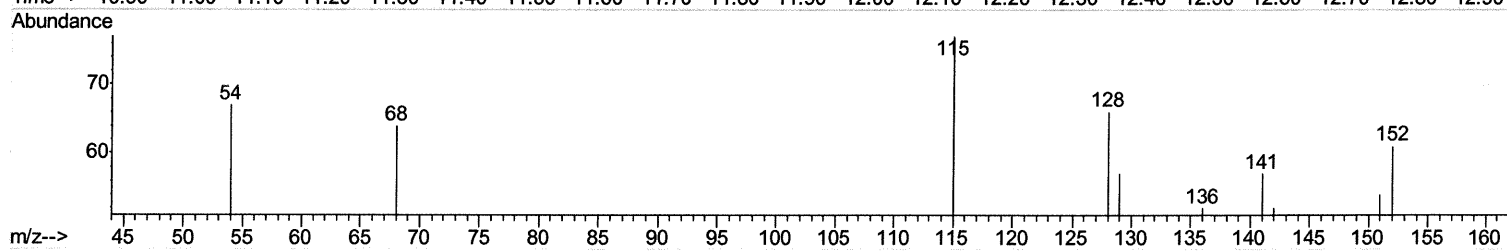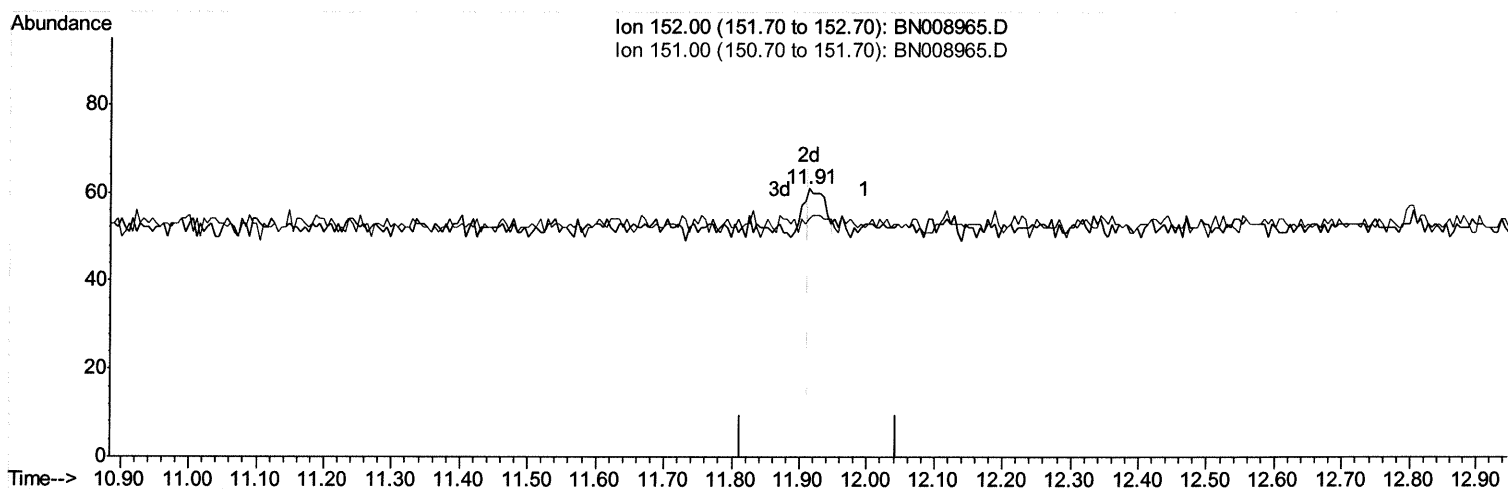

TIC: BN008965.D

(4) 2-Methylnaphthalene-d10 (SURR)

11.913min (-0.000) 0.00ng/ul m **Ju 12/16/19**

response 29

Ion	Exp%	Act%
152.00	100	100
151.00	19.50	3.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121319\
Data File : BN008966.D
Acq On : 13 Dec 2019 14:02
Operator : JU
Sample : K6089-14DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 13 14:38:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 12 00:49:42 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	5607	0.40	ng/ul	0.00
2) Naphthalene-d8	10.31	136	23061	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.18	164	14945	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.93	188	33233	0.40	ng/ul	0.00
16) Chrysene-d12	21.13	240	24736	0.40	ng/ul	0.00
20) Perylene-d12	23.27	264	21545	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.91	152	28	0.00	ng/ul	0.00
14) Fluoranthene-d10	18.96	212	42	0.00	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed