

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121418\
 Data File : BN003934.D
 Acq On : 14 Dec 2018 16:46
 Operator : JU/SJ
 Sample : J6270-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E14

Quant Time: Dec 14 22:54:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 14 22:50:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	31181	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	153186	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	94689	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	230050	20.00	ng/ul	0.00
77) Chrysene-d12	21.39	240	304542	20.00	ng/ul	0.00
85) Perylene-d12	23.71	264	320451	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	1652	3.47	ng/uL	0.00
5) Phenol-d5	6.99	99	57072	18.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	31908	19.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	46964	19.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	47374	18.44	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	24381	20.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	27689	20.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	50022	19.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	62341	26.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	161230	19.08	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	205304	20.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.66	143	29494	16.88	ng/ul	0.00
57) Fluorene-d10	15.46	176	149455	20.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.58	200	11566	6.98	ng/ul	0.00
70) Anthracene-d10	17.31	188	242262	20.84	ng/ul	0.00
78) Pyrene-d10	19.60	212	294384	21.61	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.56	264	378814	21.79	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	7.02	94	12048	3.894	ng/ul 99
44) Dimethylphthalate	13.92	163	30716	3.723	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121418\
Data File : BN003934.D
Acq On : 14 Dec 2018 16:46
Operator : JU/SJ
Sample : J6270-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E14

Quant Time: Dec 14 22:54:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 14 22:50:59 2018
Response via : Initial Calibration

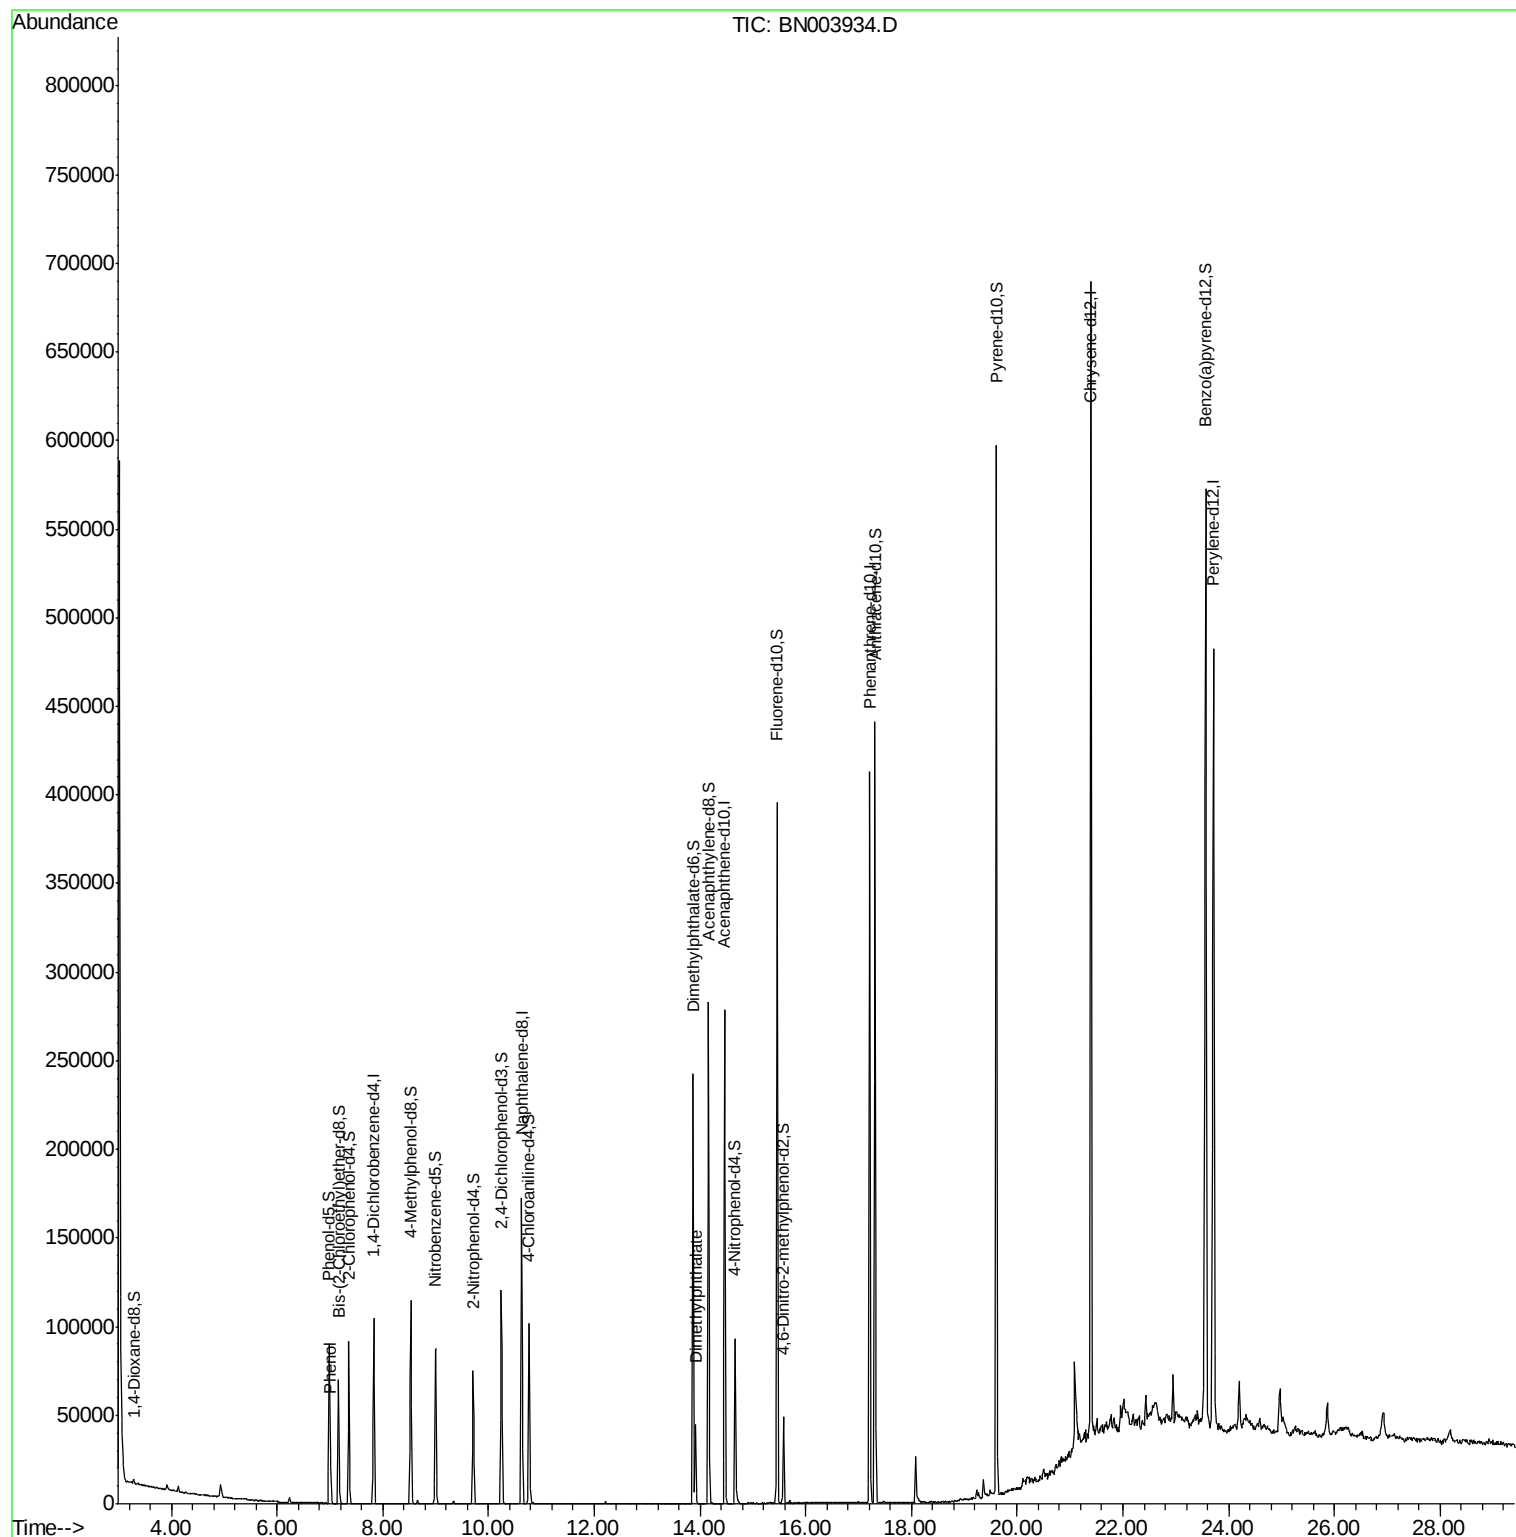

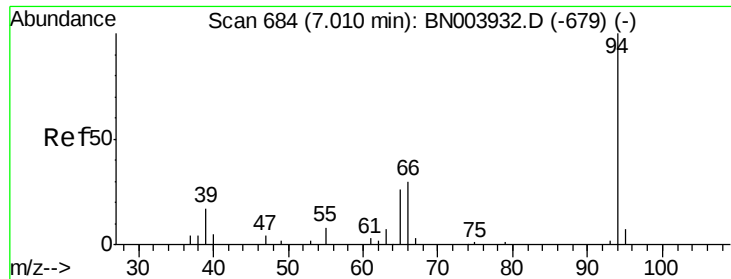

#6

Phenol

Concen: 3.894 ng/ul

RT: 7.02 min Scan# 685

Delta R.T. 0.01 min

Lab File: BN003934.D

Acq: 14 Dec 2018 16:46

Instrument :

BNA_N

ClientSampleId :

F9E14


Tot Ion: 94 Resp: 12048

Ion Ratio Lower Upper

94 100

65 27.1 21.2 31.8

66 34.5 26.9 40.3



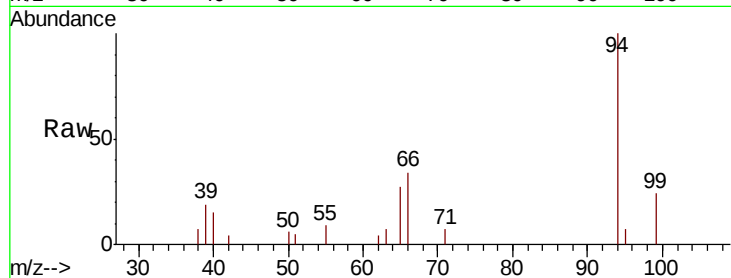


Abundance

Ion 94.00 (93.70 to 94.70): BN003932.D (-679) (-)

Ion 65.00 (64.70 to 65.70): BN003932.D (-679) (-)

Ion 66.00 (65.70 to 66.70): BN003932.D (-679) (-)

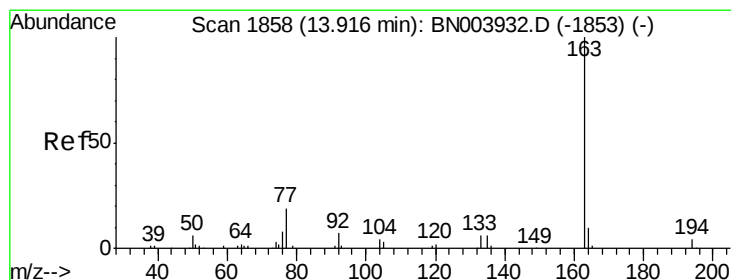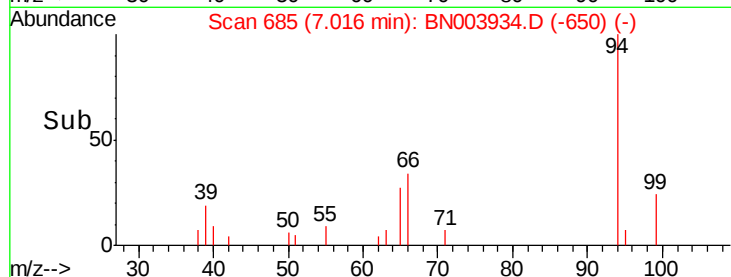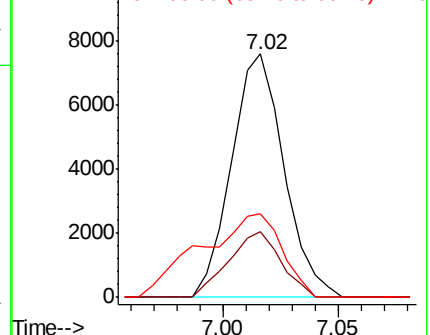

#44

Dimethylphthalate

Concen: 3.723 ng/ul

RT: 13.92 min Scan# 1858

Delta R.T. 0.00 min

Lab File: BN003934.D

Acq: 14 Dec 2018 16:46


Tgt Ion:163 Resp: 30716

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 9.9 7.9 11.9

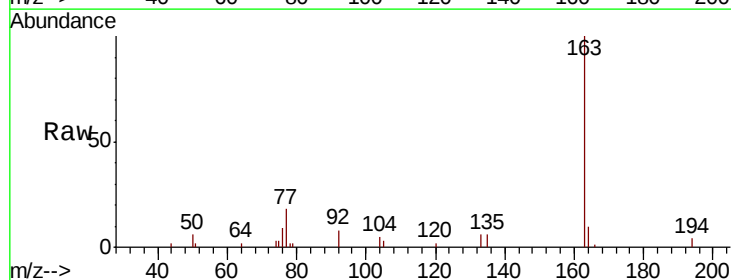

Abundance

Ion 163.00 (162.70 to 163.70): BN003932.D (-1853) (-)

Ion 194.00 (193.70 to 194.70): BN003932.D (-1853) (-)

Ion 164.00 (163.70 to 164.70): BN003932.D (-1853) (-)

