
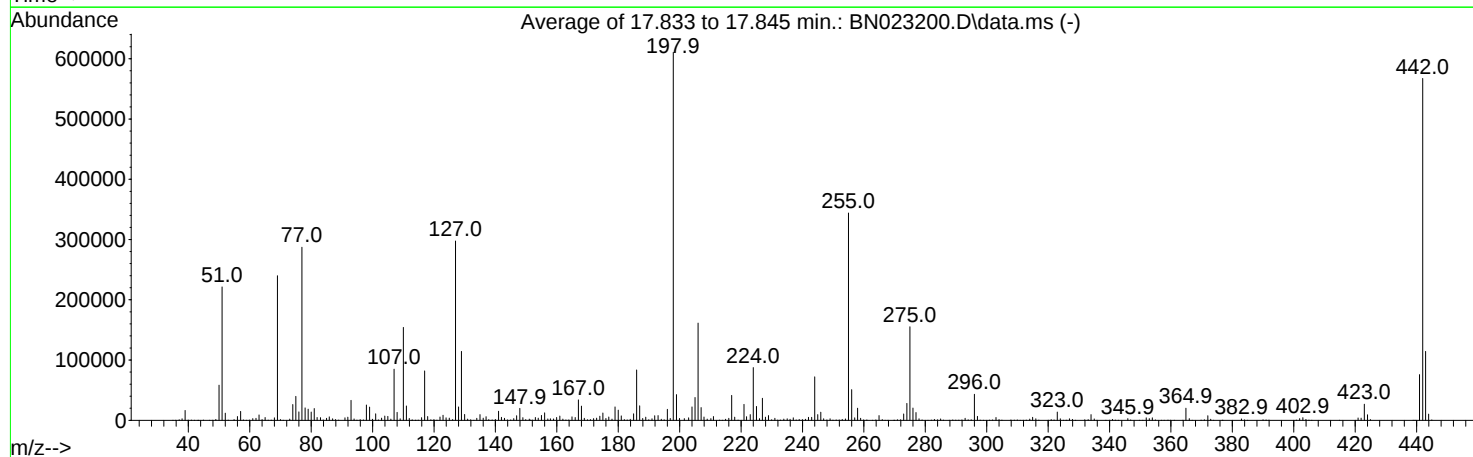


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121422\
 Data File : BN023200.D
 Acq On : 14 Dec 2022 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 12 05:18:26 2022

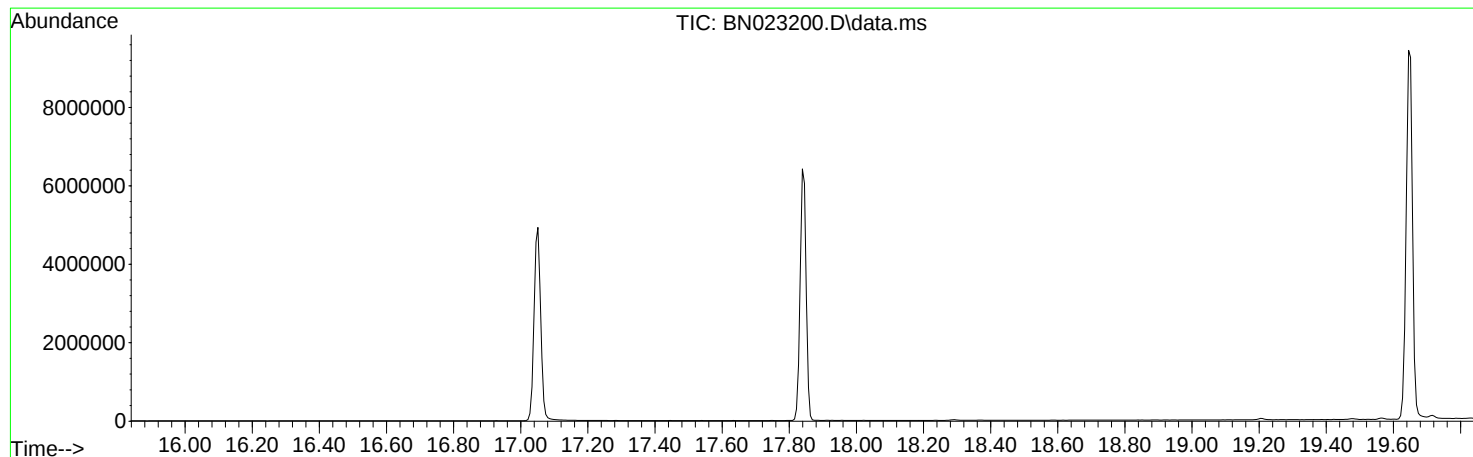




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	221312	PASS
68	69	0.00	2	1.7	4112	PASS
69	198	0.00	100	39.3	239957	PASS
70	69	0.00	2	0.5	1300	PASS
127	198	10	80	48.8	297643	PASS
197	198	0.00	2	0.5	2971	PASS
198	198	100	100	100.0	610517	PASS
199	198	5	9	7.0	42683	PASS
275	198	10	60	25.4	155320	PASS
365	198	1	100	3.3	19986	PASS
441	198	0.01	100	12.4	75819	PASS
442	442	50	100	100.0	567296	PASS
443	442	15	24	20.1	114237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121422\
 Data File : BN023200.D
 Acq On : 14 Dec 2022 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 05:45:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 05:45:01 2022
 Response via : Initial Calibration

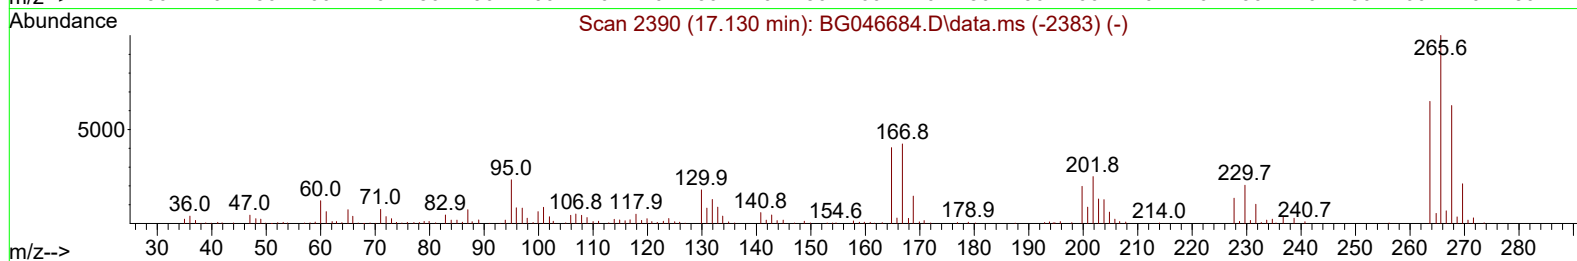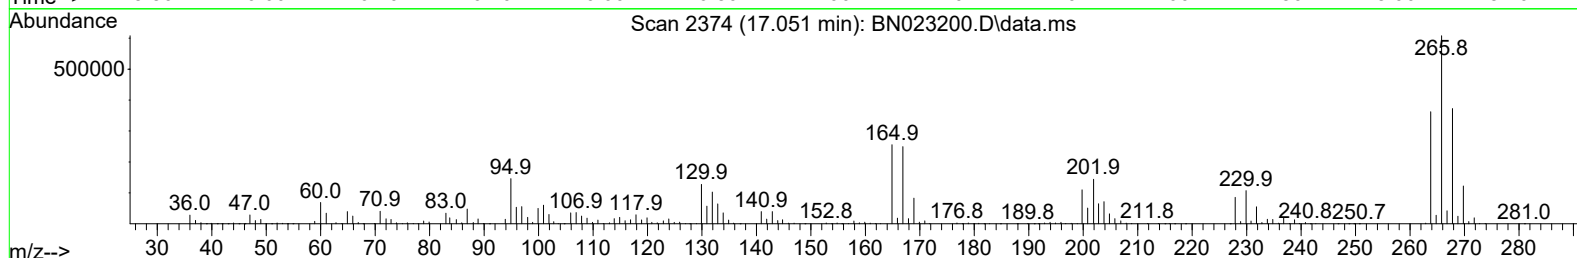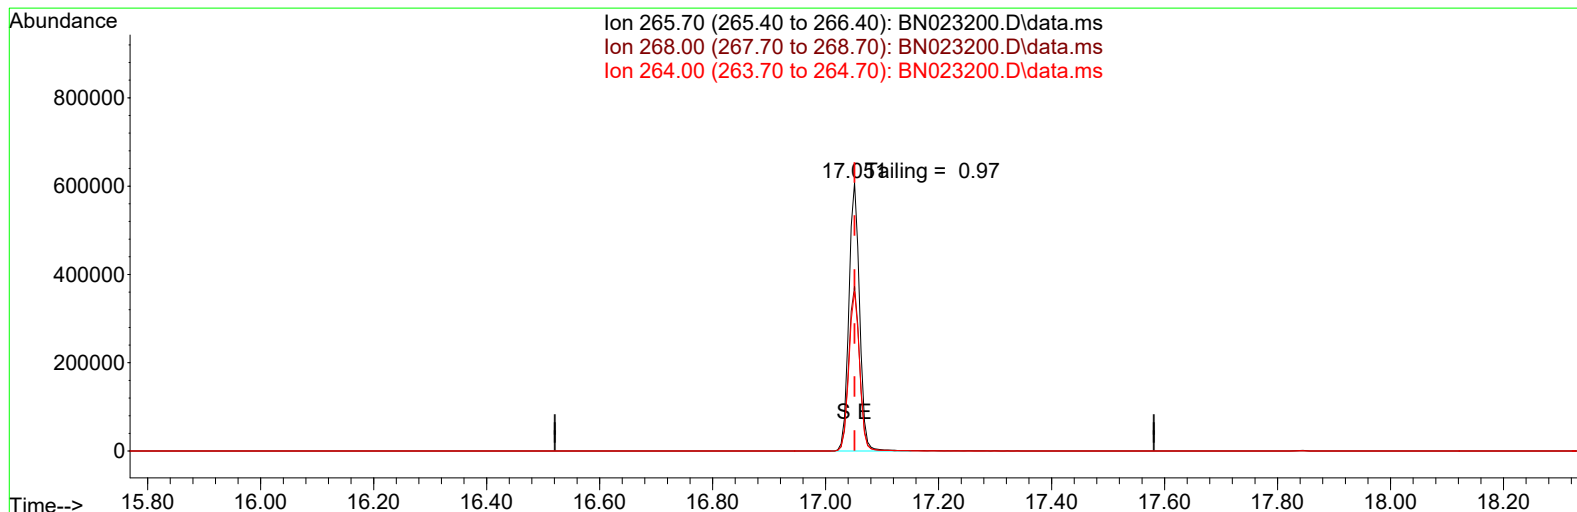

TIC: BN023200.D\data.ms

(70) Pentachlorophenol (C)

17.051min (0.000) 24941.15 ng




response 803675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.25
264.00	61.60	59.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121422\
 Data File : BN023200.D
 Acq On : 14 Dec 2022 14:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 15 05:45:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 15 05:45:01 2022
 Response via : Initial Calibration

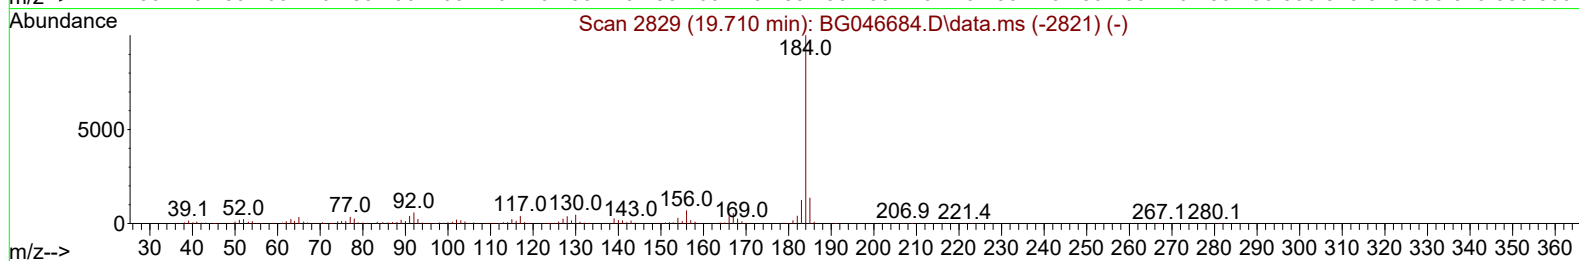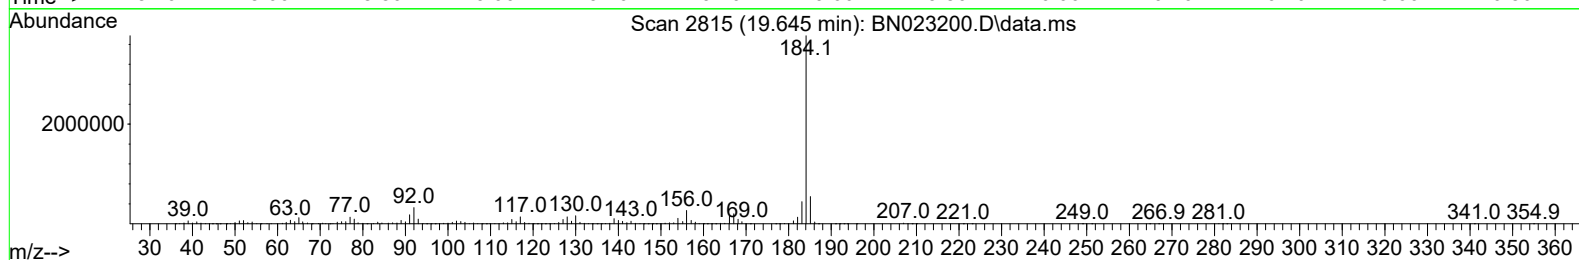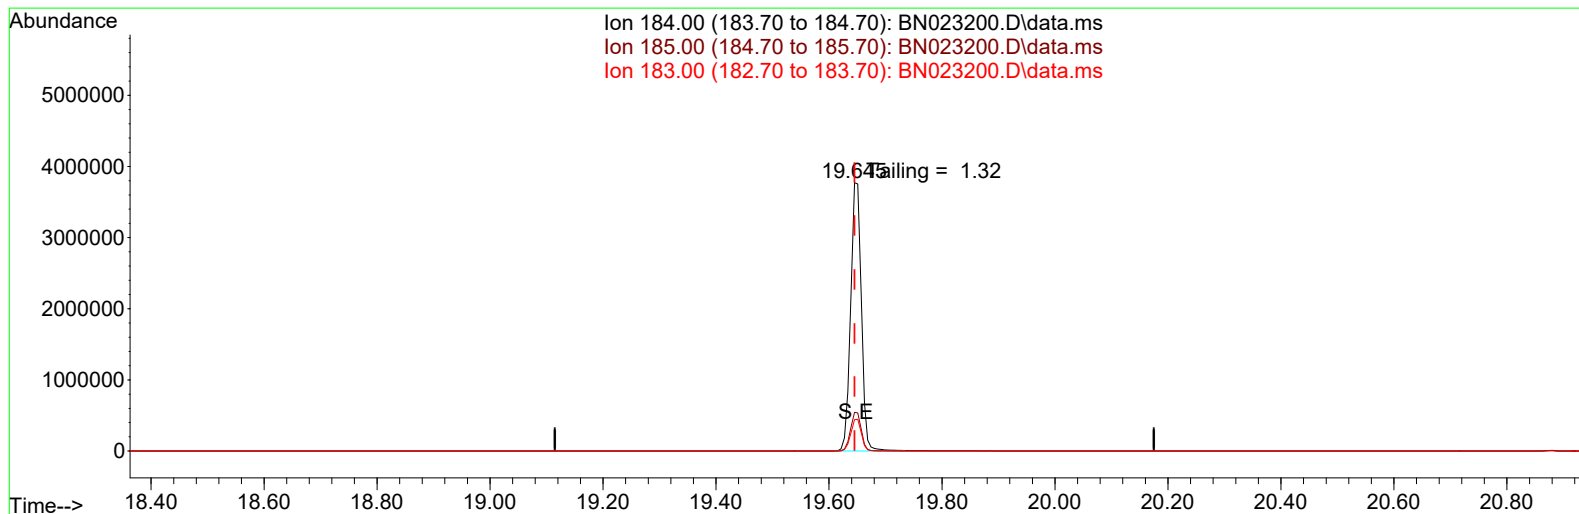

TIC: BN023200.D\data.ms

(77) Benzidine

19.645min (0.000) 215410.78 ng

response 4973448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2022	BNA_N	<u>BN023200.D</u>
Compound Name	Response	Retention Time
DDT	2143223	20.88
DDD	54141	20.433
DDE	1462	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
55603	2198826	2.53

Instrument :
BNA_N
ClientSampleId :
DFTPP