

Data File : BN003971.D
Acq On : 15 Dec 2018 22:46
Operator : JU/SJ
Sample : J6171-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y10DL

Quant Time: Dec 15 23:26:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	2058	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	10406	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	6224	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	15553	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	20164	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	18268	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	478	0.03	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1469	0.03	ng/ul	0.00
Target Compounds				Qvalue		
5) 2-Methylnaphthalene	12.29	142	539	0.026	ng/ul	97
12) Phenanthrene	17.26	178	2169	0.042	ng/ul#	91
15) Fluoranthene	19.27	202	3509	0.058	ng/ul	91
17) Pyrene	19.63	202	4844	0.067	ng/ul#	91
18) Benzo(a)anthracene	21.38	228	2314	0.036	ng/ul#	68
19) Chrysene	21.43	228	4112	0.056	ng/ul#	79
21) Benzo(b)fluoranthene	23.01	252	6164	0.082	ng/ul#	36
22) Benzo(k)fluoranthene	23.01	252	6120	0.083	ng/ul#	36
23) Benzo(a)pyrene	23.61	252	2169	0.033	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	26.07	276	2108	0.028	ng/ul#	97
26) Benzo(g,h,i)perylene	26.79	276	2639	0.040	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003971.D
Acq On : 15 Dec 2018 22:46
Operator : JU/SJ
Sample : J6171-06DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y10DL

Quant Time: Dec 15 23:26:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

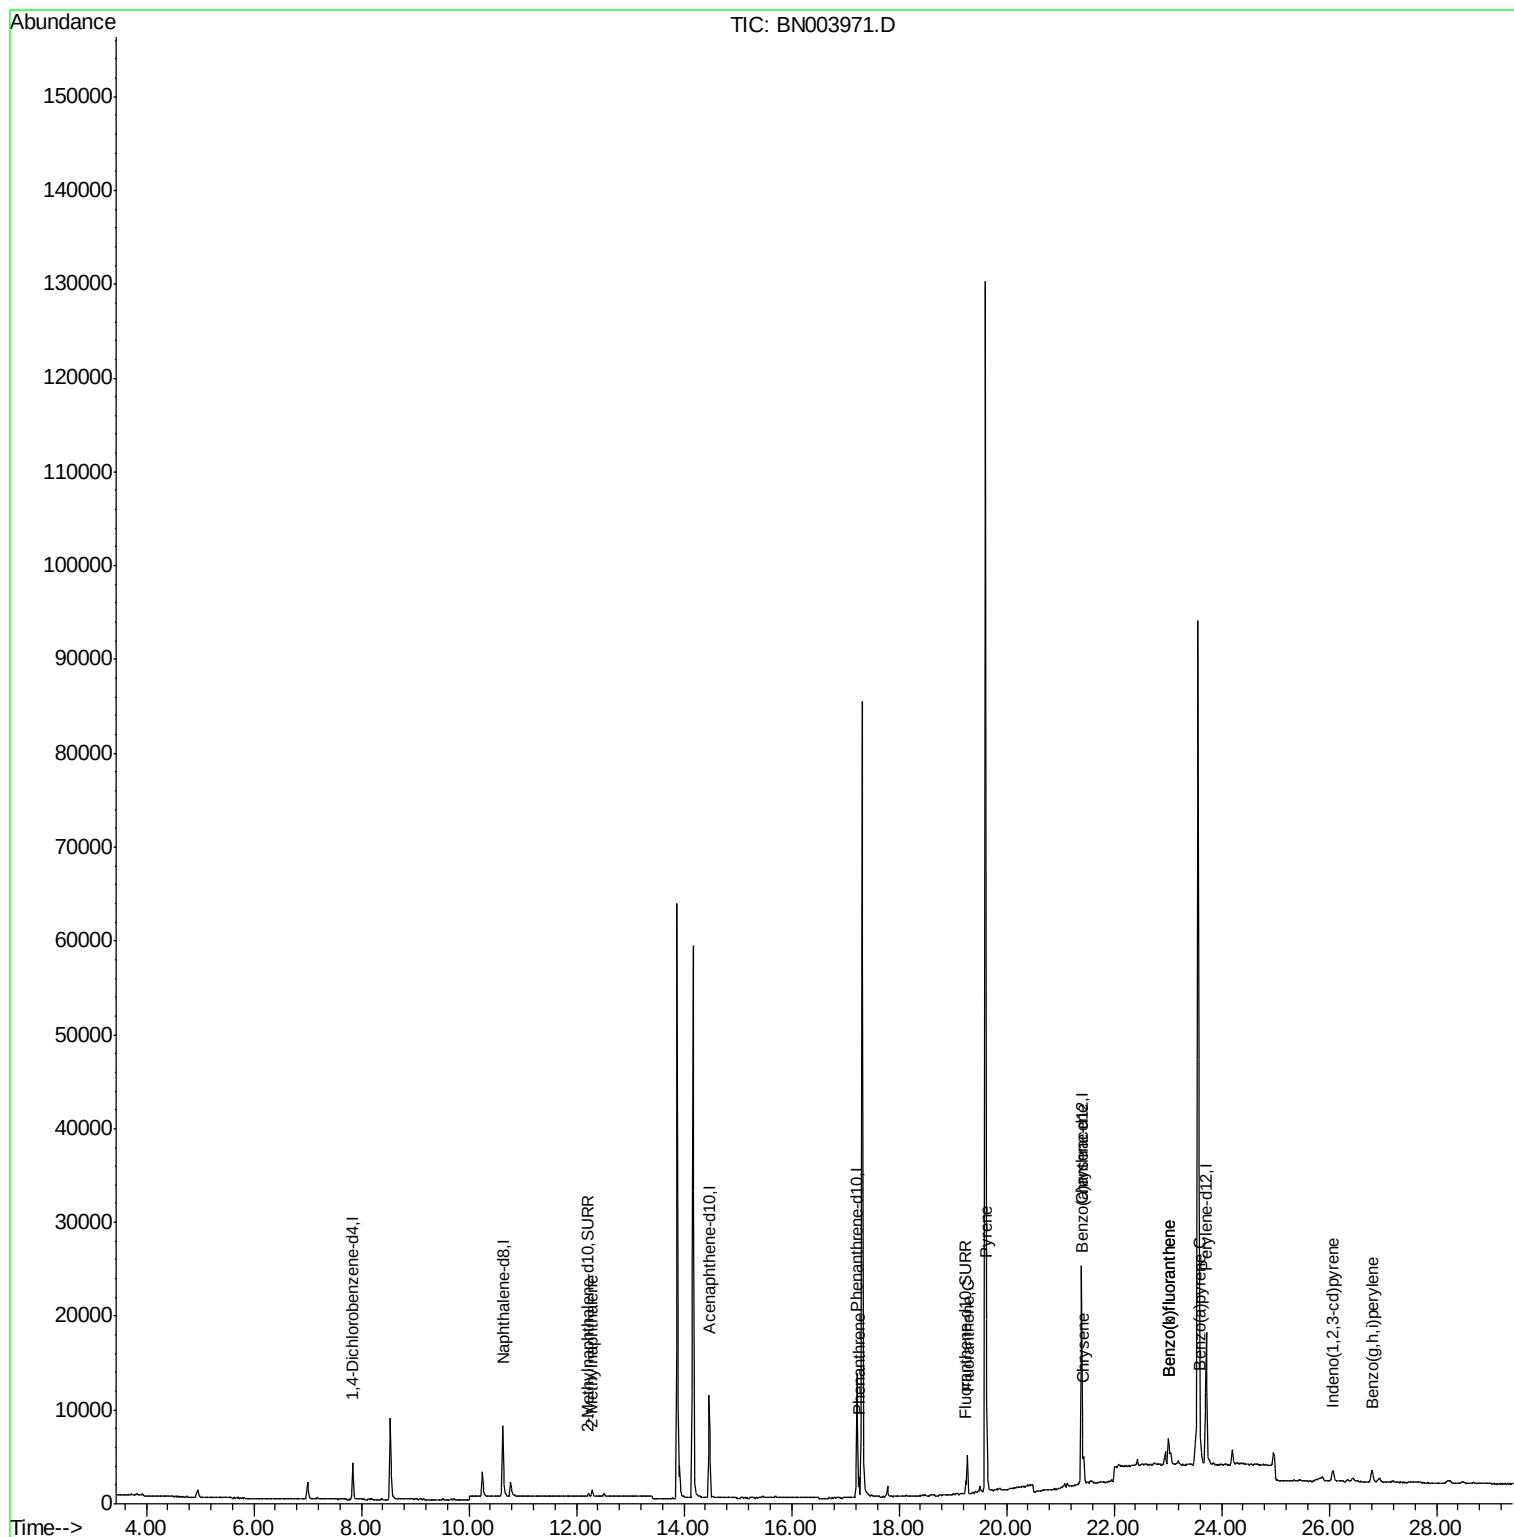

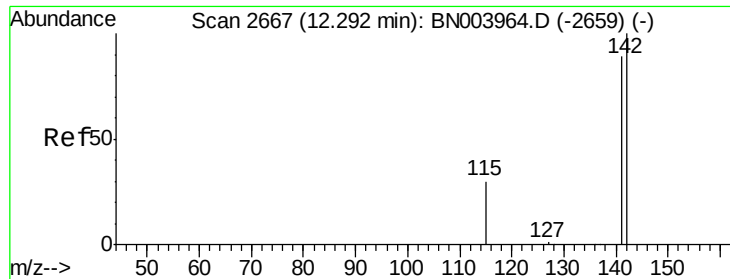

#5

2-Methylnaphthalene

Concen: 0.026 ng/ul

RT: 12.29 min Scan# 2667

Delta R.T. 0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46

Instrument :

BNA_N

ClientSampleId :


F9Y10DL

Tgt Ion:142 Resp: 539

Ion Ratio Lower Upper

142 100

141 86.6 71.5 107.3

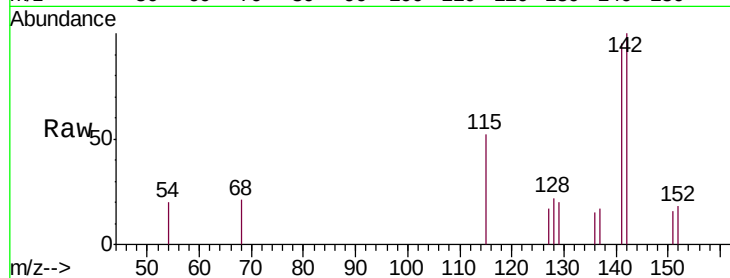

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.29

400



300

200

100

0

Time-->

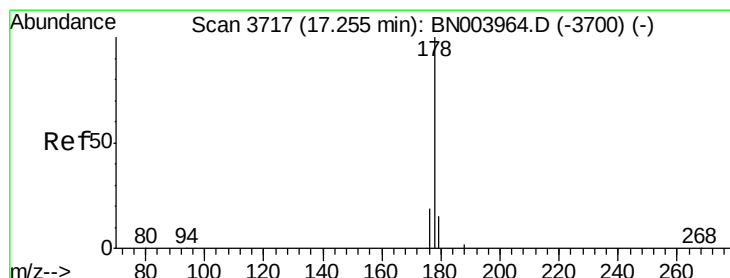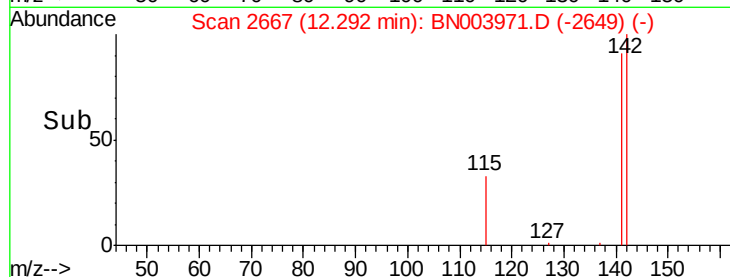

#12

Phenanthrene

Concen: 0.042 ng/ul

RT: 17.26 min Scan# 3718

Delta R.T. 0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46


Tgt Ion:178 Resp: 2169

Ion Ratio Lower Upper

178 100

179 20.2 12.5 18.7#

176 21.7 15.0 22.4

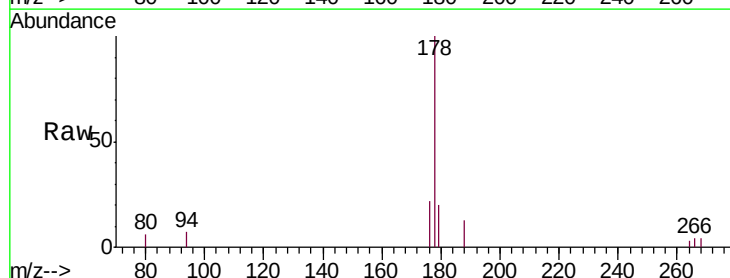

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

17.26

2000


1500


1000

500

0

Time-->

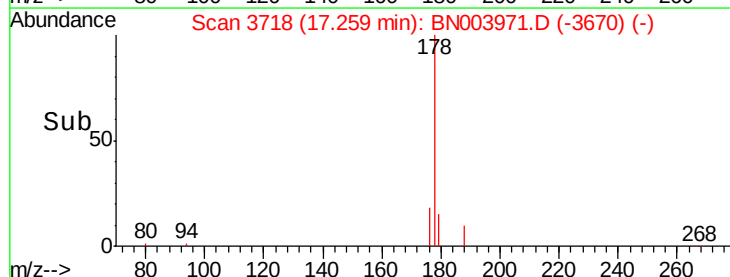


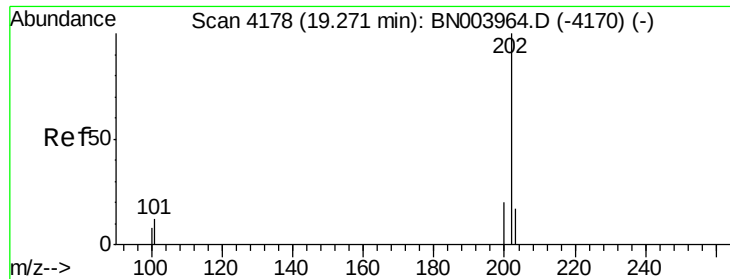




#15
Fluoranthene
Concen: 0.058 ng/ul
RT: 19.27 min Scan# 4178
Delta R.T. 0.00 min
Lab File: BN003971.D
Acq: 15 Dec 2018 22:46

Instrument :
BNA_N
ClientSampleId :
F9Y10DL

Tgt Ion:	202	Resp:	3509
Ion	Ratio	Lower	Upper
202	100		
101	14.3	0.0	30.7
100	10.7	0.0	28.1

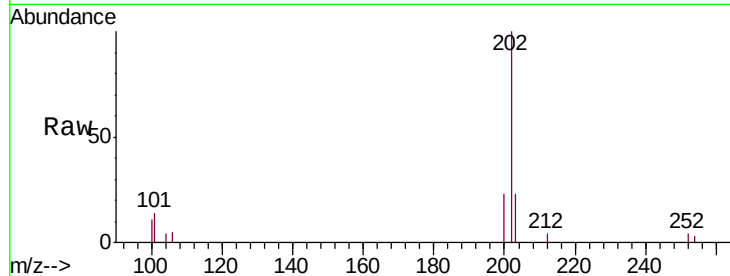


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

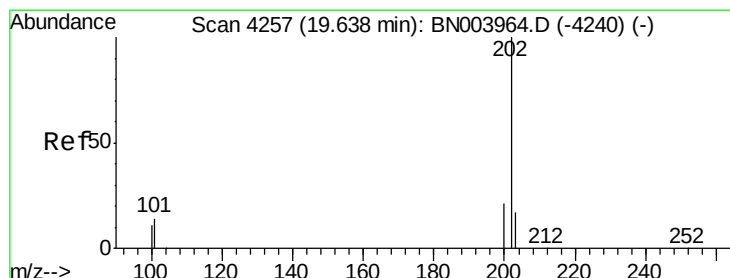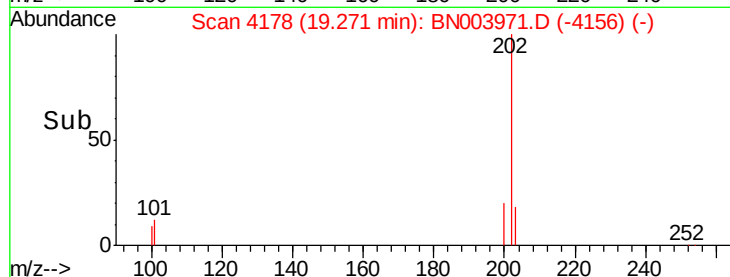
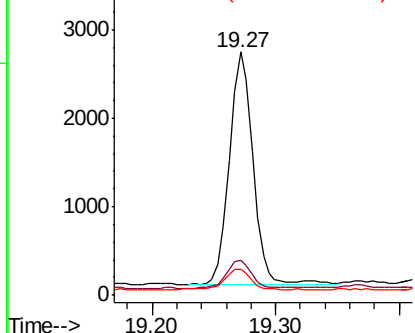



#17
Pyrene
Concen: 0.067 ng/ul
RT: 19.63 min Scan# 4256
Delta R.T. -0.00 min
Lab File: BN003971.D
Acq: 15 Dec 2018 22:46

Tgt Ion:	202	Resp:	4844
Ion	Ratio	Lower	Upper
202	100		
101	16.7	10.3	15.5#
100	13.4	8.5	12.7#

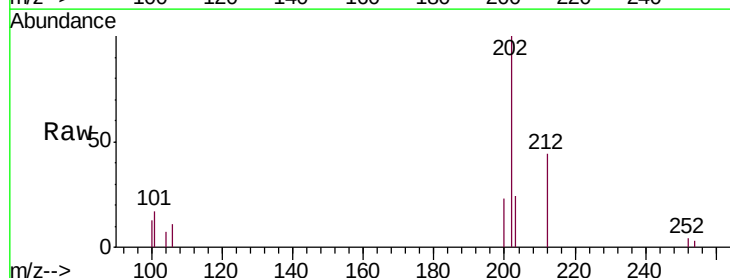

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

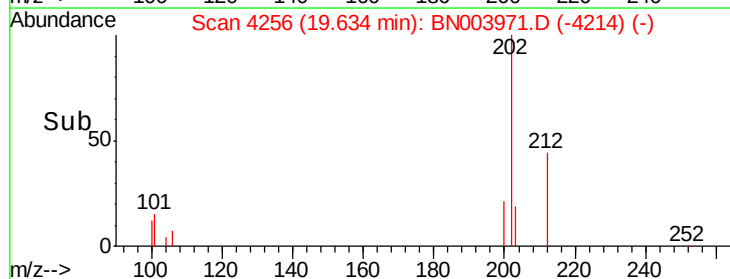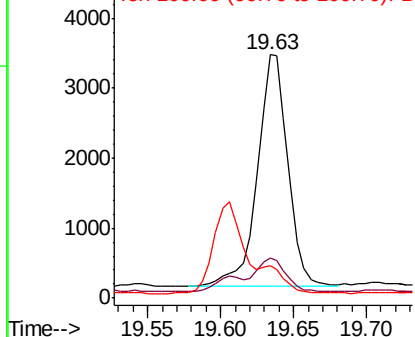

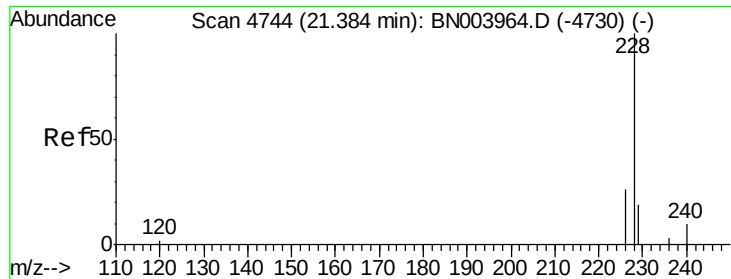

#18

Benzo(a)anthracene

Concen: 0.036 ng/ul

RT: 21.38 min Scan# 4744

Delta R.T. -0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46

Instrument :

BNA_N

ClientSampleId :

F9Y10DL


Tgt Ion:228 Resp: 2314

Ion Ratio Lower Upper

228 100

229 39.9 15.6 23.4#

226 38.3 21.1 31.7#



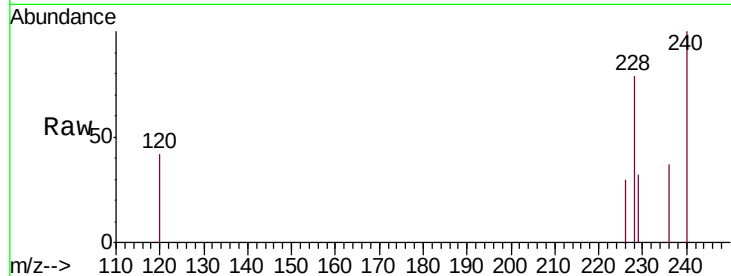


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

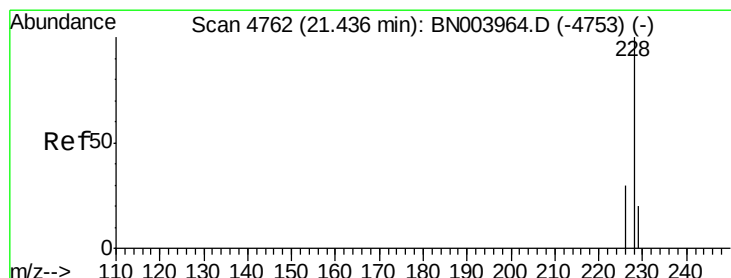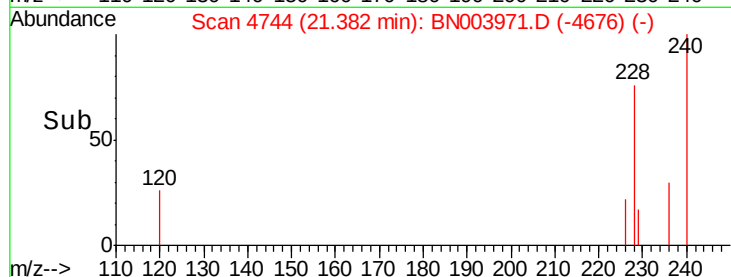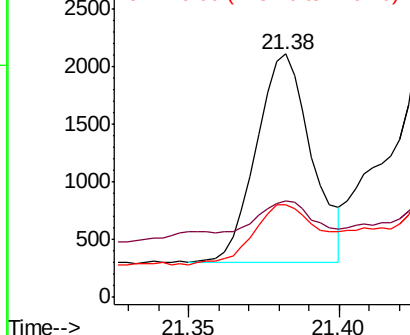

#19

Chrysene

Concen: 0.056 ng/ul

RT: 21.43 min Scan# 4762

Delta R.T. -0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46


Tgt Ion:228 Resp: 4112

Ion Ratio Lower Upper

228 100

226 37.8 24.0 36.0#

229 34.2 15.7 23.5#


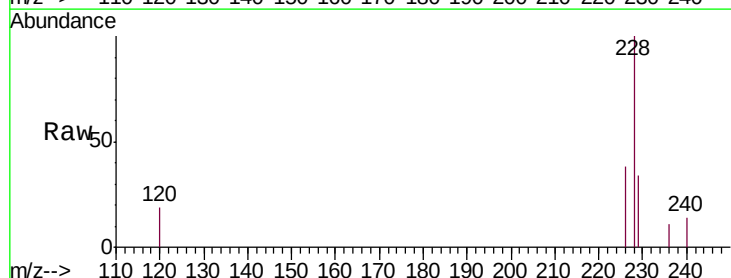



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

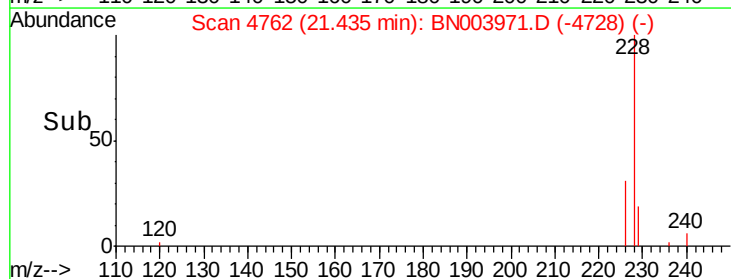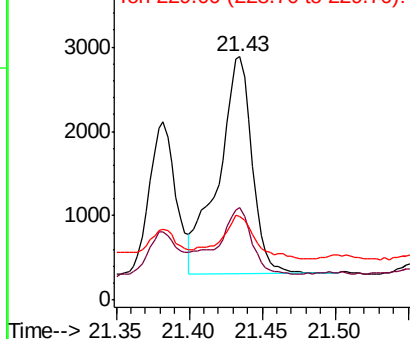

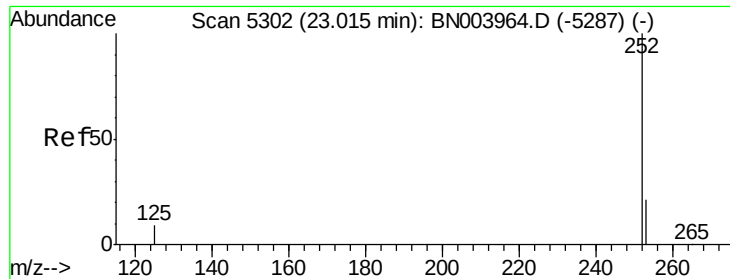

#21

Benzo(b)fluoranthene

Concen: 0.082 ng/ul

RT: 23.01 min Scan# 5301

Delta R.T. -0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46

Instrument :

BNA_N

ClientSampleId :

F9Y10DL


Tgt Ion:252 Resp: 6164

Ion Ratio Lower Upper

252 100

253 43.1 0.0 46.0




125 53.5 0.0 22.4#

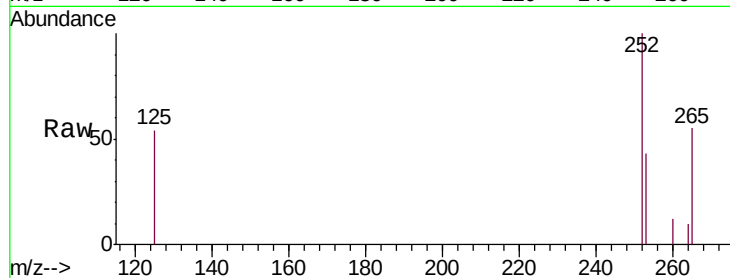

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

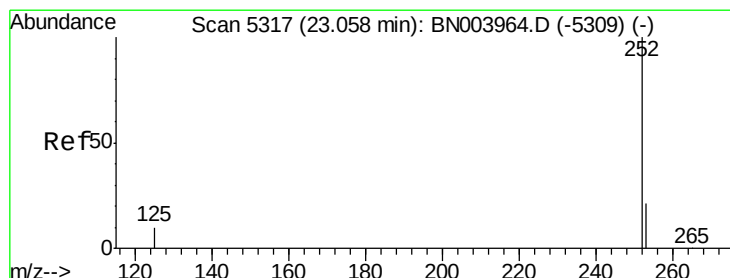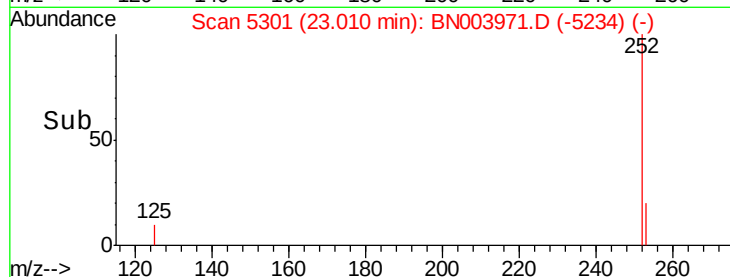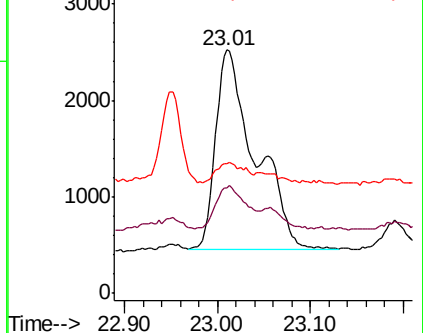

#22

Benzo(k)fluoranthene

Concen: 0.083 ng/ul

RT: 23.01 min Scan# 5301

Delta R.T. -0.05 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46


Tgt Ion:252 Resp: 6120

Ion Ratio Lower Upper

252 100

253 43.1 18.5 27.7#



125 53.5 9.0 13.6#

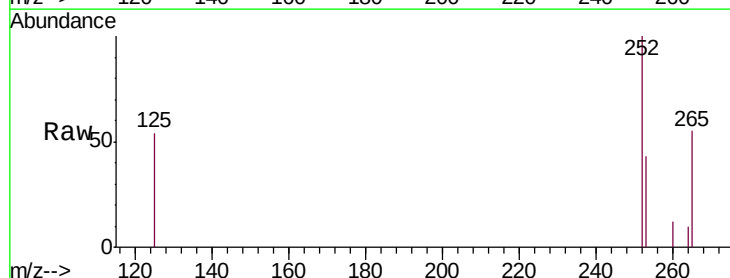


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

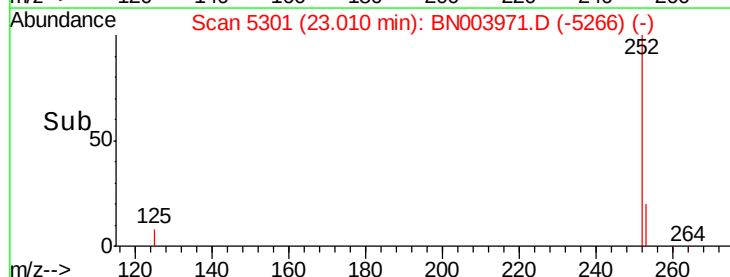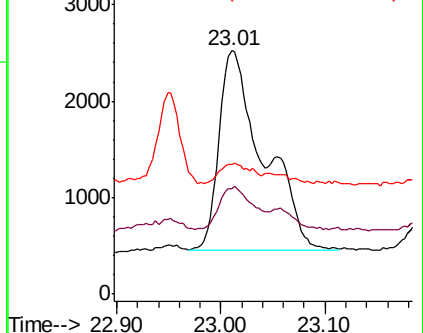

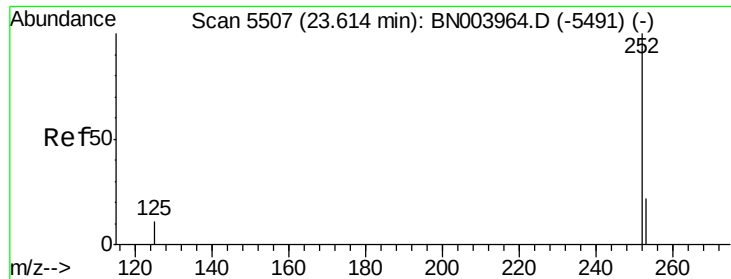

#23

Benzo(a)pyrene

Concen: 0.033 ng/ul

RT: 23.61 min Scan# 5507

Delta R.T. -0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46

Instrument :

BNA_N

ClientSampleID :

F9Y10DL


Tgt Ion: 252 Resp: 2169

Ion Ratio Lower Upper

252 100

253 57.9 19.0 28.4#




125 78.5 10.2 15.4#

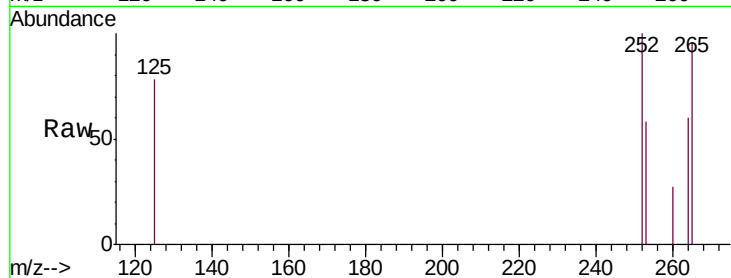

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

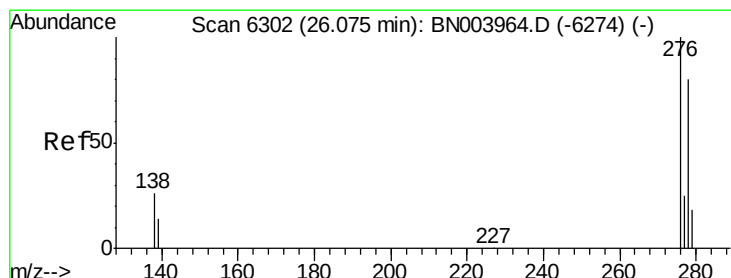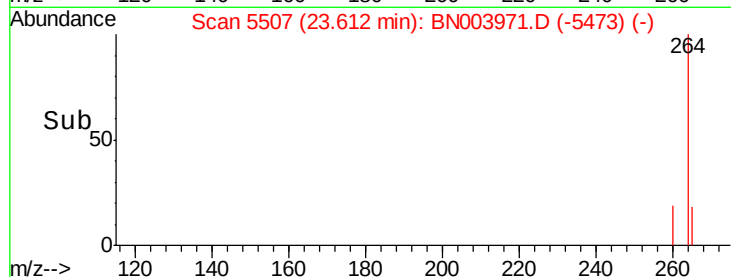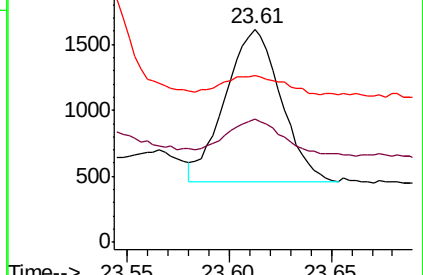

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.028 ng/ul

RT: 26.07 min Scan# 6301

Delta R.T. -0.00 min

Lab File: BN003971.D

Acq: 15 Dec 2018 22:46


Tgt Ion: 276 Resp: 2108

Ion Ratio Lower Upper

276 100

138 23.8 20.3 30.5



227 0.9 0.2 0.2#

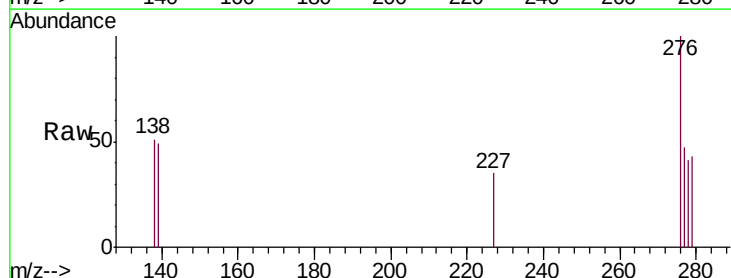


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

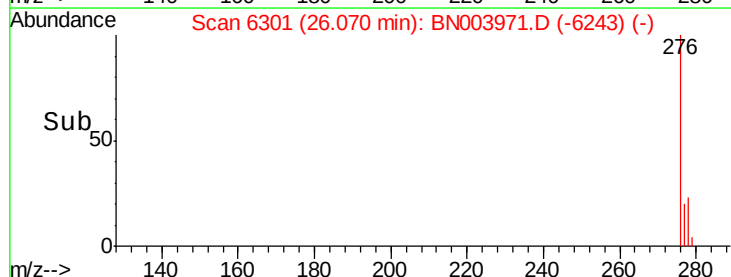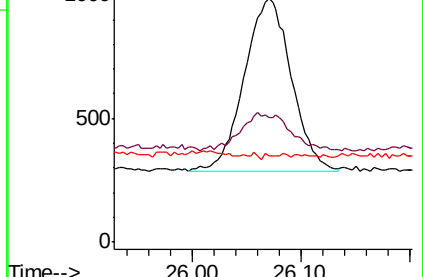

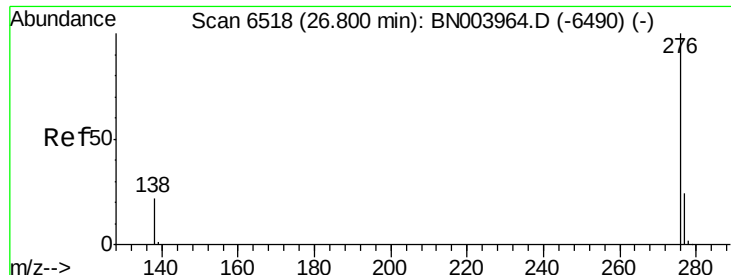

#26

Benzo(g,h,i)perylene

Concen: 0.040 ng/ul

RT: 26.79 min Scan# 6517

Delta R.T. -0.00 min

Lab File: BN003971.D


Acq: 15 Dec 2018 22:46

Instrument :

BNA_N

ClientSampleId :

F9Y10DL

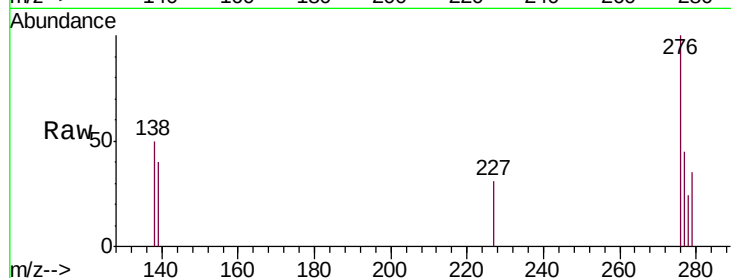


Tgt Ion: 276 Resp: 2639

Ion Ratio Lower Upper

276 100

138 50.4 17.7 26.5#

277 45.4 19.3 28.9#

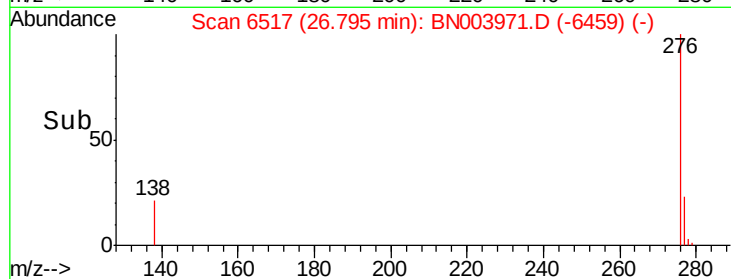

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

