

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121518\
Quantitation Report (QT Reviewed)


Data File : BN003969.D
Acq On : 15 Dec 2018 21:35
Operator : JU/SJ
Sample : J6171-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y07DL

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:22:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

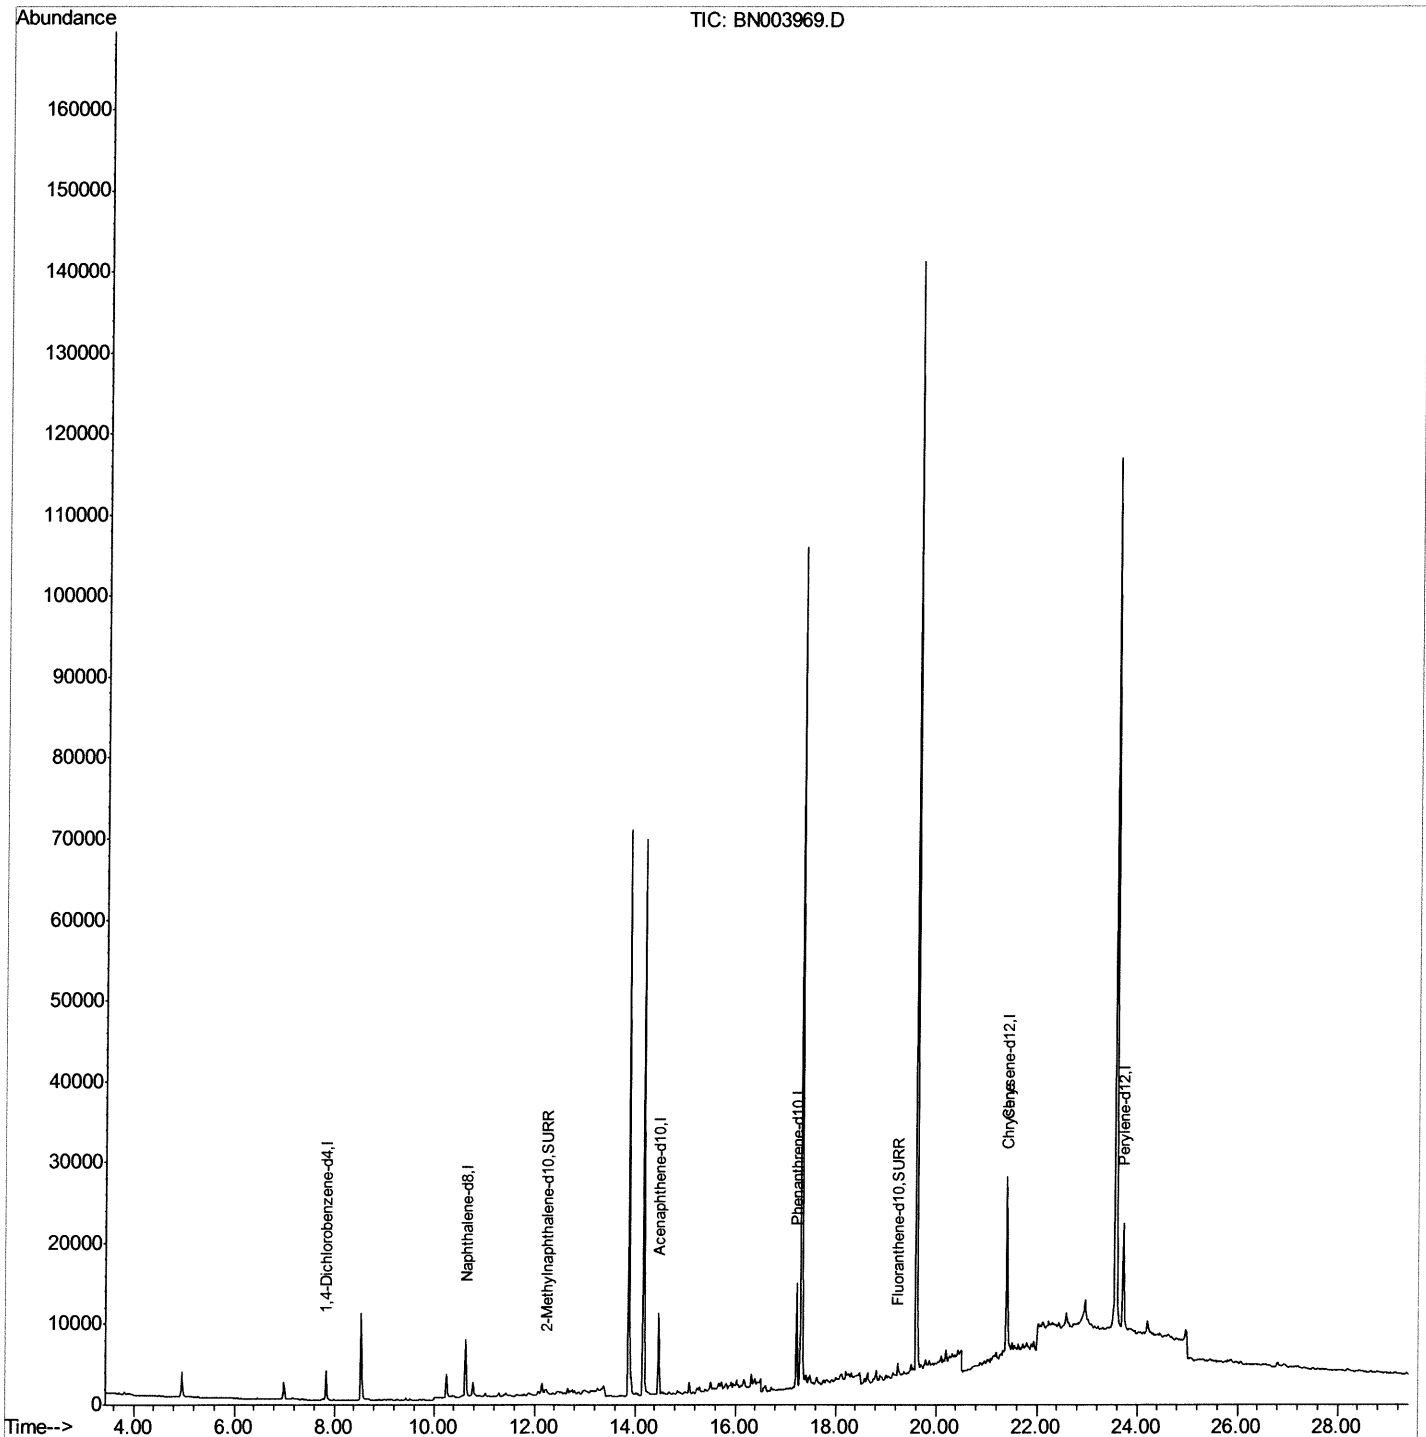

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121518\
Quantitation Report (Qedit)




Data File : BN003969.D
Acq On : 15 Dec 2018 21:35
Operator : JU/SJ
Sample : J6171-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9Y07DL

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:07:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

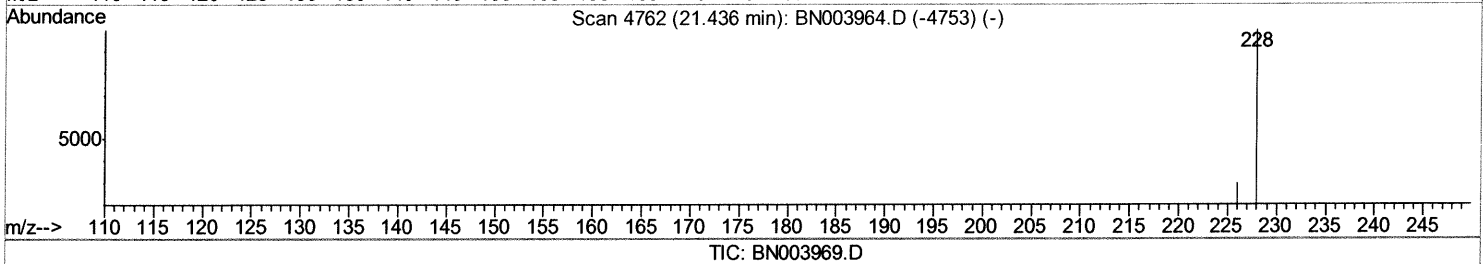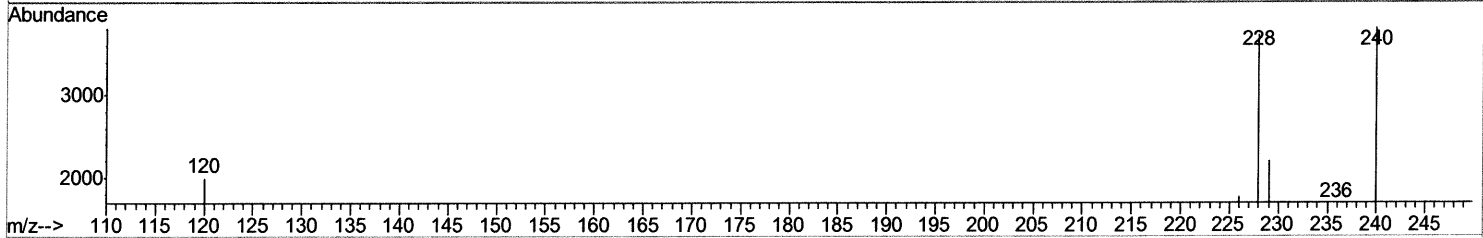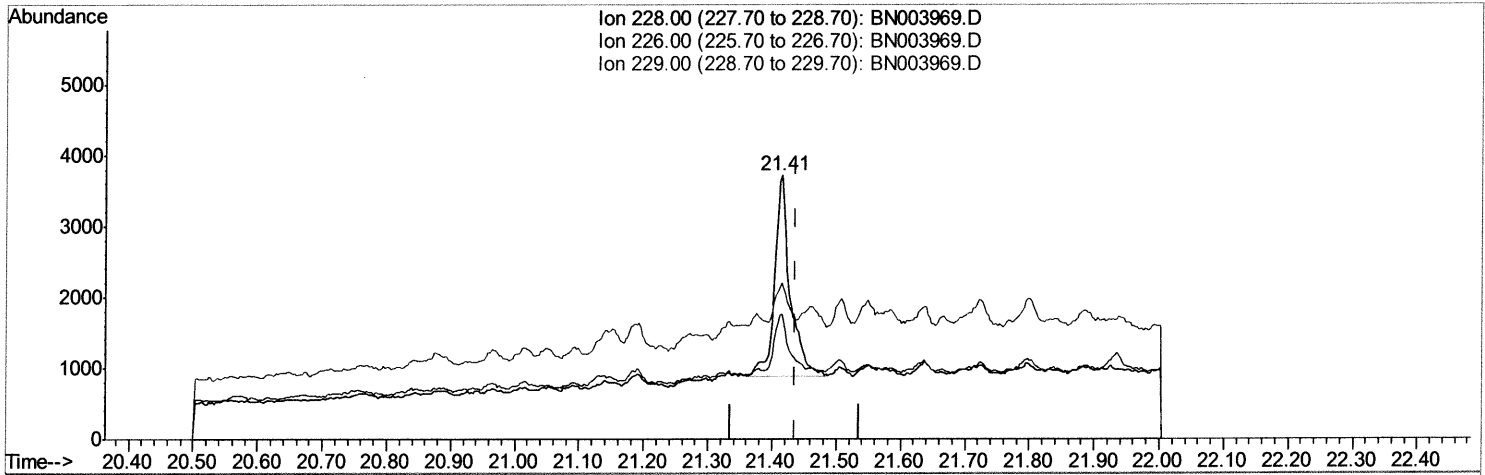

(19) Chrysene

21.414min (-0.022) 0.07ng/ul

response 4775

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	47.46#
229.00	19.60	59.01#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121518\
Quantitation Report (Qedit)




Data File : BN003969.D
Acq On : 15 Dec 2018 21:35
Operator : JU/SJ
Sample : J6171-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y07DL

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:07:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

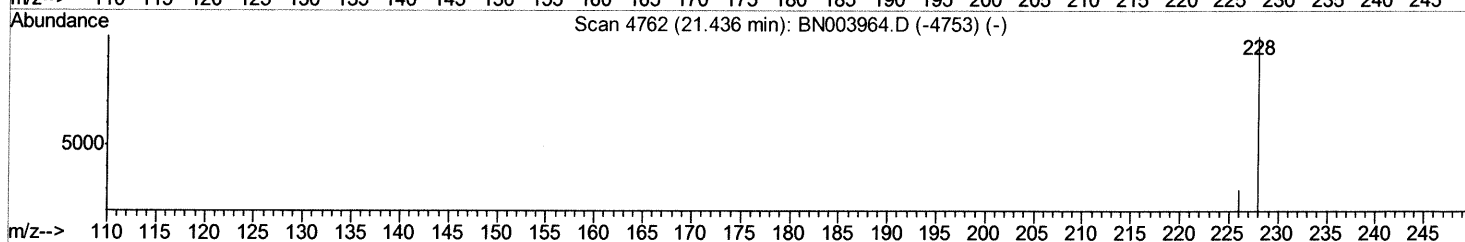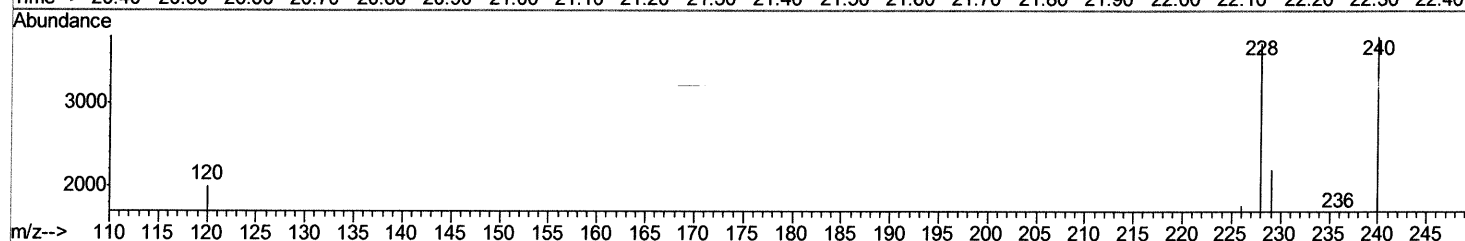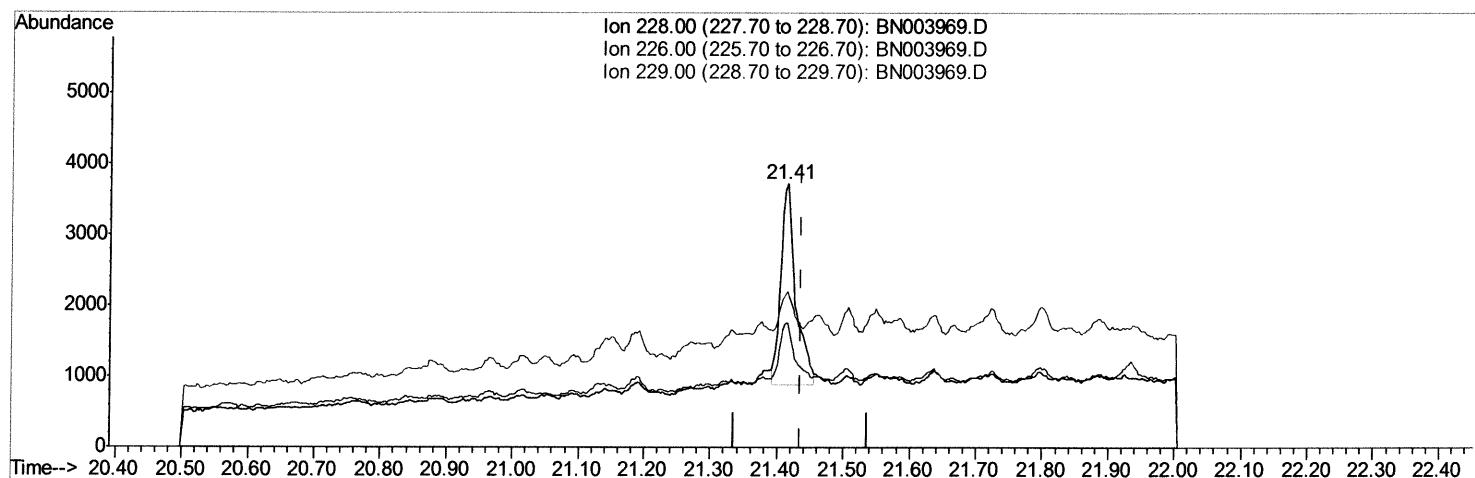

TIC: BN003969.D

(19) Chrysene

21.414min (-0.022) 0.07ng/ul m

SJ 12/17/18

response 4440

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	47.46#
229.00	19.60	59.01#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121518\
Quantitation Report (QT Reviewed)

Data File : BN003969.D
Acq On : 15 Dec 2018 21:35
Operator : JU/SJ
Sample : J6171-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y07DL

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:22:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1932	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	9529	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5916	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	14696	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	18608	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	17723	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	649	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1703	0.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) Chrysene	21.41	228	4440m)	0.066	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ

12/17/18