

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
 Data File : BN003966.D
 Acq On : 15 Dec 2018 19:49
 Operator : JU/SJ
 Sample : J6171-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y06

Manual Integrations
 APPROVED

Sohil
 12/17/2018 4:23:56 PM

Quant Time: Dec 15 23:15:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 23:04:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1986	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	9447	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5618	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	14351m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	17660m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	15596m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2737	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	9116m	0.22	ng/ul	0.00
Target Compounds						
26) Benzo(a,h,i)perylene	26.81	276	19530	0.351	ng/ul#	Ovalue 75

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
Data File : BN003966.D
Acq On : 15 Dec 2018 19:49
Operator : JU/SJ
Sample : J6171-02
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
F9Y06

Quant Time: Dec 15 23:15:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:56 PM

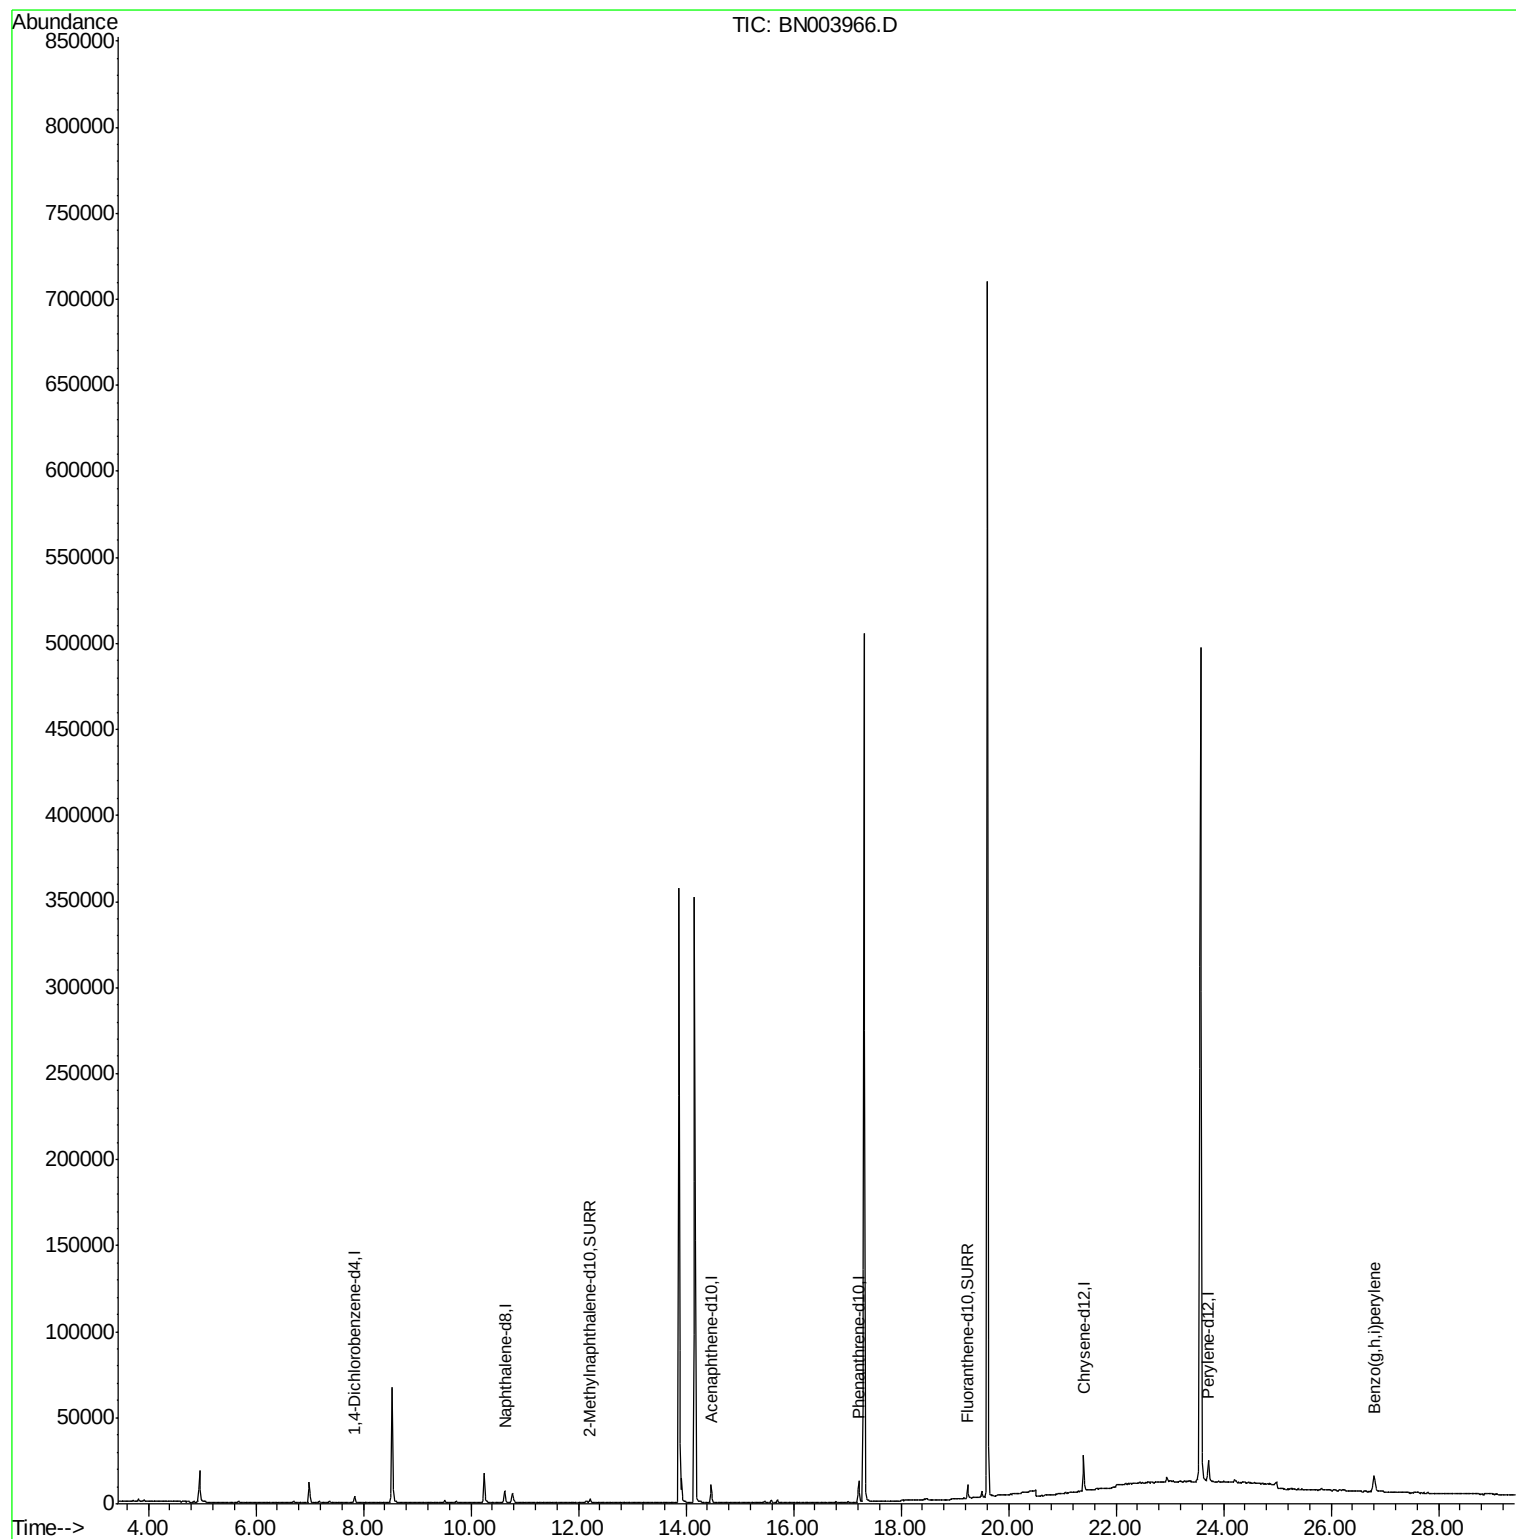

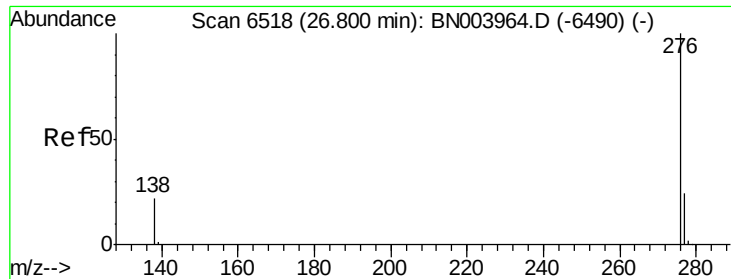


#26
 Benzo(a,h,i)perylene
 Concen: 0.351 ng/ul
 RT: 26.81 min Scan# 6520
 Delta R.T. 0.01 min
 Lab File: BN003966.D
 Acq: 15 Dec 2018 19:49

Instrument :
 BNA_N
 ClientSampleId :
 F9Y06

Tot Ion	Ratio	Lower	Upper
276	100		
138	37.1	17.7	26.5#
277	33.7	19.3	28.9#

Manual Integrations
 APPROVED

Sohil
 12/17/2018 4:23:56 PM

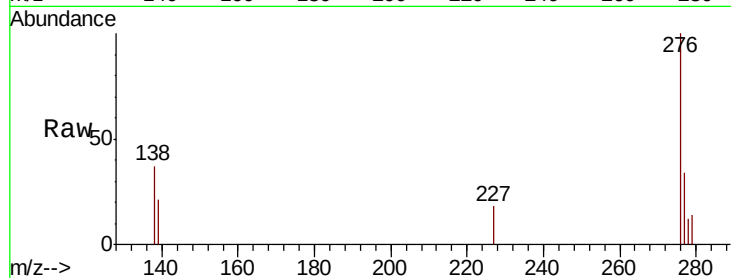

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

