

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
 Data File : BN003967.D
 Acq On : 15 Dec 2018 20:24
 Operator : JU/SJ
 Sample : J6171-02DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y06DL

Quant Time: Dec 15 23:07:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 23:04:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	2376	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	11711	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	6731	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	16536	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	19893	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	18457	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	664	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1989	0.04	ng/ul	0.00
Target Compounds						
26) Benzo(a,h,i)perylene	26.80	276	4530	0.069	ng/ul#	Ovalue 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
Data File : BN003967.D
Acq On : 15 Dec 2018 20:24
Operator : JU/SJ
Sample : J6171-02DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y06DL

Quant Time: Dec 15 23:07:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

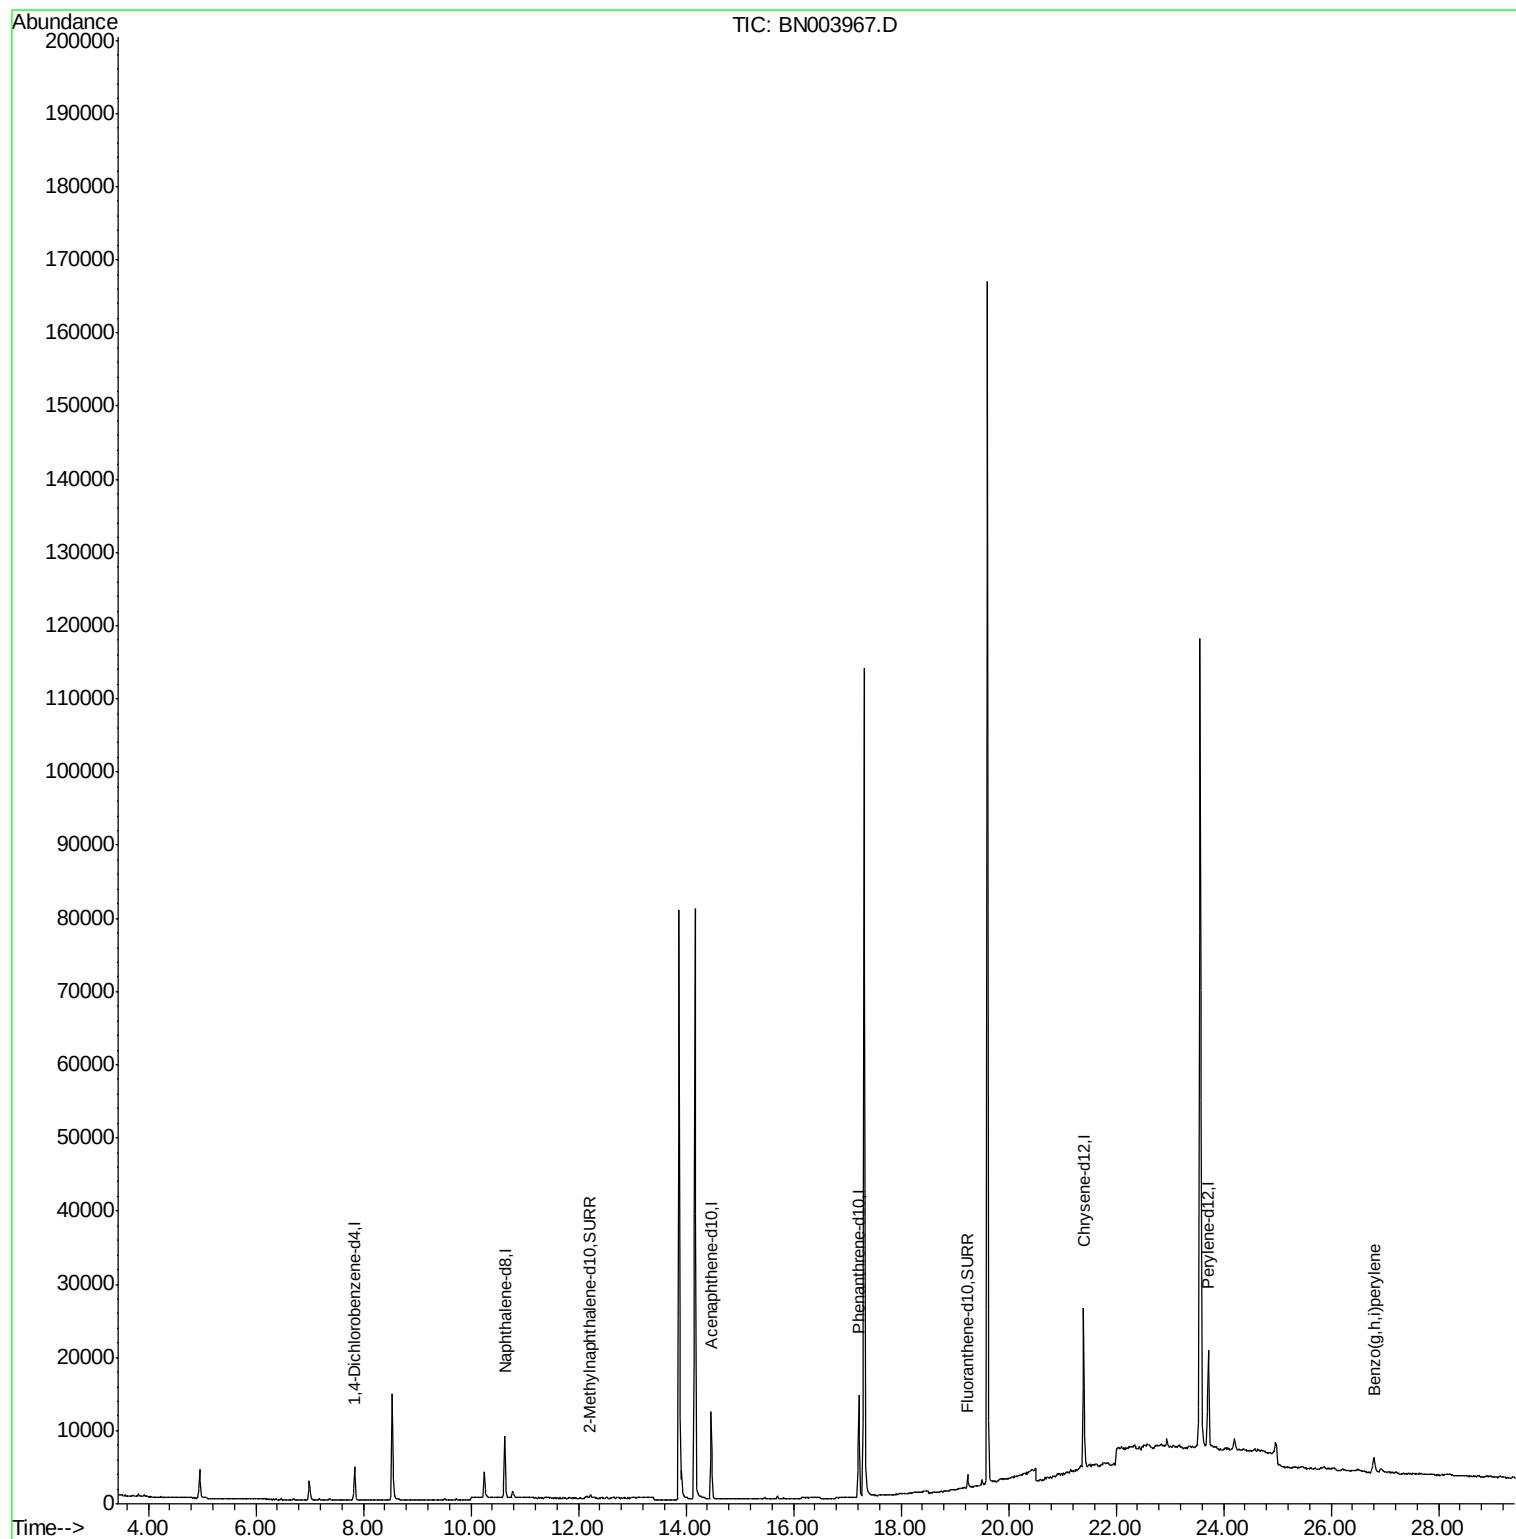

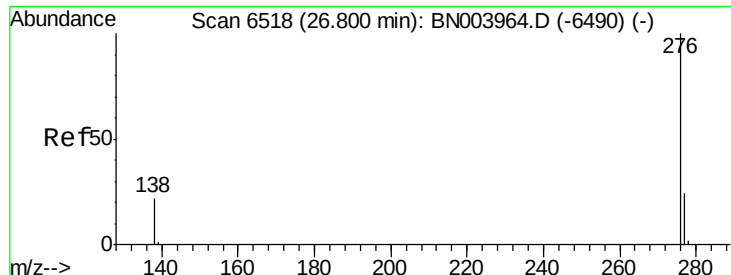

#26

Benzo(a,h,i)perylene

Concen: 0.069 ng/ul

RT: 26.80 min Scan# 6517

Delta R.T. -0.00 min

Lab File: BN003967.D

Acq: 15 Dec 2018 20:24

Instrument :

BNA_N

ClientSampleId :

F9Y06DL


Tot Ion:276 Resp: 4530

Ion Ratio Lower Upper

276 100

138 52.9 17.7 26.5#

277 45.3 19.3 28.9#

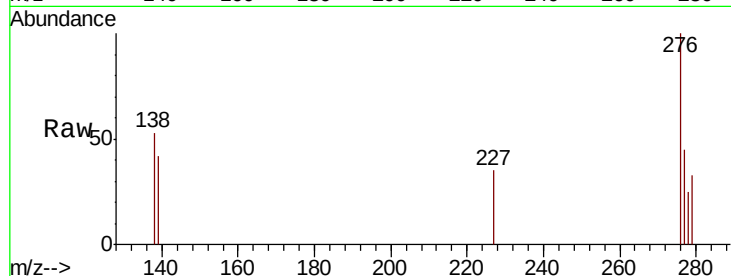

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

