

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
 Data File : BN003969.D
 Acq On : 15 Dec 2018 21:35
 Operator : JU/SJ
 Sample : J6171-03DL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9Y07DL

Manual Integrations
 APPROVED

Sohil
 12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:22:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 15 23:04:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1932	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	9529	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5916	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	14696	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	18608	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	17723	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	649	0.04	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	1703	0.04	ng/ul	0.00
Target Compounds						
19) Chrysene	21.41	228	4440m	0.066	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121518\
Data File : BN003969.D
Acq On : 15 Dec 2018 21:35
Operator : JU/SJ
Sample : J6171-03DL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
F9Y07DL

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

Quant Time: Dec 15 23:22:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 15 23:04:58 2018
Response via : Initial Calibration

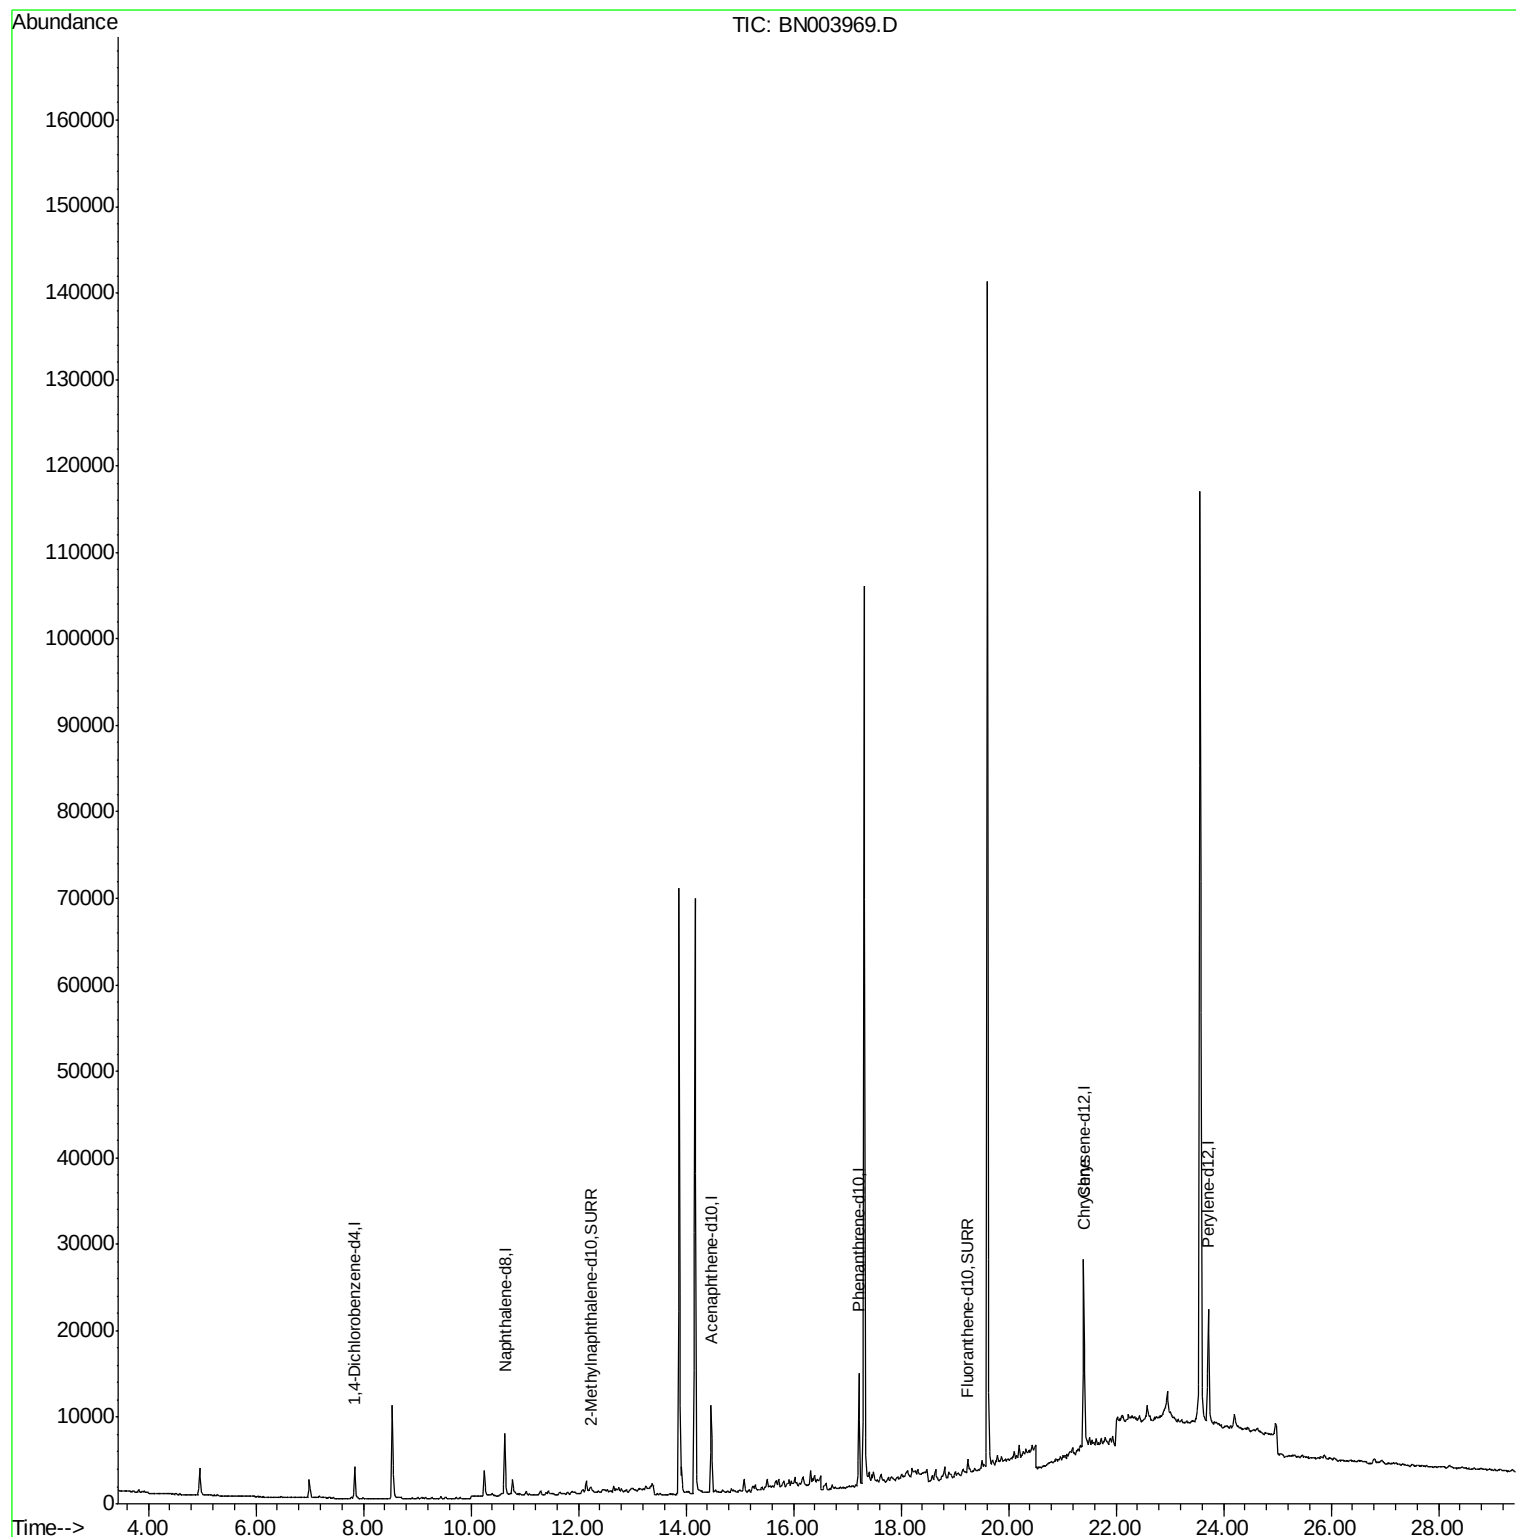

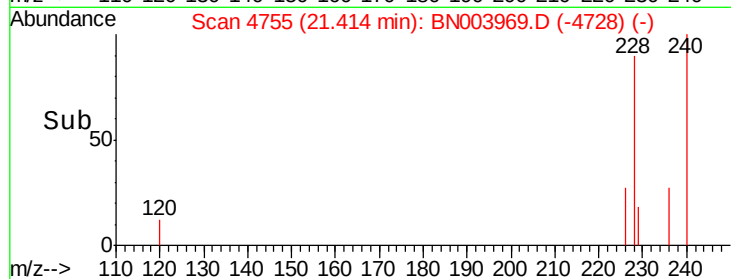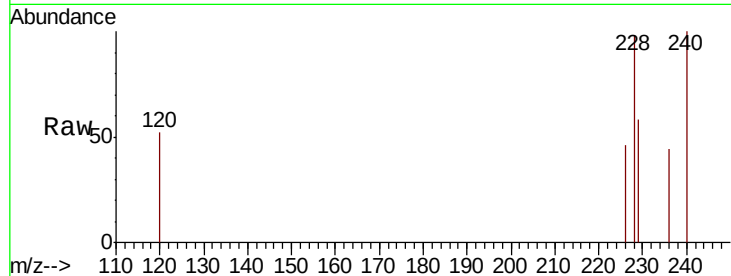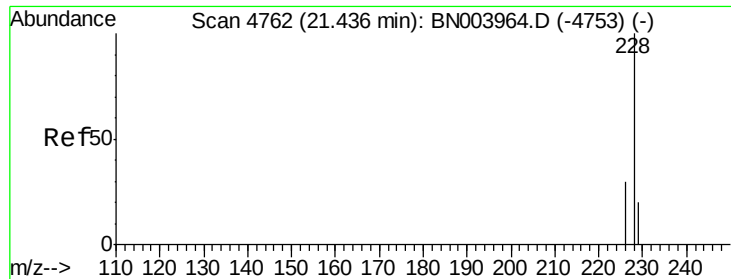

#19

Chrysene

Concen: 0.066 ng/ul m

RT: 21.41 min Scan# 4755

Delta R.T. -0.02 min

Lab File: BN003969.D

Acq: 15 Dec 2018 21:35

Instrument :

BNA_N

ClientSampleId :

F9Y07DL

Tot Ion:	228	Resp:	4440
Ion Ratio	Lower	Upper	
228	100		
226	47.5	24.0	36.0#
229	59.0	15.7	23.5#

Manual Integrations
APPROVED

Sohil
12/17/2018 4:23:59 PM

