


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121518\
 Data File : BN003949.D
 Acq On : 15 Dec 2018 08:31
 Operator : JU/SJ
 Sample : DFTPP69
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP69

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 17 06:22:23 2018

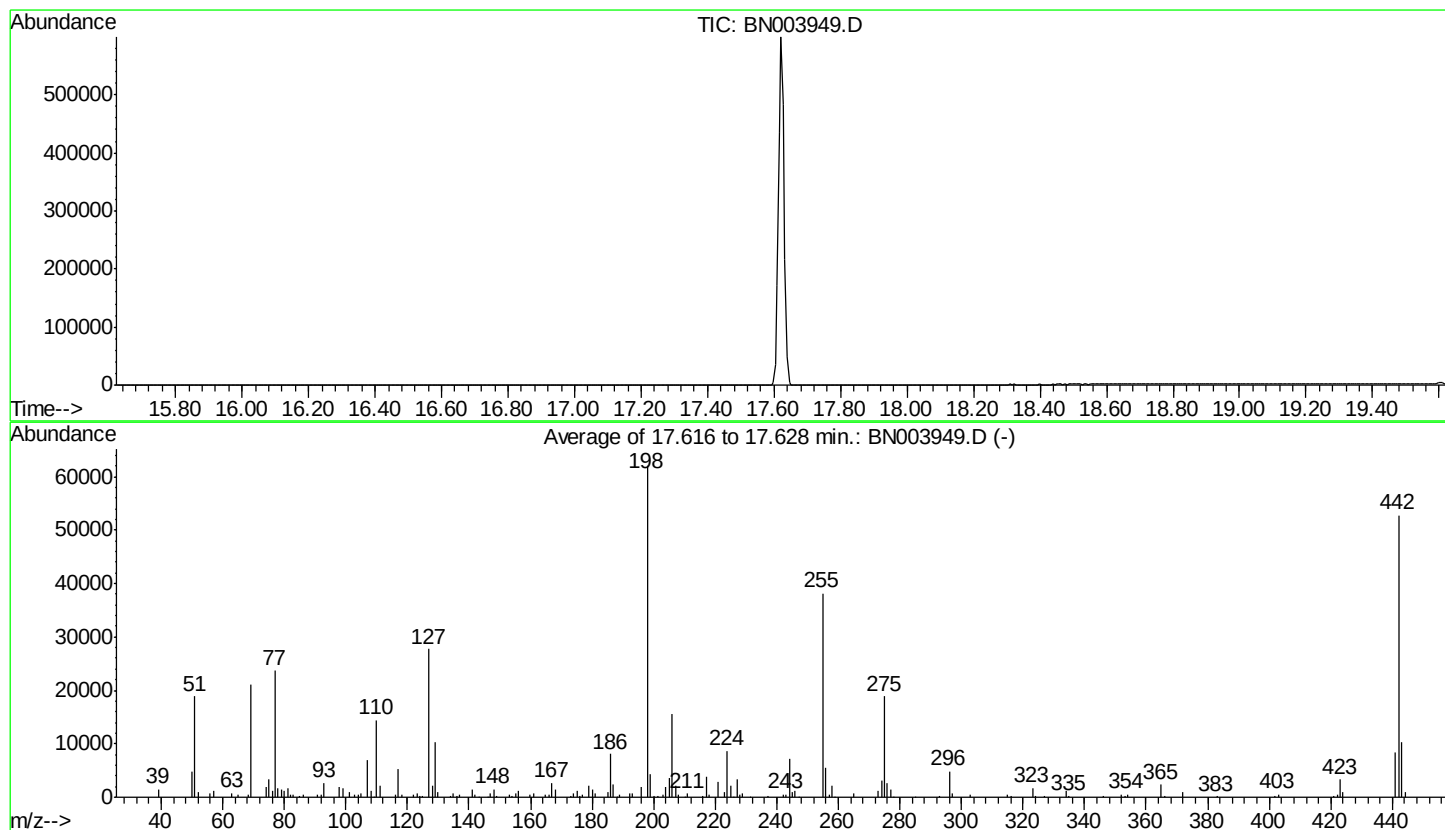

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	18849	PASS
68	69	0.00	2	1.9	390	PASS
69	198	0.00	100	34.0	21069	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.7	27765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62058	PASS
199	198	5	9	6.9	4263	PASS
275	198	10	60	30.3	18830	PASS
365	198	1	100	3.9	2391	PASS
441	198	0.01	100	13.4	8303	PASS
442	198	50	100	85.0	52752	PASS
443	442	15	24	19.4	10240	PASS

m/z	Abundance
44.00	682.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69

m/z	Abundance
39.00	1426.0
43.90	637.0
50.00	4746.0
51.00	19376.0
52.00	935.0
55.90	573.0
57.00	1292.0
63.00	803.0
65.00	368.0
68.10	410.0
69.00	21064.0
74.00	1998.0
75.00	3322.0
76.00	1125.0
77.00	23568.0
78.00	1672.0
79.00	1544.0
79.90	1150.0
81.00	1679.0
81.90	441.0
82.90	412.0
84.90	316.0
86.00	470.0
90.90	338.0
92.00	424.0
93.00	2527.0
98.00	1865.0
99.00	1673.0
101.00	948.0
103.00	387.0
104.00	573.0
104.90	609.0
107.00	6850.0
108.00	1167.0
110.00	13821.0
111.00	2089.0
115.90	370.0
117.00	5081.0
118.00	393.0
121.90	456.0
123.00	779.0
123.90	320.0
124.90	344.0
127.00	26088.0
128.00	2137.0
129.00	9803.0
130.00	869.0
135.00	714.0
137.00	475.0
141.00	1287.0
141.90	403.0
147.00	694.0
148.00	1331.0
148.90	317.0
152.90	416.0
153.90	353.0
155.00	663.0
156.00	999.0
159.90	415.0
160.90	646.0
164.90	515.0
166.00	407.0
167.00	2374.0
168.00	1376.0
173.00	318.0
173.90	547.0
175.00	965.0
176.00	324.0
177.00	476.0
179.00	1887.0
180.00	1343.0
181.00	634.0
185.00	926.0
186.00	7370.0
187.00	2133.0
189.00	411.0
192.00	609.0
193.00	677.0
196.00	1669.0
198.00	53784.0
199.00	3782.0
201.40	325.0
202.90	395.0
204.00	1774.0
205.00	3168.0
206.00	13308.0
207.00	2139.0
208.00	478.0
211.00	576.0
217.00	3346.0
217.90	432.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69

221.00	2549.0
223.00	854.0
224.00	7451.0
225.00	1743.0
227.00	2860.0
227.90	451.0
229.00	679.0
242.00	435.0
243.00	476.0
244.00	6189.0
245.00	866.0
246.00	1129.0
255.00	31696.0
256.00	4704.0
257.00	400.0
258.00	1703.0
265.00	680.0
273.00	964.0
274.00	2553.0
275.00	15076.0
276.00	2144.0
276.90	1125.0
296.00	3780.0
297.00	555.0
303.00	448.0
314.90	349.0
323.00	1326.0
334.00	834.0
351.90	389.0
354.00	461.0
365.00	1652.0
365.90	309.0
372.00	696.0
402.90	364.0
422.00	334.0
423.10	2180.0
424.00	661.0
441.10	5228.0
442.10	35024.0
443.10	6719.0
444.00	643.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69

m/z	Abundance
39.00	1743.0
44.00	681.0
50.00	5621.0
51.00	21544.0
52.00	1142.0
56.00	736.0
57.00	1544.0
63.00	909.0
65.00	455.0
68.10	436.0
69.00	24704.0
74.00	2462.0
75.00	3874.0
76.00	1277.0
77.00	27448.0
78.00	1884.0
79.00	1817.0
80.00	1334.0
81.00	1919.0
81.90	461.0
83.00	463.0
84.90	320.0
86.00	545.0
90.90	427.0
92.00	508.0
93.00	3139.0
98.00	2430.0
99.00	1900.0
101.00	1211.0
102.90	407.0
103.90	652.0
105.00	682.0
107.00	8422.0
108.00	1235.0
109.10	318.0
110.00	17224.0
111.00	2480.0
116.00	492.0
117.00	6448.0
118.00	505.0
121.90	593.0
123.00	933.0
123.90	429.0
125.00	405.0
127.00	32952.0
128.00	2544.0
129.00	11991.0
130.00	1043.0
133.90	399.0
134.90	1008.0
135.90	379.0
137.00	581.0
141.00	1495.0
141.90	610.0
143.00	364.0
146.00	307.0
146.90	849.0
148.00	1723.0
148.90	404.0
153.00	583.0
154.00	380.0
155.00	831.0
156.00	1380.0
160.00	524.0
161.00	794.0
164.90	624.0
165.90	489.0
167.00	3148.0
168.00	1549.0
172.90	400.0
174.00	729.0
175.00	1305.0
176.00	440.0
176.90	621.0
178.90	2510.0
180.00	1734.0
181.00	792.0
185.00	1177.0
186.00	9589.0
187.00	2797.0
188.00	326.0
188.90	537.0
192.00	686.0
193.00	918.0
196.00	2138.0
198.00	74112.0
199.00	5081.0
200.00	378.0
201.50	363.0
203.00	449.0
204.00	2394.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69

205.00	4048.0
206.10	18504.0
207.00	2518.0
208.00	668.0
210.00	311.0
211.00	773.0
215.90	366.0
217.00	4500.0
217.90	604.0
221.00	3420.0
223.00	1047.0
224.00	10223.0
225.00	2601.0
226.00	372.0
227.00	4039.0
228.00	685.0
229.00	861.0
231.10	356.0
237.00	391.0
242.00	542.0
243.10	626.0
244.00	8312.0
245.00	1050.0
246.00	1522.0
247.00	356.0
255.00	44968.0
256.00	6563.0
257.00	570.0
258.00	2424.0
258.90	373.0
264.90	1003.0
273.00	1377.0
274.00	3549.0
275.00	22104.0
276.00	3045.0
277.00	1677.0
278.00	316.0
285.00	331.0
293.00	429.0
296.00	5881.0
297.00	802.0
303.00	752.0
315.00	655.0
316.00	393.0
323.00	2021.0
324.00	383.0
326.90	430.0
334.00	1297.0
335.00	416.0
345.90	418.0
352.00	642.0
352.90	448.0
354.00	668.0
365.00	2787.0
366.00	411.0
372.00	1180.0
383.00	329.0
401.90	423.0
403.00	688.0
420.90	549.0
422.00	493.0
423.10	3978.0
424.10	1014.0
441.10	9703.0
442.10	61064.0
443.10	12522.0
444.00	1254.0

Instrument :

BNA_N

ClientSampleId :

DFTPP69

m/z	Abundance
39.00	1231.0
43.90	686.0
50.00	3863.0
51.00	15629.0
52.00	846.0
56.00	530.0
57.00	1108.0
63.00	653.0
65.00	366.0
68.10	326.0
69.00	17440.0
74.00	1619.0
75.00	2747.0
76.10	1031.0
77.00	20104.0
78.00	1386.0
79.00	1326.0
79.90	979.0
81.00	1463.0
82.00	343.0
83.00	327.0
85.90	377.0
90.90	424.0
92.00	392.0
93.00	2273.0
98.00	1804.0
99.00	1469.0
101.00	792.0
103.00	315.0
104.00	514.0
104.90	548.0
107.00	5920.0
108.00	960.0
110.00	12304.0
111.00	1693.0
116.00	307.0
117.00	4573.0
118.00	355.0
121.90	366.0
123.00	728.0
127.00	24256.0
128.00	1780.0
129.00	9198.0
130.00	823.0
133.90	316.0
135.00	748.0
136.00	310.0
136.90	352.0
141.00	1225.0
141.90	399.0
147.00	636.0
148.00	1364.0
149.00	308.0
152.90	336.0
154.00	319.0
155.00	678.0
156.00	955.0
160.00	371.0
160.90	582.0
165.00	460.0
166.00	374.0
167.00	2525.0
168.00	1251.0
172.90	368.0
174.00	581.0
175.00	1126.0
175.90	315.0
176.90	517.0
178.90	1940.0
180.00	1280.0
180.90	595.0
185.00	1000.0
186.00	7174.0
187.00	2085.0
188.90	478.0
192.00	663.0
193.00	712.0
196.00	1834.0
198.00	58280.0
199.00	3927.0
199.90	321.0
201.50	301.0
203.00	351.0
204.00	1954.0
205.00	3231.0
206.00	14717.0
207.00	2095.0
208.00	464.0
211.00	591.0
215.90	325.0
217.00	3983.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69

218.00	487.0
221.00	2730.0
223.00	887.0
224.00	8386.0
225.00	2173.0
227.00	3288.0
228.00	439.0
229.00	727.0
237.00	324.0
242.00	499.0
243.00	514.0
244.10	6818.0
245.00	1019.0
246.00	1274.0
255.00	37840.0
256.00	5435.0
257.00	402.0
258.00	2187.0
265.00	810.0
273.00	1223.0
274.00	3174.0
275.00	19312.0
276.00	2571.0
277.00	1409.0
293.00	381.0
296.00	4945.0
296.90	660.0
303.00	612.0
314.90	577.0
316.00	406.0
323.00	1893.0
323.90	323.0
334.00	1182.0
335.00	336.0
346.00	359.0
352.00	557.0
353.00	403.0
353.90	639.0
365.00	2734.0
366.00	331.0
372.00	1076.0
383.00	301.0
402.00	462.0
403.00	652.0
421.00	489.0
422.10	539.0
423.00	3629.0
424.00	865.0
441.10	9980.0
442.10	62168.0
443.10	11480.0
444.10	1069.0

Instrument :
BNA_N
ClientSampleId :
DFTPP69