

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
 Data File : BN023222.D
 Acq On : 15 Dec 2022 19:15
 Operator : CG/JU
 Sample : N5962-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	48	rBV	44004	56785	0.64%	0.083%
2	3.805	120	122	131	rBV	16825	39803	0.45%	0.058%
3	4.022	154	159	166	rVB	23374	37834	0.43%	0.055%
4	4.116	171	175	183	rVB	17127	26752	0.30%	0.039%
5	4.664	264	268	272	rVB4	7892	9815	0.11%	0.014%
6	5.069	332	337	344	rVB2	18171	28373	0.32%	0.041%
7	7.157	684	692	700	rVB	214394	338717	3.81%	0.492%
8	7.328	714	721	735	rVB	739369	1124713	12.63%	1.635%
9	7.528	748	755	766	rVV	619066	952278	10.70%	1.385%
10	8.005	828	836	843	rBV	873134	1368186	15.37%	1.989%
11	8.710	949	956	968	rBV	526532	860375	9.67%	1.251%
12	9.169	1027	1034	1045	rBV	918638	1486817	16.70%	2.162%
13	9.593	1101	1106	1111	rVB3	9245	16659	0.19%	0.024%
14	9.899	1148	1158	1172	rBV	640512	1008824	11.33%	1.467%
15	10.440	1242	1250	1266	rBV	869232	1449171	16.28%	2.107%
16	10.822	1307	1315	1326	rBV	1343436	2187145	24.57%	3.180%
17	10.957	1331	1338	1353	rVV	527218	885990	9.95%	1.288%
18	12.404	1577	1584	1591	rBV	23570	40112	0.45%	0.058%
19	13.016	1680	1688	1694	rBV6	6333	13334	0.15%	0.019%
20	13.545	1772	1778	1783	rBV5	13188	21605	0.24%	0.031%
21	13.928	1835	1843	1848	rBV3	7899	14631	0.16%	0.021%
22	14.057	1859	1865	1877	rBV	2462936	3355726	37.70%	4.879%
23	14.345	1907	1914	1928	rBV	2852409	4064750	45.66%	5.910%
24	14.651	1958	1966	1976	rBV	2289462	3269229	36.73%	4.753%
25	14.839	1991	1998	2016	rBV	239407	426867	4.80%	0.621%
26	15.063	2031	2036	2041	rBV3	24635	35561	0.40%	0.052%
27	15.439	2094	2100	2103	rBV5	6328	11223	0.13%	0.016%
28	15.639	2127	2134	2147	rBV	3716272	5510951	61.91%	8.012%
29	15.751	2147	2153	2170	rVV	1089975	1529623	17.18%	2.224%
30	15.881	2170	2175	2181	rVB2	20297	32983	0.37%	0.048%
31	16.004	2192	2196	2200	rBV3	10023	13200	0.15%	0.019%
32	17.398	2426	2433	2439	rBV	3082679	4196705	47.14%	6.102%
33	17.498	2443	2450	2462	rVV	4921396	6756173	75.90%	9.823%
34	17.575	2462	2463	2470	rVB7	9398	12394	0.14%	0.018%
35	18.069	2541	2547	2550	rBV6	9068	14198	0.16%	0.021%
36	18.286	2580	2584	2594	rBV2	54767	93037	1.05%	0.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
 Data File : BN023222.D
 Acq On : 15 Dec 2022 19:15
 Operator : CG/JU
 Sample : N5962-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZ50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

37	18.363	2594	2597	2601	rVB2	13339	17491	0.20%	0.025%
38	18.716	2654	2657	2660	rBV5	8685	9376	0.11%	0.014%
39	19.351	2761	2765	2772	rVB	62845	85379	0.96%	0.124%
40	19.422	2772	2777	2782	rBV	69171	108887	1.22%	0.158%
41	19.563	2798	2801	2806	rBV3	44510	62357	0.70%	0.091%
42	19.710	2824	2826	2830	rVB4	15560	16789	0.19%	0.024%
43	19.786	2833	2839	2854	rVV	5861319	8269727	92.90%	12.023%
44	21.580	3139	3144	3153	rVB	3927303	4887489	54.90%	7.106%
45	23.874	3526	3534	3551	rVB2	4364711	8901881	100.00%	12.942%
46	24.033	3554	3561	3574	rVB2	2489997	5130570	57.63%	7.459%




Sum of corrected areas: 68780485

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023222.D
Acq On : 15 Dec 2022 19:15
Operator : CG/JU
Sample : N5962-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

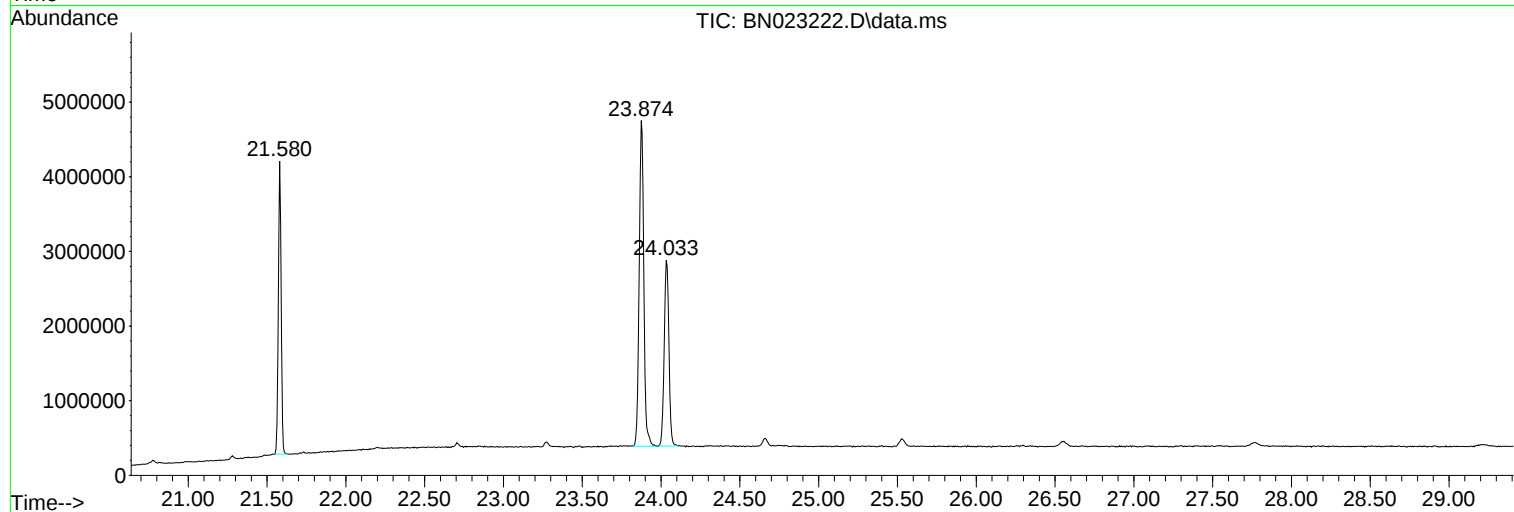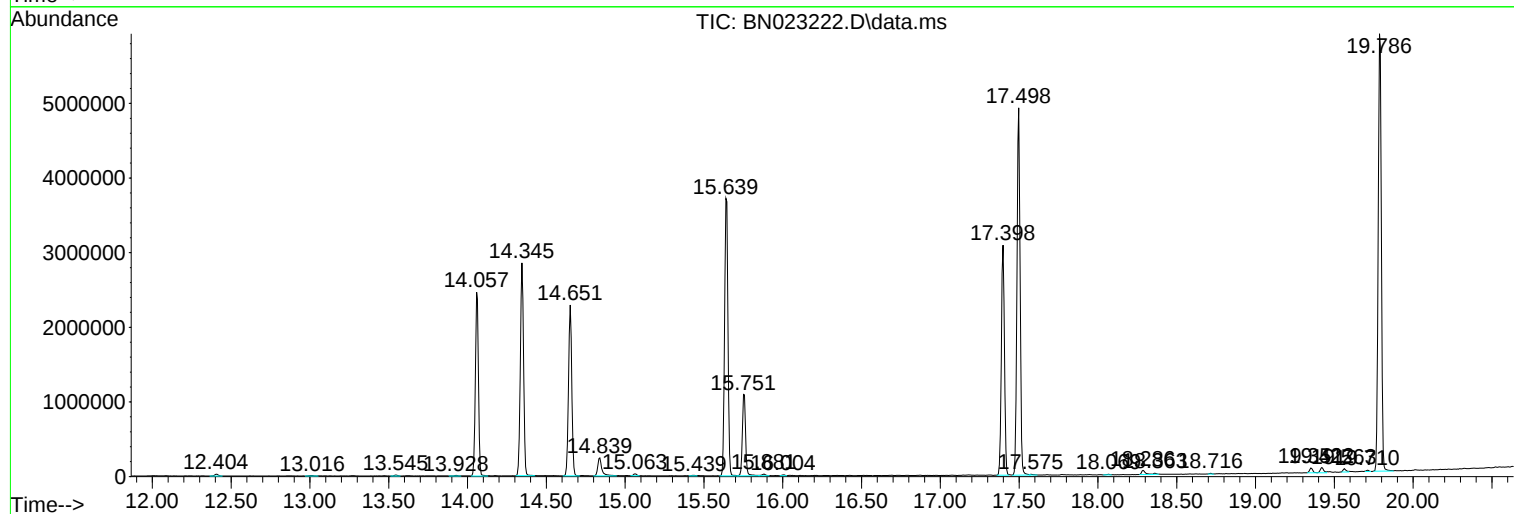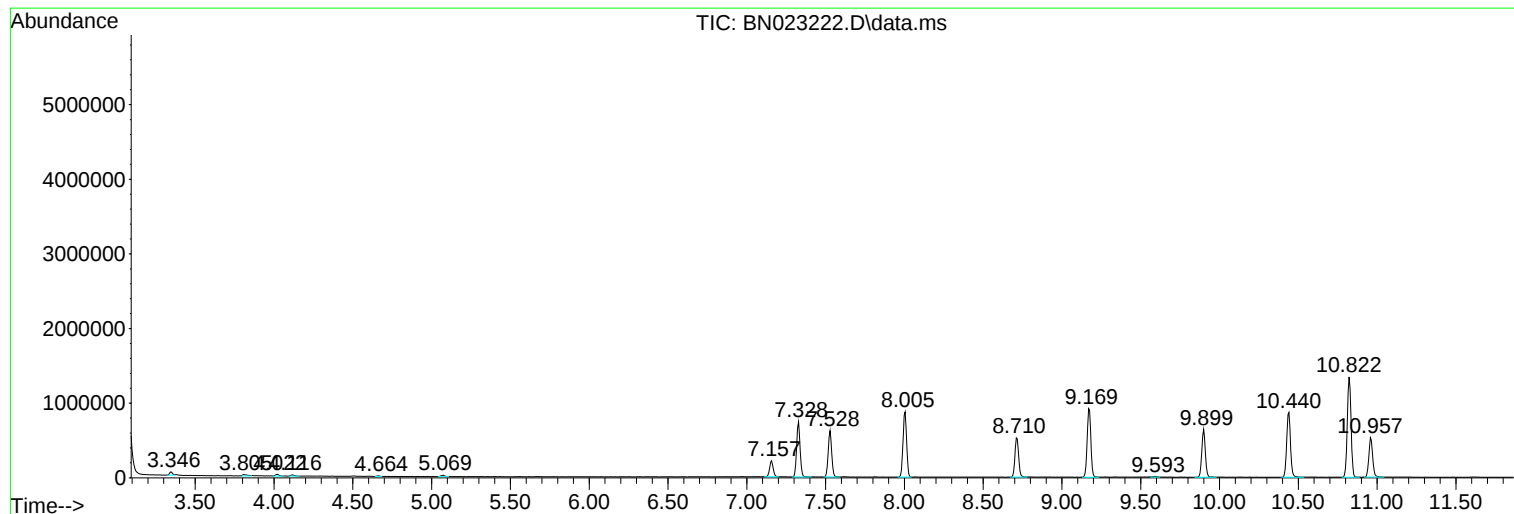

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023222.D
Acq On : 15 Dec 2022 19:15
Operator : CG/JU
Sample : N5962-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023222.D
Acq On : 15 Dec 2022 19:15
Operator : CG/JU
Sample : N5962-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFZ50

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc