

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
 Data File : BN023227.D
 Acq On : 15 Dec 2022 22:58
 Operator : CG/JU
 Sample : PB149615BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK615

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	58	rVB	80888	125964	1.25%	0.133%
2	3.775	114	117	145	rBV	1028258	1650998	16.38%	1.738%
3	4.117	170	175	189	rVB	157374	244951	2.43%	0.258%
4	7.158	684	692	708	rBV	1376284	2129857	21.13%	2.242%
5	7.328	714	721	733	rVB	1132950	1728664	17.15%	1.820%
6	7.528	748	755	766	rBV	1404338	2153203	21.36%	2.267%
7	8.005	828	836	844	rBV	1087647	1740145	17.26%	1.832%
8	8.710	949	956	972	rBV	1664878	2703969	26.83%	2.847%
9	9.169	1026	1034	1047	rBV	1320643	2165712	21.49%	2.280%
10	9.899	1150	1158	1174	rBV	1127434	1798388	17.84%	1.893%
11	10.434	1242	1249	1264	rBV	1668733	2778467	27.57%	2.925%
12	10.822	1307	1315	1325	rBV	1653608	2707983	26.87%	2.851%
13	10.957	1331	1338	1356	rBV	1770080	3041596	30.18%	3.202%
14	12.010	1507	1517	1523	rBV9	4855	13208	0.13%	0.014%
15	12.404	1577	1584	1592	rVB	32513	52674	0.52%	0.055%
16	13.010	1679	1687	1693	rBV5	5525	13574	0.13%	0.014%
17	14.063	1859	1866	1874	rBV	3251146	4550336	45.15%	4.791%
18	14.345	1907	1914	1930	rBV	3747953	5406718	53.64%	5.692%
19	14.651	1958	1966	1976	rBV	2769260	3904733	38.74%	4.111%
20	14.840	1990	1998	2023	rBV	1741536	2615141	25.95%	2.753%
21	15.004	2024	2026	2032	rVV7	6518	11370	0.11%	0.012%
22	15.057	2032	2035	2040	rVB7	7569	10655	0.11%	0.011%
23	15.434	2093	2099	2103	rBV5	6417	11217	0.11%	0.012%
24	15.645	2127	2135	2146	rBV	4678881	6730031	66.77%	7.085%
25	15.757	2147	2154	2165	rBV	1627899	2169992	21.53%	2.285%
26	15.881	2171	2175	2180	rVB	24921	36963	0.37%	0.039%
27	17.186	2392	2397	2401	rBV3	6799	10207	0.10%	0.011%
28	17.398	2426	2433	2442	rBV	3599359	4971671	49.33%	5.234%
29	17.498	2443	2450	2470	rVV	5437440	7577172	75.18%	7.977%
30	17.769	2493	2496	2501	rBV5	7129	12092	0.12%	0.013%
31	18.063	2543	2546	2550	rBV5	7649	10402	0.10%	0.011%
32	19.351	2760	2765	2770	rBV	71968	100302	1.00%	0.106%
33	19.422	2772	2777	2782	rBV	71491	99673	0.99%	0.105%
34	19.786	2833	2839	2851	rBV	6952158	9382812	93.09%	9.878%
35	21.580	3138	3144	3152	rBV2	4656567	6028127	59.81%	6.346%
36	23.874	3526	3534	3551	rVB2	4836761	10079061	100.00%	10.611%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023227.D
Acq On : 15 Dec 2022 22:58
Operator : CG/JU
Sample : PB149615BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK615

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Title : SVOA CALIBRATION

37	24.033	3553	3561	3572	rVV2	3171360	6216636	61.68%	6.545%
----	--------	------	------	------	------	---------	---------	--------	--------


Sum of corrected areas: 94984664

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023227.D
Acq On : 15 Dec 2022 22:58
Operator : CG/JU
Sample : PB149615BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK615

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

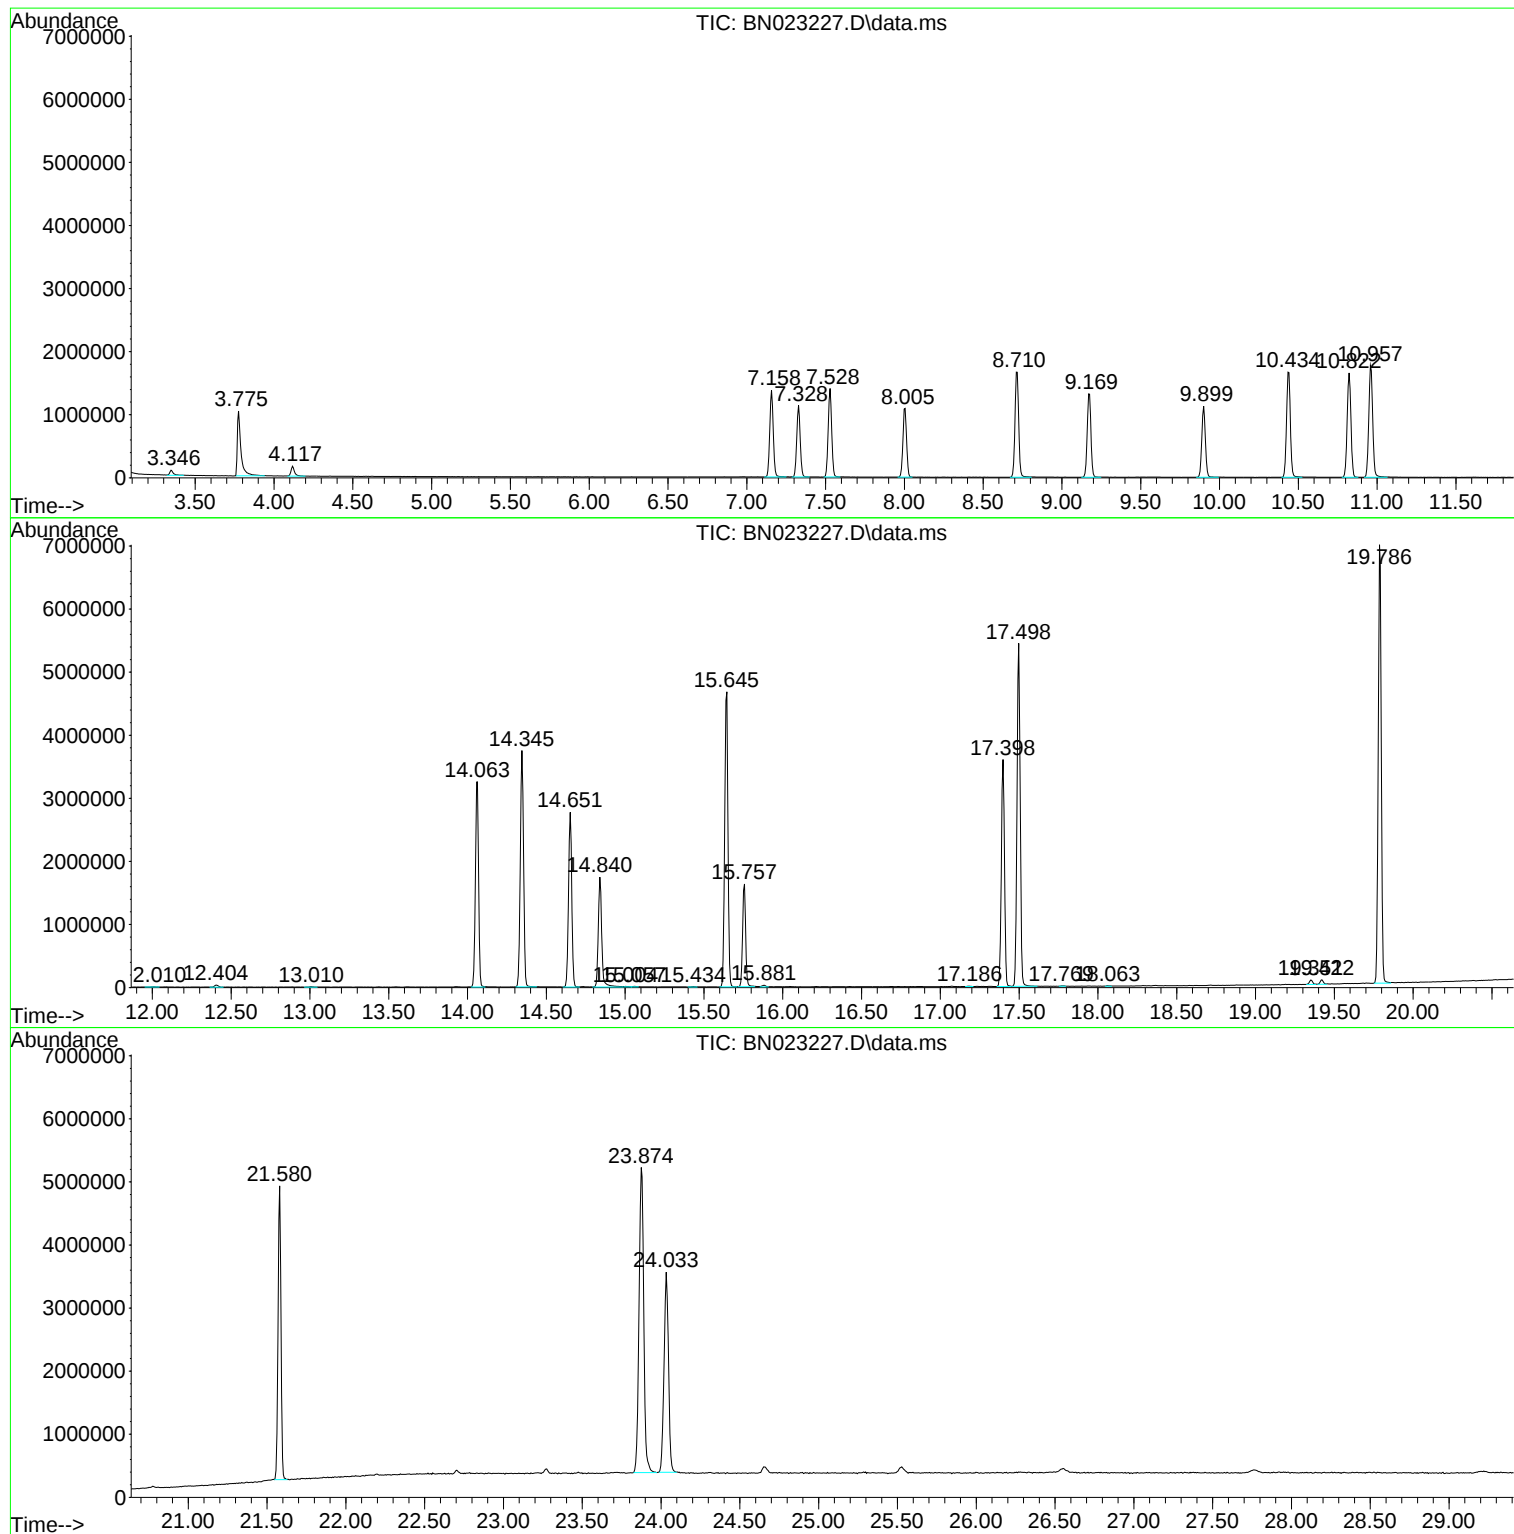

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023227.D
Acq On : 15 Dec 2022 22:58
Operator : CG/JU
Sample : PB149615BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK615










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.117	2.82 ng/ul	244951	1,4-Dichlorobenzene-d4	7.999

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Toluene			92	C7H8	000108-88-3	95
2	Toluene			92	C7H8	000108-88-3	95
3	Toluene			92	C7H8	000108-88-3	94
4	Toluene			92	C7H8	000108-88-3	87
5	1,3,5-Cycloheptatriene			92	C7H8	000544-25-2	87

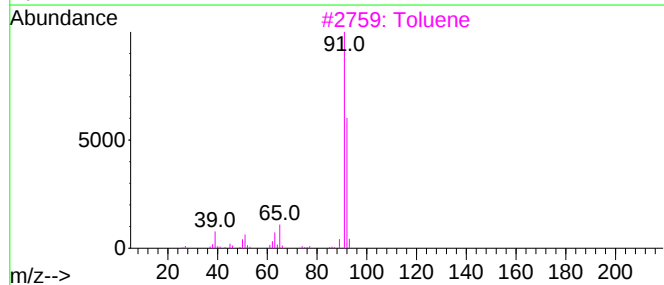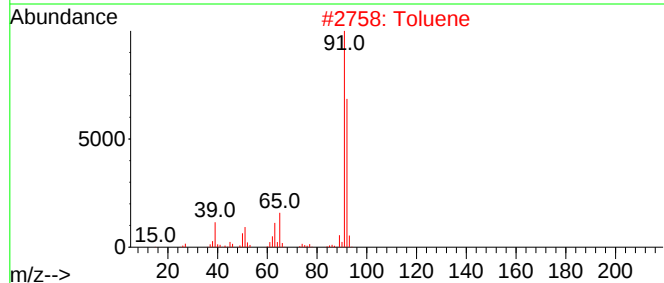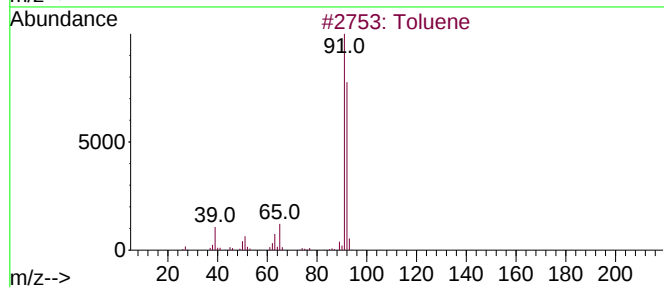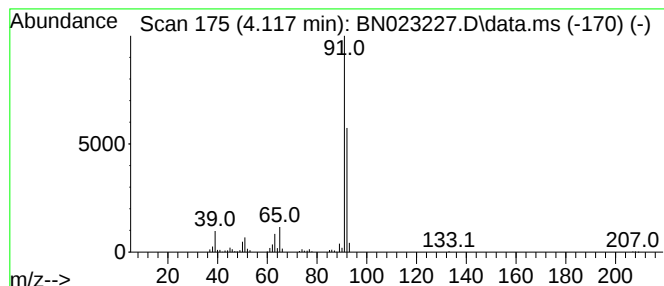

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023227.D
Acq On : 15 Dec 2022 22:58
Operator : CG/JU
Sample : PB149615BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK615

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	4.117	2.8	ng/u1	244951	1	7.999	1740150	20.0