

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
 Data File : BN023231.D
 Acq On : 16 Dec 2022 01:26
 Operator : CG/JU
 Sample : N5983-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023231.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	56	rVB	51730	88024	0.99%	0.123%
2	3.781	116	118	139	rBV	184836	353504	3.98%	0.492%
3	4.022	154	159	170	rVB	32251	60382	0.68%	0.084%
4	4.116	171	175	182	rVB	18505	28910	0.33%	0.040%
5	5.069	333	337	343	rVB	24353	34222	0.39%	0.048%
6	7.157	683	692	701	rBV	260358	423150	4.77%	0.589%
7	7.328	714	721	733	rBV	900921	1415601	15.95%	1.972%
8	7.528	747	755	765	rBV	850619	1322336	14.90%	1.842%
9	7.616	765	770	776	rVB9	6907	13198	0.15%	0.018%
10	8.005	828	836	846	rBV	846449	1355699	15.27%	1.889%
11	8.710	949	956	968	rBV	712227	1114324	12.55%	1.552%
12	8.916	986	991	999	rVB6	3832	9273	0.10%	0.013%
13	9.169	1026	1034	1044	rBV	1088938	1763261	19.87%	2.456%
14	9.587	1100	1105	1113	rVB2	27490	43204	0.49%	0.060%
15	9.899	1150	1158	1172	rBV	785741	1265147	14.25%	1.762%
16	10.434	1242	1249	1264	rBV	1216330	1977946	22.28%	2.755%
17	10.822	1307	1315	1324	rBV	1283555	2100329	23.66%	2.926%
18	10.957	1331	1338	1357	rBV	1321876	2195852	24.74%	3.059%
19	12.004	1510	1516	1523	rBV9	4103	9149	0.10%	0.013%
20	12.093	1525	1531	1539	rVB	21931	36670	0.41%	0.051%
21	12.404	1578	1584	1591	rBV	26223	44074	0.50%	0.061%
22	13.010	1682	1687	1691	rBV6	7345	11574	0.13%	0.016%
23	13.969	1846	1850	1856	rVB7	8946	13001	0.15%	0.018%
24	14.057	1859	1865	1880	rVV	2678749	3674685	41.40%	5.119%
25	14.345	1907	1914	1925	rBV	3178457	4491611	50.60%	6.257%
26	14.651	1959	1966	1975	rBV	2150737	3065470	34.54%	4.271%
27	14.834	1991	1997	2010	rBV	187292	309116	3.48%	0.431%
28	15.063	2031	2036	2041	rBV	52285	68752	0.77%	0.096%
29	15.445	2094	2101	2106	rBV	38447	56546	0.64%	0.079%
30	15.639	2127	2134	2147	rBV	3997854	5702892	64.25%	7.945%
31	15.751	2147	2153	2166	rVV	888183	1182745	13.33%	1.648%
32	15.881	2171	2175	2180	rVB	18962	28333	0.32%	0.039%
33	17.069	2374	2377	2382	rVB6	5942	9096	0.10%	0.013%
34	17.398	2426	2433	2442	rBV	2757234	3921389	44.18%	5.463%
35	17.498	2443	2450	2460	rVV	4692234	6530382	73.57%	9.097%
36	17.580	2460	2464	2469	rVB	43174	62096	0.70%	0.087%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
 Data File : BN023231.D
 Acq On : 16 Dec 2022 01:26
 Operator : CG/JU
 Sample : N5983-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLE8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

37	17.680	2476	2481	2485	rVB	9086	13190	0.15%	0.018%
38	17.769	2494	2496	2502	rVB5	7598	13114	0.15%	0.018%
39	18.292	2581	2585	2589	rBV7	14220	22294	0.25%	0.031%
40	18.363	2594	2597	2601	rVB	12293	15397	0.17%	0.021%
41	18.716	2654	2657	2661	rBV5	8180	11475	0.13%	0.016%
42	19.351	2761	2765	2770	rBV3	56697	80755	0.91%	0.112%
43	19.422	2773	2777	2783	rVV	55516	77622	0.87%	0.108%
44	19.563	2799	2801	2804	rBV4	10585	11366	0.13%	0.016%
45	19.710	2824	2826	2830	rVB3	14235	15503	0.17%	0.022%
46	19.792	2833	2840	2849	rBV	5799448	8089662	91.14%	11.270%
47	21.580	3139	3144	3154	rBV	3428095	4594682	51.76%	6.401%
48	23.880	3527	3535	3551	rVB2	4205080	8876068	100.00%	12.365%
49	24.039	3554	3562	3572	rVB	2432945	4766567	53.70%	6.640%
50	24.662	3663	3668	3678	rVB2	203954	412615	4.65%	0.575%




Sum of corrected areas: 71782253

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023231.D
Acq On : 16 Dec 2022 01:26
Operator : CG/JU
Sample : N5983-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

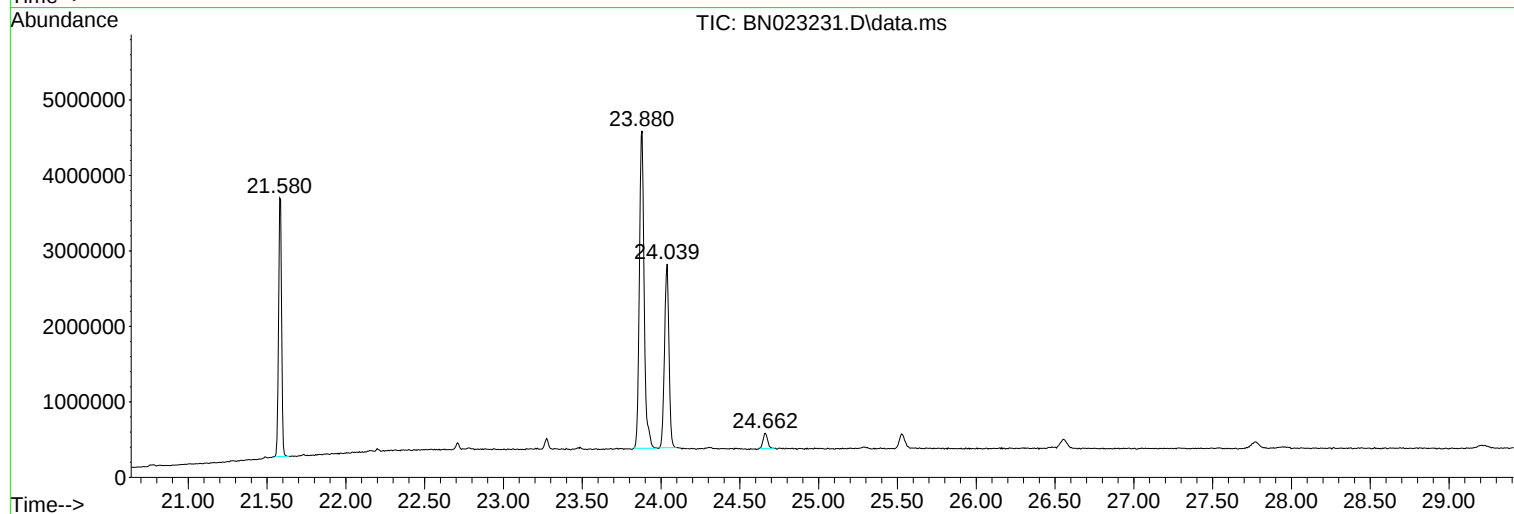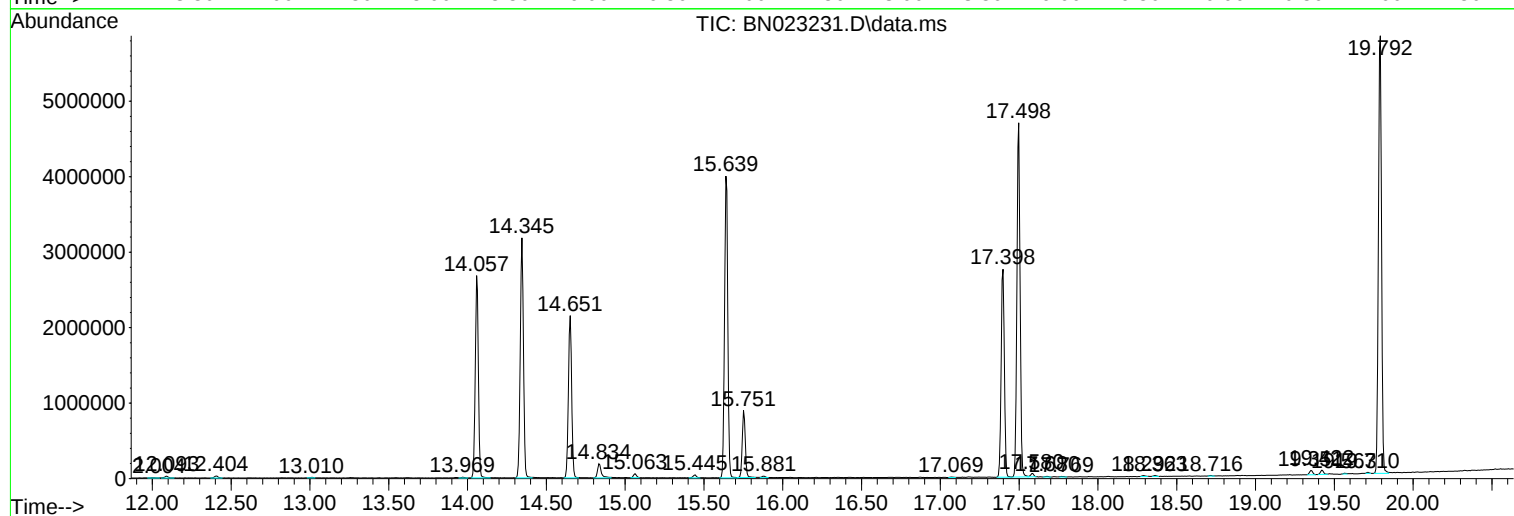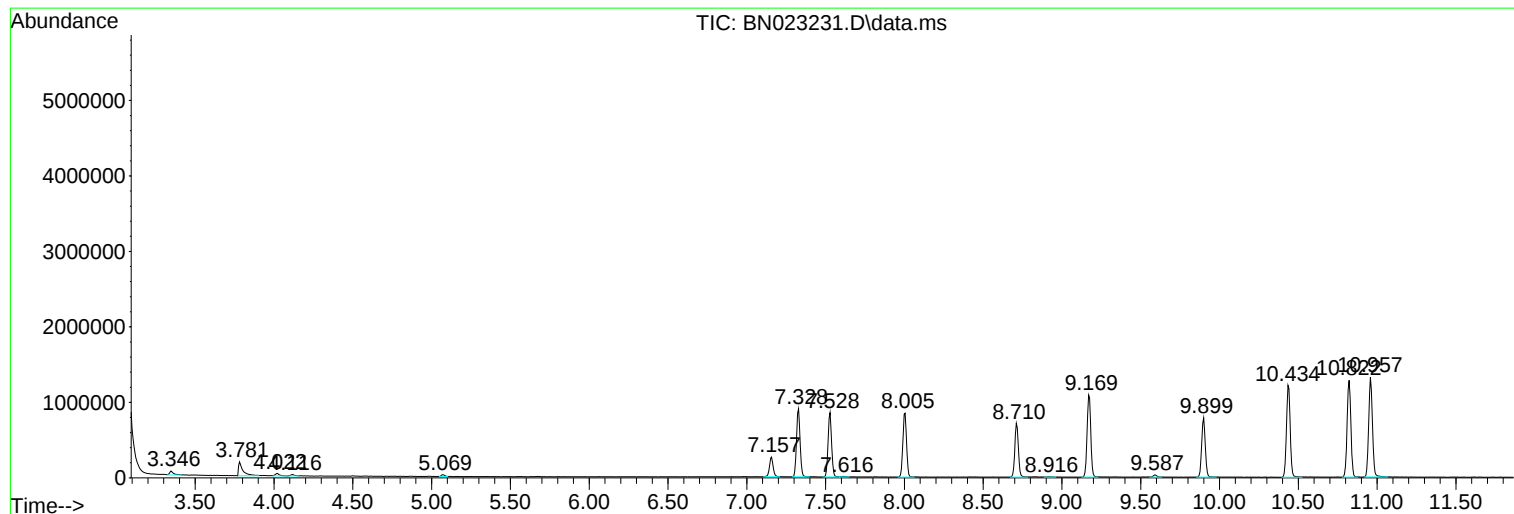

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023231.D
Acq On : 16 Dec 2022 01:26
Operator : CG/JU
Sample : N5983-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121522\
Data File : BN023231.D
Acq On : 16 Dec 2022 01:26
Operator : CG/JU
Sample : N5983-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLE8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
