
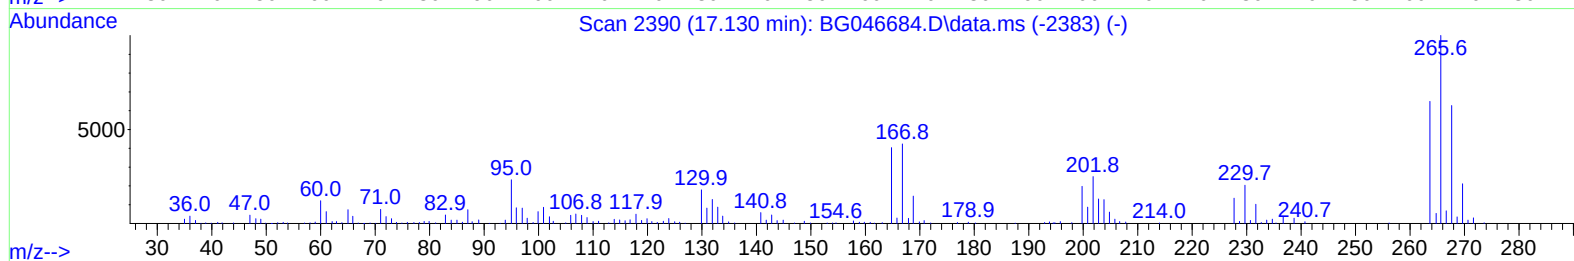
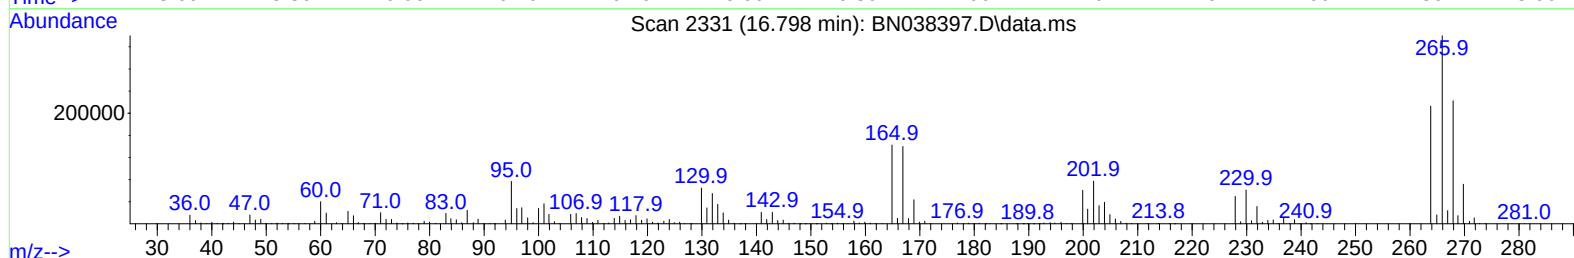


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038397.D
Acq On : 15 Dec 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 10:09:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

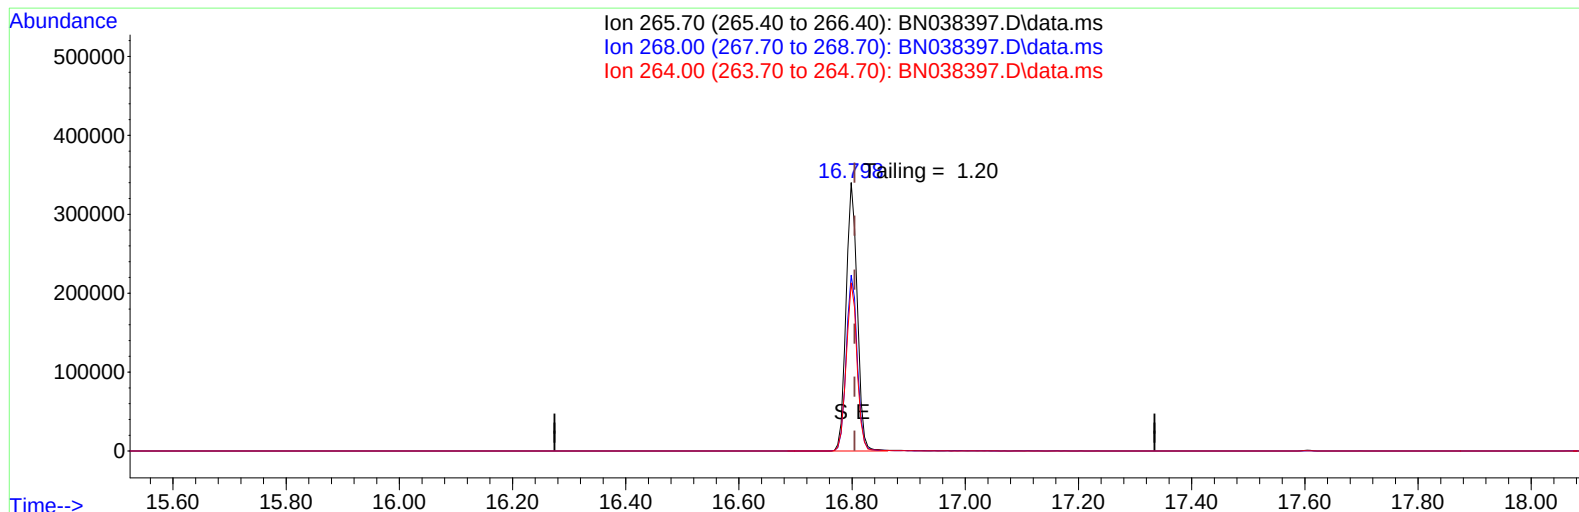

TIC: BN038397.D\data.ms

(70) Pentachlorophenol (C)




16.798min (-0.006) 553107.47 ng

response 468790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.49
264.00	61.60	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038397.D
Acq On : 15 Dec 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 10:09:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

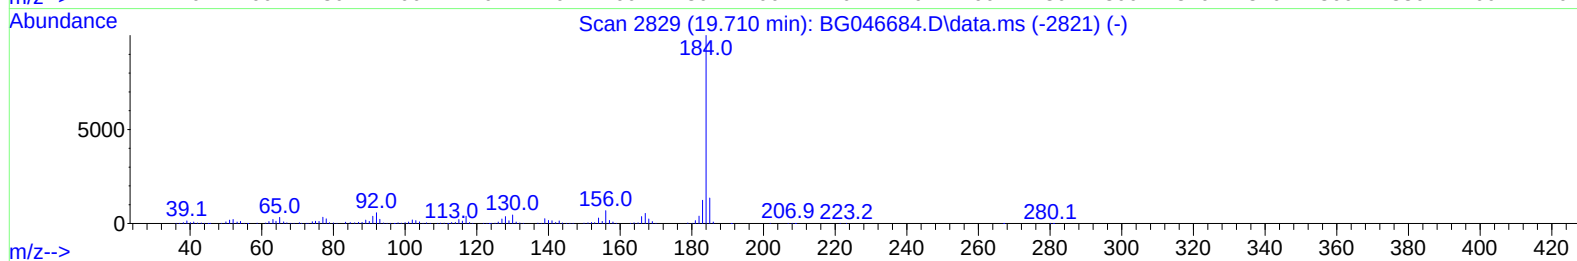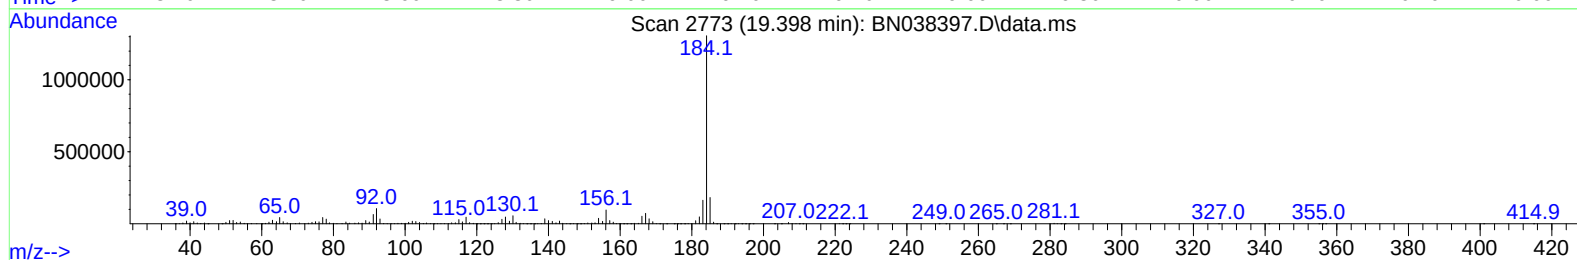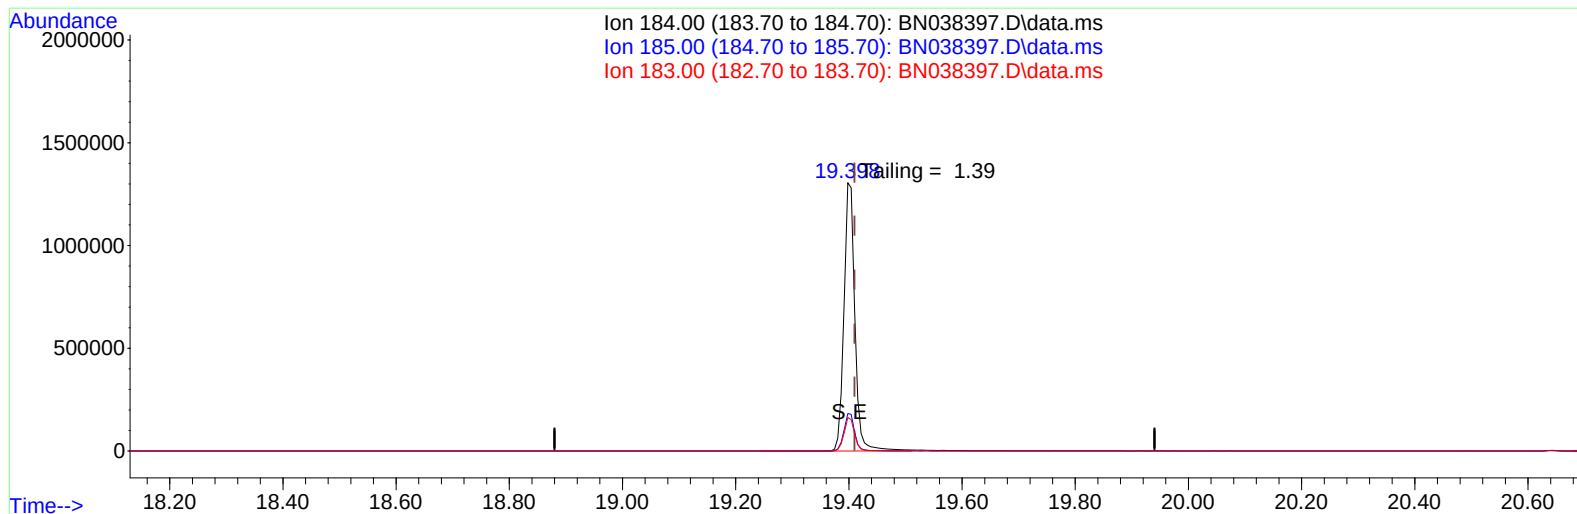

TIC: BN038397.D\data.ms

(77) Benzidine**19.398min (-0.012) 4213.74 ng****response 1763907**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.49
0.00	0.00	0.00