
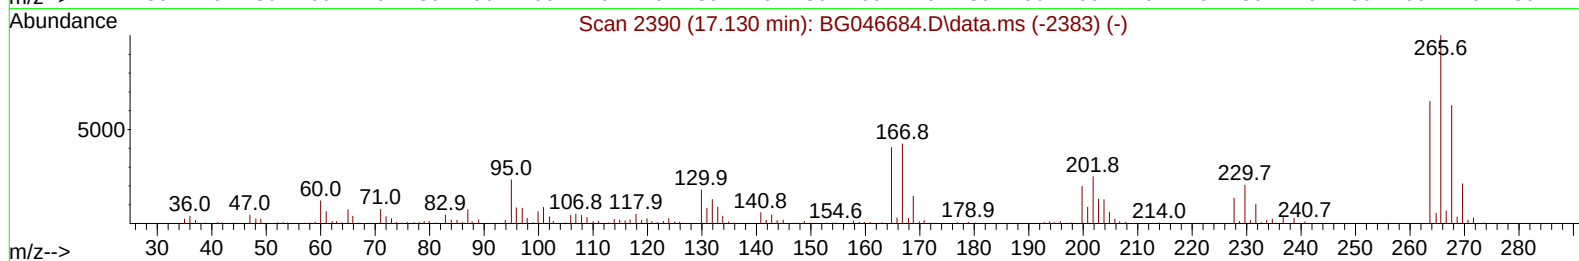
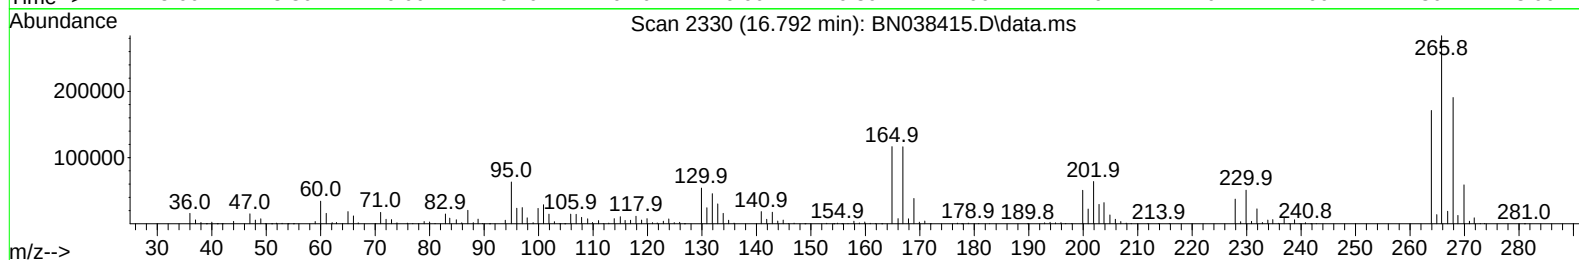


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038415.D
Acq On : 15 Dec 2025 22:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 00:22:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

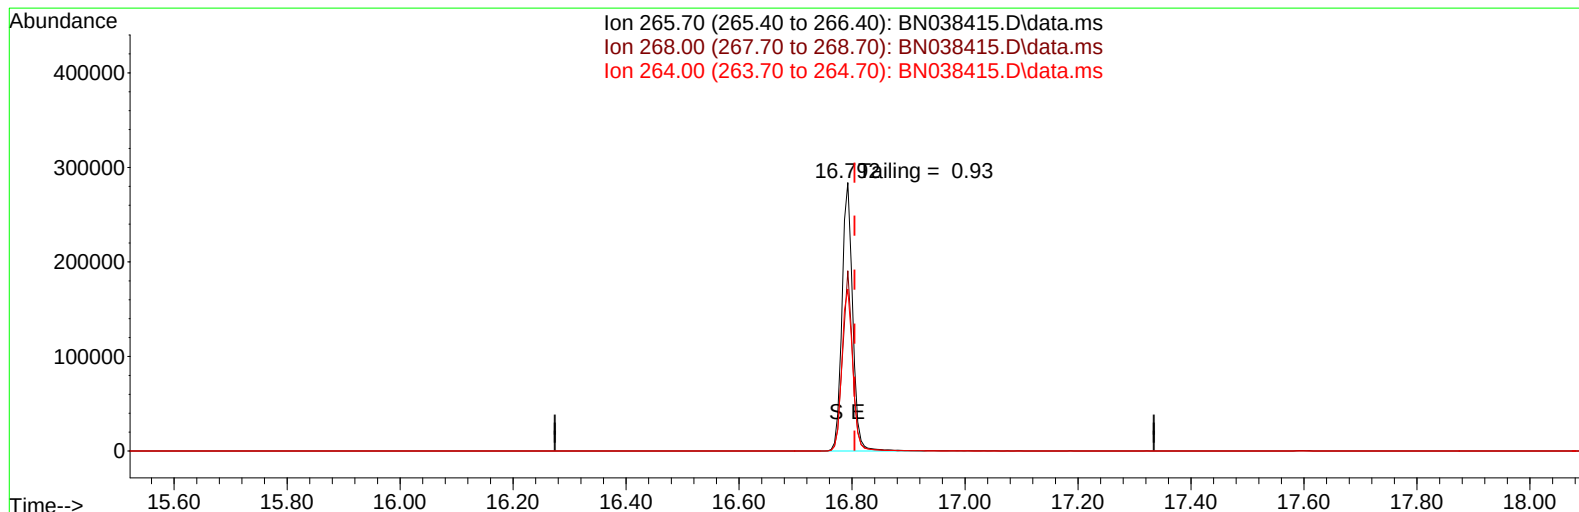

TIC: BN038415.D\data.ms




(70) Pentachlorophenol (C)

16.792min (-0.012) 591376.64 ng

response 371278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.13
264.00	61.60	60.26
0.00	0.00	0.00

Quant Time: Dec 16 00:22:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

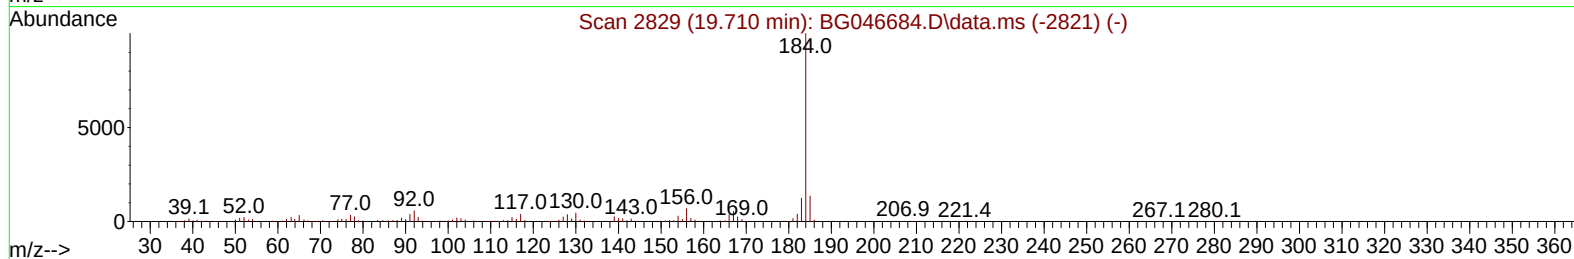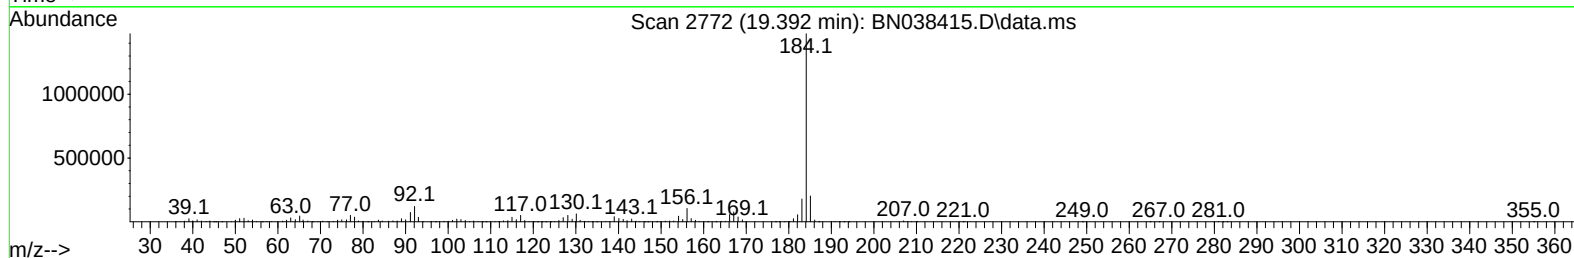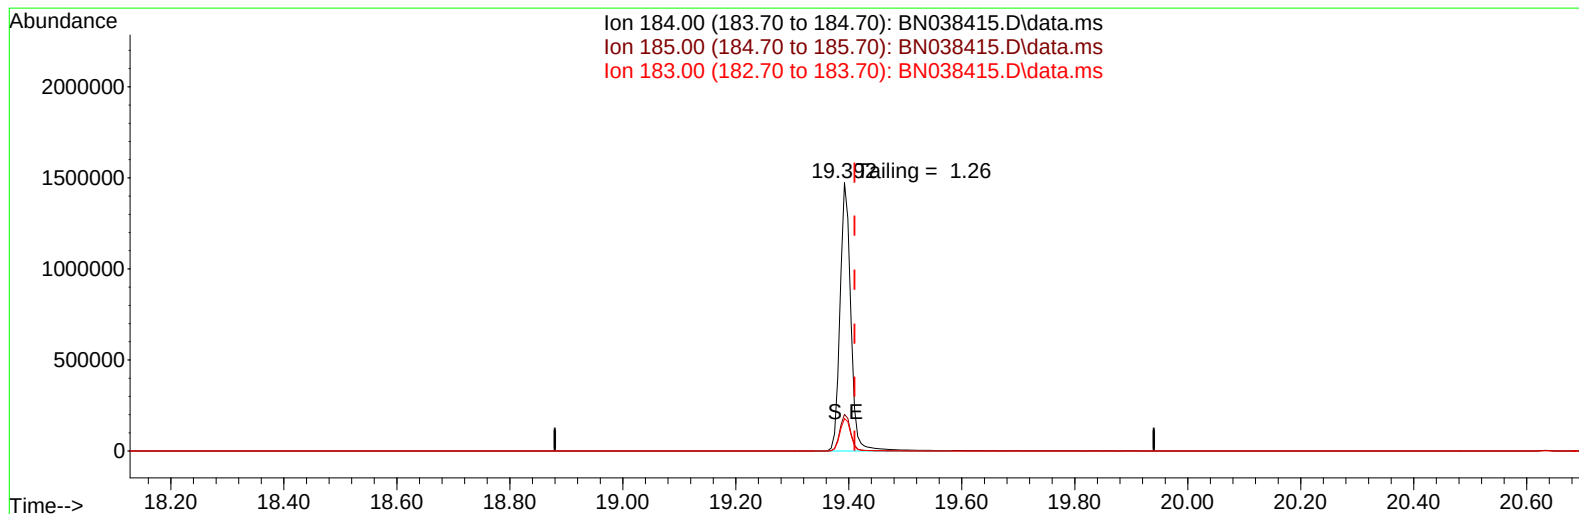

TIC: BN038415.D\data.ms

(77) Benzidine

19.392min (-0.018) 4654.56 ng

response **1952601**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.50	13.69
--------	-------	-------

183.00	13.20	12.10
--------	-------	-------

0.00 0.00 0.00