

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
 Data File : BN038425.D
 Acq On : 16 Dec 2025 04:42
 Operator : RC/JU
 Sample : Q3839-23
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AT5

Quant Time: Dec 16 05:33:56 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 10 13:56:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	5025	0.400	ng	-0.01
7) Naphthalene-d8	10.509	136	13773	0.400	ng	#-0.02
13) Acenaphthene-d10	14.388	164	7488	0.400	ng	-0.01
19) Phenanthrene-d10	17.136	188	14044	0.400	ng	#-0.01
29) Chrysene-d12	21.331	240	11274	0.400	ng	0.00
35) Perylene-d12	23.619	264	11544	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.283	112	1643	0.131	ng	0.00
5) Phenol-d6	6.879	99	1168	0.079	ng	0.00
8) Nitrobenzene-d5	8.865	82	3417	0.294	ng	-0.01
11) 2-Methylnaphthalene-d10	12.116	152	5455	0.281	ng	-0.01
14) 2,4,6-Tribromophenol	15.882	330	1162	0.350	ng	-0.01
15) 2-Fluorobiphenyl	13.003	172	13153	0.365	ng	0.00
27) Fluoranthene-d10	19.174	212	12079	0.348	ng	-0.01
31) Terphenyl-d14	19.777	244	10254	0.408	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.189	88	820	0.142	ng	# 59
9) Naphthalene	10.562	128	971	0.024	ng	# 76
25) Phenanthrene	17.173	178	1774	0.036	ng	97
34) Bis(2-ethylhexyl)phtha...	21.259	149	1401	0.059	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038425.D
Acq On : 16 Dec 2025 04:42
Operator : RC/JU
Sample : Q3839-23
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AT5

Quant Time: Dec 16 05:33:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 10 13:56:50 2025
Response via : Initial Calibration



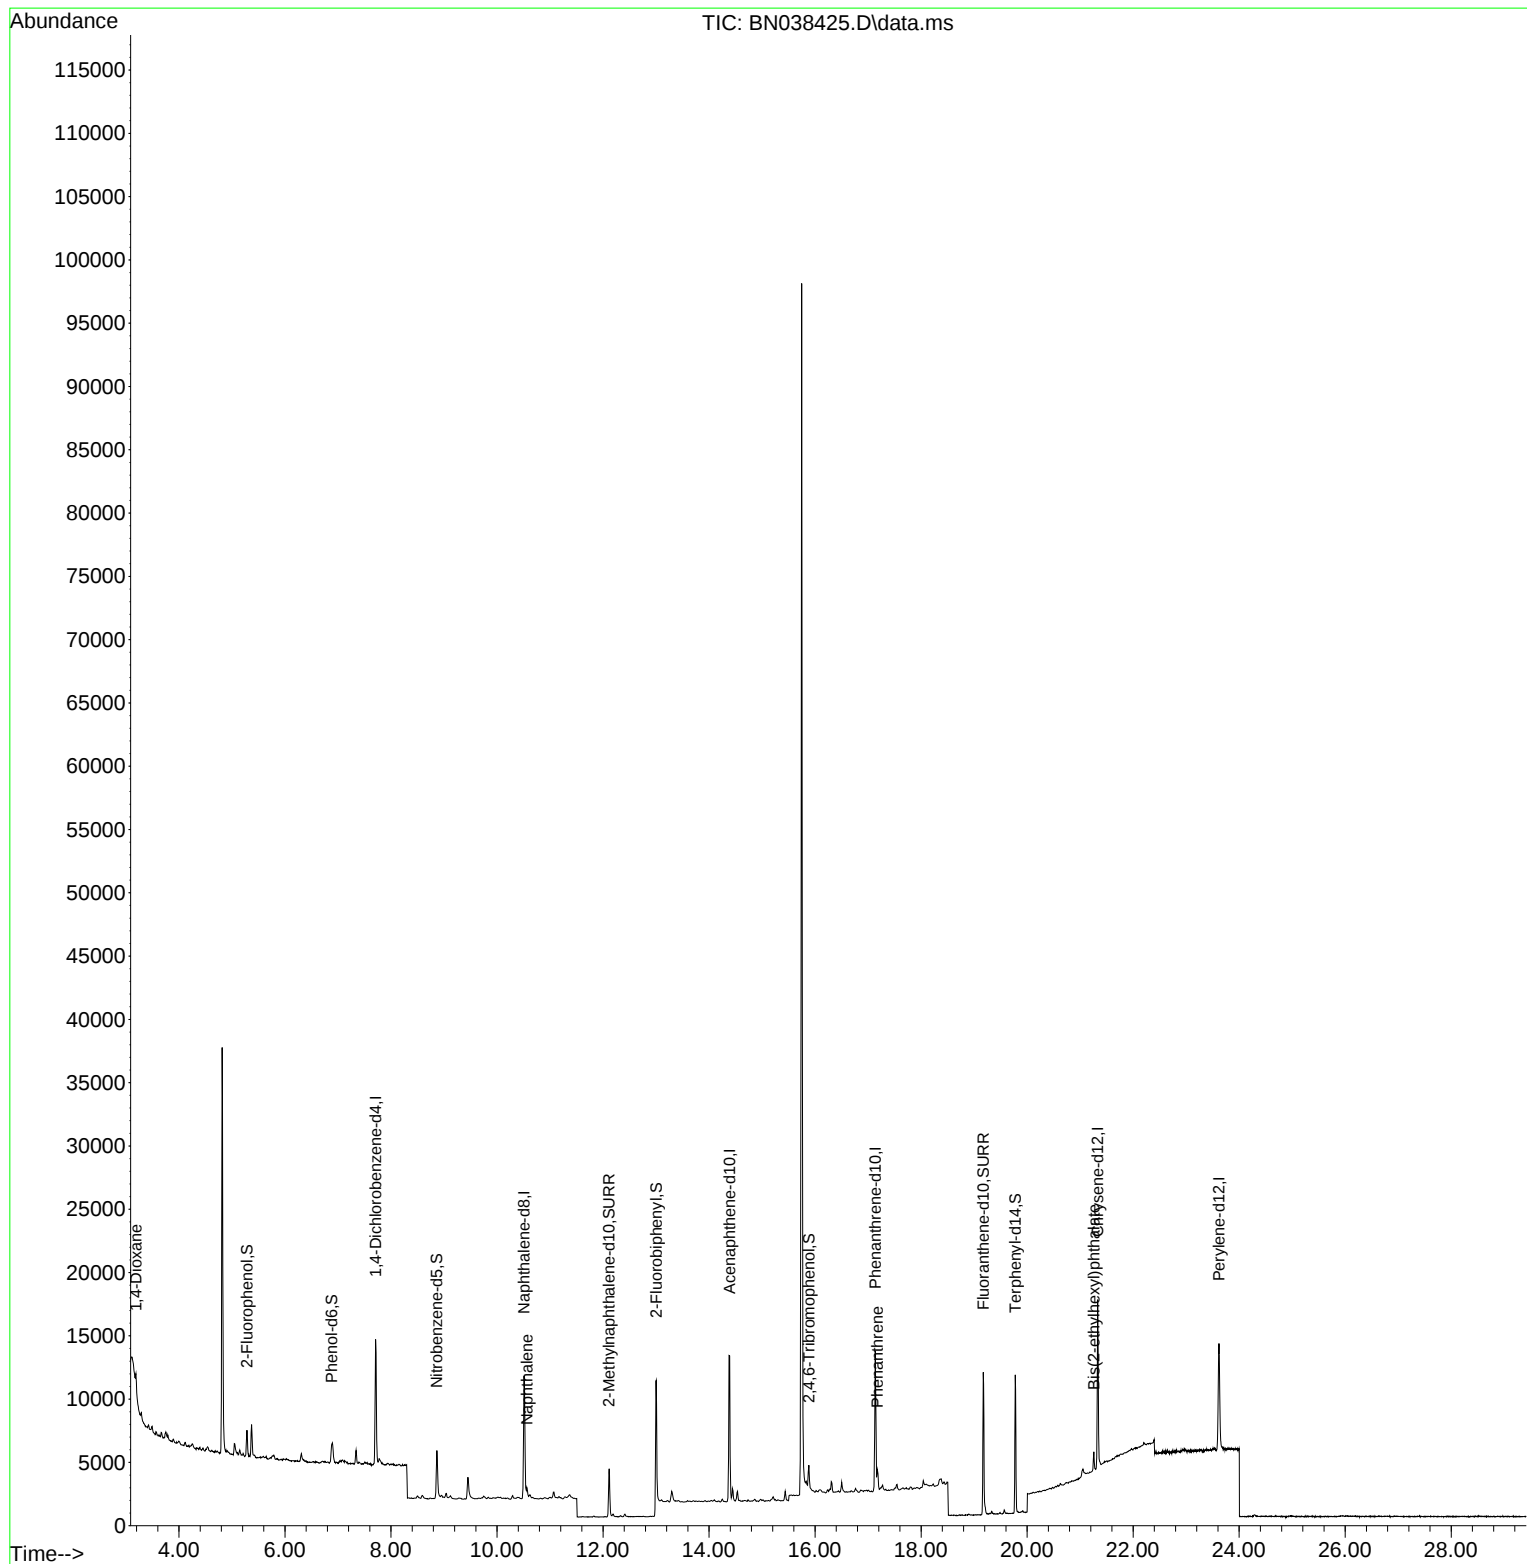




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.710 min Scan# 64
 Delta R.T. -0.014 min
 Lab File: BN038425.D
 Acq: 16 Dec 2025 04:42




Instrument :
 BNA_N
 ClientSampleId :
 C0AT5


Tgt Ion:152 Resp: 5025
 Ion Ratio Lower Upper
 152 100
 150 155.2 122.4 183.6
 115 61.8 47.3 70.9

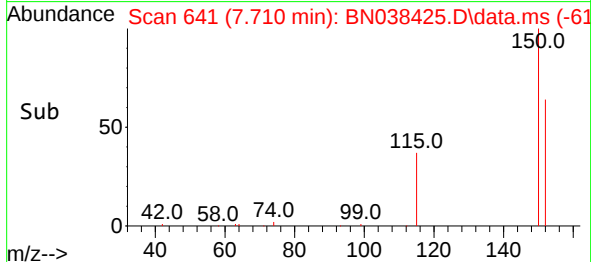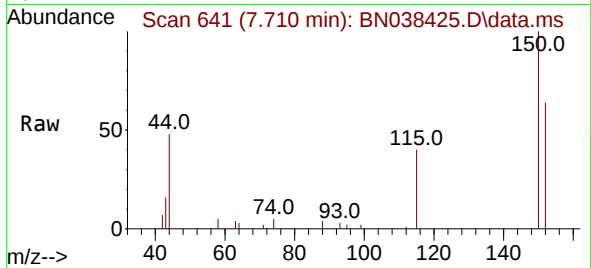

#2
 1,4-Dioxane
 Concen: 0.142 ng
 RT: 3.189 min Scan# 15
 Delta R.T. -0.007 min
 Lab File: BN038425.D
 Acq: 16 Dec 2025 04:42

Tgt Ion: 88 Resp: 820
 Ion Ratio Lower Upper
 88 100
 43 104.5 24.9 37.3#
 58 79.9 61.4 92.0


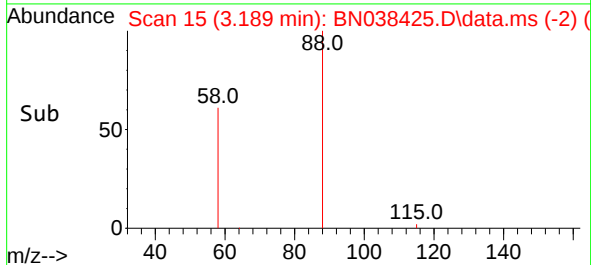

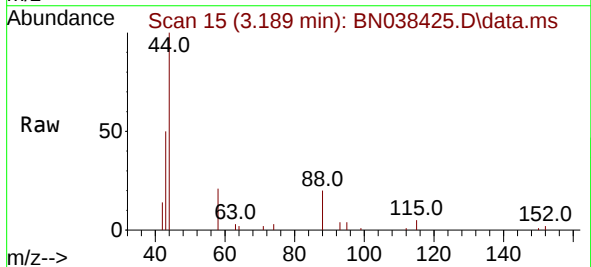


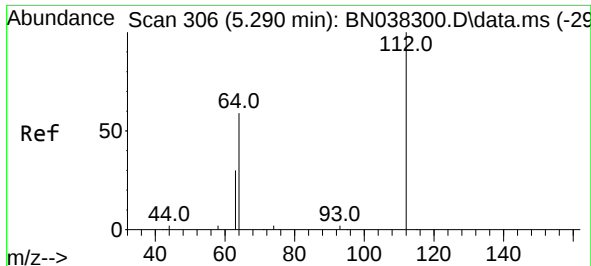

#4
2-Fluorophenol
Concen: 0.131 ng
RT: 5.283 min Scan# 306
Delta R.T. -0.007 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42




Instrument :
BNA_N
ClientSampleId :
C0AT5


Tgt Ion:112 Resp: 1643
Ion Ratio Lower Upper
112 100
64 56.8 44.4 66.6
63 31.0 23.4 35.0

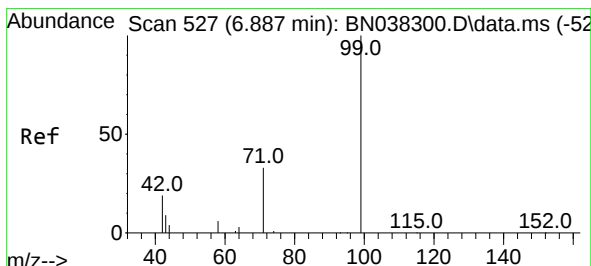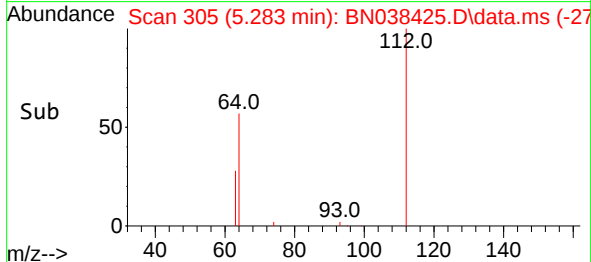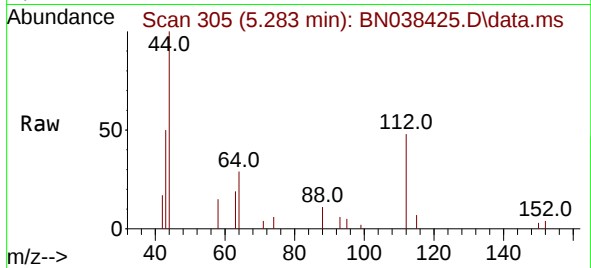

#5
Phenol-d6
Concen: 0.079 ng
RT: 6.879 min Scan# 526
Delta R.T. -0.007 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion: 99 Resp: 1168
Ion Ratio Lower Upper
99 100
42 27.5 16.5 24.7#
71 44.7 24.9 37.3#


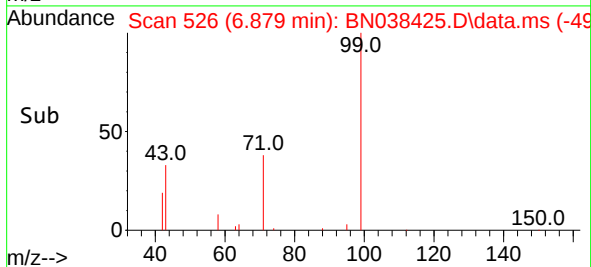

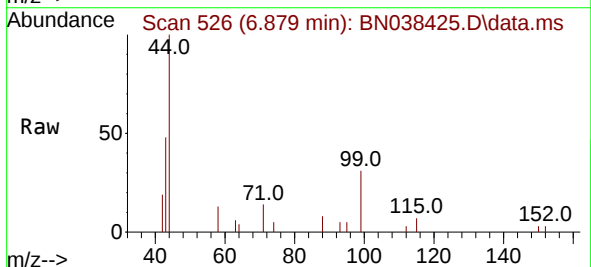


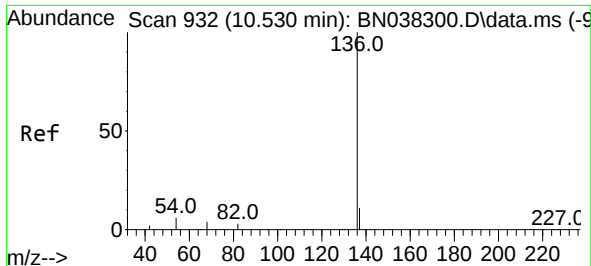

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.509 min Scan# 91
Delta R.T. -0.021 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42




Instrument :
BNA_N
ClientSampleId :
C0AT5


Tgt Ion:136 Resp: 13773
Ion Ratio Lower Upper
136 100
137 11.9 9.1 13.7
54 11.2 5.2 7.8#
68 8.3 4.1 6.1#

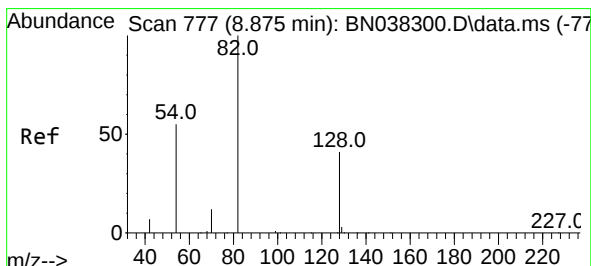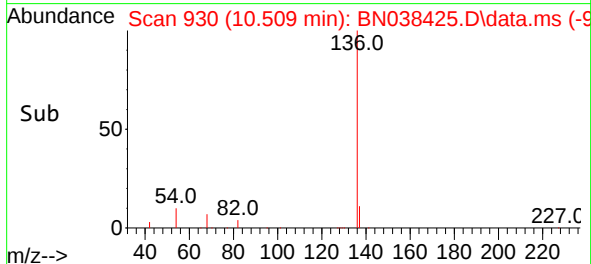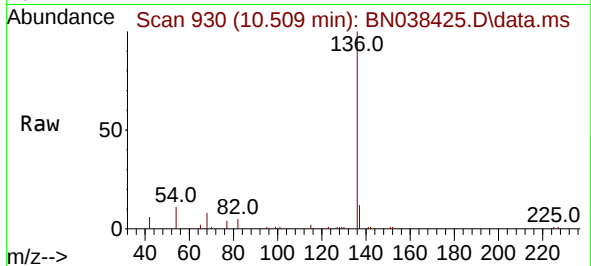

#8
Nitrobenzene-d5
Concen: 0.294 ng
RT: 8.865 min Scan# 776
Delta R.T. -0.011 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion: 82 Resp: 3417
Ion Ratio Lower Upper
82 100
128 44.2 34.0 51.0
54 58.8 44.4 66.6


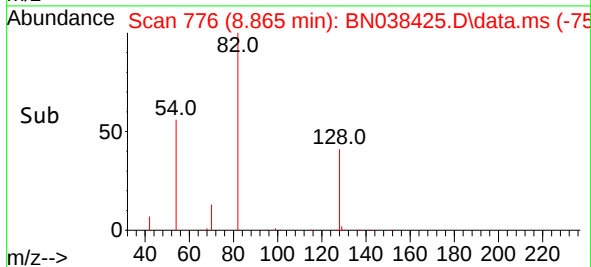

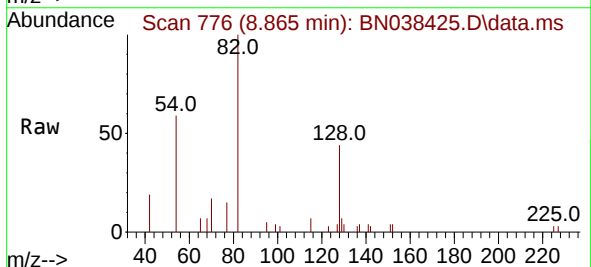


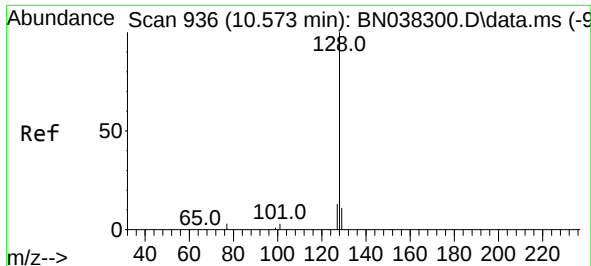

#9
Naphthalene
Concen: 0.024 ng
RT: 10.562 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42




Instrument :
BNA_N
ClientSampleId :
C0AT5


Tgt Ion:128 Resp: 971
Ion Ratio Lower Upper
128 100
129 22.2 9.1 13.7#
127 21.7 10.9 16.3#

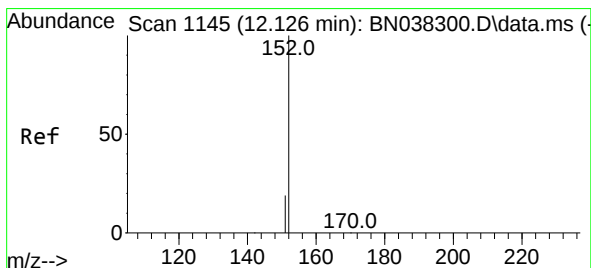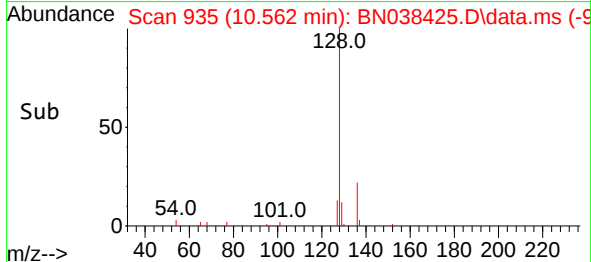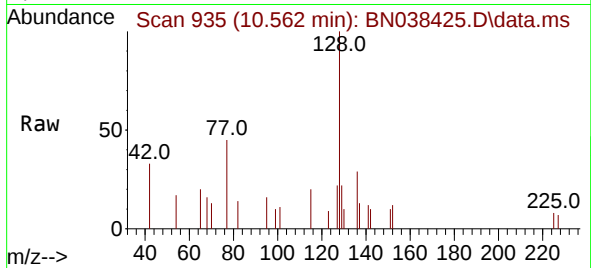

#11
2-Methylnaphthalene-d10
Concen: 0.281 ng
RT: 12.116 min Scan# 1143
Delta R.T. -0.010 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion:152 Resp: 5455
Ion Ratio Lower Upper
152 100
151 21.1 17.0 25.6


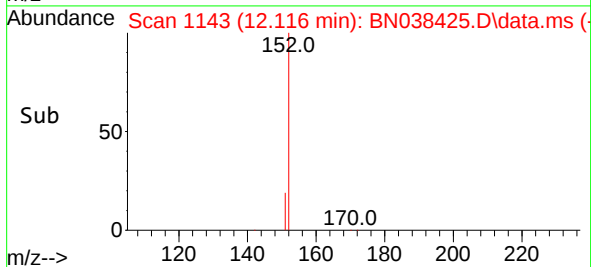

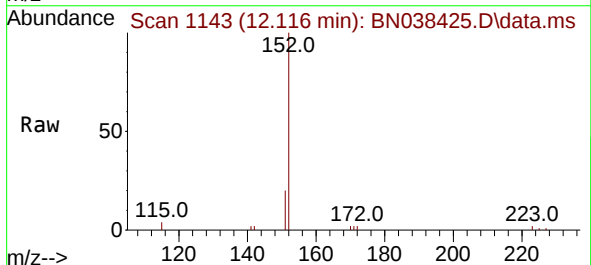


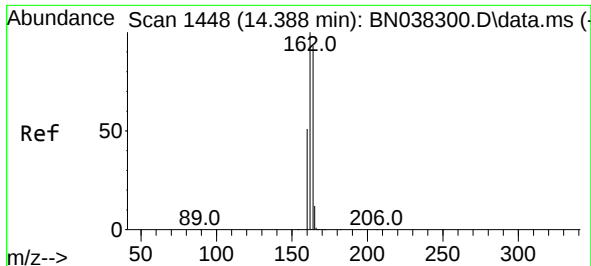

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.388 min Scan# 1448
Delta R.T. -0.011 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42




Instrument :
BNA_N
ClientSampleId :
C0AT5

Tgt Ion:164 Resp: 7488
Ion Ratio Lower Upper
164 100
162 103.0 86.2 129.4
160 49.9 44.6 67.0

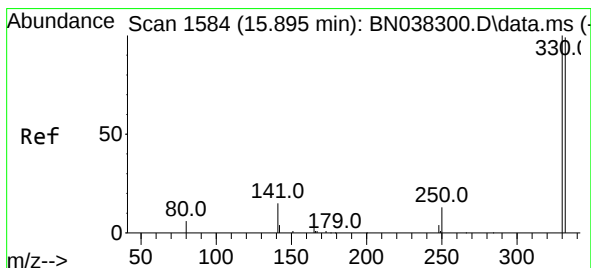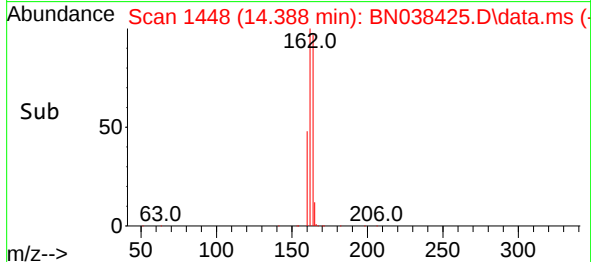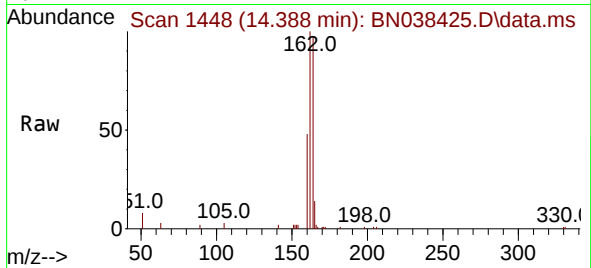

#14
2,4,6-Tribromophenol
Concen: 0.350 ng
RT: 15.882 min Scan# 1583
Delta R.T. -0.012 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion:330 Resp: 1162
Ion Ratio Lower Upper
330 100
332 98.1 75.8 113.6
141 40.8 31.8 47.8


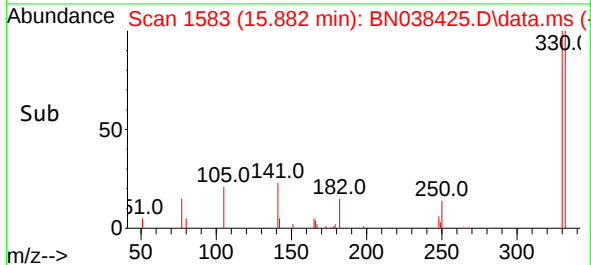

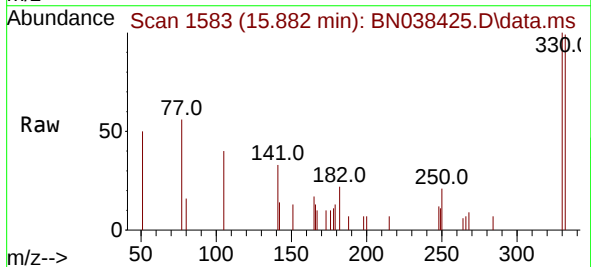




#15
2-Fluorobiphenyl
Concen: 0.365 ng
RT: 13.003 min Scan# 11
Delta R.T. -0.005 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42




Instrument :
BNA_N
ClientSampleId :
C0AT5


Tgt Ion:	172	Resp:	13153
Ion	Ratio	Lower	Upper
172	100		
171	35.5	28.6	42.8
170	23.1	19.3	28.9

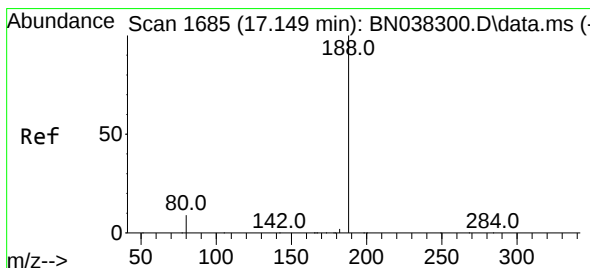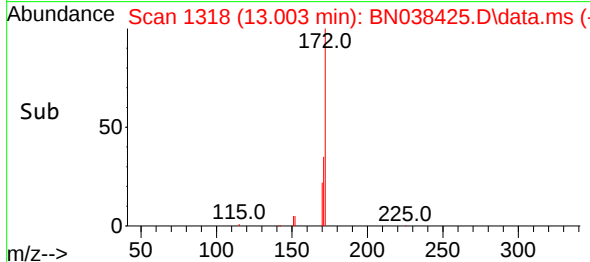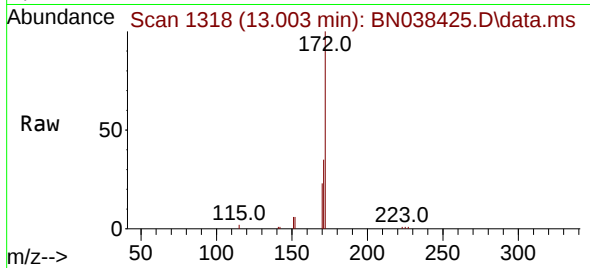

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.136 min Scan# 1684
Delta R.T. -0.012 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion:	188	Resp:	14044
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.3	7.4	11.0


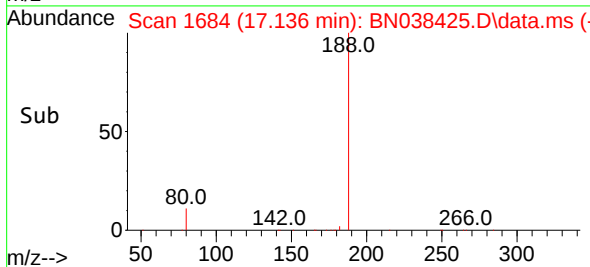

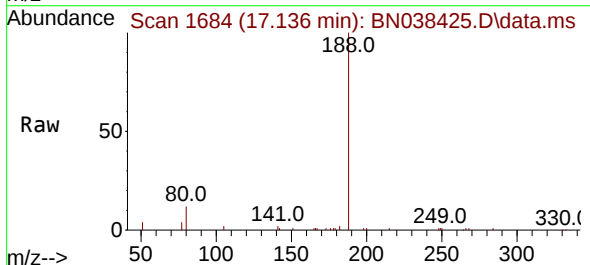


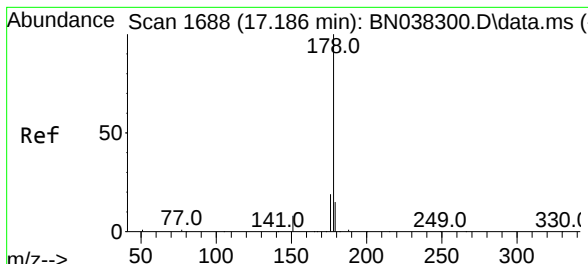

#25
 Phenanthrene
 Concen: 0.036 ng
 RT: 17.173 min Scan# 1687
 Delta R.T. -0.012 min
 Lab File: BN038425.D
 Acq: 16 Dec 2025 04:42




Instrument :
 BNA_N
 ClientSampleId :
 C0AT5


Tgt Ion:	178	Resp:	1774
Ion	Ratio	Lower	Upper
178	100		
176	21.2	15.5	23.3
179	16.2	12.2	18.2

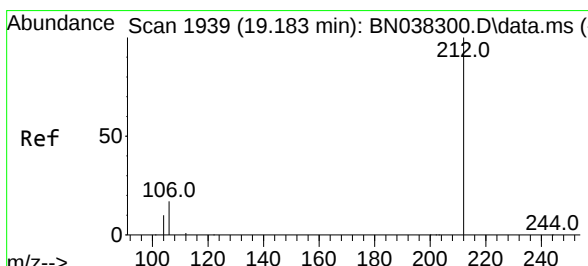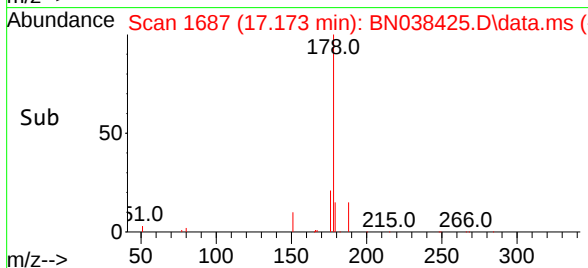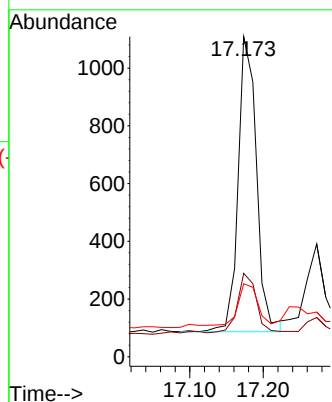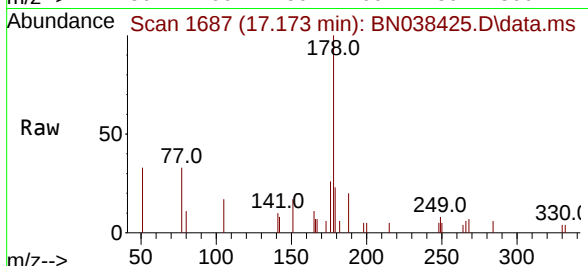

#27
 Fluoranthene-d10
 Concen: 0.348 ng
 RT: 19.174 min Scan# 1937
 Delta R.T. -0.014 min
 Lab File: BN038425.D
 Acq: 16 Dec 2025 04:42

Tgt Ion:	212	Resp:	12079
Ion	Ratio	Lower	Upper
212	100		
106	17.6	13.7	20.5
104	10.4	7.8	11.8

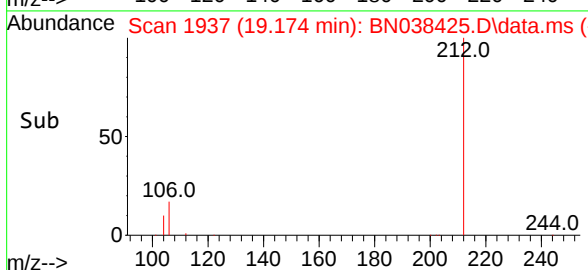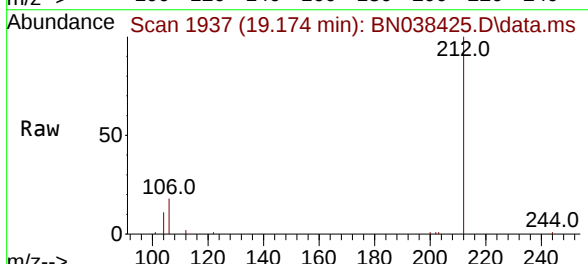

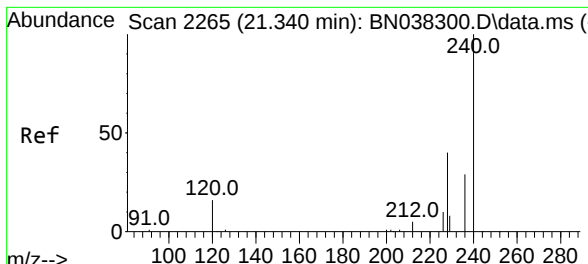

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.331 min Scan# 21

Delta R.T. -0.009 min

Lab File: BN038425.D

Acq: 16 Dec 2025 04:42

Instrument :

BNA_N

ClientSampleId :

C0AT5





Tgt Ion:240 Resp: 11274

Ion Ratio Lower Upper

240 100

120 20.1 15.4 23.2

236 29.7 23.9 35.9

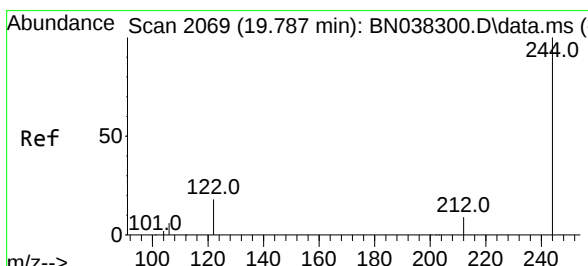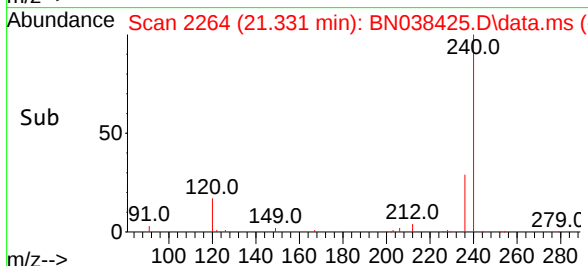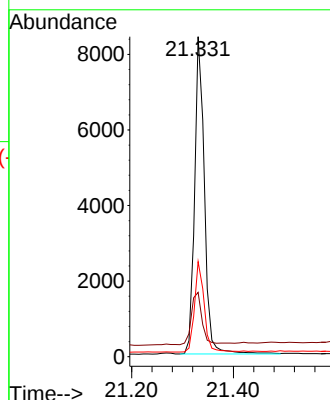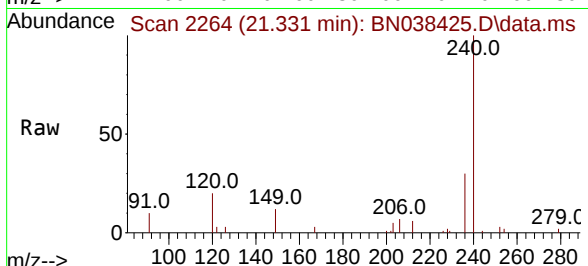

#31

Terphenyl-d14

Concen: 0.408 ng

RT: 19.777 min Scan# 2067

Delta R.T. -0.014 min

Lab File: BN038425.D

Acq: 16 Dec 2025 04:42




Tgt Ion:244 Resp: 10254


Ion Ratio Lower Upper

244 100

212 9.7 7.9 11.9

122 20.5 15.0 22.6


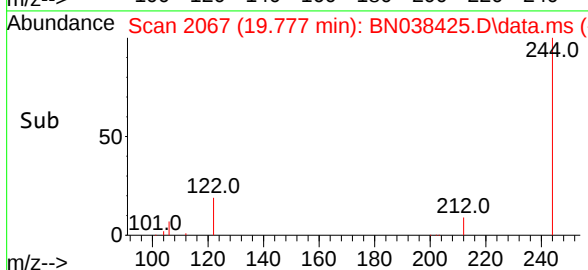
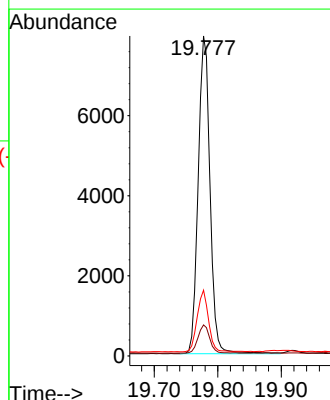
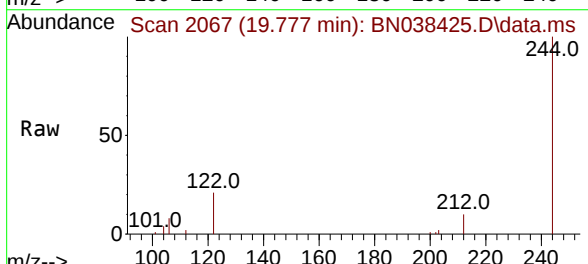


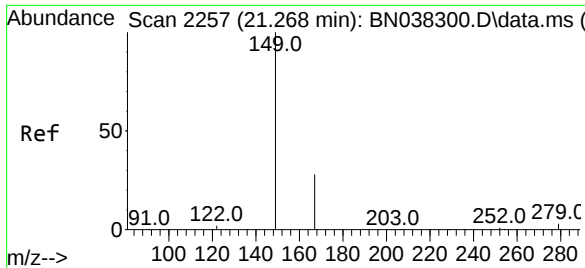

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.059 ng
RT: 21.259 min Scan# 21256
Delta R.T. -0.009 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Instrument :
BNA_N
ClientSampleId :
C0AT5

Tgt Ion:149 Resp: 1401
Ion Ratio Lower Upper
149 100
167 28.7 21.4 32.0
279 5.8 2.4 3.6#

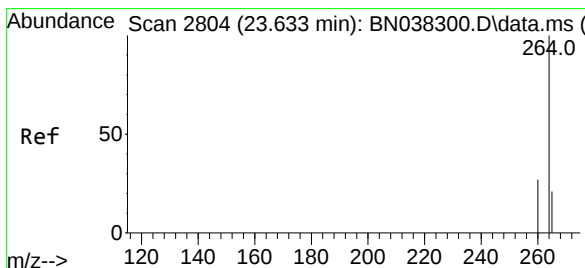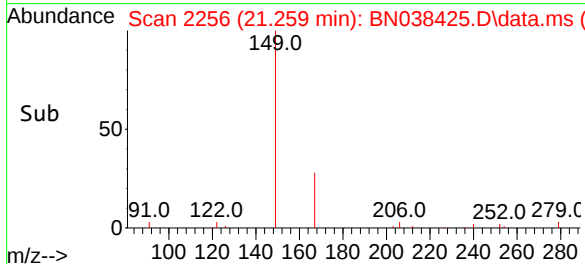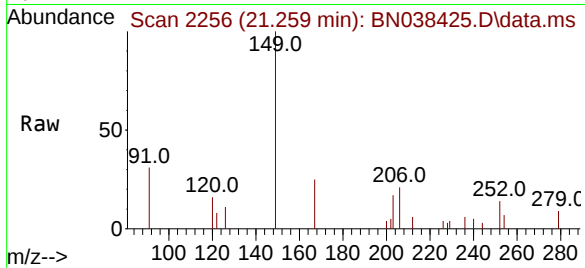

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.619 min Scan# 2799
Delta R.T. -0.015 min
Lab File: BN038425.D
Acq: 16 Dec 2025 04:42

Tgt Ion:264 Resp: 11544
Ion Ratio Lower Upper
264 100
260 27.4 22.2 33.2
265 84.2 80.2 120.2

