


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038397.D
Acq On : 15 Dec 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

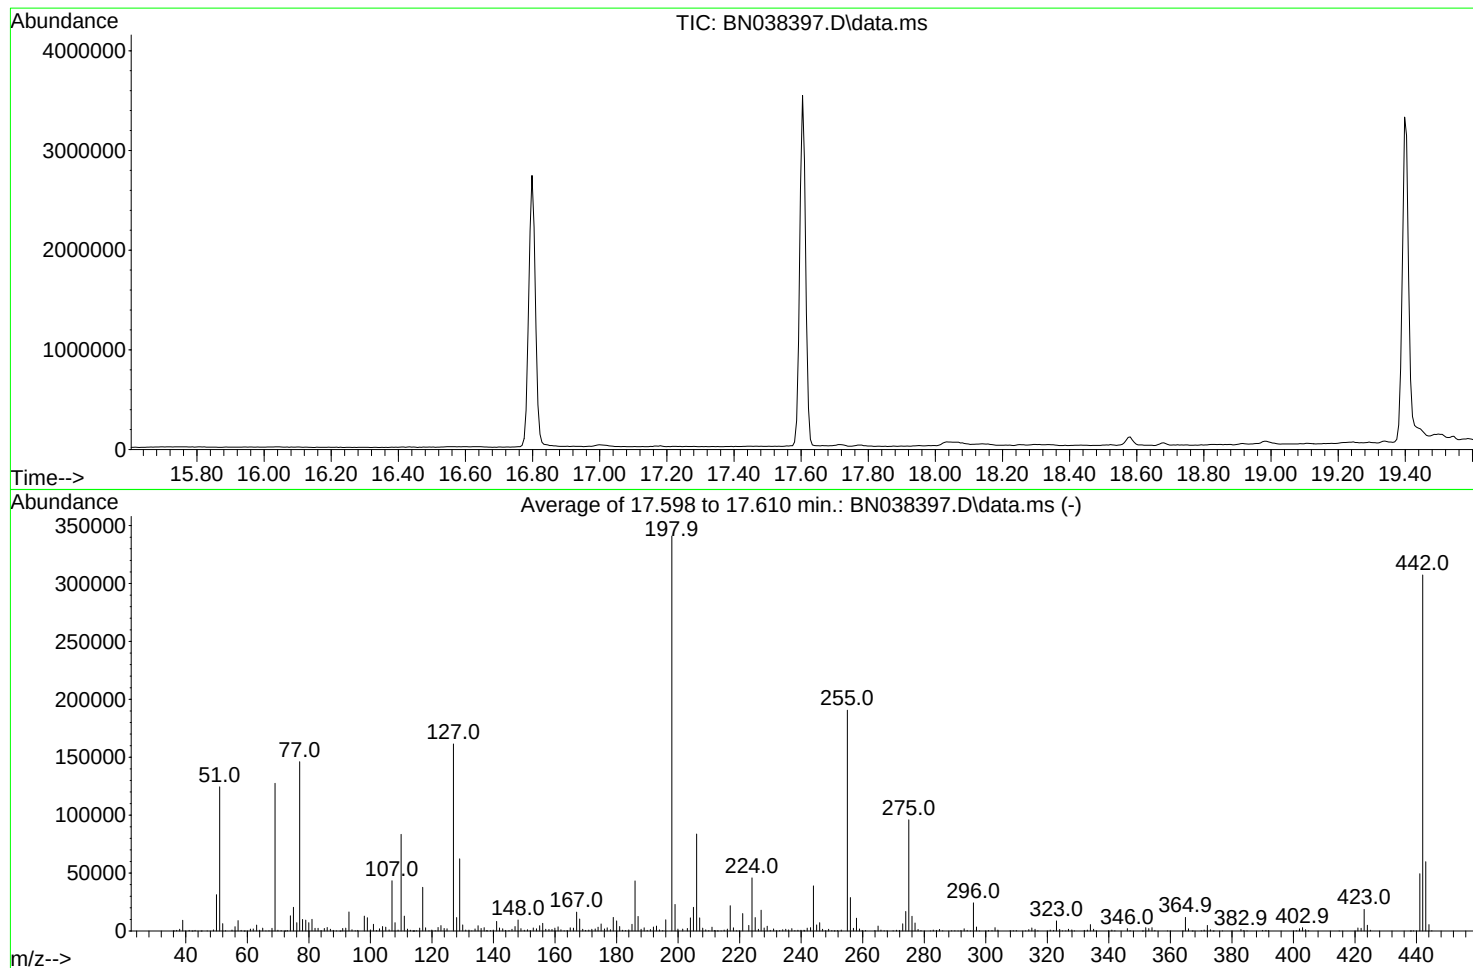




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	2335	PASS
69	69	100	100	100.0	127541	PASS
70	69	0.00	2	0.5	650	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	340885	PASS
199	198	5	9	6.7	22952	PASS
365	198	1	100	3.5	11811	PASS
441	443	0.01	150	82.8	49504	PASS
442	442	100	100	100.0	307392	PASS
443	442	15	24	19.4	59784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038397.D
Acq On : 15 Dec 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 10:09:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

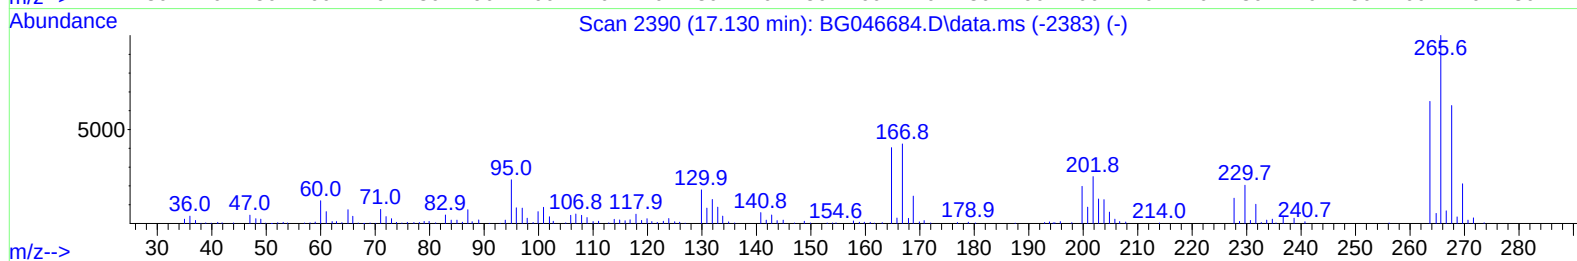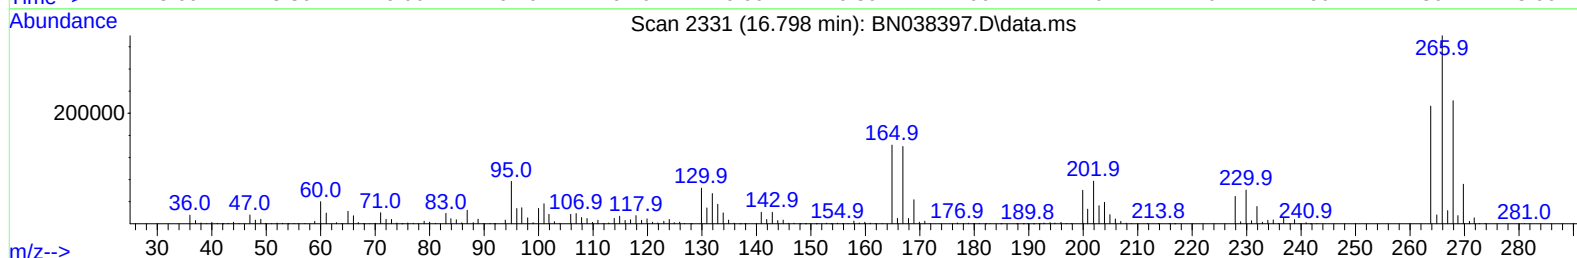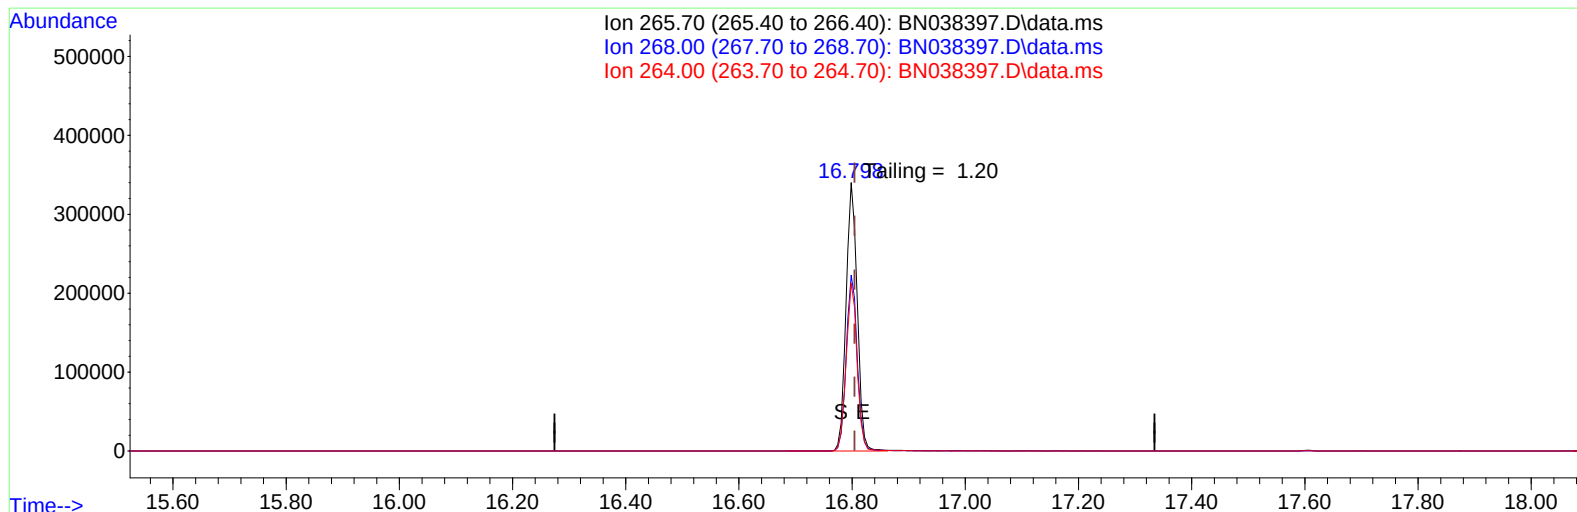

TIC: BN038397.D\data.ms

(70) Pentachlorophenol (C)

16.798min (-0.006) 553107.47 ng




response 468790

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.49
264.00	61.60	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038397.D
Acq On : 15 Dec 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 15 10:09:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

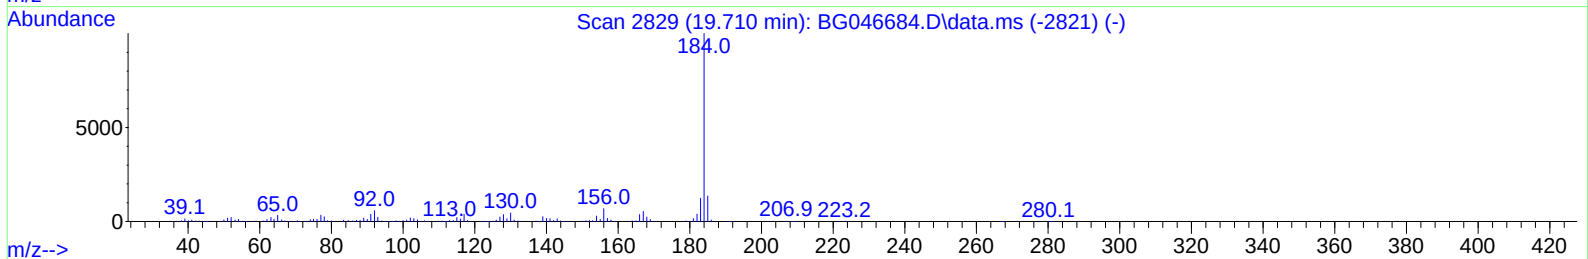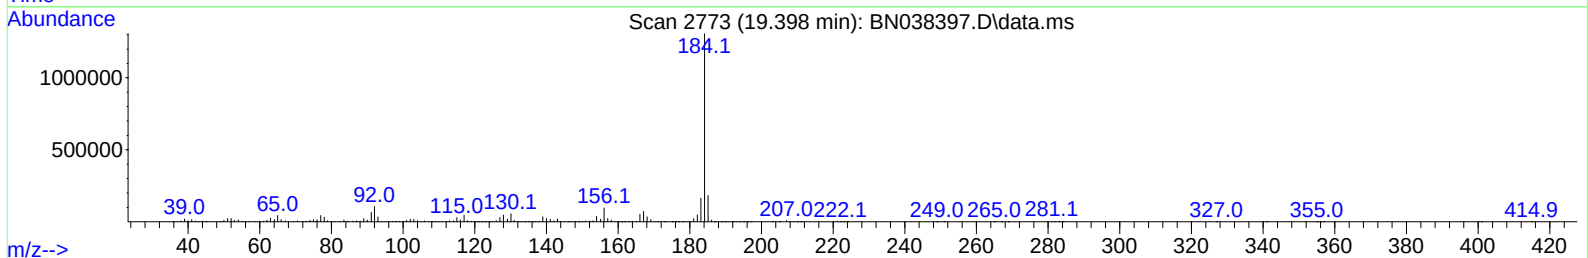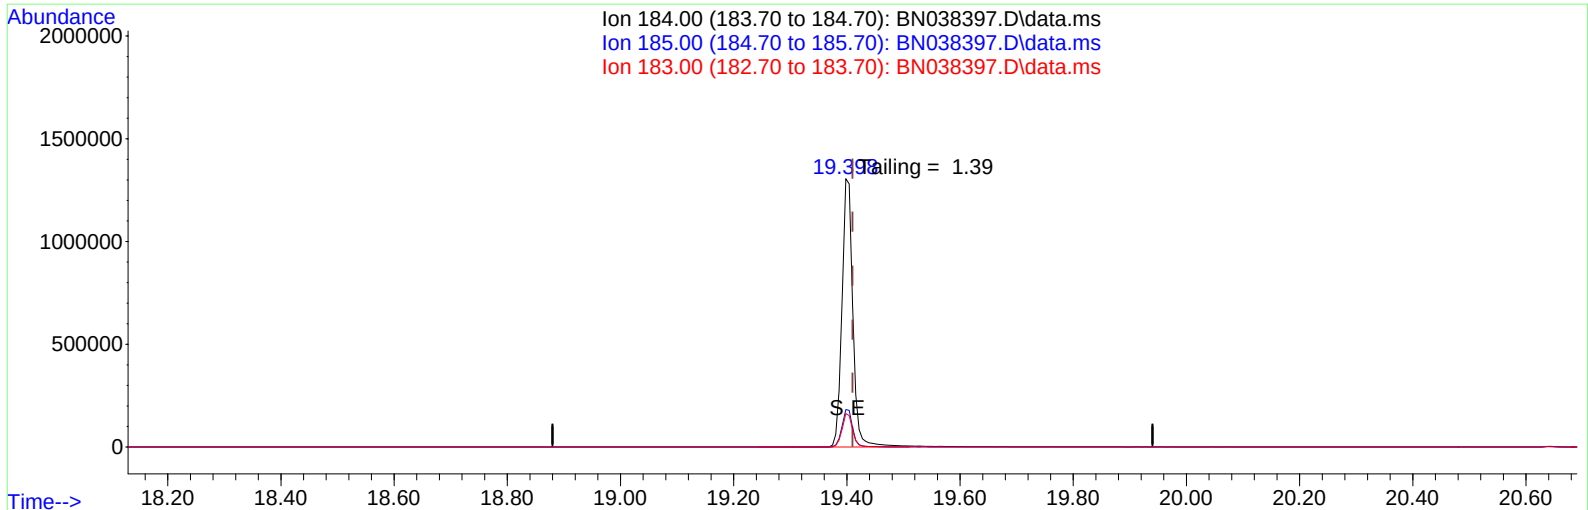

TIC: BN038397.D\data.ms

(77) Benzidine

19.398min (-0.012) 4213.74 ng

response 1763907

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.97
183.00	13.20	12.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2025	BNA_N	<u>BN038397.D</u>
Compound Name	Response	Retention Time
DDT	935587	20.645
DDD	80387	20.204
DDE	3165	19.638
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
83552	1019139	8.20

S

Instrument :
BNA_N
ClientSampleId :
DFTPP