
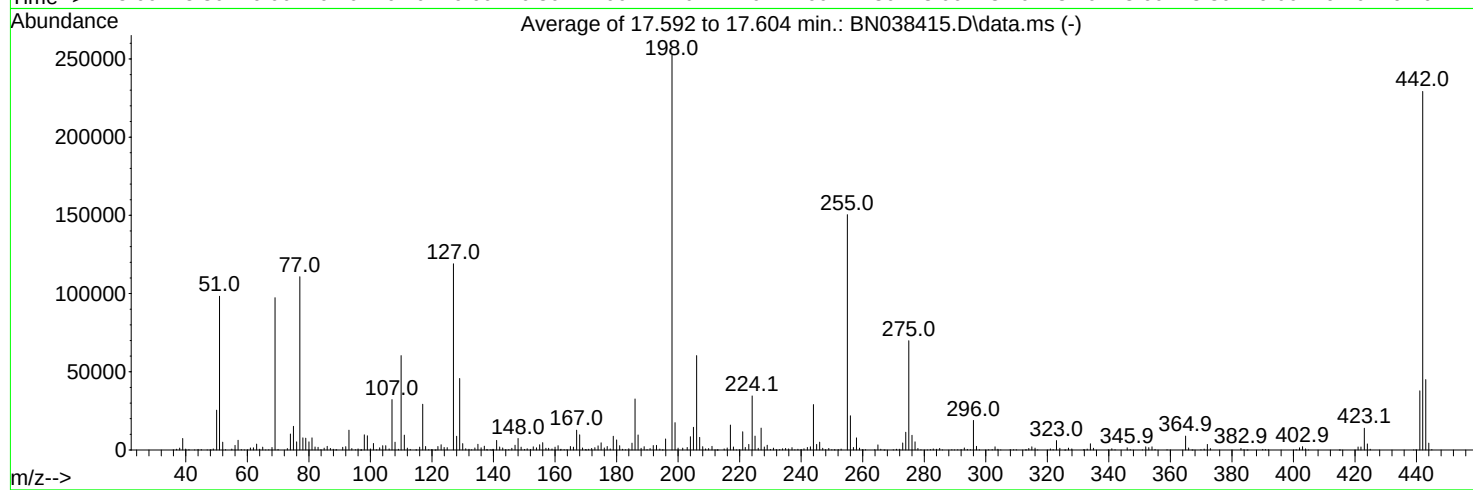


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038415.D
Acq On : 15 Dec 2025 22:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

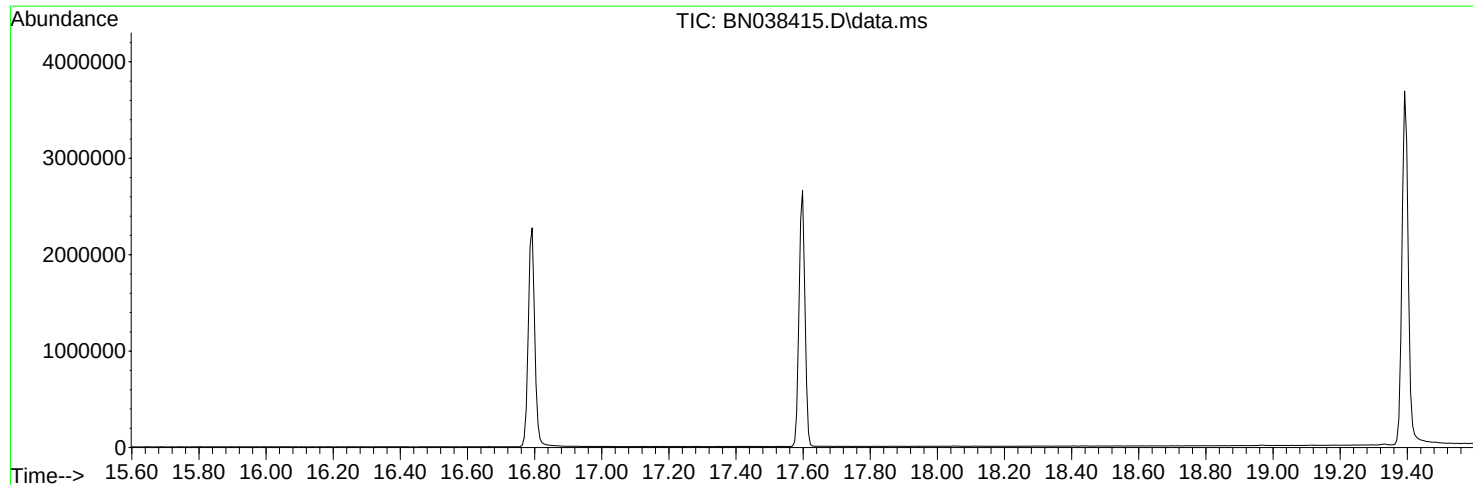




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	1668	PASS
69	69	100	100	100.0	97435	PASS
70	69	0.00	2	0.5	460	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	252395	PASS
199	198	5	9	6.9	17487	PASS
365	198	1	100	3.5	8934	PASS
441	443	0.01	150	84.1	37851	PASS
442	442	100	100	100.0	229248	PASS
443	442	15	24	19.6	45005	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038415.D
Acq On : 15 Dec 2025 22:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 16 00:22:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

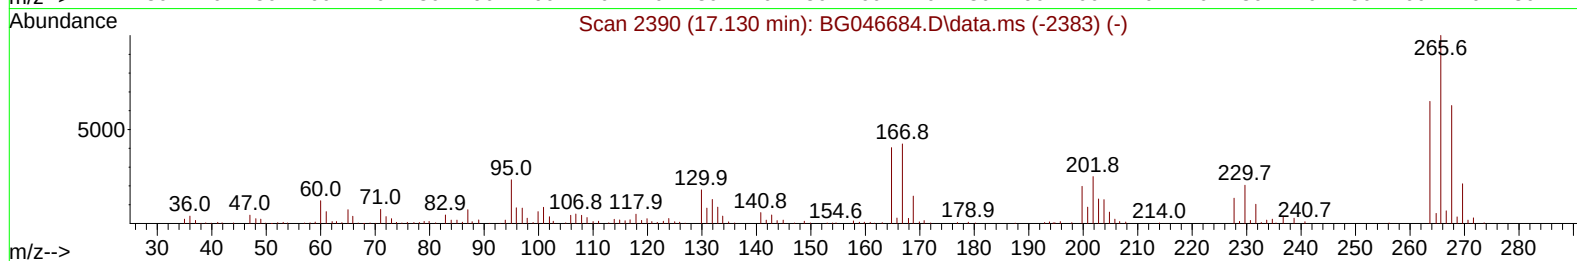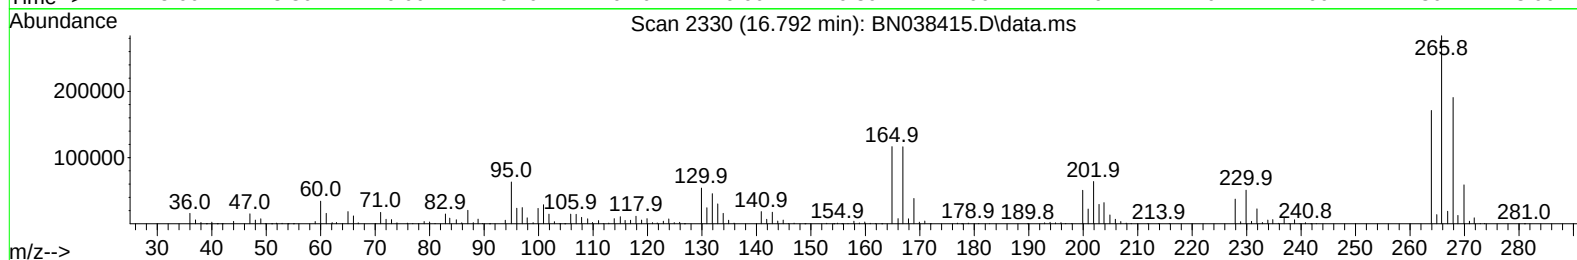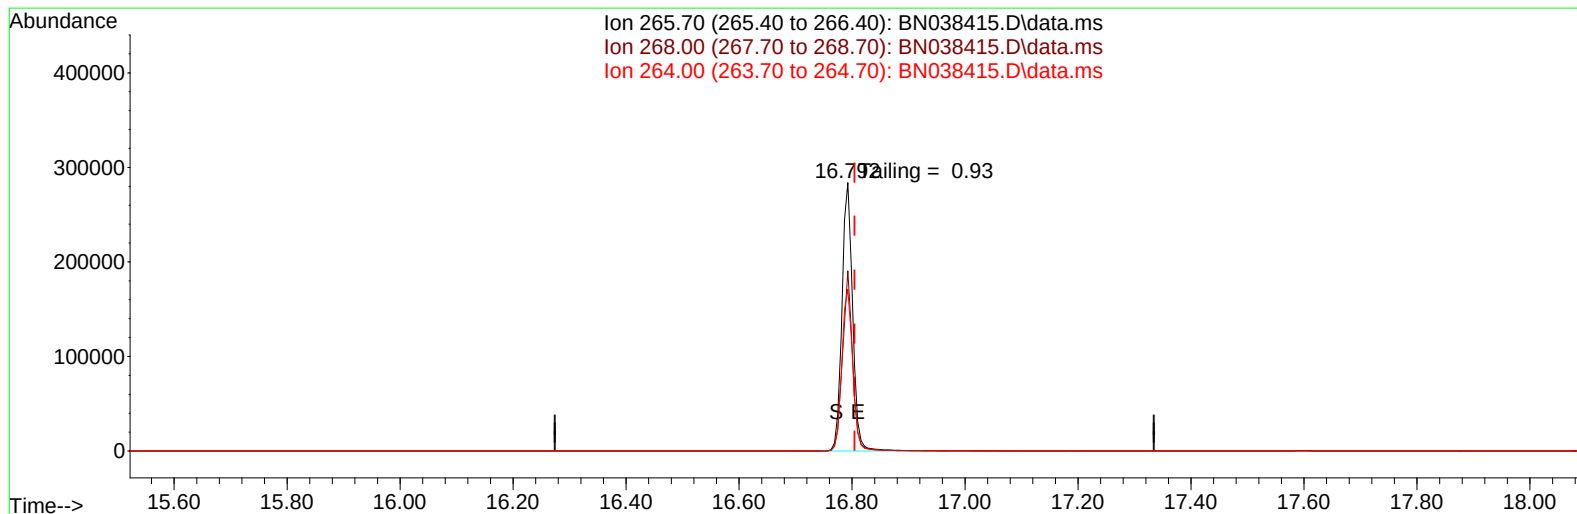

TIC: BN038415.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.012) 591376.64 ng




response 371278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.13
264.00	61.60	60.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121525\
Data File : BN038415.D
Acq On : 15 Dec 2025 22:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 16 00:22:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

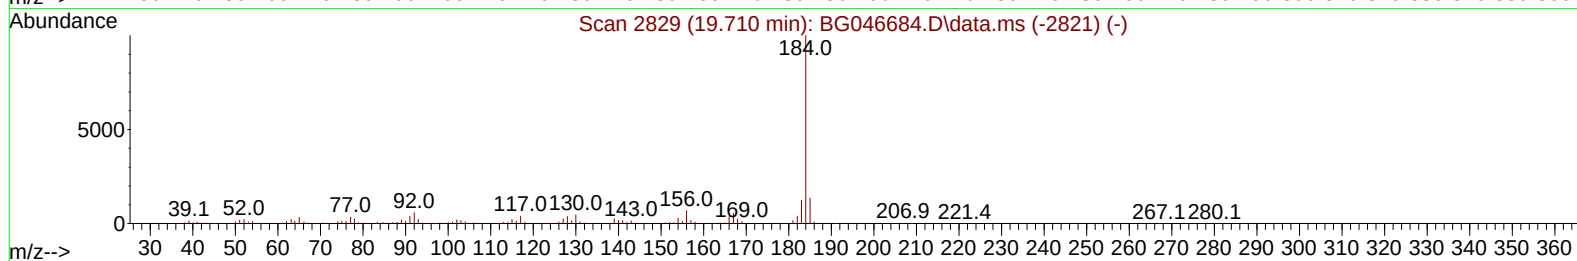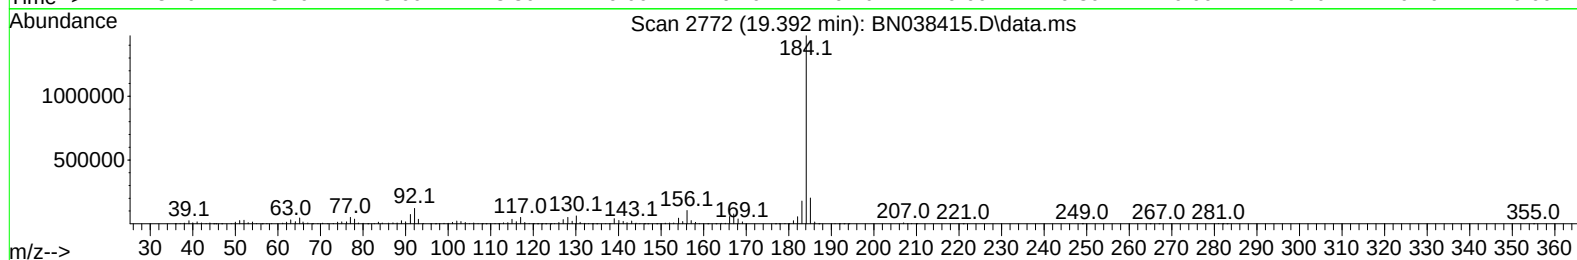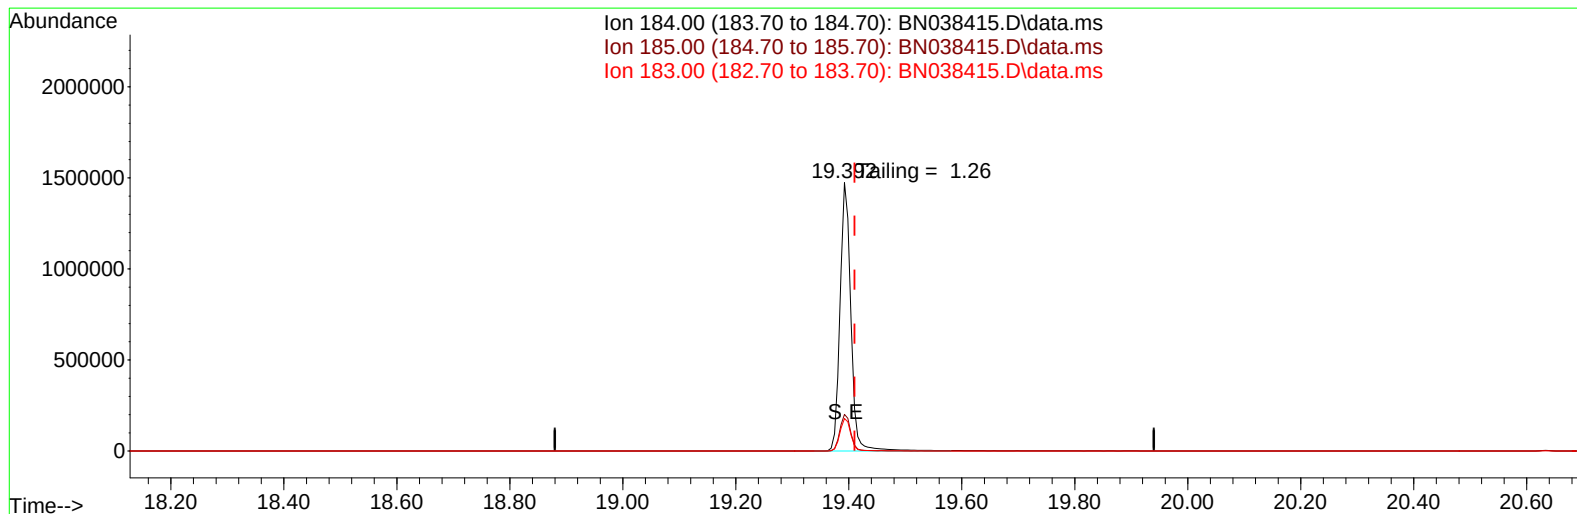

TIC: BN038415.D\data.ms

(77) Benzidine

19.392min (-0.018) 4654.56 ng

response 1952601

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.69
183.00	13.20	12.10
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2025	BNA_N	<u>BN038415.D</u>
Compound Name	Response	Retention Time
DDT	894528	20.633
DDD	56011	20.192
DDE	1434	19.686
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57445	951973	6.03

S

Instrument :
BNA_N
ClientSampleId :
DFTPP