

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (QT Reviewed)


Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:54:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

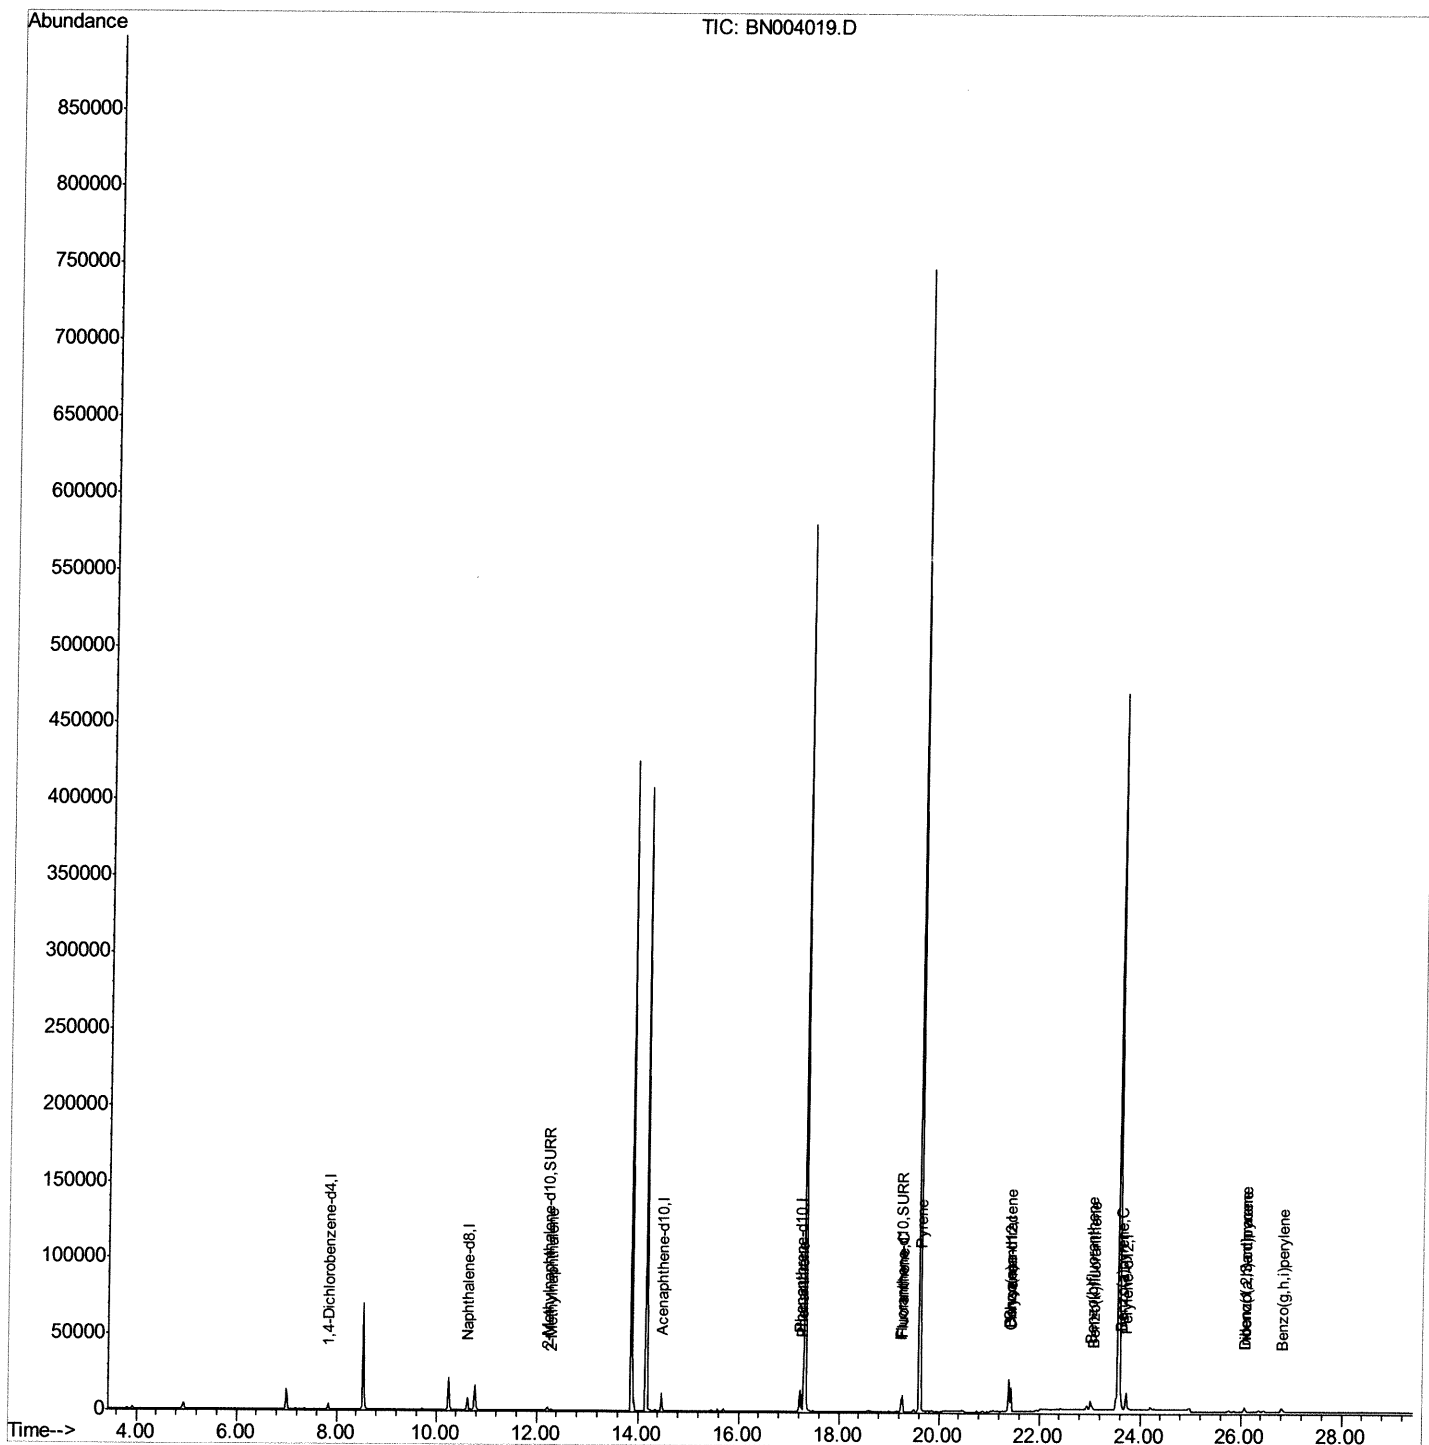

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 06:26:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

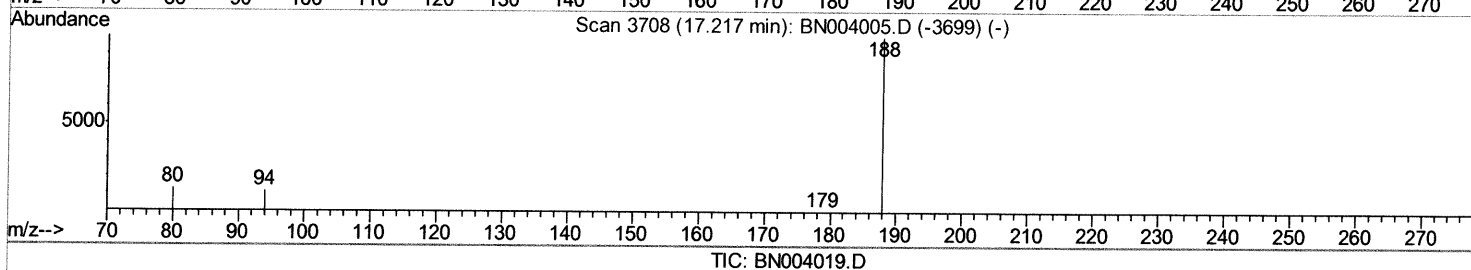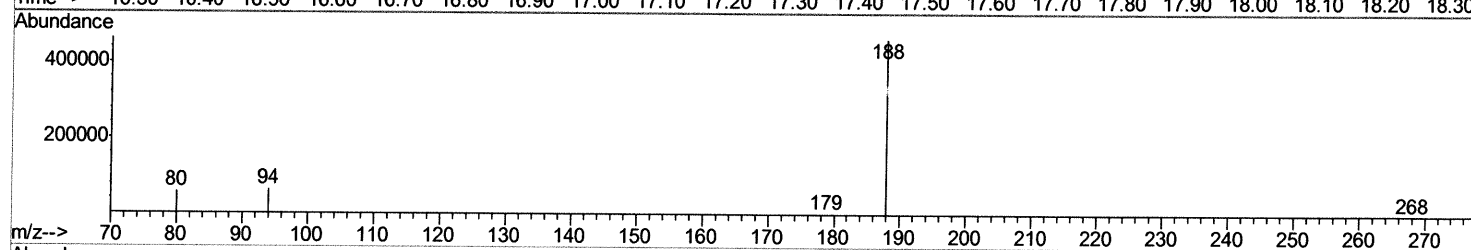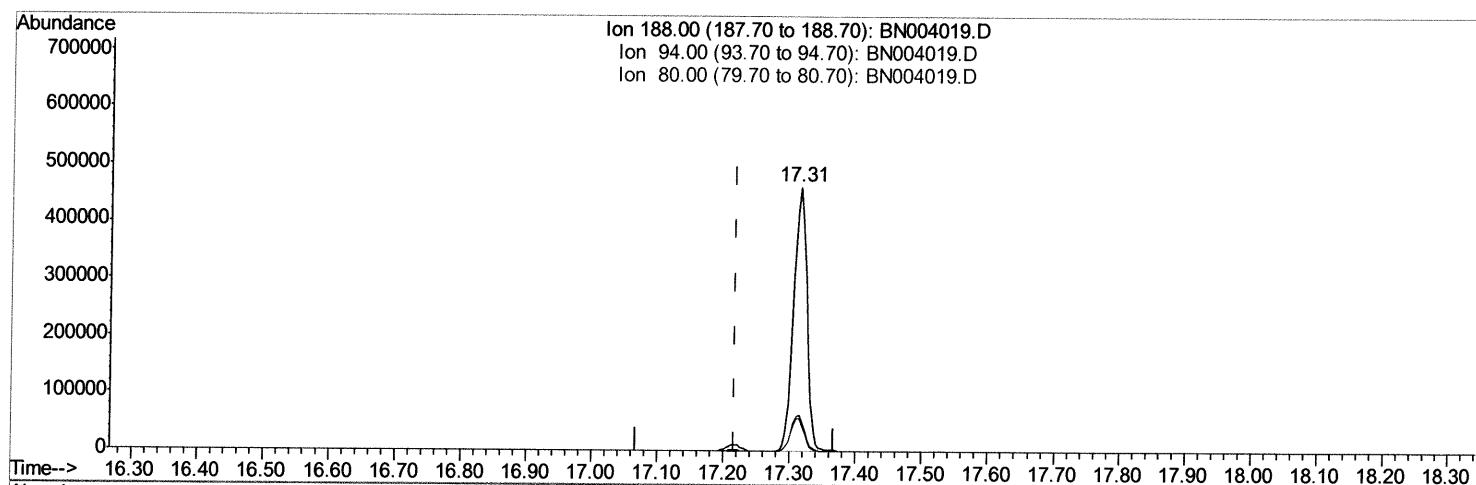

(10) Phenanthrene-d10 (I)
17.314min (+0.097) 0.40ng/ul
response 637137

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	13.45#
80.00	11.60	12.14
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 06:26:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

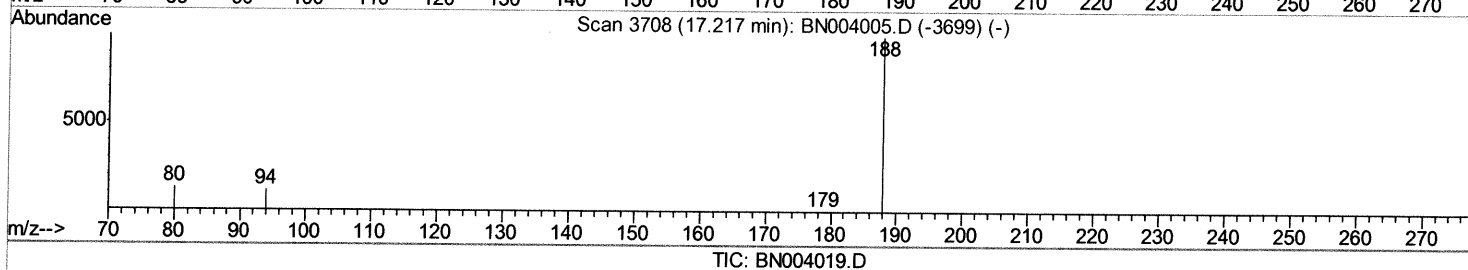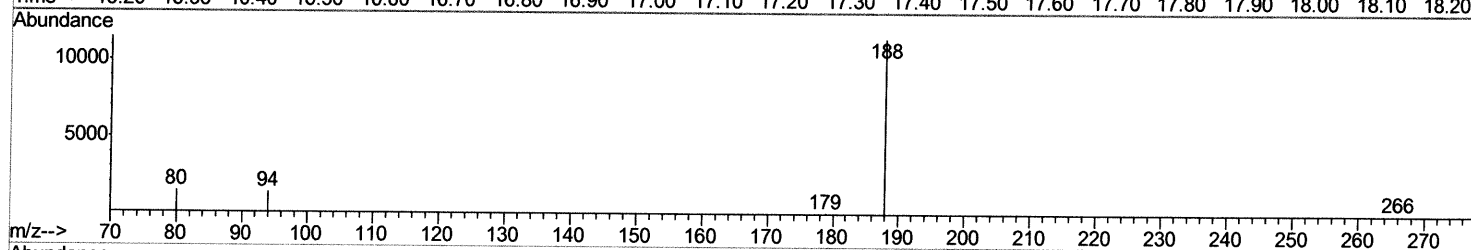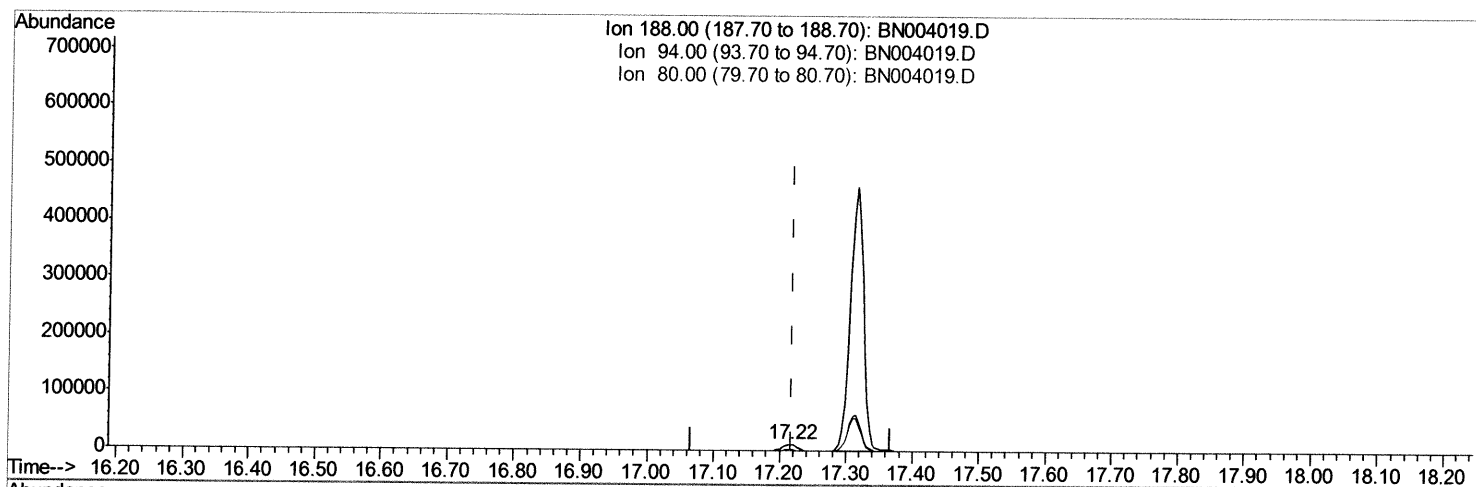

(10) Phenanthrene-d10 (I)

17.217min (-0.000) 0.40ng/ul m

response 16299

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.75
80.00	11.60	12.54
0.00	0.00	0.00

> SJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

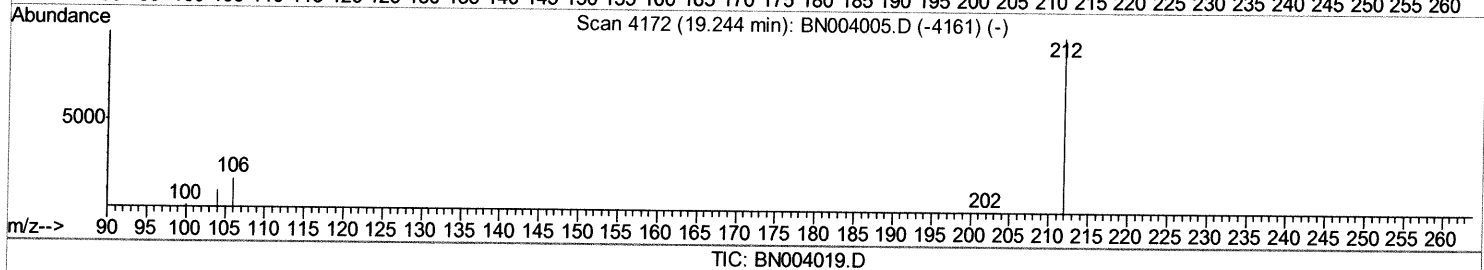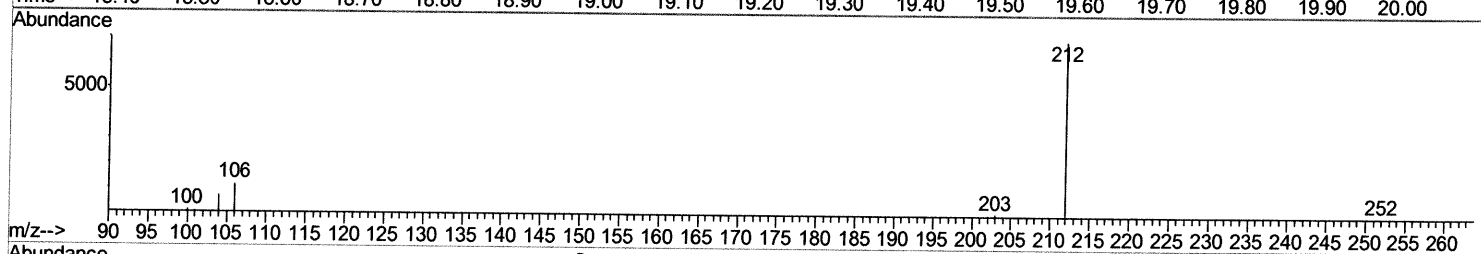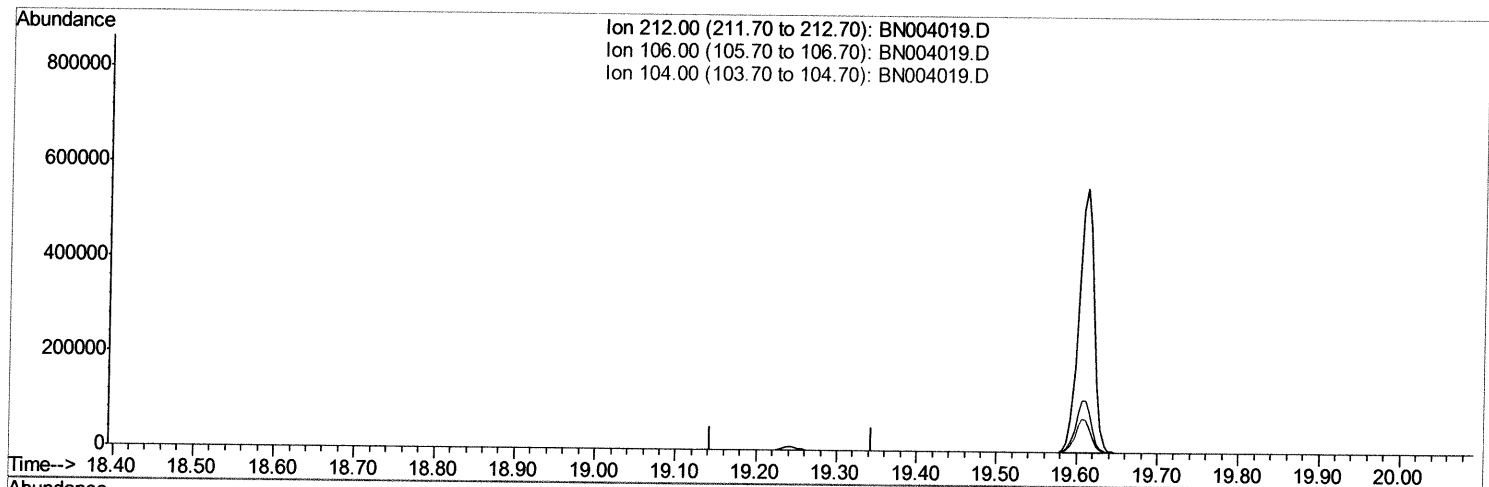

(14) Fluoranthene-d10 (SURR)

19.244min (-19.244) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

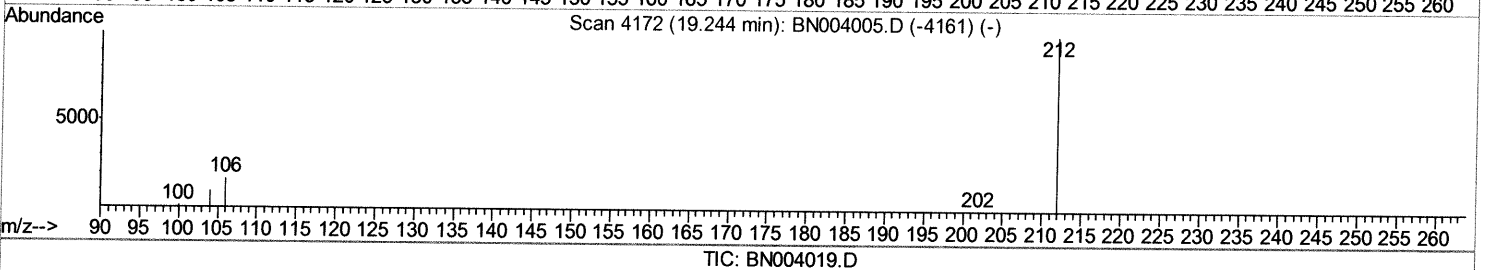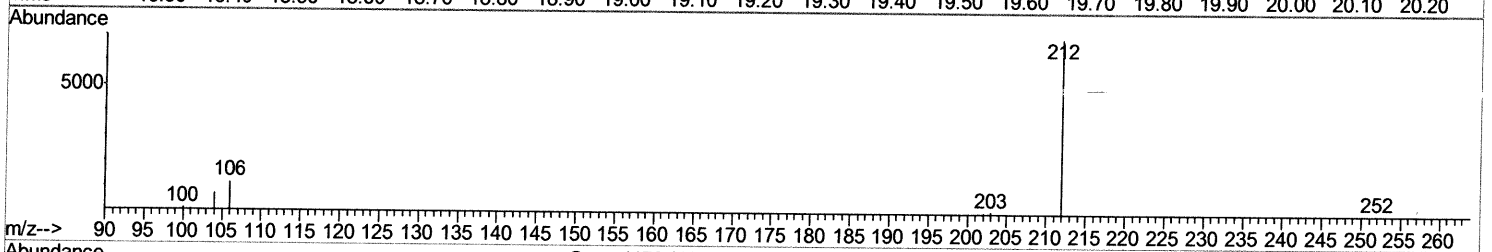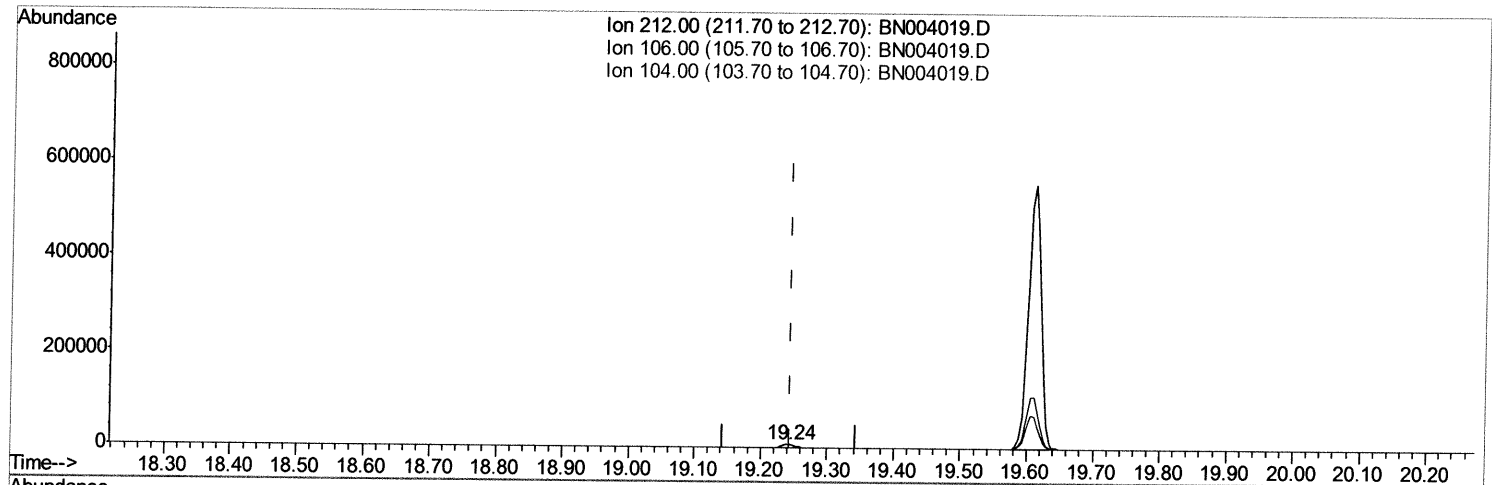

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.20ng/ul m

response 9500

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)


Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

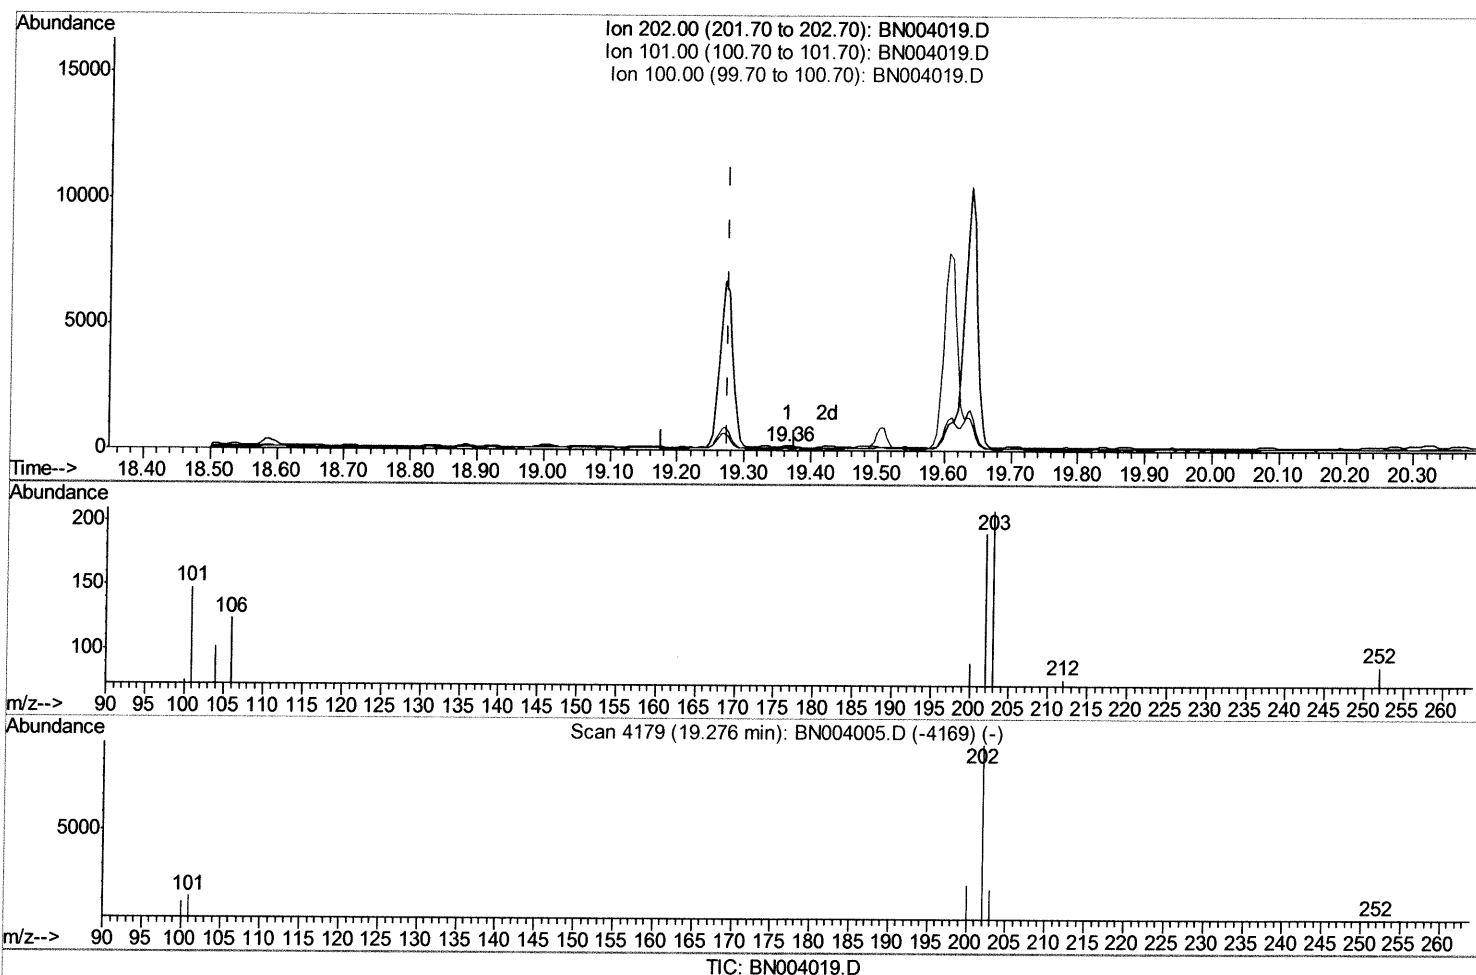

(15) Fluoranthene (C)

19.364min (+0.088) 0.00ng/ul

response 102

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	77.49#
100.00	8.10	39.79#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)


Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

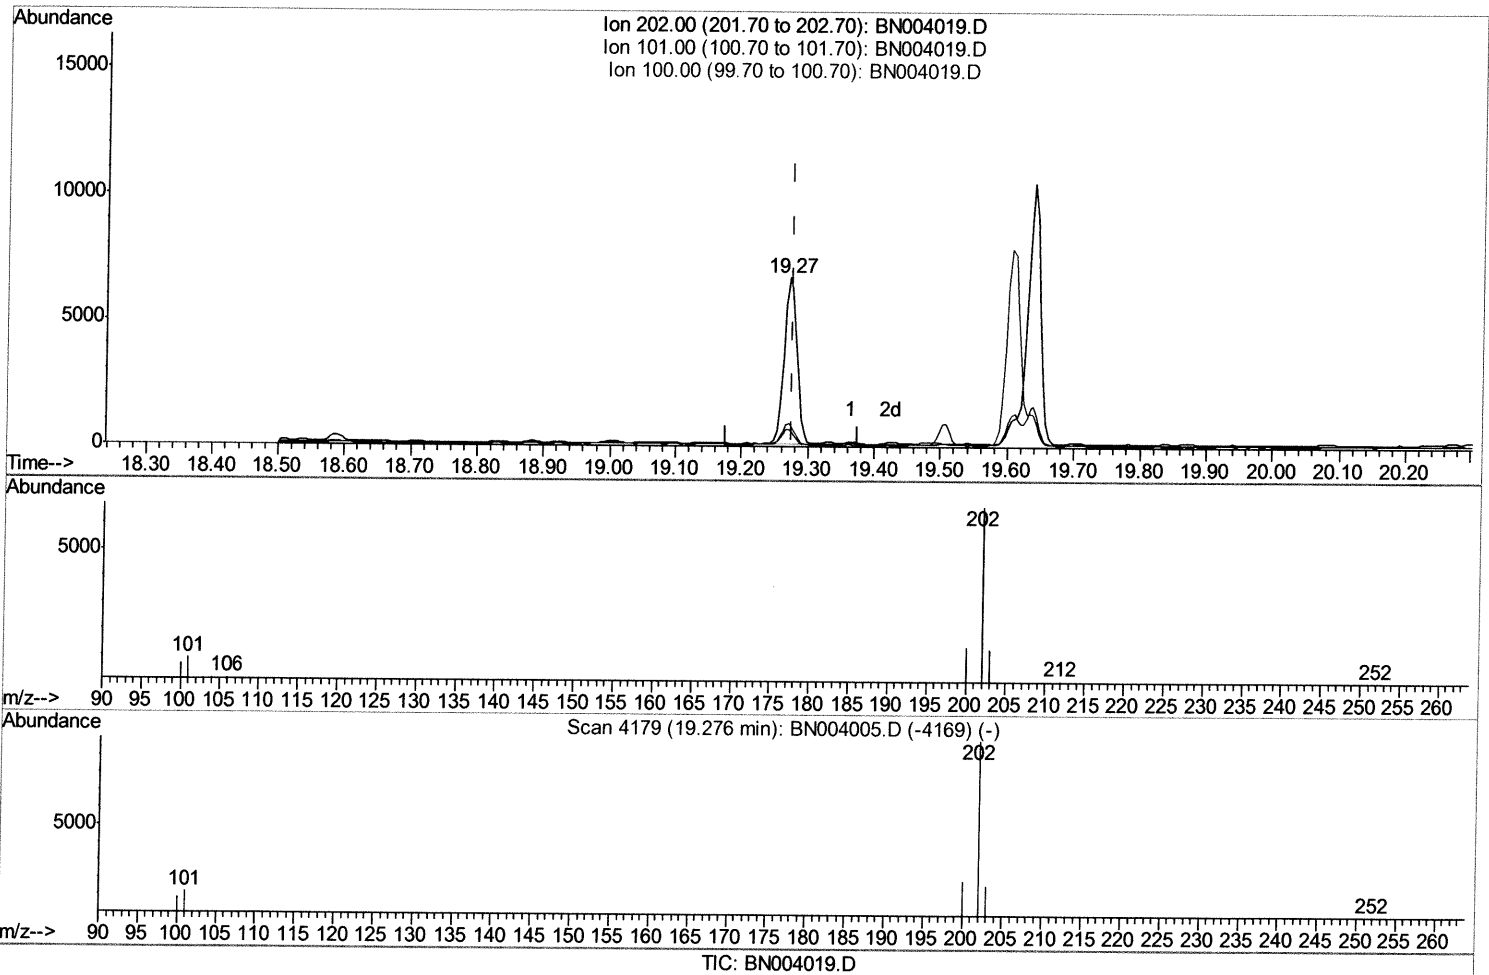

(15) Fluoranthene (C)

19.271min (-0.005) 0.14ng/ul m

> $\frac{57}{12/17/18}$

response 8943

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	13.25
100.00	8.10	9.81
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

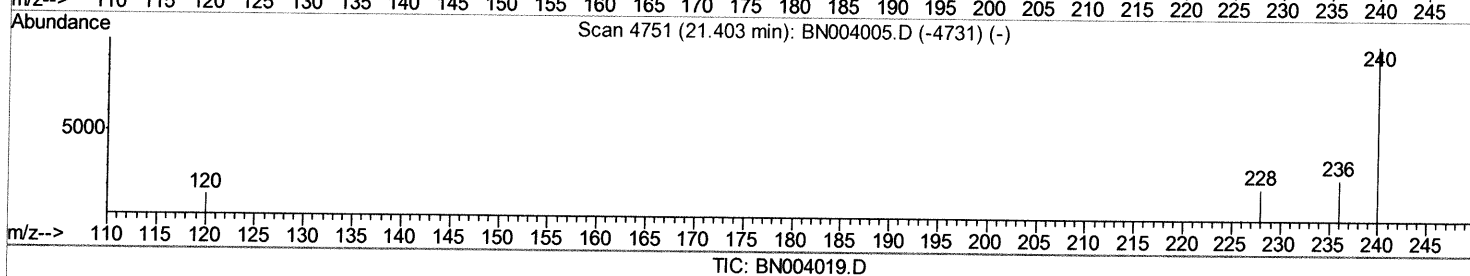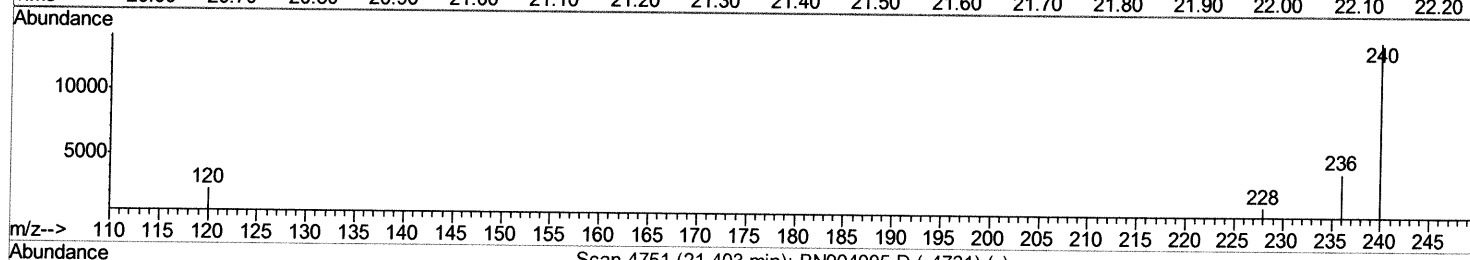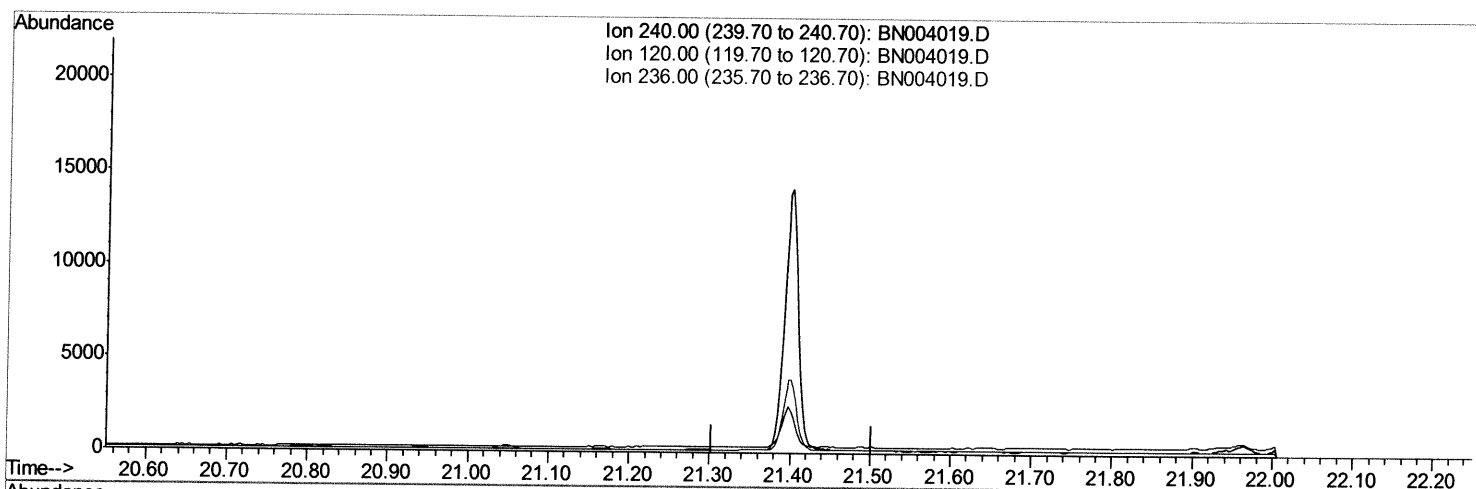

(16) Chrysene-d12 (I)

21.403min (-21.403) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:51:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

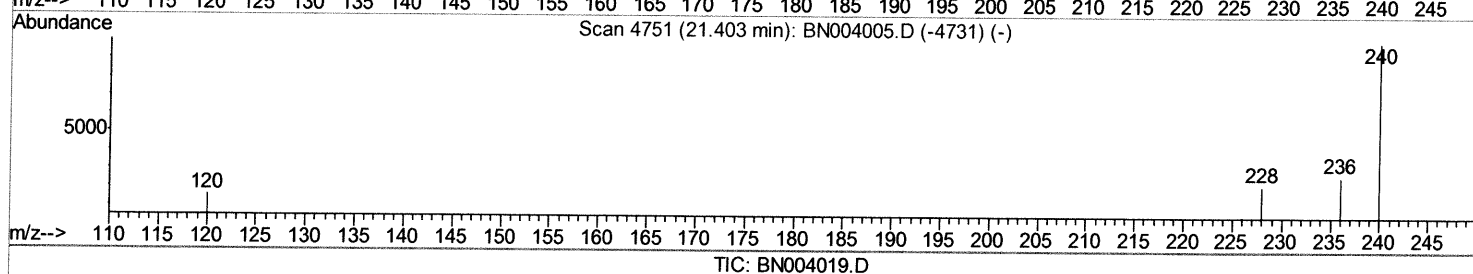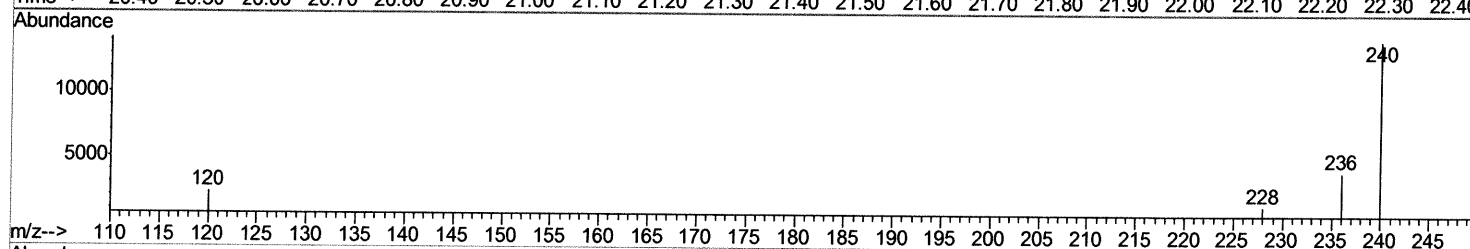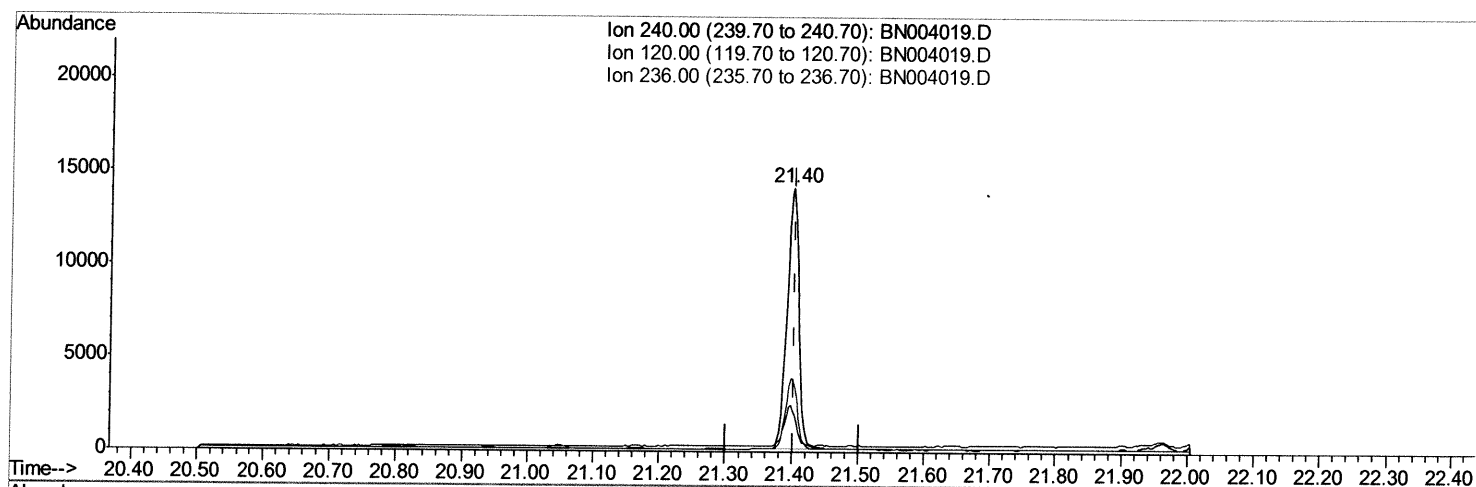

(16) Chrysene-d12 (I)

21.401min (-0.001) 0.40ng/ul m

response 17216

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	15.84
236.00	27.60	27.93
0.00	0.00	0.00

> JJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

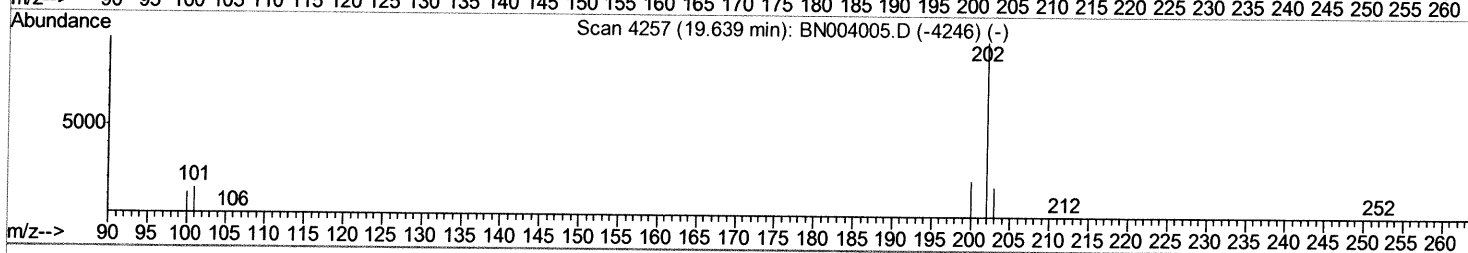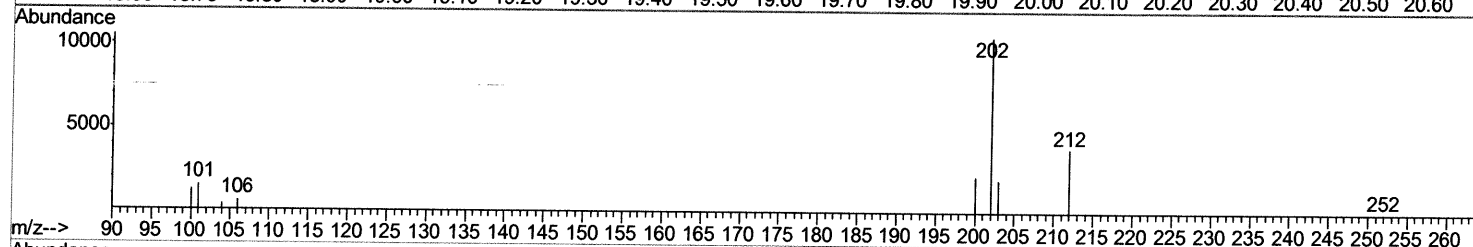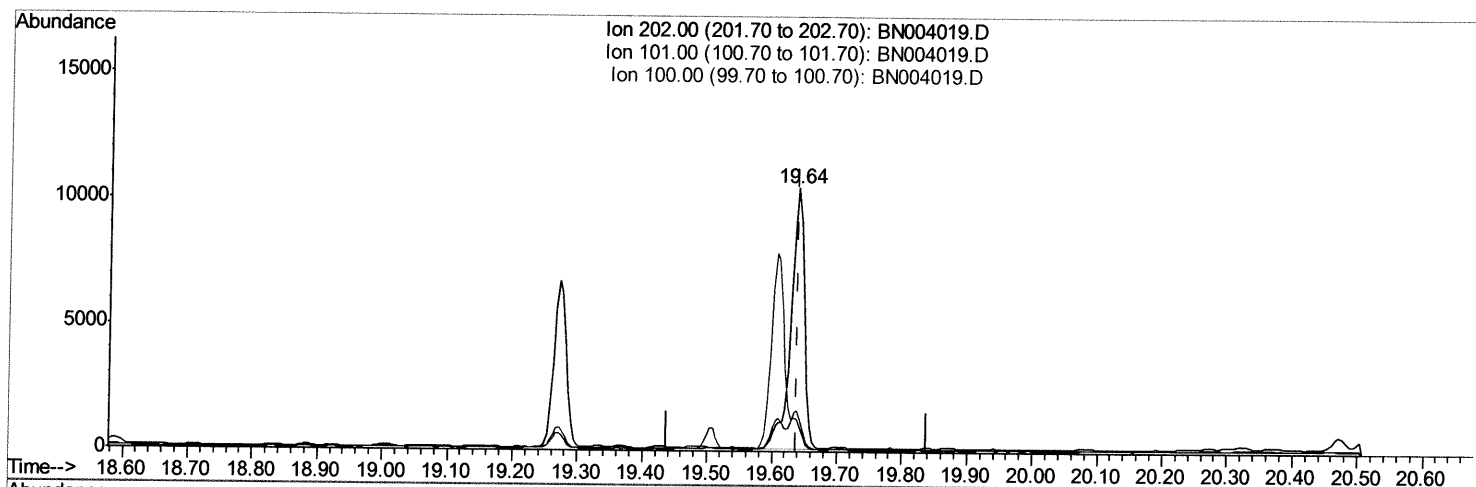

TIC: BN004019.D

(17) Pyrene

19.638min (-0.000) 0.23ng/ul

response 14508

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.25
100.00	10.60	12.17
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

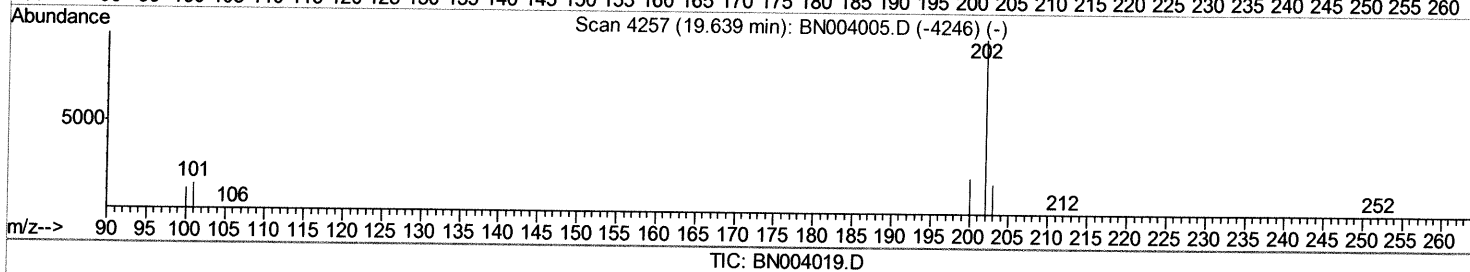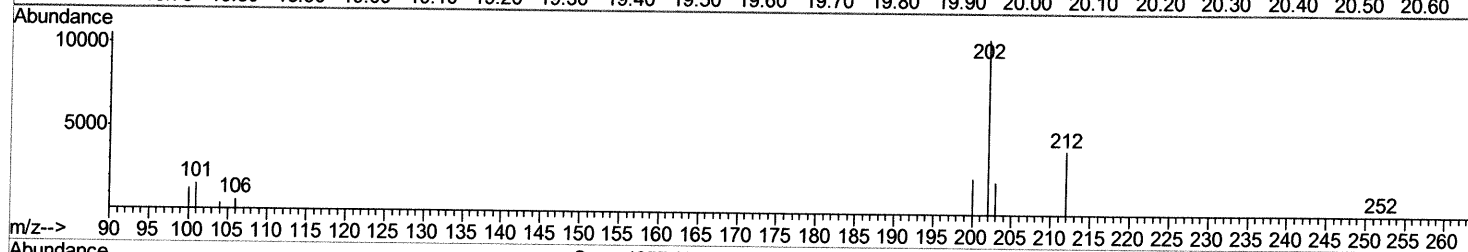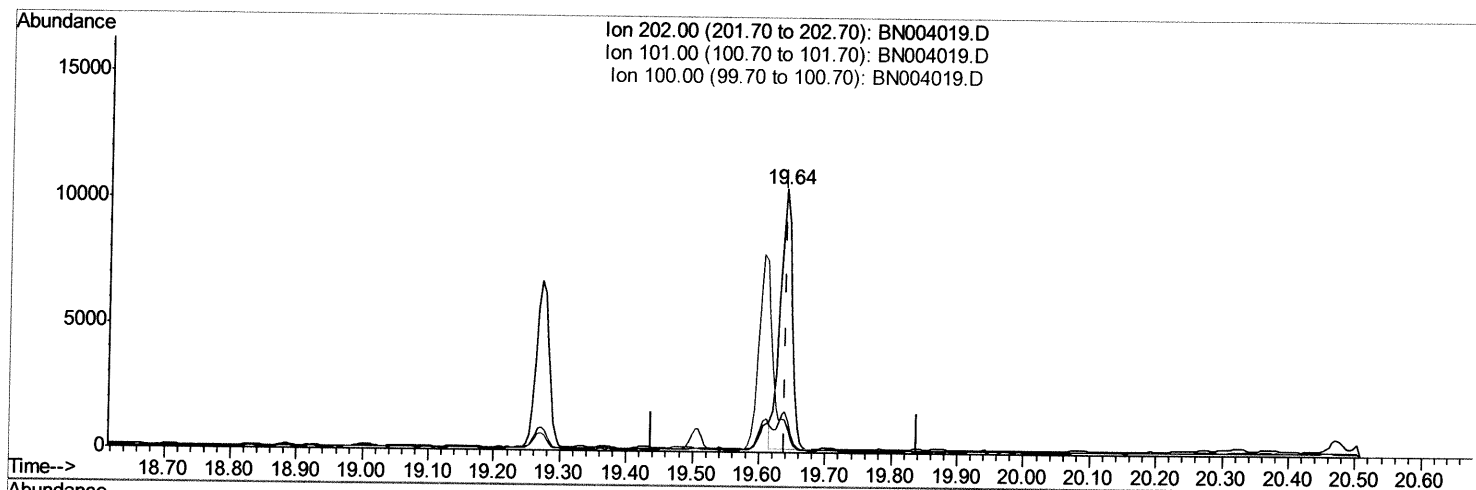

(17) Pyrene

19.638min (-0.000) 0.22ng/ul m

response 13345

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.25
100.00	10.60	12.17
0.00	0.00	0.00

> $\frac{57}{12/17/18}$

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

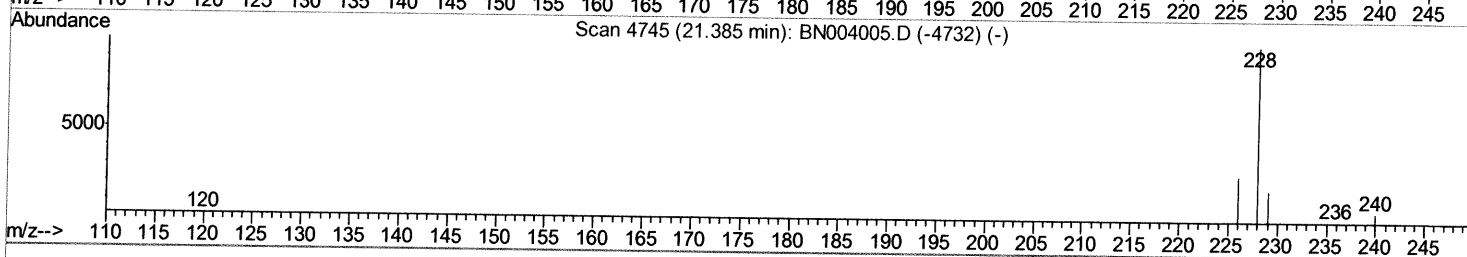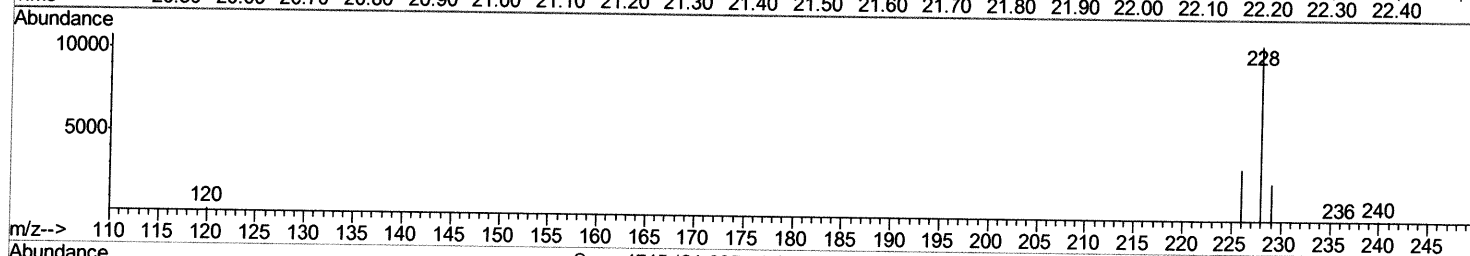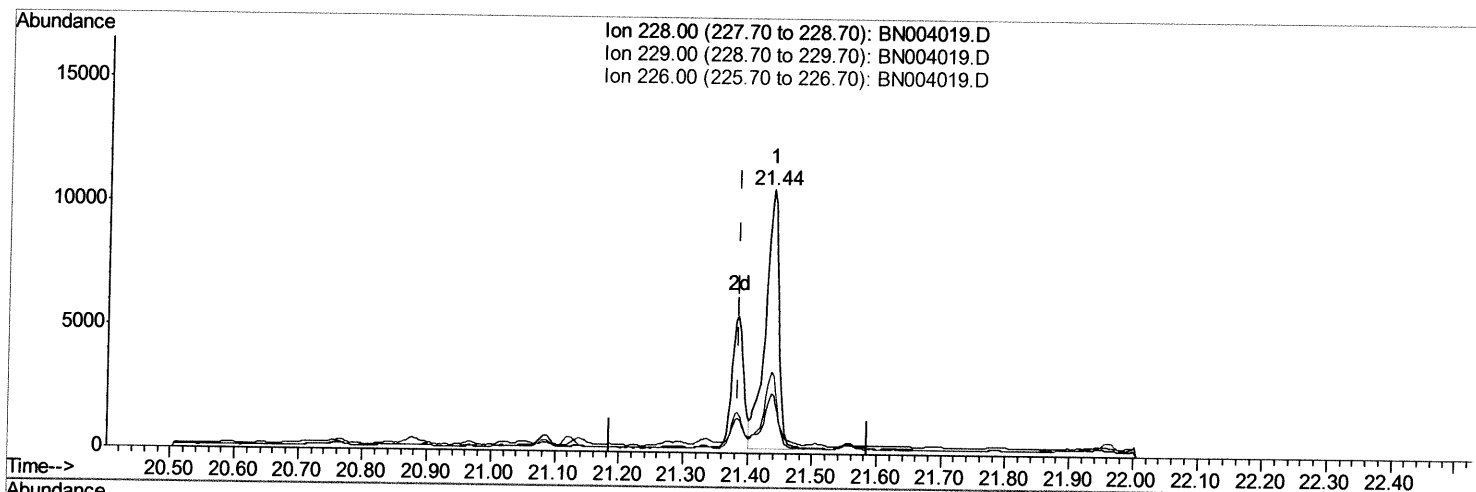

TIC: BN004019.D

(18) Benzo(a)anthracene

21.436min (+0.051) 0.28ng/ul

response 15392

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	22.53
226.00	26.40	31.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

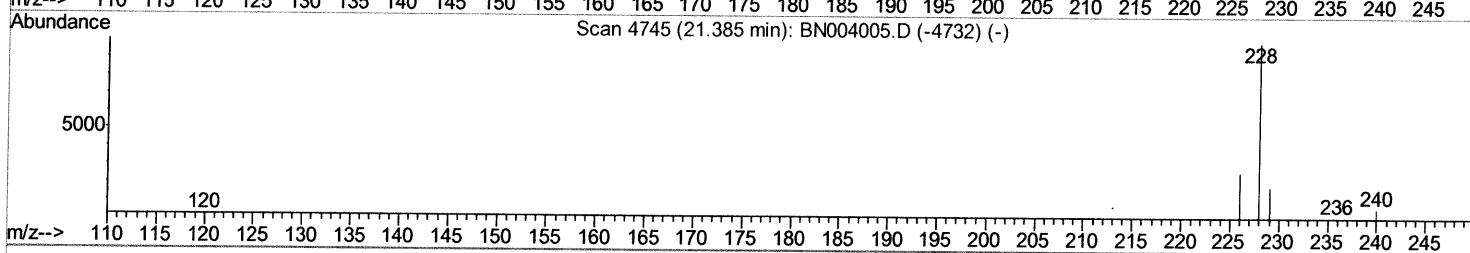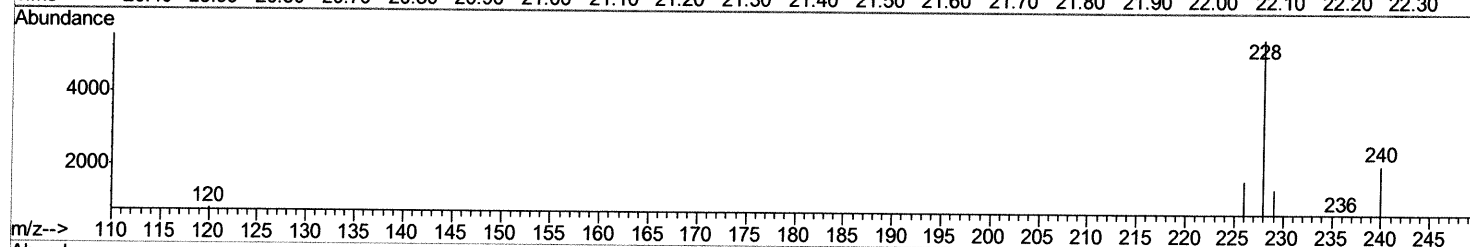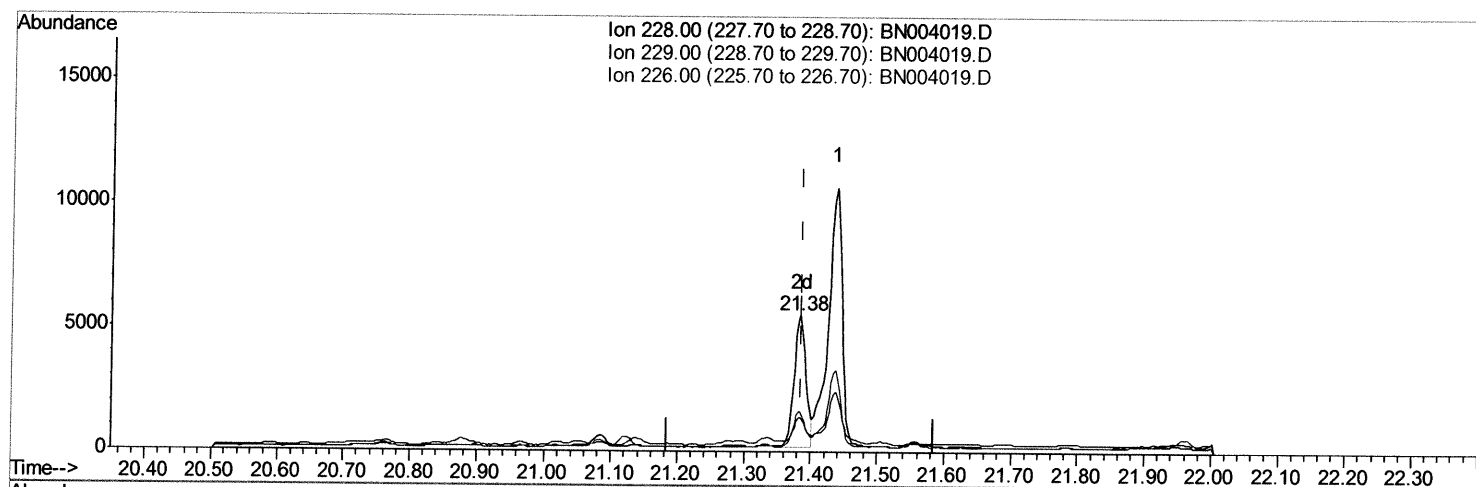

TIC: BN004019.D

(18) Benzo(a)anthracene

21.384min (-0.001) 0.12ng/ul m

response 6669

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	25.56#
226.00	26.40	29.83
0.00	0.00	0.00

> SJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

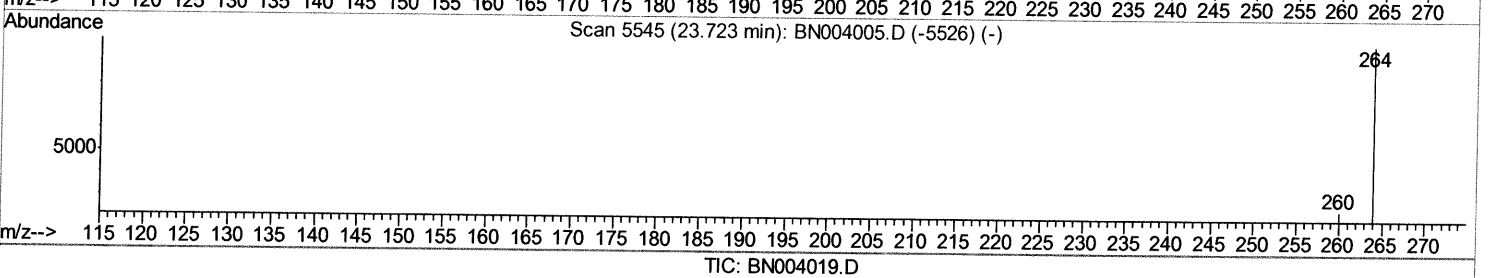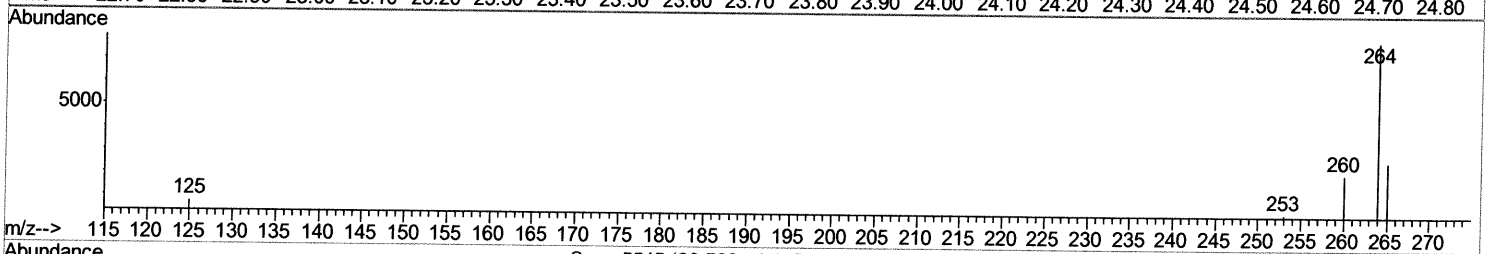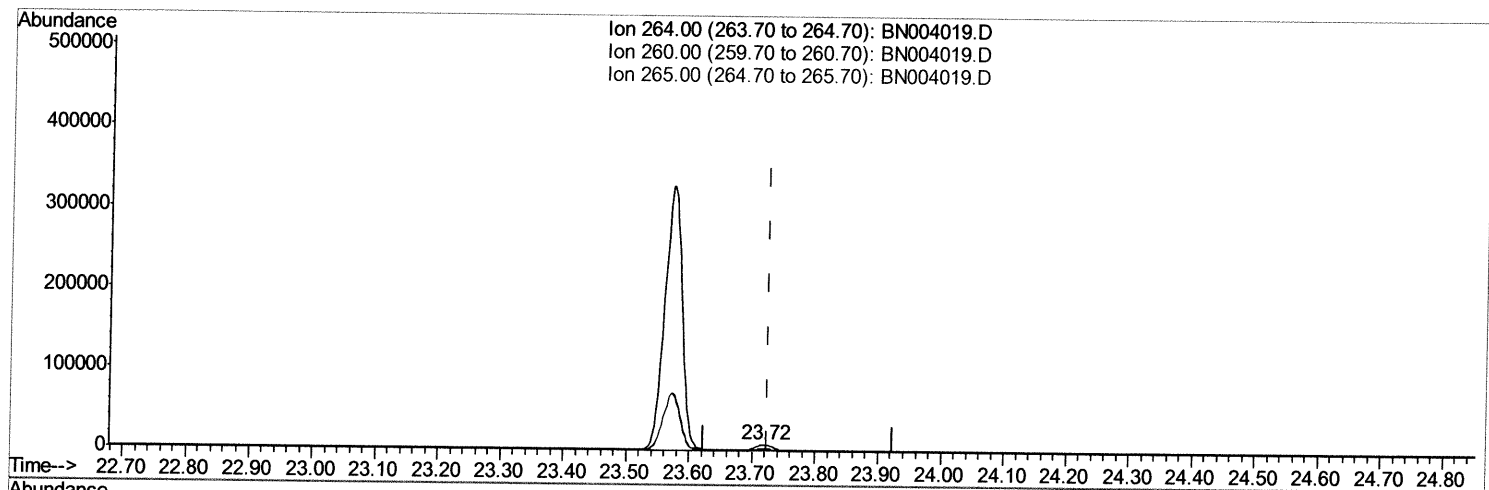

(20) Perylene-d12 (I)
23.719min (-0.004) 0.40ng/ul
response 15729

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.34
265.00	33.50	34.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:52:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

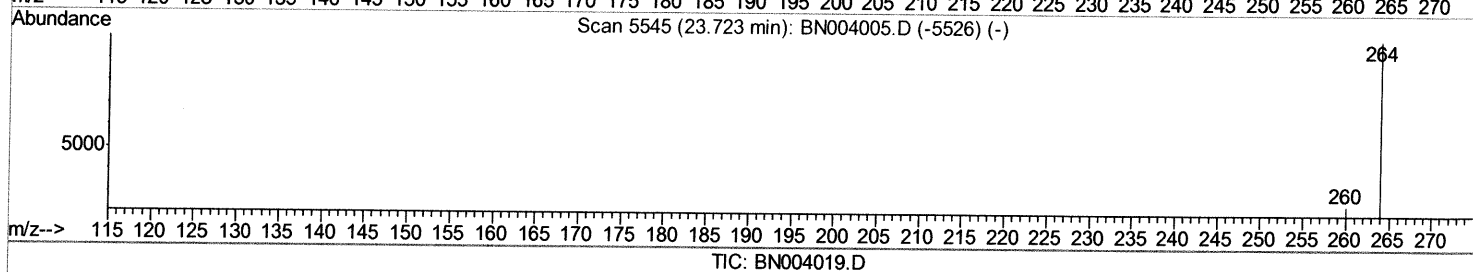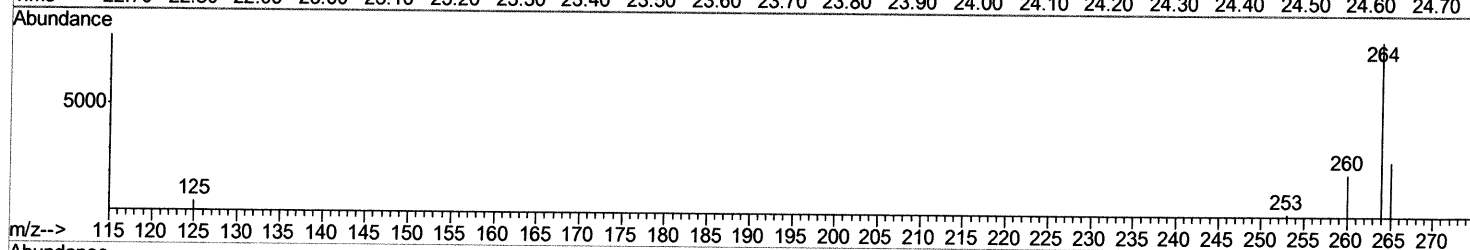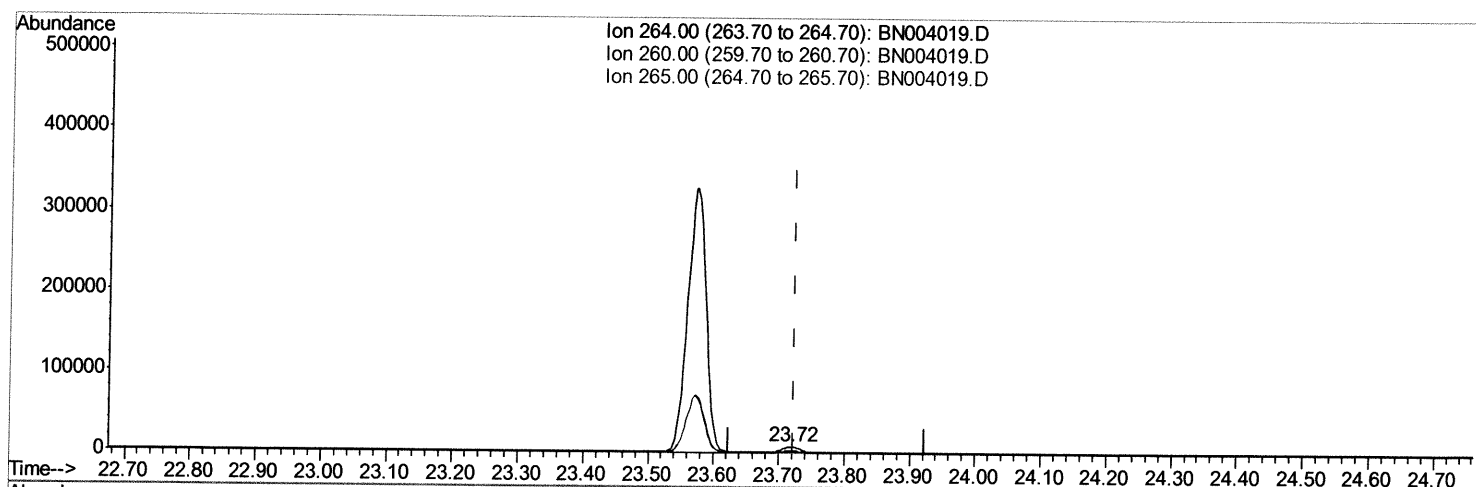

(20) Perylene-d12 (I)

23.719min (-0.004) 0.40ng/ul m

response 14999

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.34
265.00	33.50	34.47
0.00	0.00	0.00

> SJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:53:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

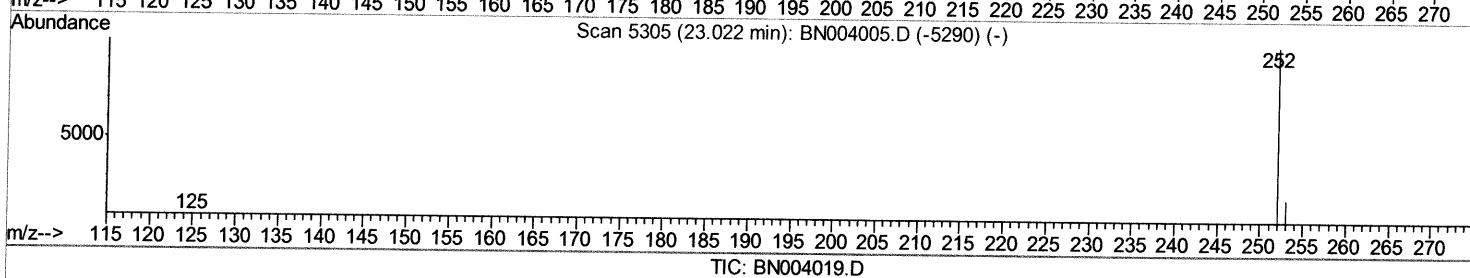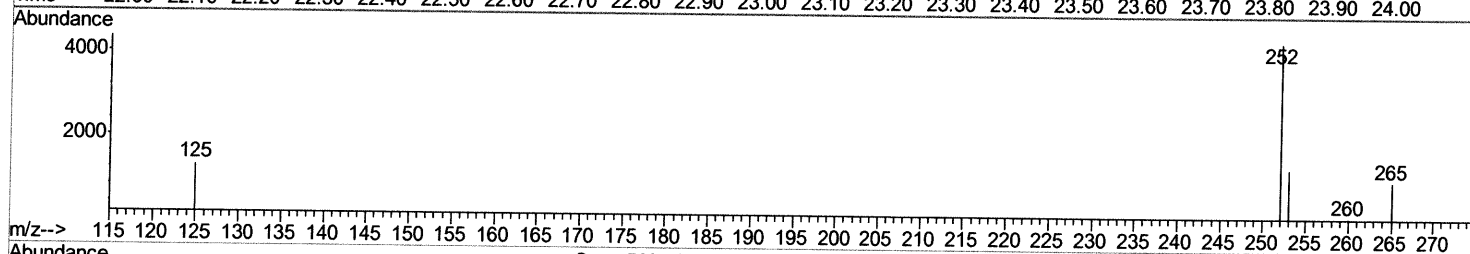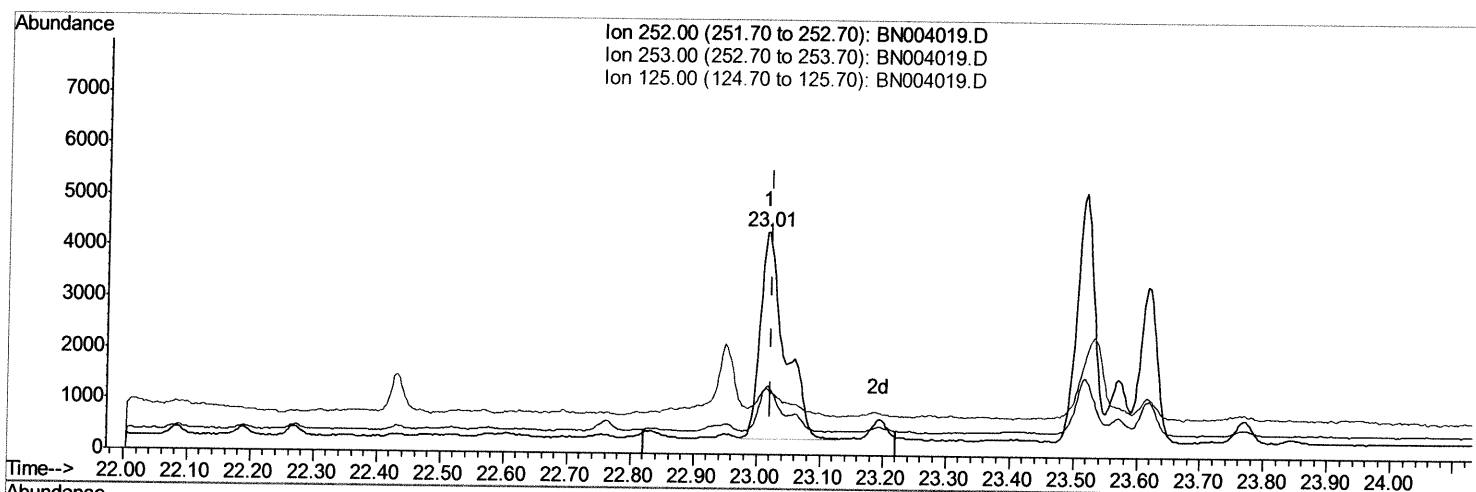

(21) Benzo(b)fluoranthene

23.015min (-0.007) 0.18ng/ul

response 10877

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	30.52
125.00	11.20	29.46#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:53:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

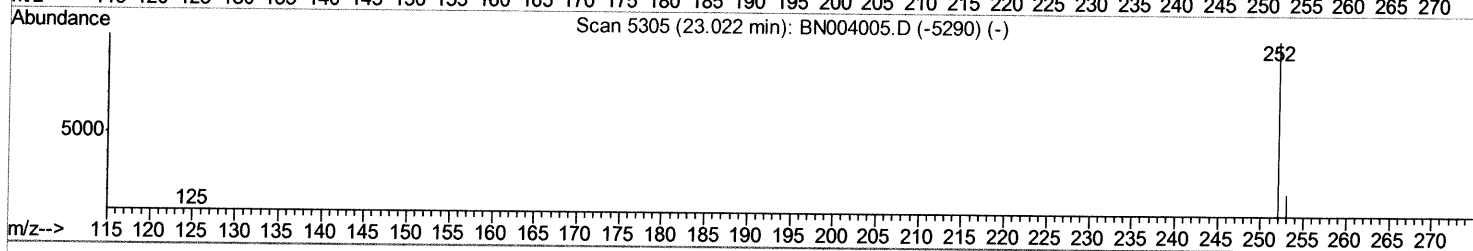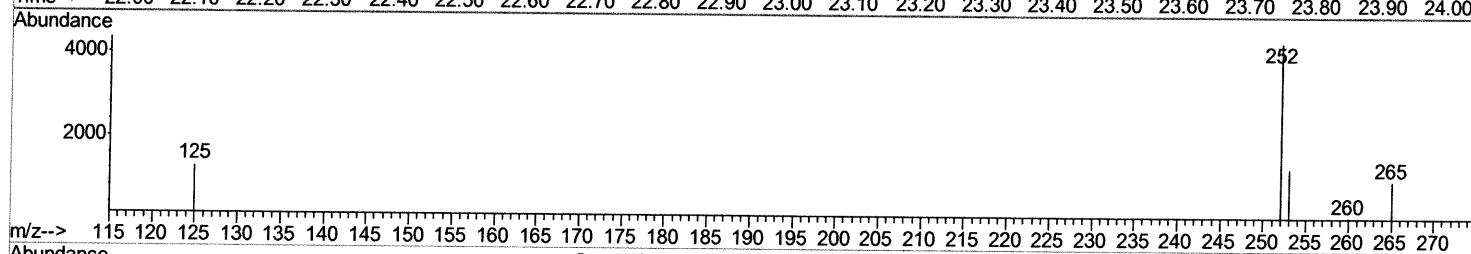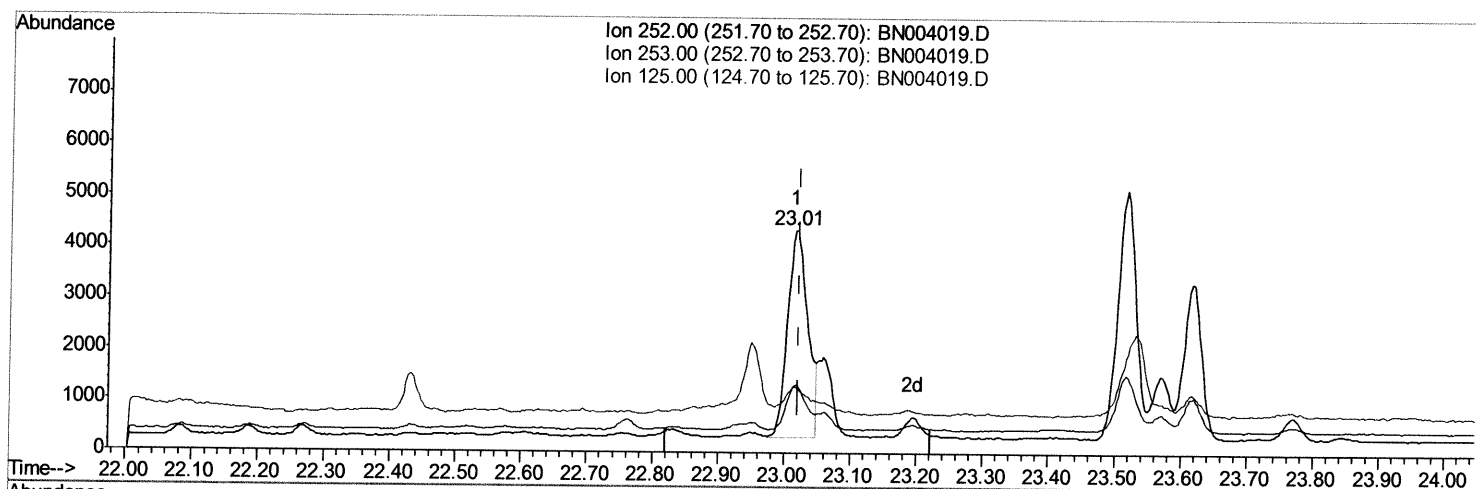

TIC: BN004019.D

(21) Benzo(b)fluoranthene

23.015min (-0.007) 0.14ng/ul m

response 8508

Ion Exp% Act%

252.00 100 100

253.00 23.00 30.52

125.00 11.20 29.46#

0.00 0.00 0.00

> JJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:53:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

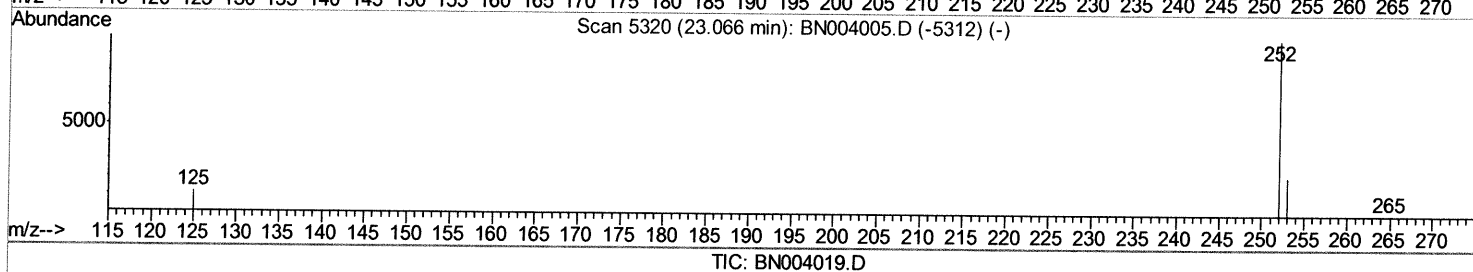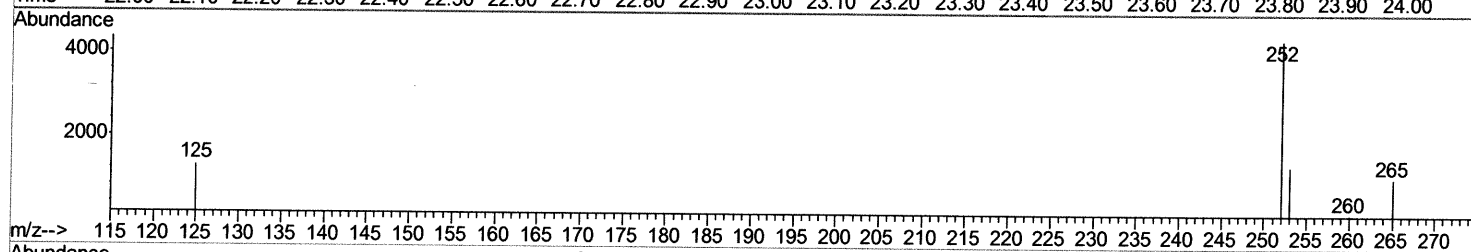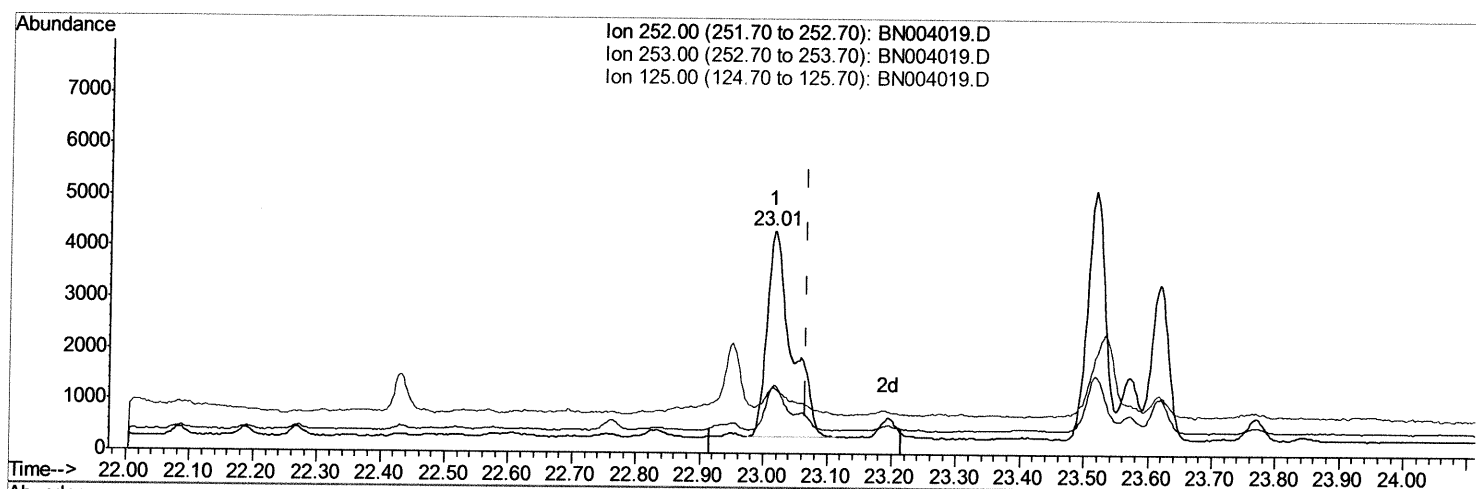

(22) Benzo(k)fluoranthene

23.015min (-0.051) 0.18ng/ul

response 10854

Ion	Exp%	Act%
-----	------	------

252.00	100	100
--------	-----	-----

253.00	23.10	30.52#
--------	-------	--------

125.00	11.30	29.46#
--------	-------	--------

0.00	0.00	0.00
------	------	------

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (Qedit)




Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:53:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

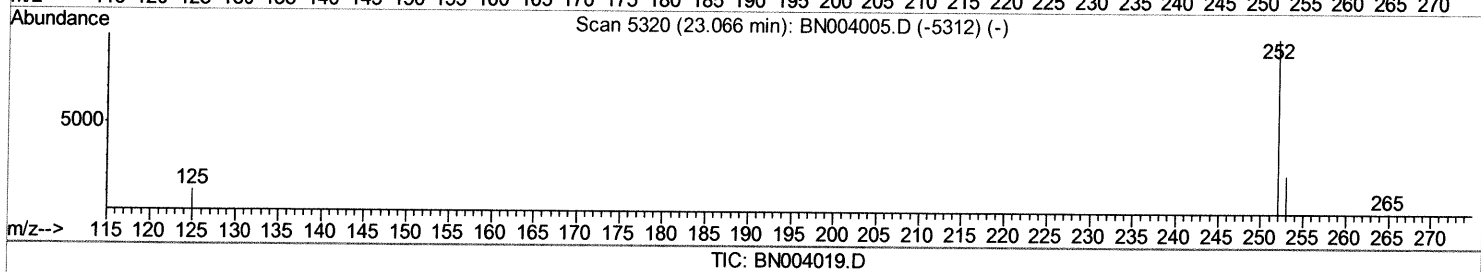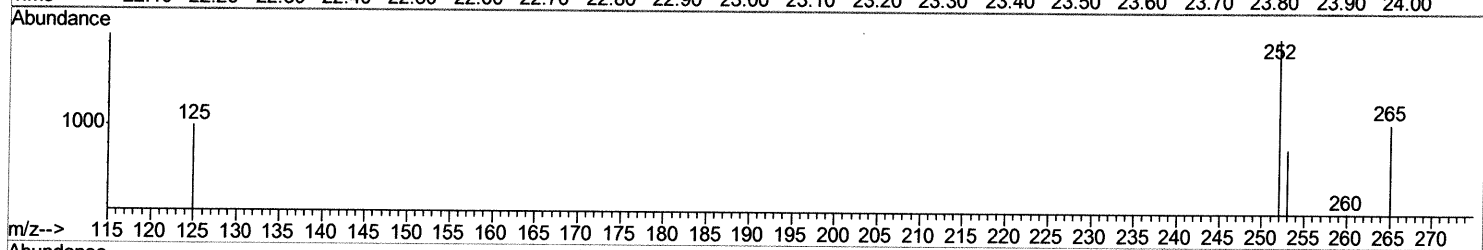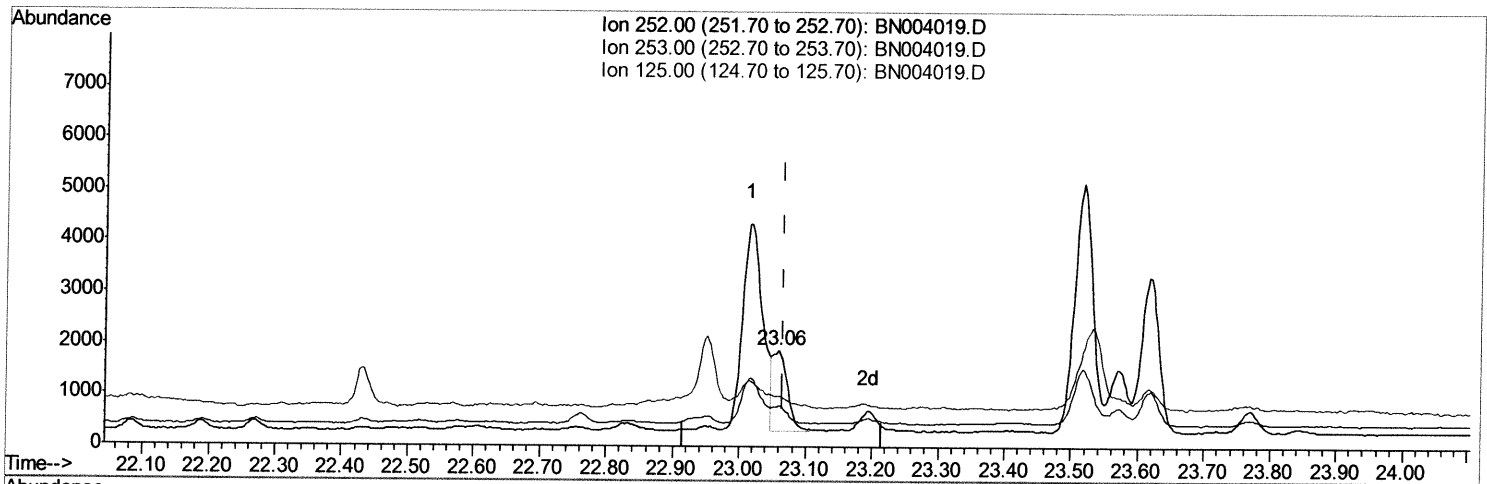

(22) Benzo(k)fluoranthene

23.058min (-0.007) 0.04ng/ul m

response 2428

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	42.36#
125.00	11.30	52.49#
0.00	0.00	0.00

> SJ
12/17/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121618\
Quantitation Report (QT Reviewed)

Data File : BN004019.D
Acq On : 17 Dec 2018 05:24
Operator : JU/SJ
Sample : J6236-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E98

Manual Integrations
APPROVED

Sohil
12/17/2018 4:28:28 PM

Quant Time: Dec 17 07:54:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 17 06:22:23 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	2130	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	10691	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	6463	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	16299m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	17216m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	14999m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	3093	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	9500m	0.20	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) 2-Methylnaphthalene	12.29	142	722	0.034	ng/ul	99
12) Phenanthrene	17.26	178	11579	0.216	ng/ul	99
15) Fluoranthene	19.27	202	8943m	0.142	ng/ul	
17) Pyrene	19.64	202	13345m	0.216	ng/ul	
18) Benzo(a)anthracene	21.38	228	6669m	0.123	ng/ul	
19) Chrysene	21.44	228	15145	0.243	ng/ul	96
21) Benzo(b)fluoranthene	23.01	252	8508m	0.137	ng/ul	
22) Benzo(k)fluoranthene	23.06	252	2428m	0.040	ng/ul	
23) Benzo(a)pyrene	23.62	252	5659	0.105	ng/ul#	69
24) Indeno(1,2,3-cd)pyrene	26.08	276	3962	0.064	ng/ul#	99
25) Dibenzo(a,h)anthracene	26.08	278	1878	0.038	ng/ul#	20
26) Benzo(g,h,i)perylene	26.81	276	5220	0.097	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JJ
12/17/18