

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023238.D
 Acq On : 16 Dec 2022 13:56
 Operator : CG/JU
 Sample : N5983-18
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLF4

Quant Time: Dec 16 21:43:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	301093	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1396456	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	947745	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	2174776	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	2180968	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	2246381	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	30073	4.132	ng/uL	0.00
4) Pyridine-d5	3.787	84	61590	2.867	ng/ul	0.01
7) Phenol-d5	7.158	99	152818	5.457	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	475355	29.170	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132	467531	22.157	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	313262	13.933	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	326110	30.225	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	329688	29.012	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	564060	26.293	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	650714	18.851	ng/ul	0.00
46) Dimethylphthalate-d6	14.063	166	2240815	31.550	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	2454304	30.814	ng/ul	0.00
54) 4-Nitrophenol-d4	14.840	143	72563	4.574	ng/ul	0.00
60) Fluorene-d10	15.645	176	1973743	32.624	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	345990	27.026	ng/ul	0.00
73) Anthracene-d10	17.498	188	3346362	34.334	ng/ul	0.00
81) Pyrene-d10	19.792	212	4051617	34.151	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.886	264	3822831	34.719	ng/ul	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.492	149	337221	3.976	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023238.D
Acq On : 16 Dec 2022 13:56
Operator : CG/JU
Sample : N5983-18
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLF4

Quant Time: Dec 16 21:43:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

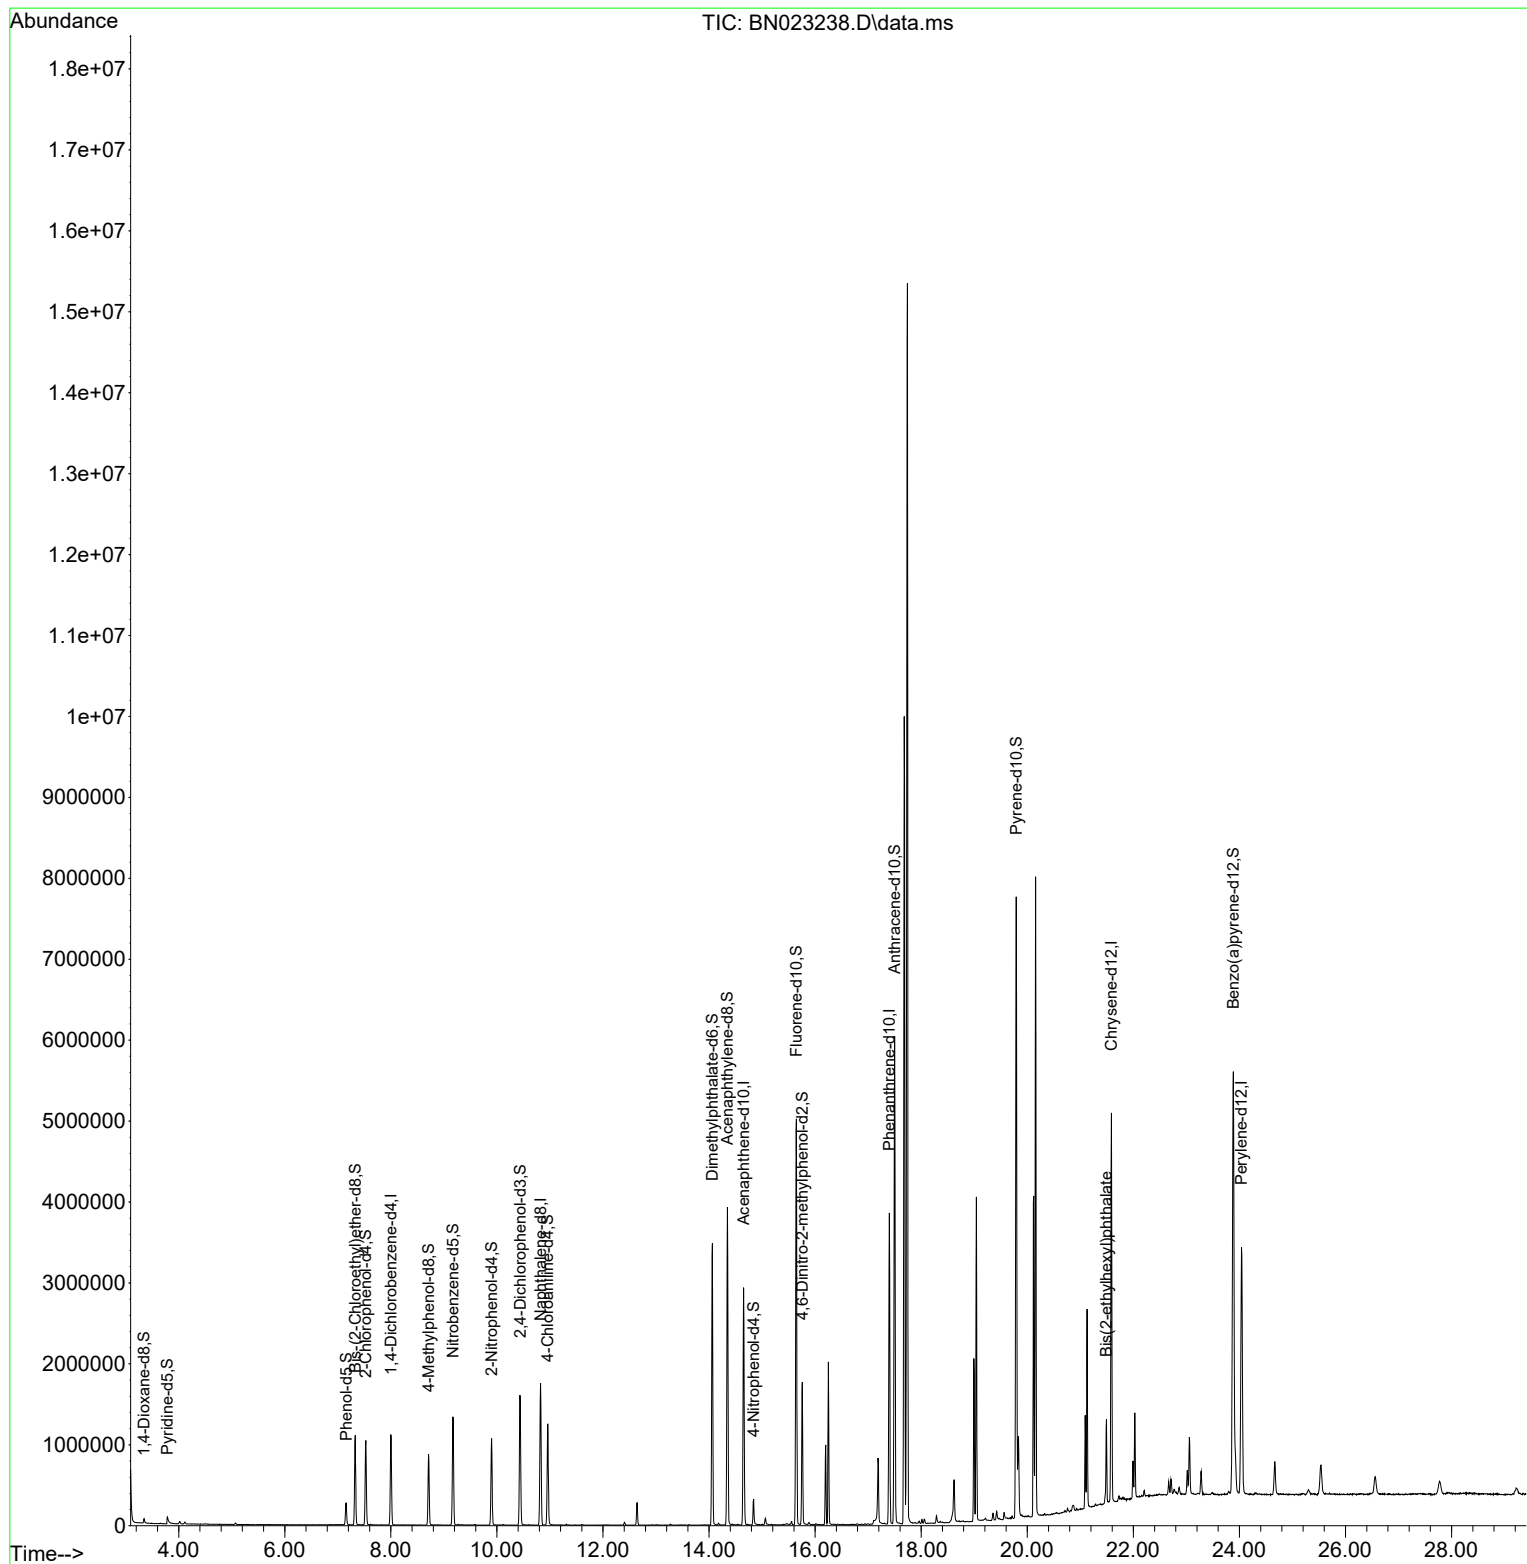

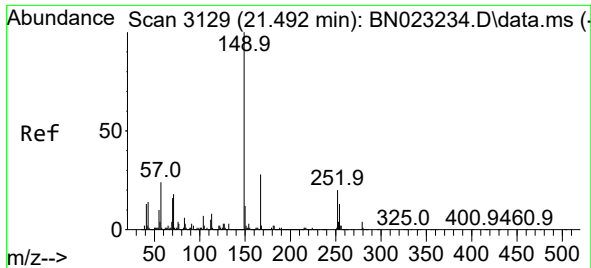

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.976 ng/ul
 RT: 21.492 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BN023238.D
 Acq: 16 Dec 2022 13:56

Instrument :
 BNA_N
 ClientSampleId :
 COLF4

Tgt Ion:149 Resp: 337221
 Ion Ratio Lower Upper
 149 100
 167 28.4 21.9 32.9
 279 3.6 3.4 5.0

