

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023239.D
 Acq On : 16 Dec 2022 14:33
 Operator : CG/JU
 Sample : N6018-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBYJ8

Quant Time: Dec 16 21:43:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	266876	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1231788	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	836423	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1924907	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1916673	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	2019078	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	31679	4.911	ng/uL	0.00
4) Pyridine-d5	3.781	84	143067	7.514	ng/ul	0.00
7) Phenol-d5	7.158	99	169808	6.841	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	465916	32.256	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132	452039	24.169	ng/ul	0.00
15) 4-Methylphenol-d8	8.711	113	308729	15.492	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	319576	33.579	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	302807	30.209	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	512494	27.083	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	832236	27.333	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	2076011	33.120	ng/ul	0.00
49) Acenaphthylene-d8	14.346	160	2391909	34.027	ng/ul	0.00
54) 4-Nitrophenol-d4	14.834	143	55197	3.943	ng/ul	-0.01
60) Fluorene-d10	15.645	176	1865057	34.930	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	229505	20.254	ng/ul	0.00
73) Anthracene-d10	17.498	188	3021419	35.024	ng/ul	0.00
81) Pyrene-d10	19.792	212	3720731	35.686	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	3480412	35.168	ng/ul	0.00
Target Compounds						
					Qvalue	
48) 2,6-Dinitrotoluene	14.063	165	12891	1.053	ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023239.D
Acq On : 16 Dec 2022 14:33
Operator : CG/JU
Sample : N6018-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBYJ8


Quant Time: Dec 16 21:43:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

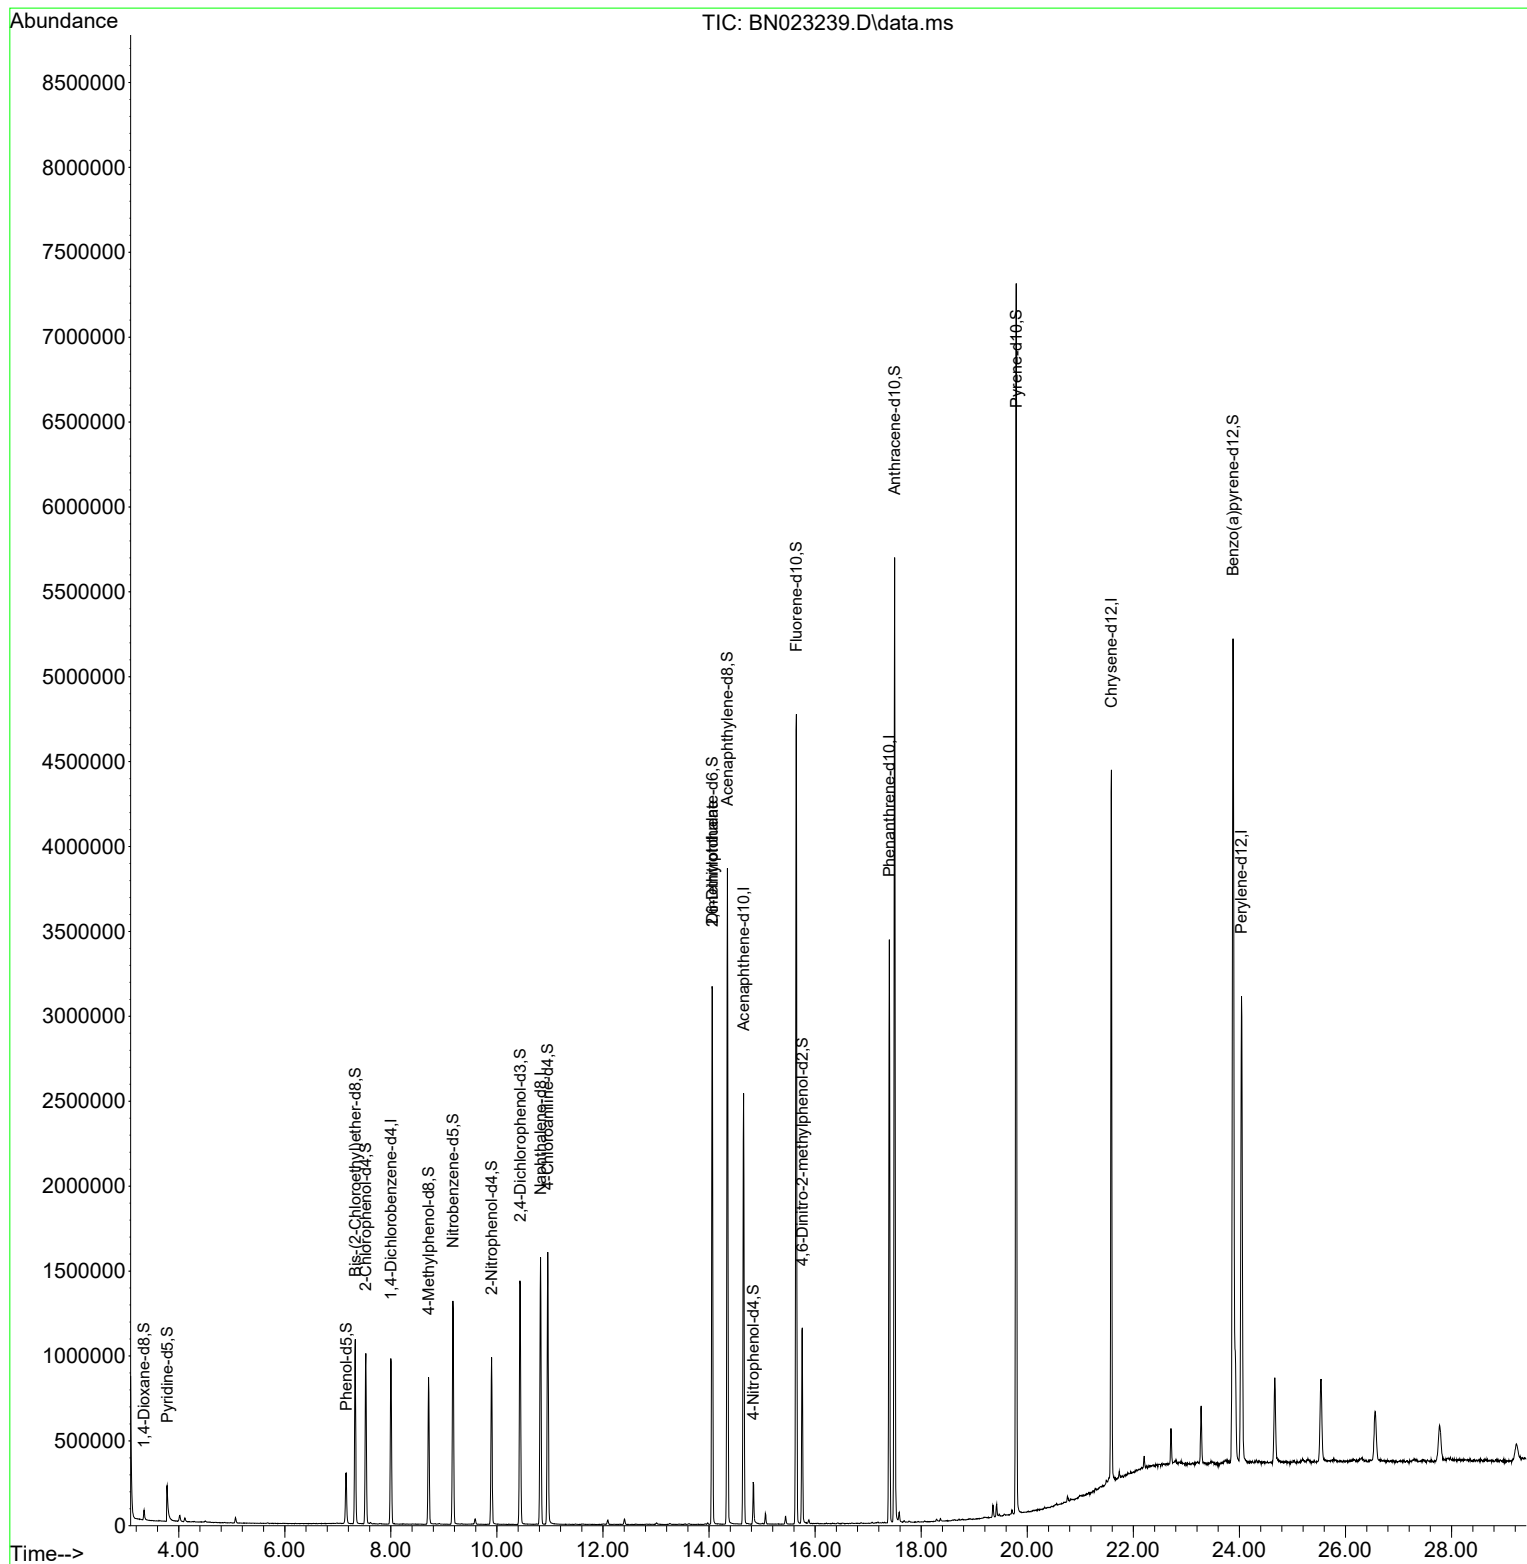

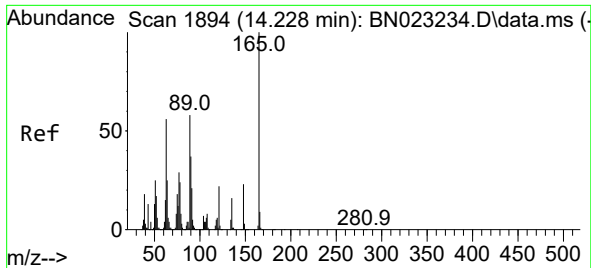

#48
 2,6-Dinitrotoluene
 Concen: 1.053 ng/ul
 RT: 14.063 min Scan# 11
 Delta R.T. -0.165 min
 Lab File: BN023239.D
 Acq: 16 Dec 2022 14:33

Instrument :
 BNA_N
 ClientSampleId :
 DBYJ8

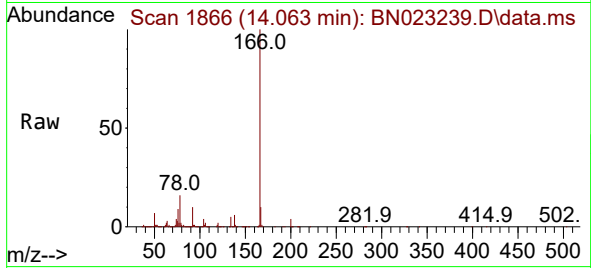

Tgt Ion:165 Resp: 12891
 Ion Ratio Lower Upper
 165 100
 89 2.6 47.7 71.5#
 121 42.1 17.8 26.8#

