

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023247.D
 Acq On : 16 Dec 2022 19:32
 Operator : CG/JU
 Sample : N5983-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0LC4

Quant Time: Dec 16 21:45:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	253412	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1187211	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	811444	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1888112	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1887742	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	1858692	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	25150	4.106	ng/uL	0.00
4) Pyridine-d5	3.775	84	362312	20.039	ng/ul	0.00
7) Phenol-d5	7.152	99	513384	21.782	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	323623	23.595	ng/ul	0.00
11) 2-Chlorophenol-d4	7.528	132	416239	23.437	ng/ul	0.00
15) 4-Methylphenol-d8	8.711	113	435683	23.024	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	220091	23.994	ng/ul	0.00
24) 2-Nitrophenol-d4	9.899	143	236702	24.500	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	428829	23.513	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	624578	21.283	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1534122	25.228	ng/ul	0.00
49) Acenaphthylene-d8	14.346	160	1732870	25.411	ng/ul	0.00
54) 4-Nitrophenol-d4	14.840	143	283396	20.867	ng/ul	0.00
60) Fluorene-d10	15.640	176	1357615	26.209	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	216577	19.486	ng/ul	0.00
73) Anthracene-d10	17.498	188	2168153	25.623	ng/ul	0.00
81) Pyrene-d10	19.792	212	2670923	26.010	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	2443540	26.821	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.269	232	19553	1.293	ng/ul	96
71) Pentachlorophenol	17.045	266	263801	18.756	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023247.D
Acq On : 16 Dec 2022 19:32
Operator : CG/JU
Sample : N5983-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC4

Quant Time: Dec 16 21:45:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

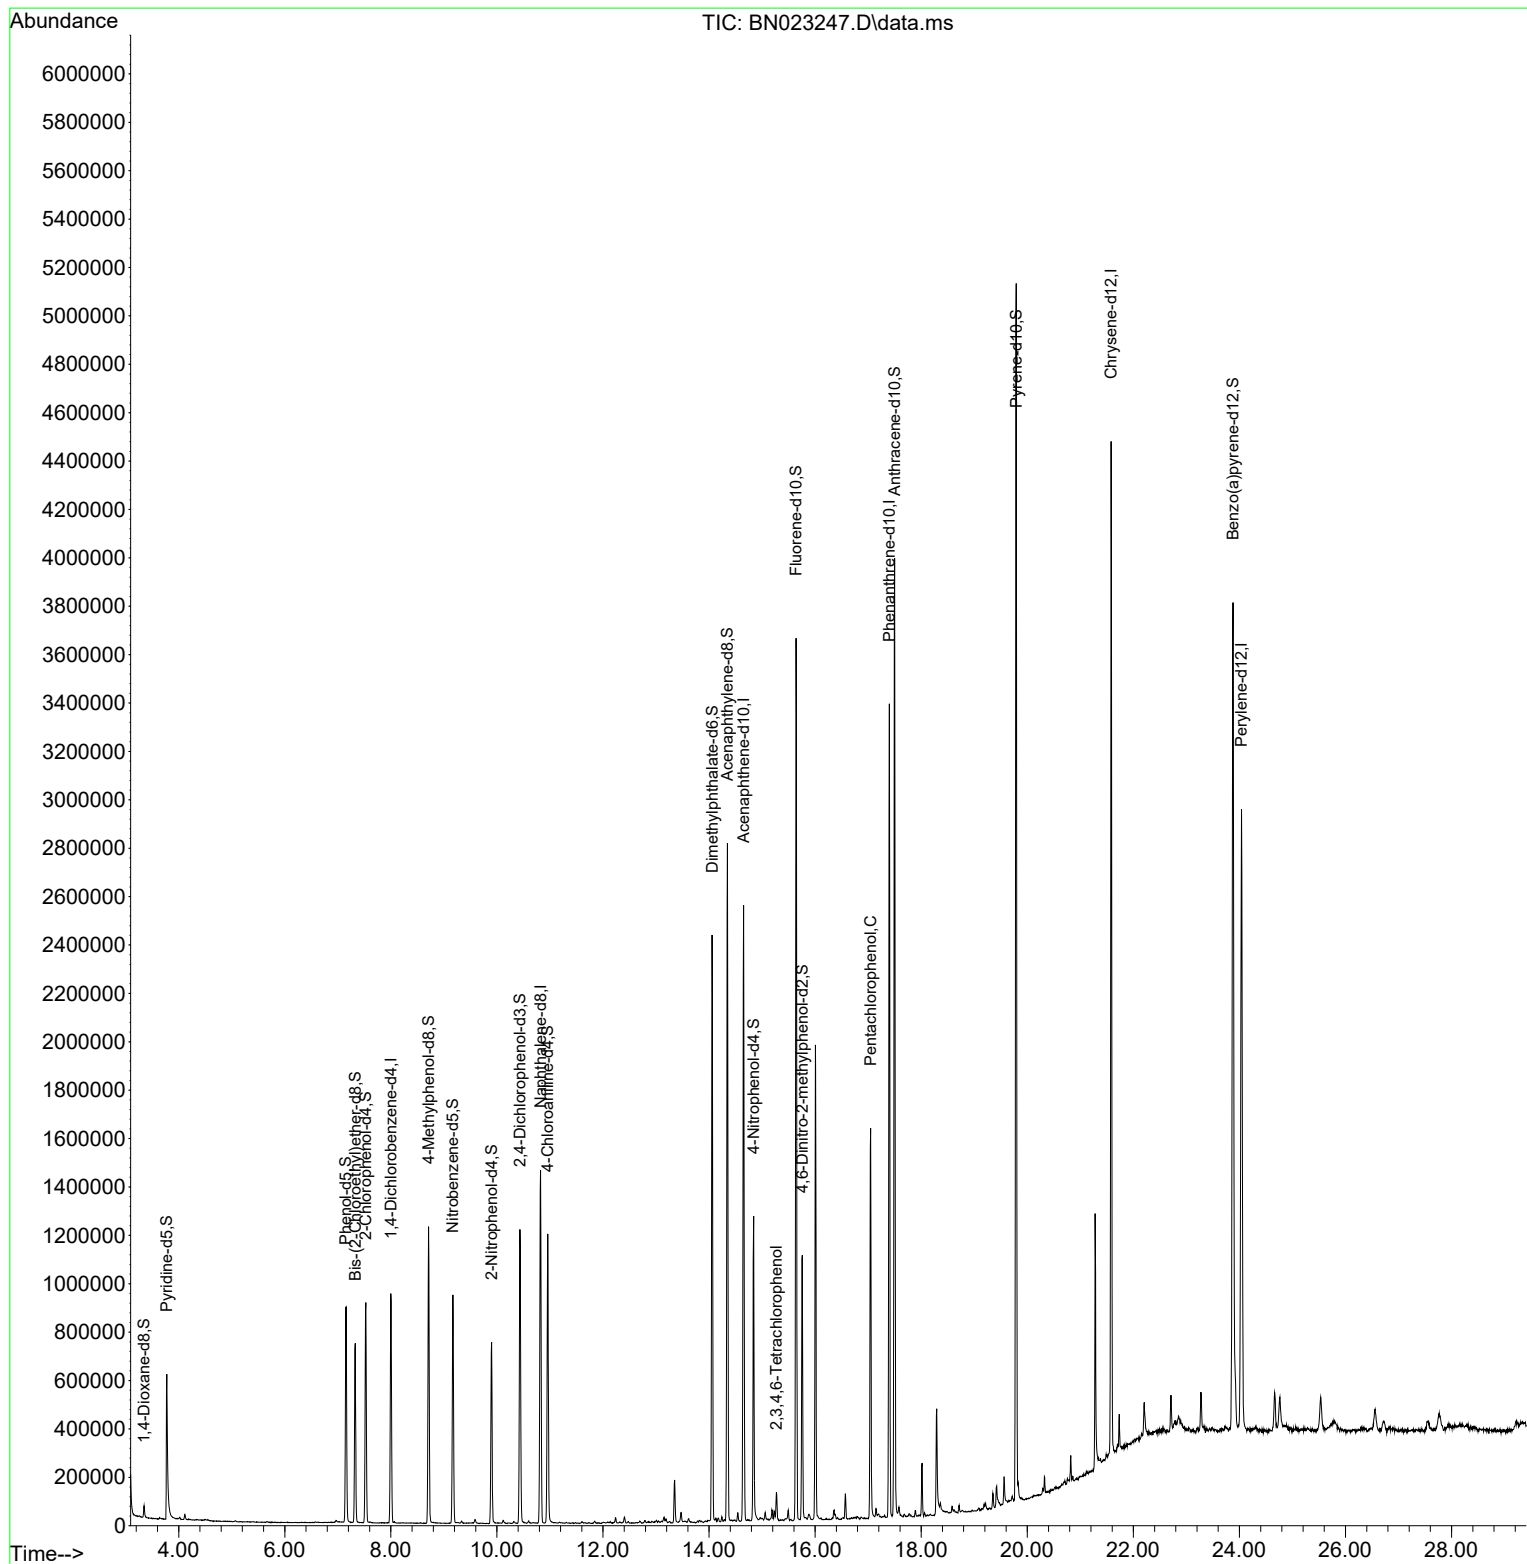




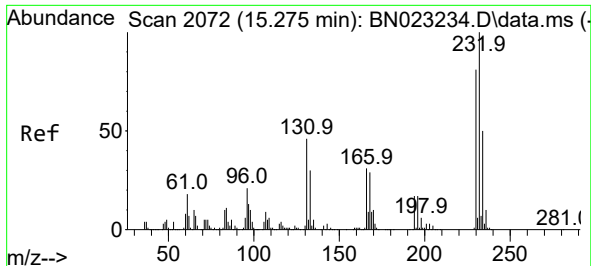


#58
2,3,4,6-Tetrachlorophenol
Concen: 1.293 ng/ul
RT: 15.269 min Scan# 2072
Delta R.T. -0.006 min
Lab File: BN023247.D
Acq: 16 Dec 2022 19:32

Instrument :
BNA_N
ClientSampleId :
COLC4

Tgt Ion:232 Resp: 19553

Ion	Ratio	Lower	Upper
232	100		
131	49.2	37.9	56.9
130	2.8	1.9	2.9
166	33.9	23.8	35.8

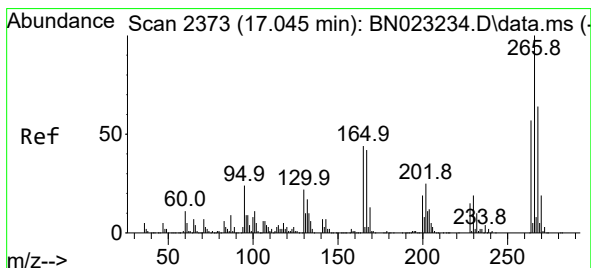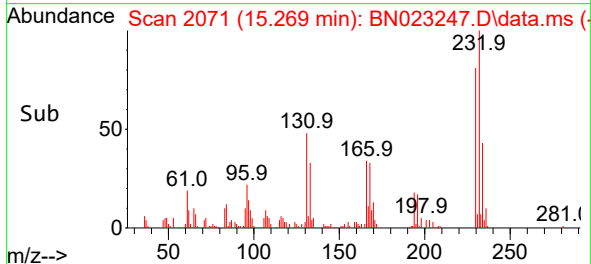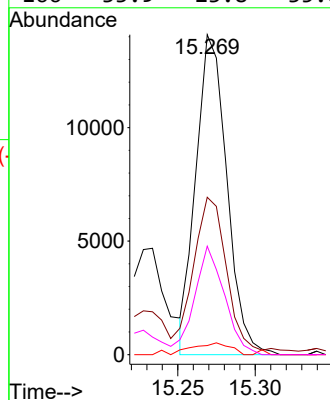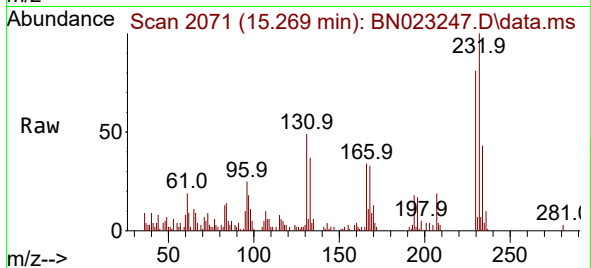

#71
Pentachlorophenol
Concen: 18.756 ng/ul
RT: 17.045 min Scan# 2373
Delta R.T. 0.000 min
Lab File: BN023247.D
Acq: 16 Dec 2022 19:32

Tgt Ion:266 Resp: 263801

Ion	Ratio	Lower	Upper
266	100		
264	62.7	50.5	75.7
268	64.5	52.6	78.8

