

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023263.D
 Acq On : 17 Dec 2022 06:02
 Operator : CG/JU
 Sample : N5925-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBYC8

Quant Time: Dec 19 00:12:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	266227	20.000	ng/ul	0.00
20) Naphthalene-d8	10.816	136	1233721	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	826664	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	1906836	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1846708	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	1773446	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	25810	4.011	ng/uL	0.00
4) Pyridine-d5	3.787	84	50695	2.669	ng/ul	0.01
7) Phenol-d5	7.152	99	595785	24.062	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	358635	24.890	ng/ul	0.00
11) 2-Chlorophenol-d4	7.522	132	476507	25.539	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	366095	18.415	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	249351	26.159	ng/ul	0.00
24) 2-Nitrophenol-d4	9.893	143	272037	27.096	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	495934	26.167	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	332180	10.893	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1716118	27.702	ng/ul	0.00
49) Acenaphthylene-d8	14.345	160	1945279	28.000	ng/ul	0.00
54) 4-Nitrophenol-d4	14.839	143	281173	20.322	ng/ul	0.00
60) Fluorene-d10	15.639	176	1506934	28.556	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	237762	21.182	ng/ul	0.00
73) Anthracene-d10	17.498	188	2358562	27.599	ng/ul	0.00
81) Pyrene-d10	19.786	212	2960486	29.470	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	2493419	28.684	ng/ul	0.00
Target Compounds						
10) Bis(2-Chloroethyl)ether	7.434	93	34890	1.796	ng/ul#	25
91) Benzo(k)fluoranthene	23.280	252	108671	1.021	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023263.D
Acq On : 17 Dec 2022 06:02
Operator : CG/JU
Sample : N5925-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBYC8

Quant Time: Dec 19 00:12:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration




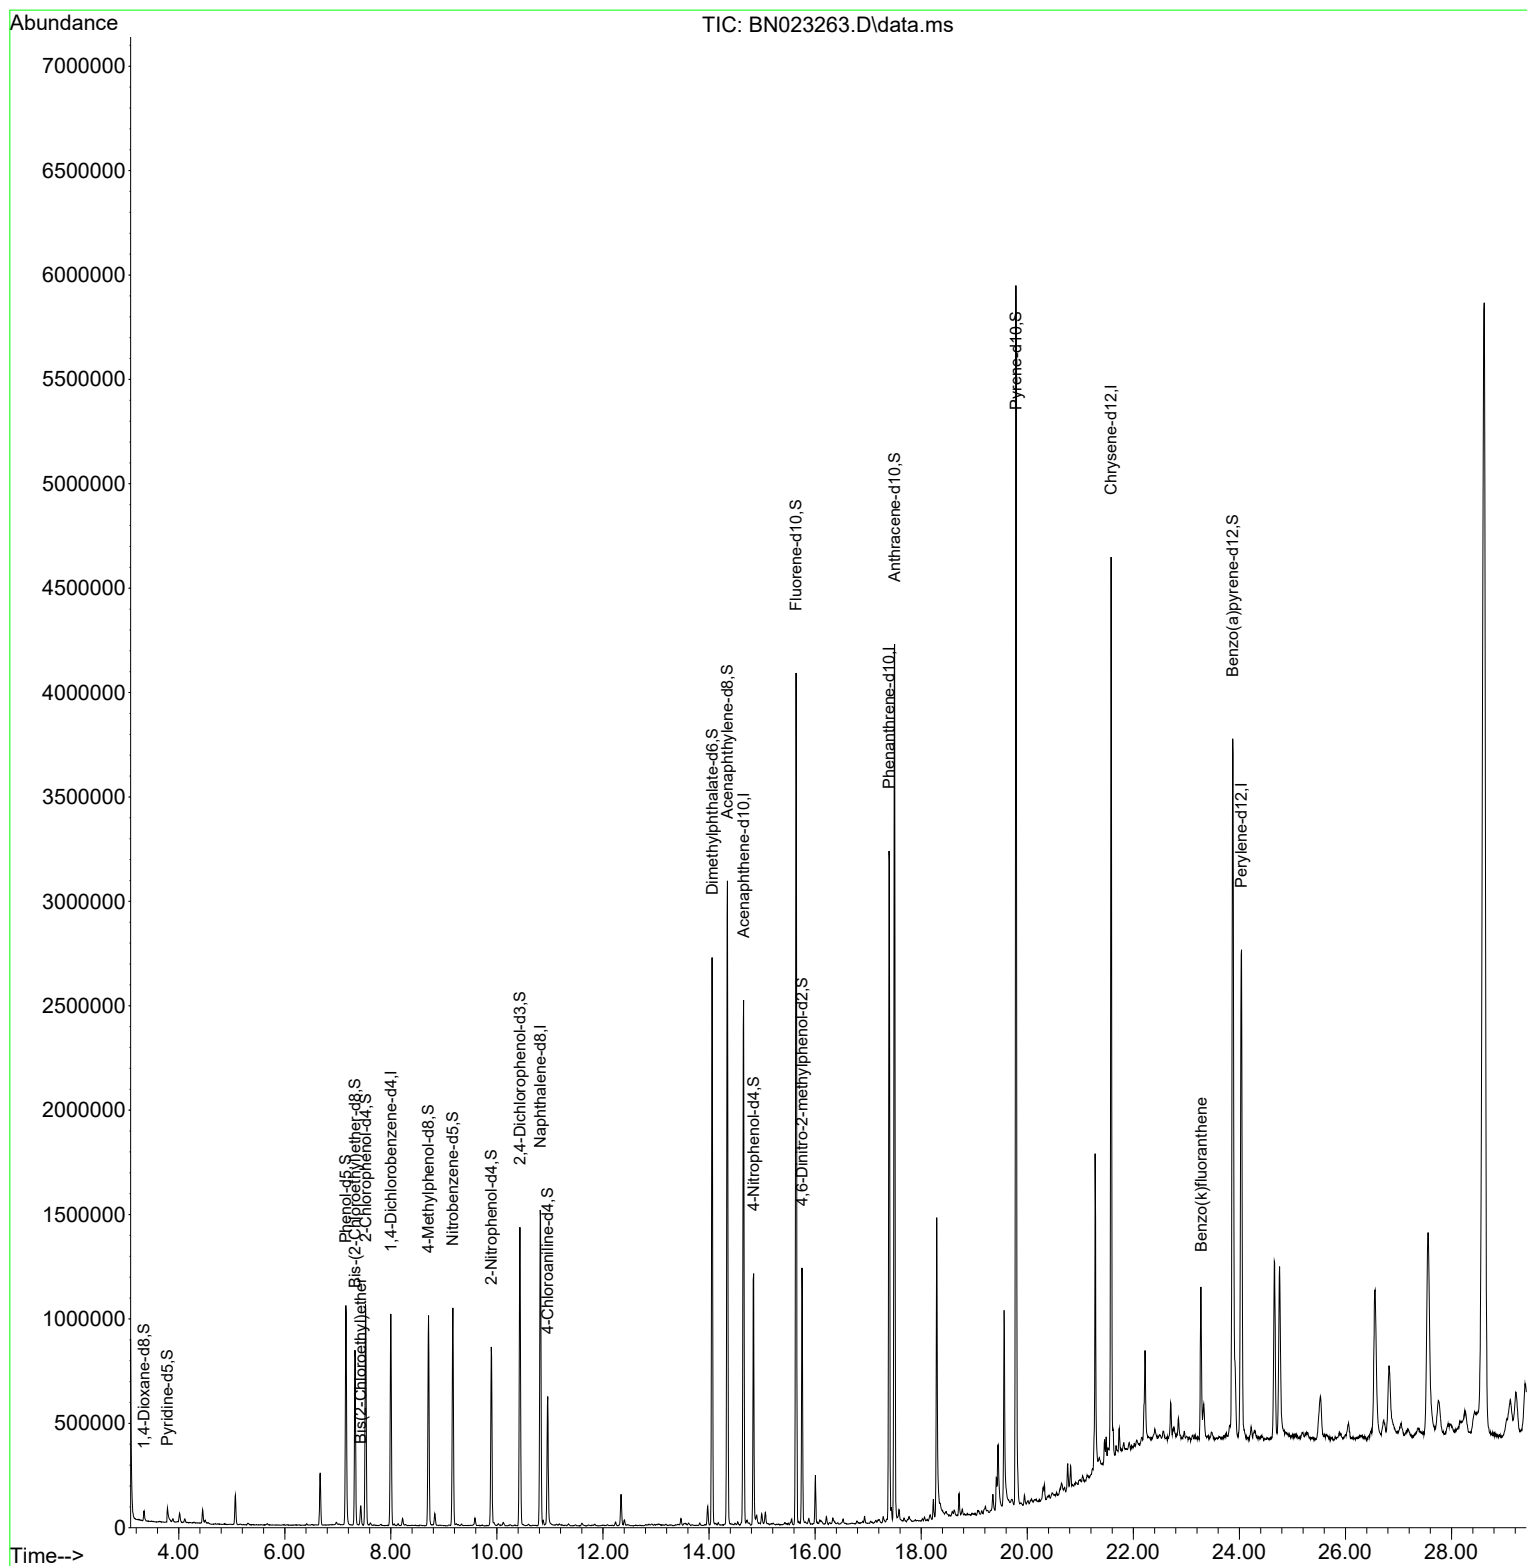


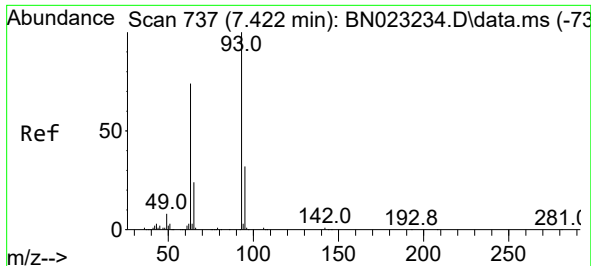

#10
Bis(2-Chloroethyl)ether
Concen: 1.796 ng/ul
RT: 7.434 min Scan# 71
Delta R.T. 0.012 min
Lab File: BN023263.D
Acq: 17 Dec 2022 06:02

Instrument :
BNA_N
ClientSampleId :
DBYC8

Tgt Ion: 93 Resp: 34890
Ion Ratio Lower Upper
93 100
63 2.5 58.9 88.3#
95 2.8 26.2 39.4#

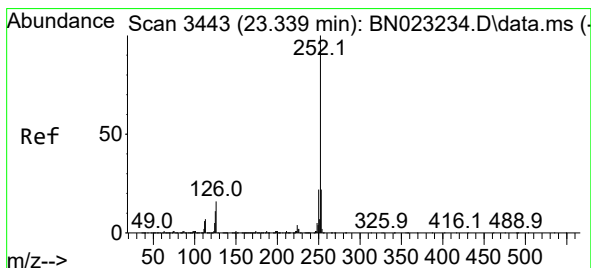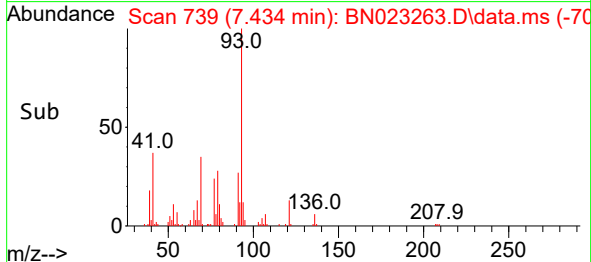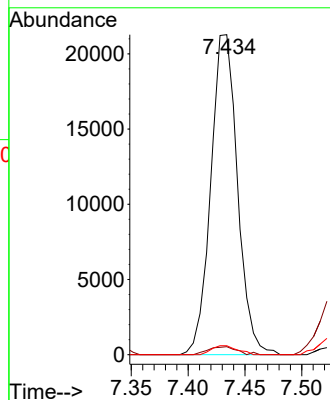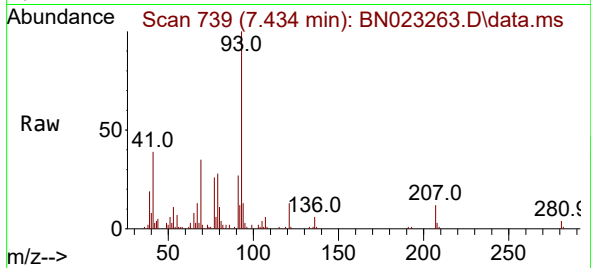

#91
Benzo(k)fluoranthene
Concen: 1.021 ng/ul
RT: 23.280 min Scan# 3433
Delta R.T. -0.053 min
Lab File: BN023263.D
Acq: 17 Dec 2022 06:02

Tgt Ion: 252 Resp: 108671
Ion Ratio Lower Upper
252 100
253 26.1 17.9 26.9
125 20.1 9.0 13.6#

