

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023269.D
 Acq On : 17 Dec 2022 09:43
 Operator : CG/JU
 Sample : N5925-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBXV4

Quant Time: Dec 19 00:14:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	297650	20.000	ng/ul	0.00
20) Naphthalene-d8	10.816	136	1373797	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.651	164	911150	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	2004441	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	1780459	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	1679932	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	30027	4.174	ng/uL	0.00
4) Pyridine-d5	3.781	84	101469	4.778	ng/ul	0.00
7) Phenol-d5	7.157	99	719796	26.001	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.322	67	411952	25.572	ng/ul	0.00
11) 2-Chlorophenol-d4	7.522	132	573553	27.495	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	566011	25.465	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	302174	28.468	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	338197	30.252	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	611310	28.966	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	454281	13.378	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1873071	27.432	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	2192501	28.632	ng/ul	0.00
54) 4-Nitrophenol-d4	14.839	143	368522	24.165	ng/ul	0.00
60) Fluorene-d10	15.639	176	1656024	28.471	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	311644	26.412	ng/ul	0.00
73) Anthracene-d10	17.498	188	2481491	27.624	ng/ul	0.00
81) Pyrene-d10	19.792	212	2970297	30.668	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	2269660	27.564	ng/ul	0.00


Target Compounds					Qvalue
16) Acetophenone	8.828	105	72758	2.164 ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023269.D
Acq On : 17 Dec 2022 09:43
Operator : CG/JU
Sample : N5925-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBXV4


Quant Time: Dec 19 00:14:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

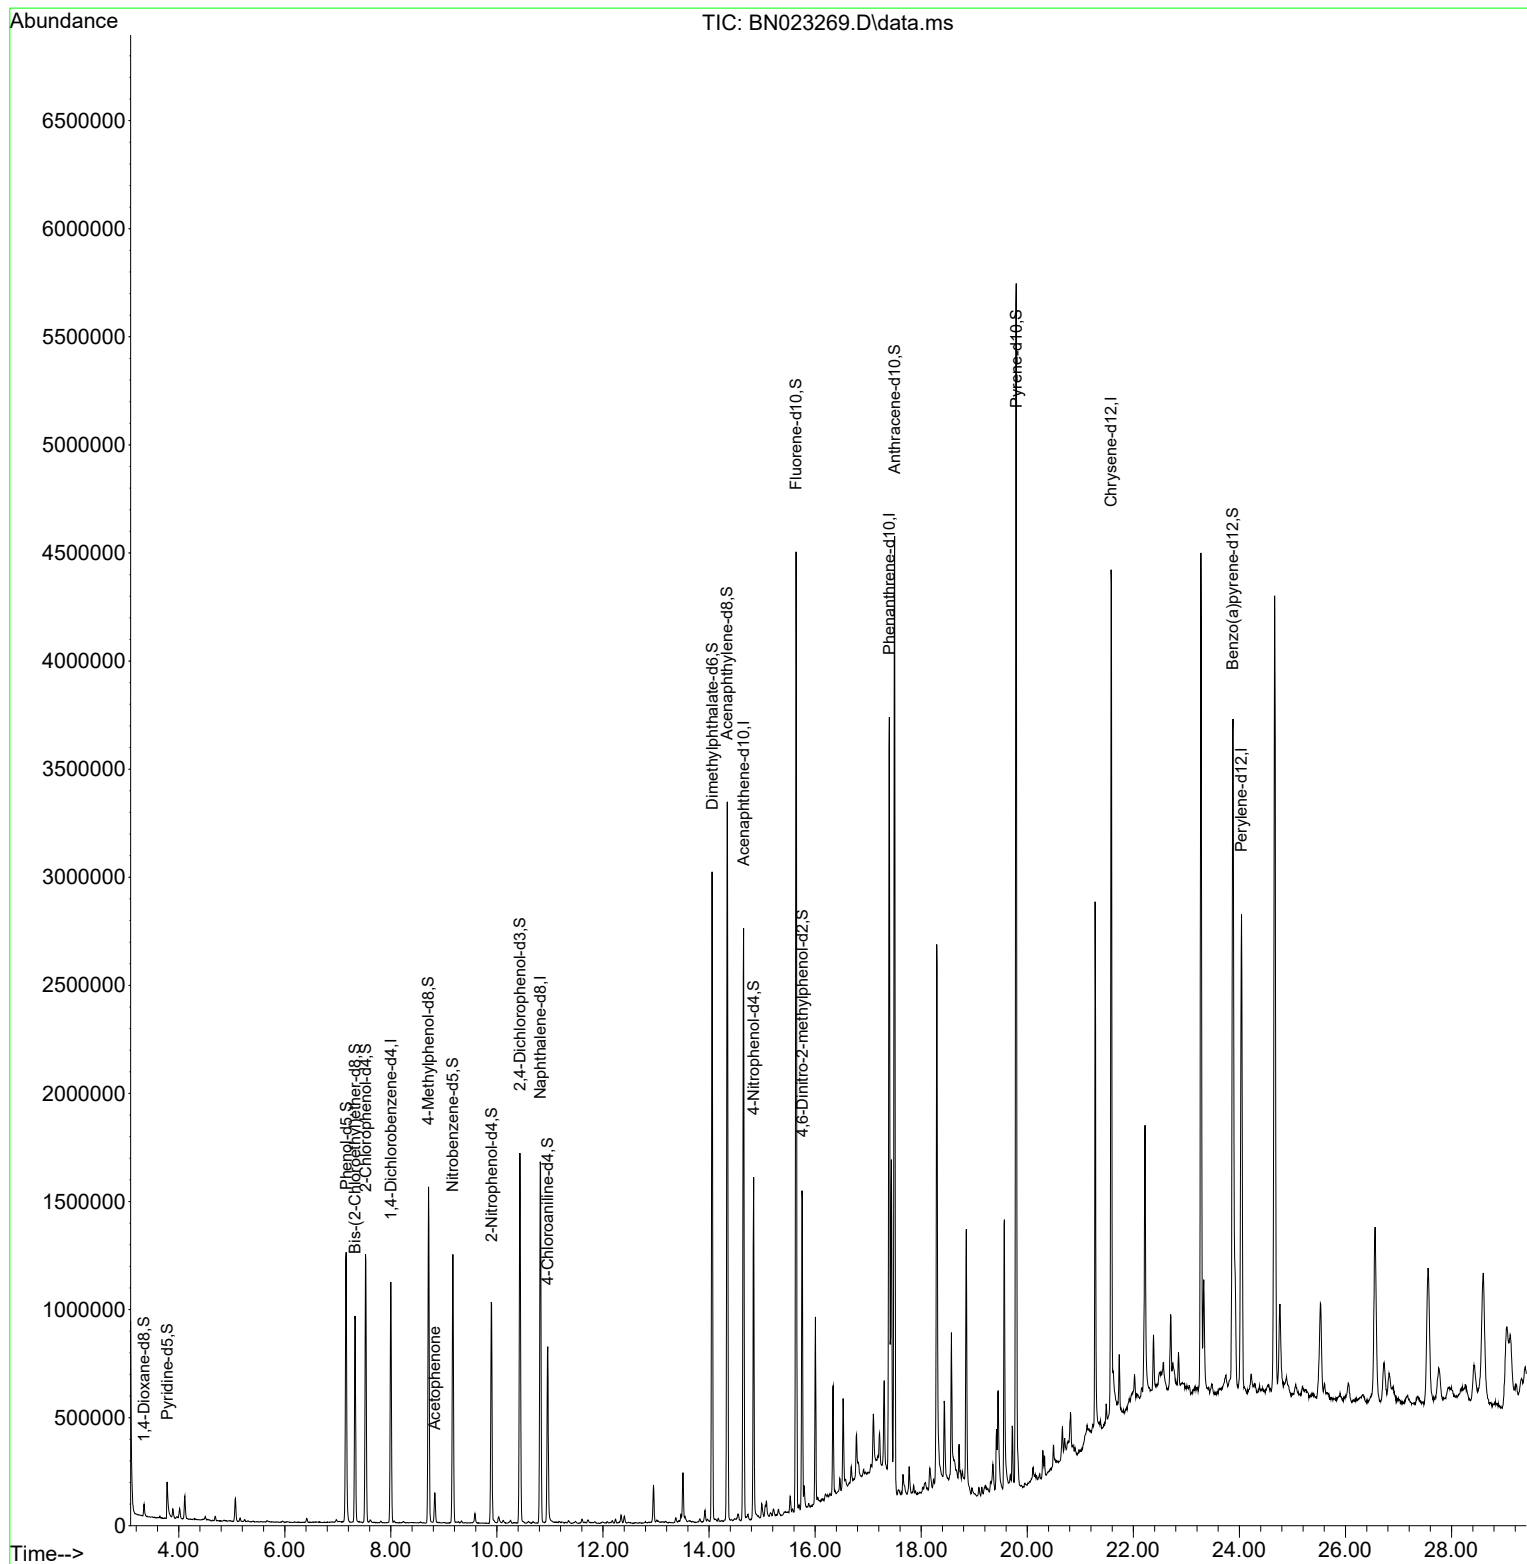

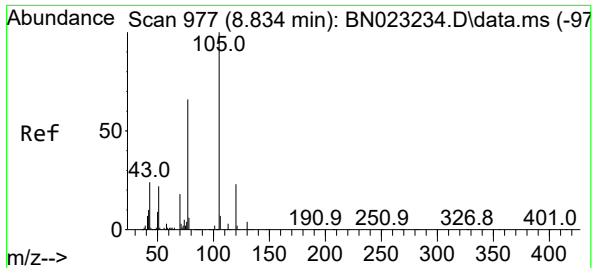

#16
 Acetophenone
 Concen: 2.164 ng/ul
 RT: 8.828 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN023269.D
 Acq: 17 Dec 2022 09:43

Instrument :
 BNA_N
 ClientSampleId :
 DBXV4

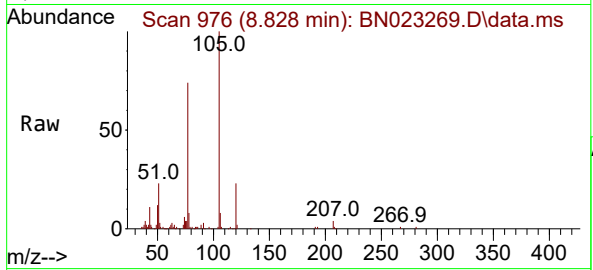

Tgt Ion:	105	Resp:	72758
Ion	Ratio	Lower	Upper
105	100		
77	73.8	61.4	92.0
51	23.1	20.0	30.0

