

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023245.D
 Acq On : 16 Dec 2022 18:18
 Operator : CG/JU
 Sample : N5983-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLE9

Quant Time: Dec 16 21:44:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	279283	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1287235	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	861537	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2024563	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	2010013	20.000	ng/u1	0.00
88) Perylene-d12	24.045	264	2045510	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	32247	4.777	ng/uL	0.00
4) Pyridine-d5	3.775	84	489857	24.583	ng/u1	0.00
7) Phenol-d5	7.158	99	711600	27.396	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	431714	28.561	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	565499	28.892	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	602903	28.909	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	306383	30.806	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	337365	32.206	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.440	165	590134	29.843	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	876114	27.534	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	2132584	33.031	ng/u1	0.00
49) Acenaphthylene-d8	14.346	160	2363494	32.643	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	427015	29.613	ng/u1	0.00
60) Fluorene-d10	15.640	176	1824254	33.170	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	336093	28.201	ng/u1	0.00
73) Anthracene-d10	17.498	188	2913324	32.109	ng/u1	0.00
81) Pyrene-d10	19.792	212	3623329	33.138	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.886	264	3442061	34.331	ng/u1	0.01
Target Compounds						
71) Pentachlorophenol	17.045	266	115754	7.675	ng/u1	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023245.D
Acq On : 16 Dec 2022 18:18
Operator : CG/JU
Sample : N5983-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLE9

Quant Time: Dec 16 21:44:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

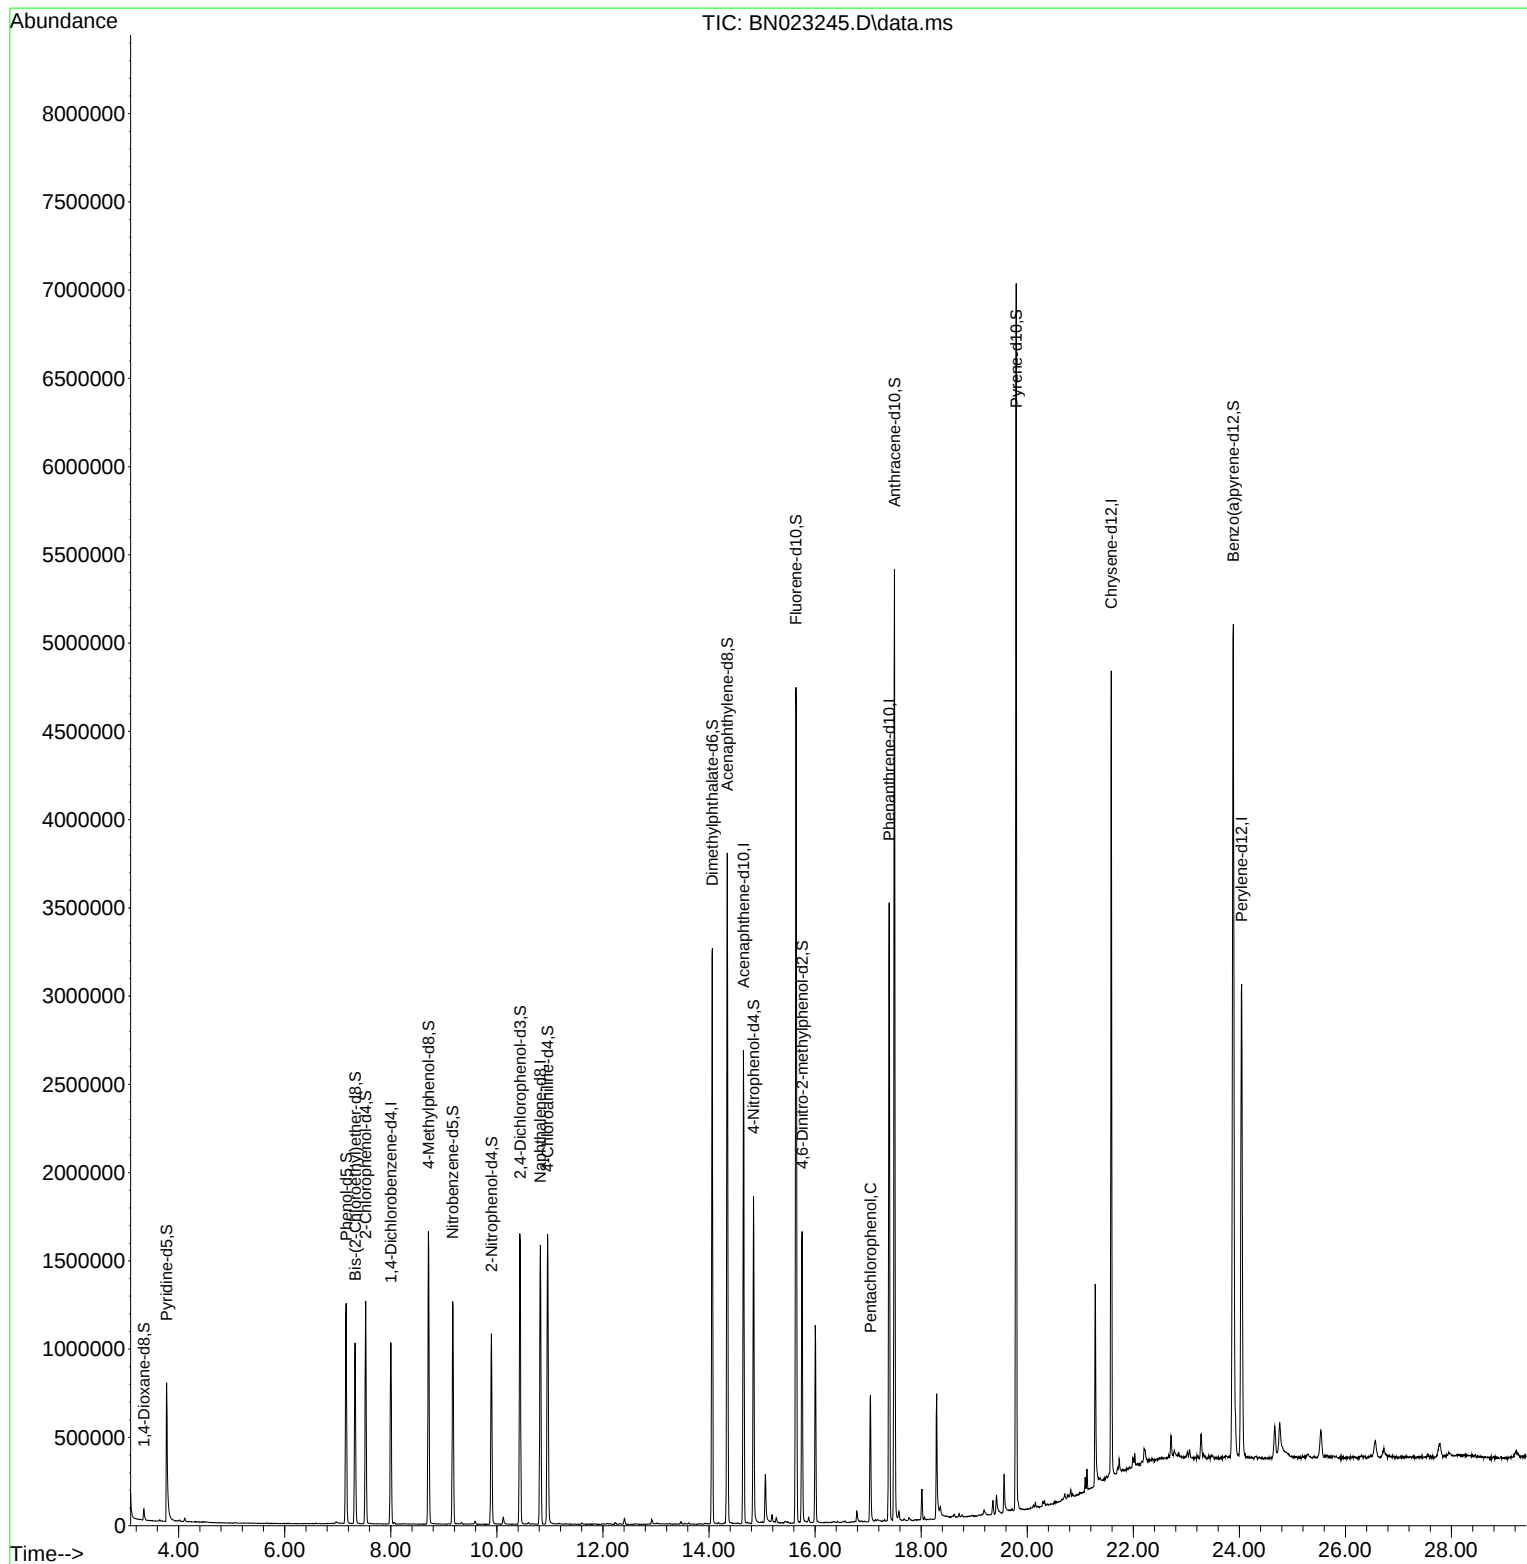

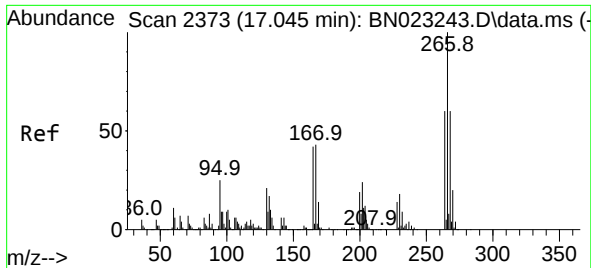

#71
 Pentachlorophenol
 Concen: 7.675 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023245.D
 Acq: 16 Dec 2022 18:18

Instrument :
 BNA_N
 ClientSampleId :
 COLE9

Tgt Ion:266 Resp: 115754
 Ion Ratio Lower Upper
 266 100
 264 58.6 50.5 75.7
 268 61.2 52.6 78.8

