

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023246.D
 Acq On : 16 Dec 2022 18:55
 Operator : CG/JU
 Sample : N5983-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLB4

Quant Time: Dec 16 21:44:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	293621	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1376052	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	922653	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2167013	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	2131104	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	2149784	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	27639	3.895	ng/uL	0.00
4) Pyridine-d5	3.775	84	389006	18.569	ng/u1	0.00
7) Phenol-d5	7.158	99	570895	20.905	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	357246	22.480	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	469241	22.803	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	487170	22.219	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	247270	23.258	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	262813	23.470	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	474535	22.448	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	707495	20.800	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	1684370	24.361	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	1913337	24.675	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	311583	20.177	ng/u1	0.00
60) Fluorene-d10	15.639	176	1487337	25.252	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	231810	18.172	ng/u1	0.00
73) Anthracene-d10	17.498	188	2352414	24.222	ng/u1	0.00
81) Pyrene-d10	19.792	212	2904127	25.051	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	2616533	24.831	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	17.045	266	76461	4.737	ng/u1	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023246.D
Acq On : 16 Dec 2022 18:55
Operator : CG/JU
Sample : N5983-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLB4


Quant Time: Dec 16 21:44:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

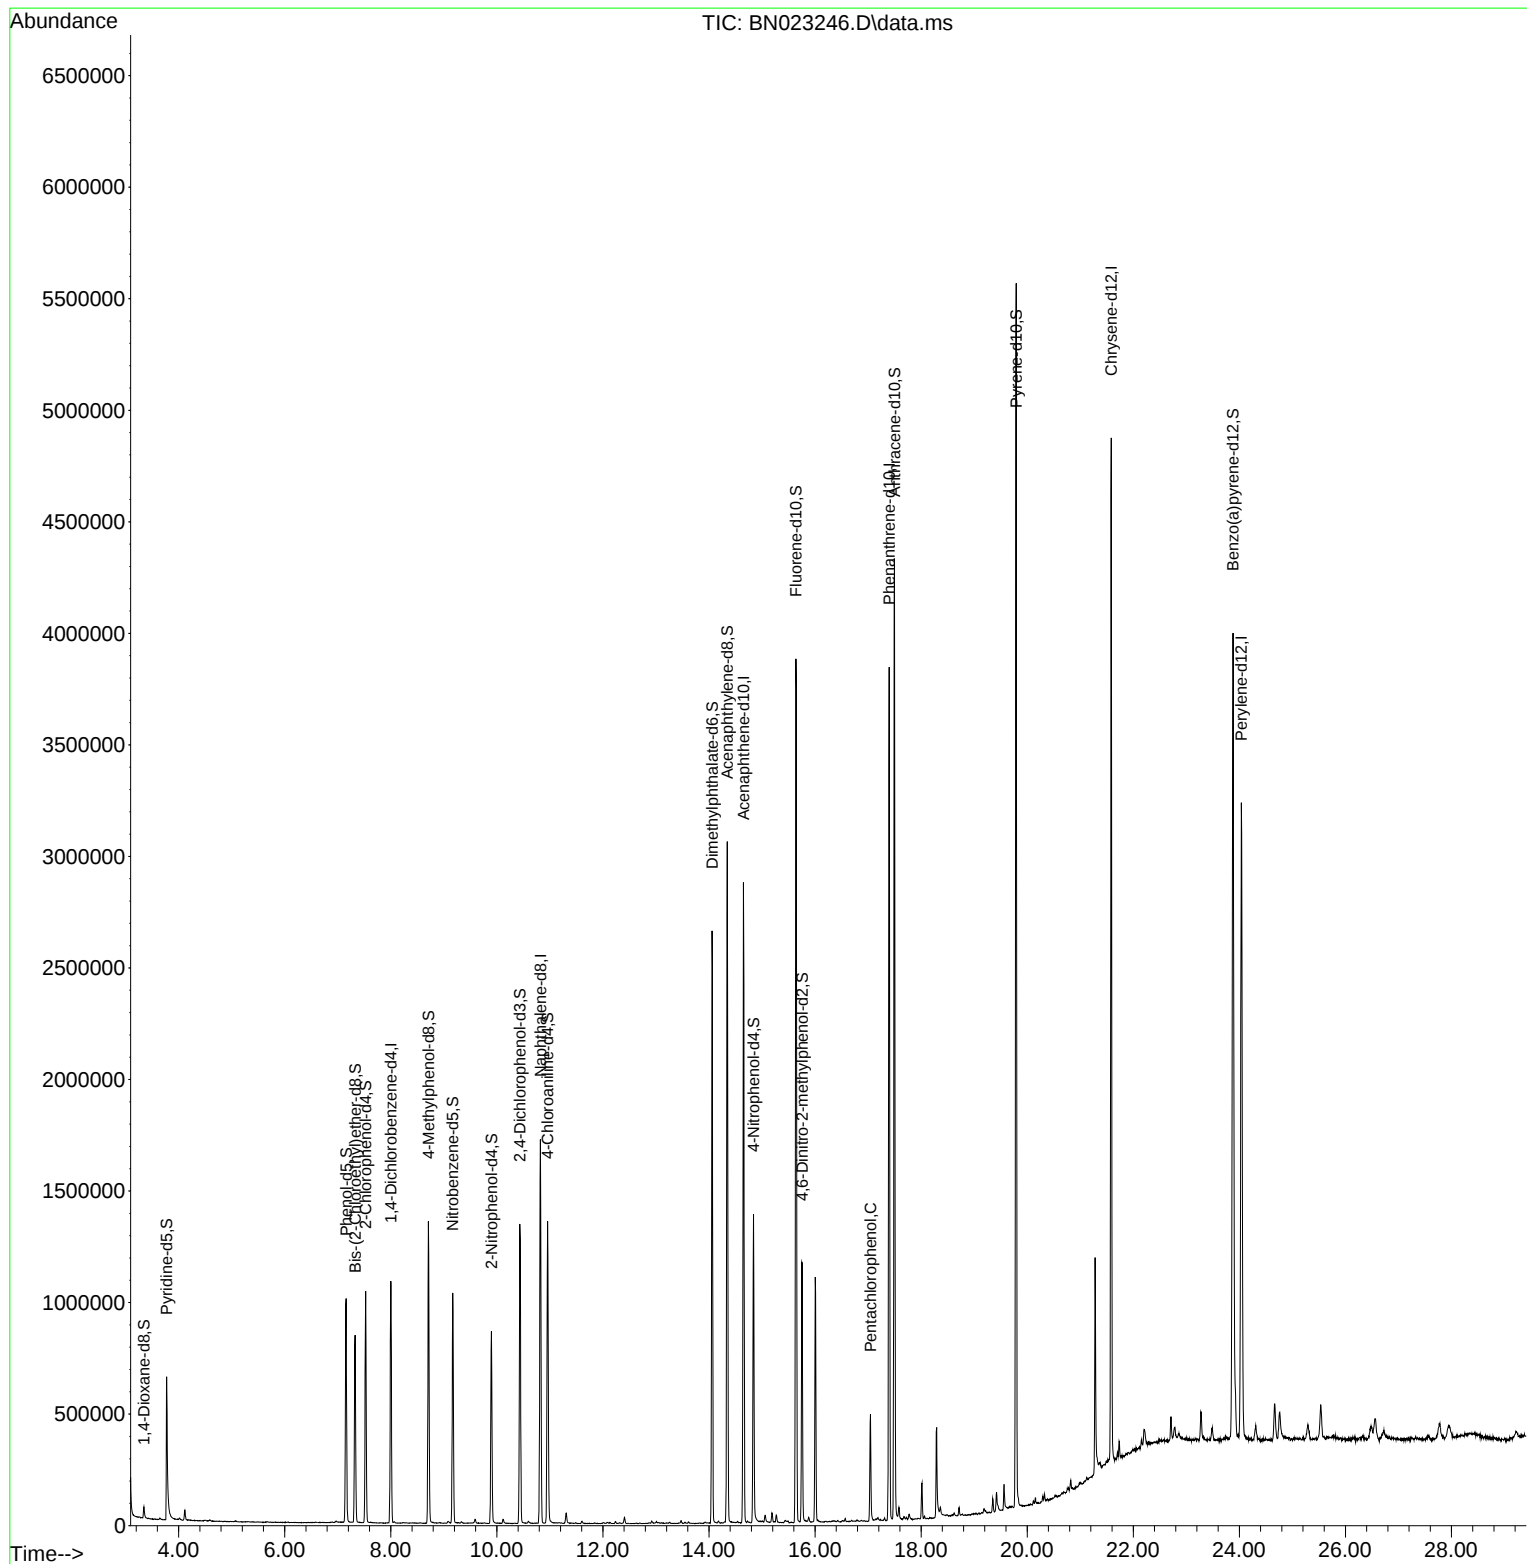

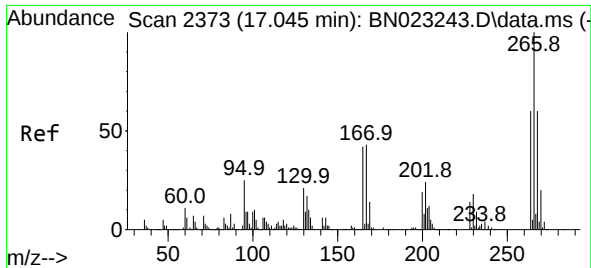

#71
 Pentachlorophenol
 Concen: 4.737 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023246.D
 Acq: 16 Dec 2022 18:55

Instrument :
 BNA_N
 ClientSampleId :
 COLB4

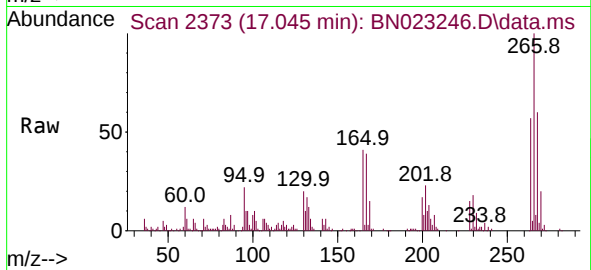

Tgt Ion:266 Resp: 76461
 Ion Ratio Lower Upper
 266 100
 264 57.1 50.5 75.7
 268 60.0 52.6 78.8

