

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023248.D
 Acq On : 16 Dec 2022 20:10
 Operator : CG/JU
 Sample : N5983-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLB7

Quant Time: Dec 16 21:45:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	295935	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1356966	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	935899	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2169515	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	2127883	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	2171374	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	30270	4.232	ng/uL	0.00
4) Pyridine-d5	3.775	84	429583	20.345	ng/u1	0.00
7) Phenol-d5	7.158	99	625201	22.715	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	378952	23.659	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	500858	24.150	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	523778	23.702	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	263293	25.113	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	286017	25.901	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	507644	24.352	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	744231	22.188	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	1822862	25.990	ng/u1	0.00
49) Acenaphthylene-d8	14.346	160	2016308	25.635	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	342628	21.873	ng/u1	0.00
60) Fluorene-d10	15.640	176	1573488	26.337	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	258913	20.273	ng/u1	0.00
73) Anthracene-d10	17.498	188	2487785	25.587	ng/u1	0.00
81) Pyrene-d10	19.786	212	3032919	26.202	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	2802225	26.329	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	17.045	266	73878	4.571	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023248.D
Acq On : 16 Dec 2022 20:10
Operator : CG/JU
Sample : N5983-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLB7


Quant Time: Dec 16 21:45:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

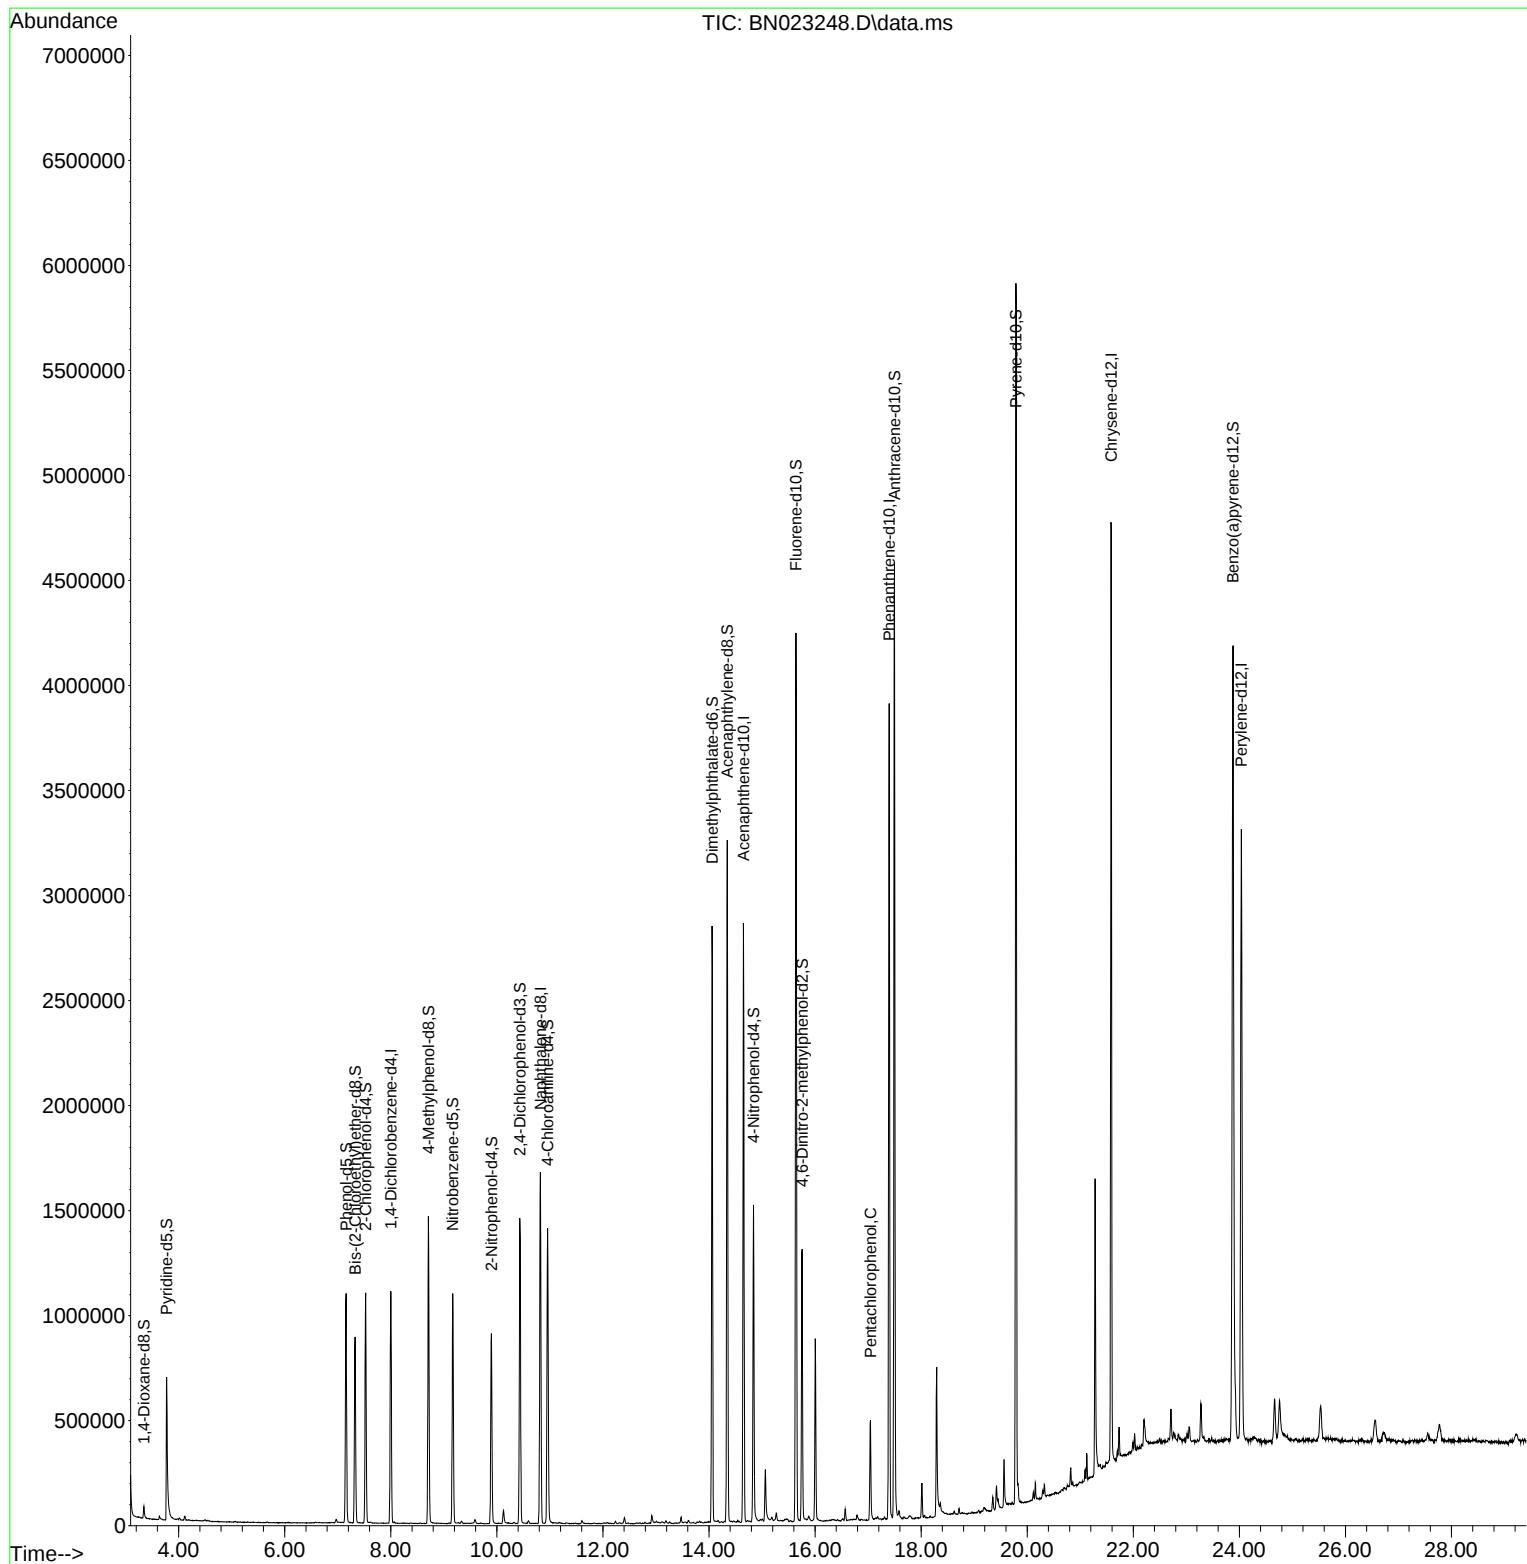

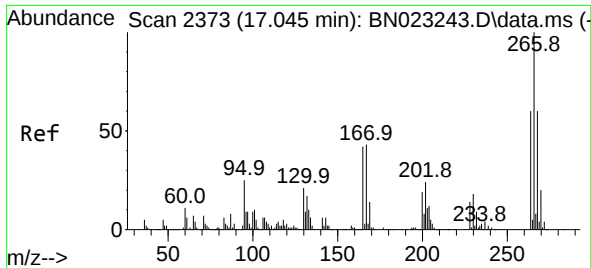

#71
 Pentachlorophenol
 Concen: 4.571 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023248.D
 Acq: 16 Dec 2022 20:10

Instrument :
 BNA_N
 ClientSampleId :
 COLB7

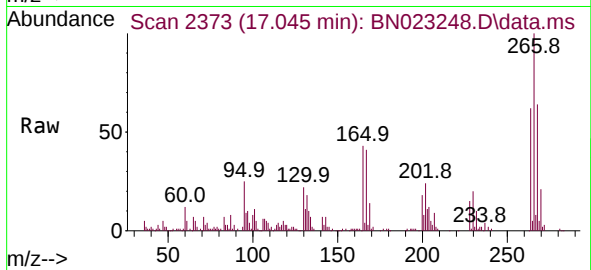

Tgt Ion:	266	Resp:	73878
Ion Ratio	Lower	Upper	
266	100		
264	61.9	50.5	75.7
268	64.5	52.6	78.8

