

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023249.D
 Acq On : 16 Dec 2022 20:47
 Operator : CG/JU
 Sample : N5983-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLC0

Quant Time: Dec 16 21:45:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	275571	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1280581	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	865987	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2034211	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1970278	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	1945469	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	19965	2.997	ng/uL	0.00
4) Pyridine-d5	3.781	84	121677	6.189	ng/u1	0.00
7) Phenol-d5	7.152	99	429823	16.770	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	281385	18.866	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	358834	18.580	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	372367	18.095	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	190099	19.213	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	198258	19.025	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	350734	17.829	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	508088	16.051	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	1339604	20.642	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	1428347	19.626	ng/u1	0.00
54) 4-Nitrophenol-d4	14.840	143	193891	13.377	ng/u1	0.00
60) Fluorene-d10	15.640	176	1169245	21.151	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	153860	12.849	ng/u1	0.00
73) Anthracene-d10	17.492	188	1909985	20.951	ng/u1	0.00
81) Pyrene-d10	19.786	212	2415309	22.535	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	2157347	22.624	ng/u1	0.00
Target Compounds						Qvalue
71) Pentachlorophenol	17.045	266	78342	5.170	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023249.D
Acq On : 16 Dec 2022 20:47
Operator : CG/JU
Sample : N5983-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLC0


Quant Time: Dec 16 21:45:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

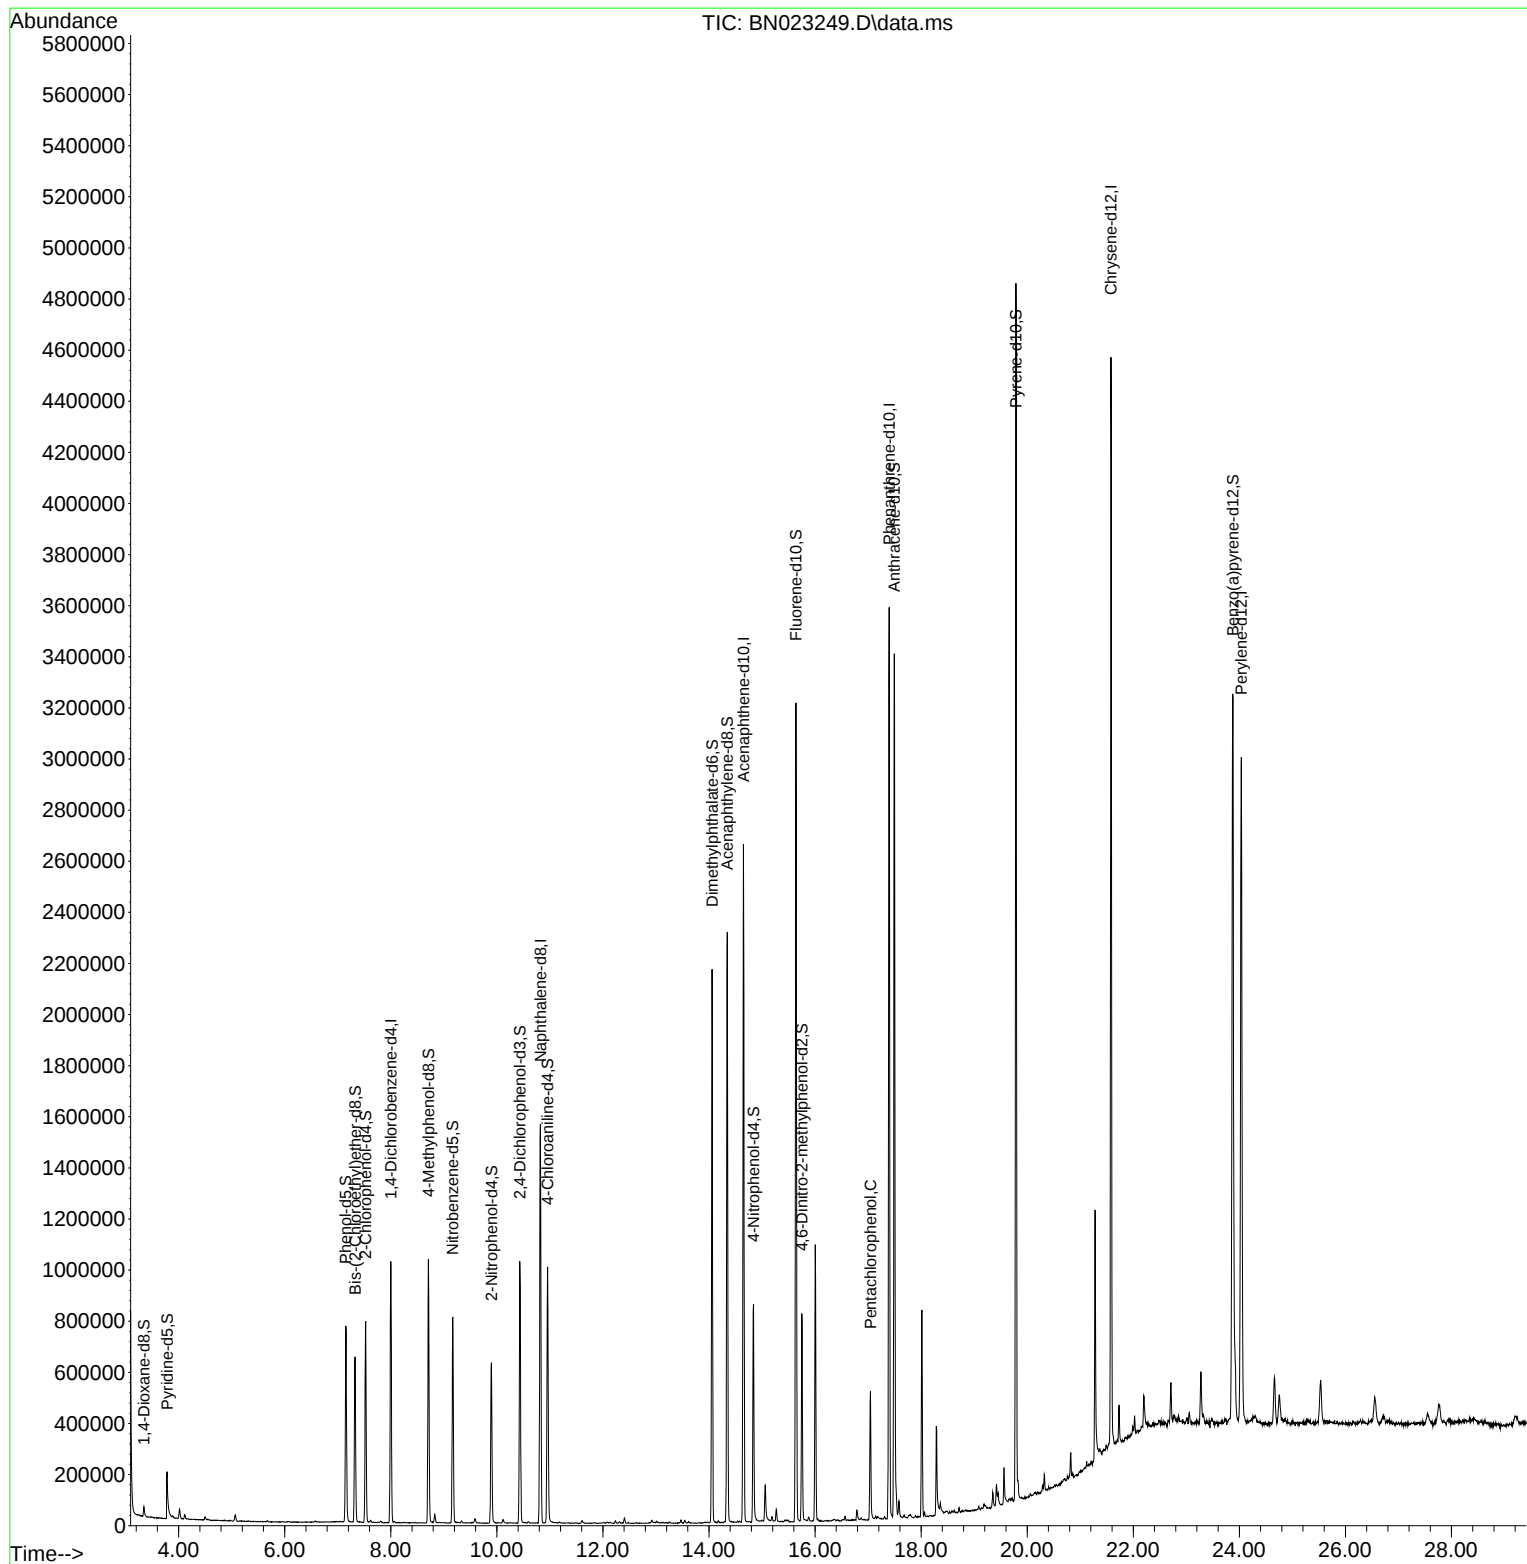

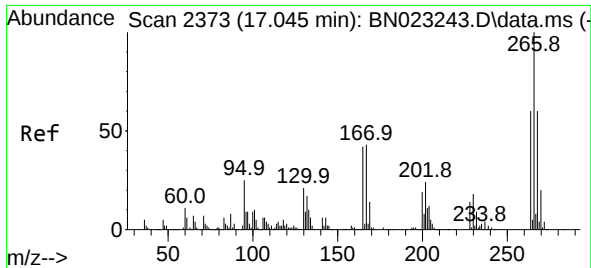

#71
 Pentachlorophenol
 Concen: 5.170 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023249.D
 Acq: 16 Dec 2022 20:47

Instrument :
 BNA_N
 ClientSampleId :
 COLC0

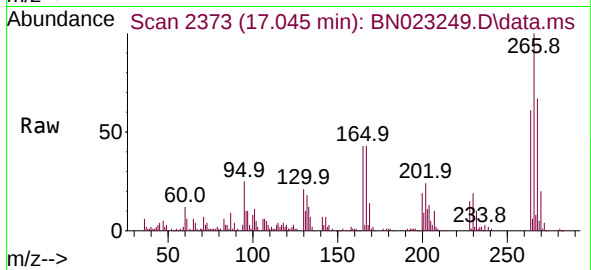

Tgt Ion:	266	Resp:	78342
Ion Ratio	Lower	Upper	
266	100		
264	60.7	50.5	75.7
268	66.9	52.6	78.8

