

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023251.D
 Acq On : 16 Dec 2022 22:01
 Operator : CG/JU
 Sample : N5983-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLB9

Quant Time: Dec 16 23:06:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	290108	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1352028	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	925012	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2132510	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	2009487	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	2044741	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	32926	4.696	ng/uL	0.00
4) Pyridine-d5	3.775	84	479022	23.143	ng/u1	0.00
7) Phenol-d5	7.158	99	654030	24.240	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	435356	27.727	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	522376	25.693	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	577525	26.659	ng/u1	0.00
21) Nitrobenzene-d5	9.169	128	301611	28.873	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	265232	24.107	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	545909	26.283	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	860623	25.751	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2058380	29.694	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	2349926	30.228	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	323151	20.872	ng/u1	0.00
60) Fluorene-d10	15.639	176	1830808	31.005	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	211949	16.884	ng/u1	0.00
73) Anthracene-d10	17.498	188	2843135	29.749	ng/u1	0.00
81) Pyrene-d10	19.792	212	3460657	31.659	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	3106287	30.994	ng/u1	0.00
Target Compounds						Qvalue
71) Pentachlorophenol	17.045	266	125344	7.890	ng/u1	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023251.D
Acq On : 16 Dec 2022 22:01
Operator : CG/JU
Sample : N5983-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLB9


Quant Time: Dec 16 23:06:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

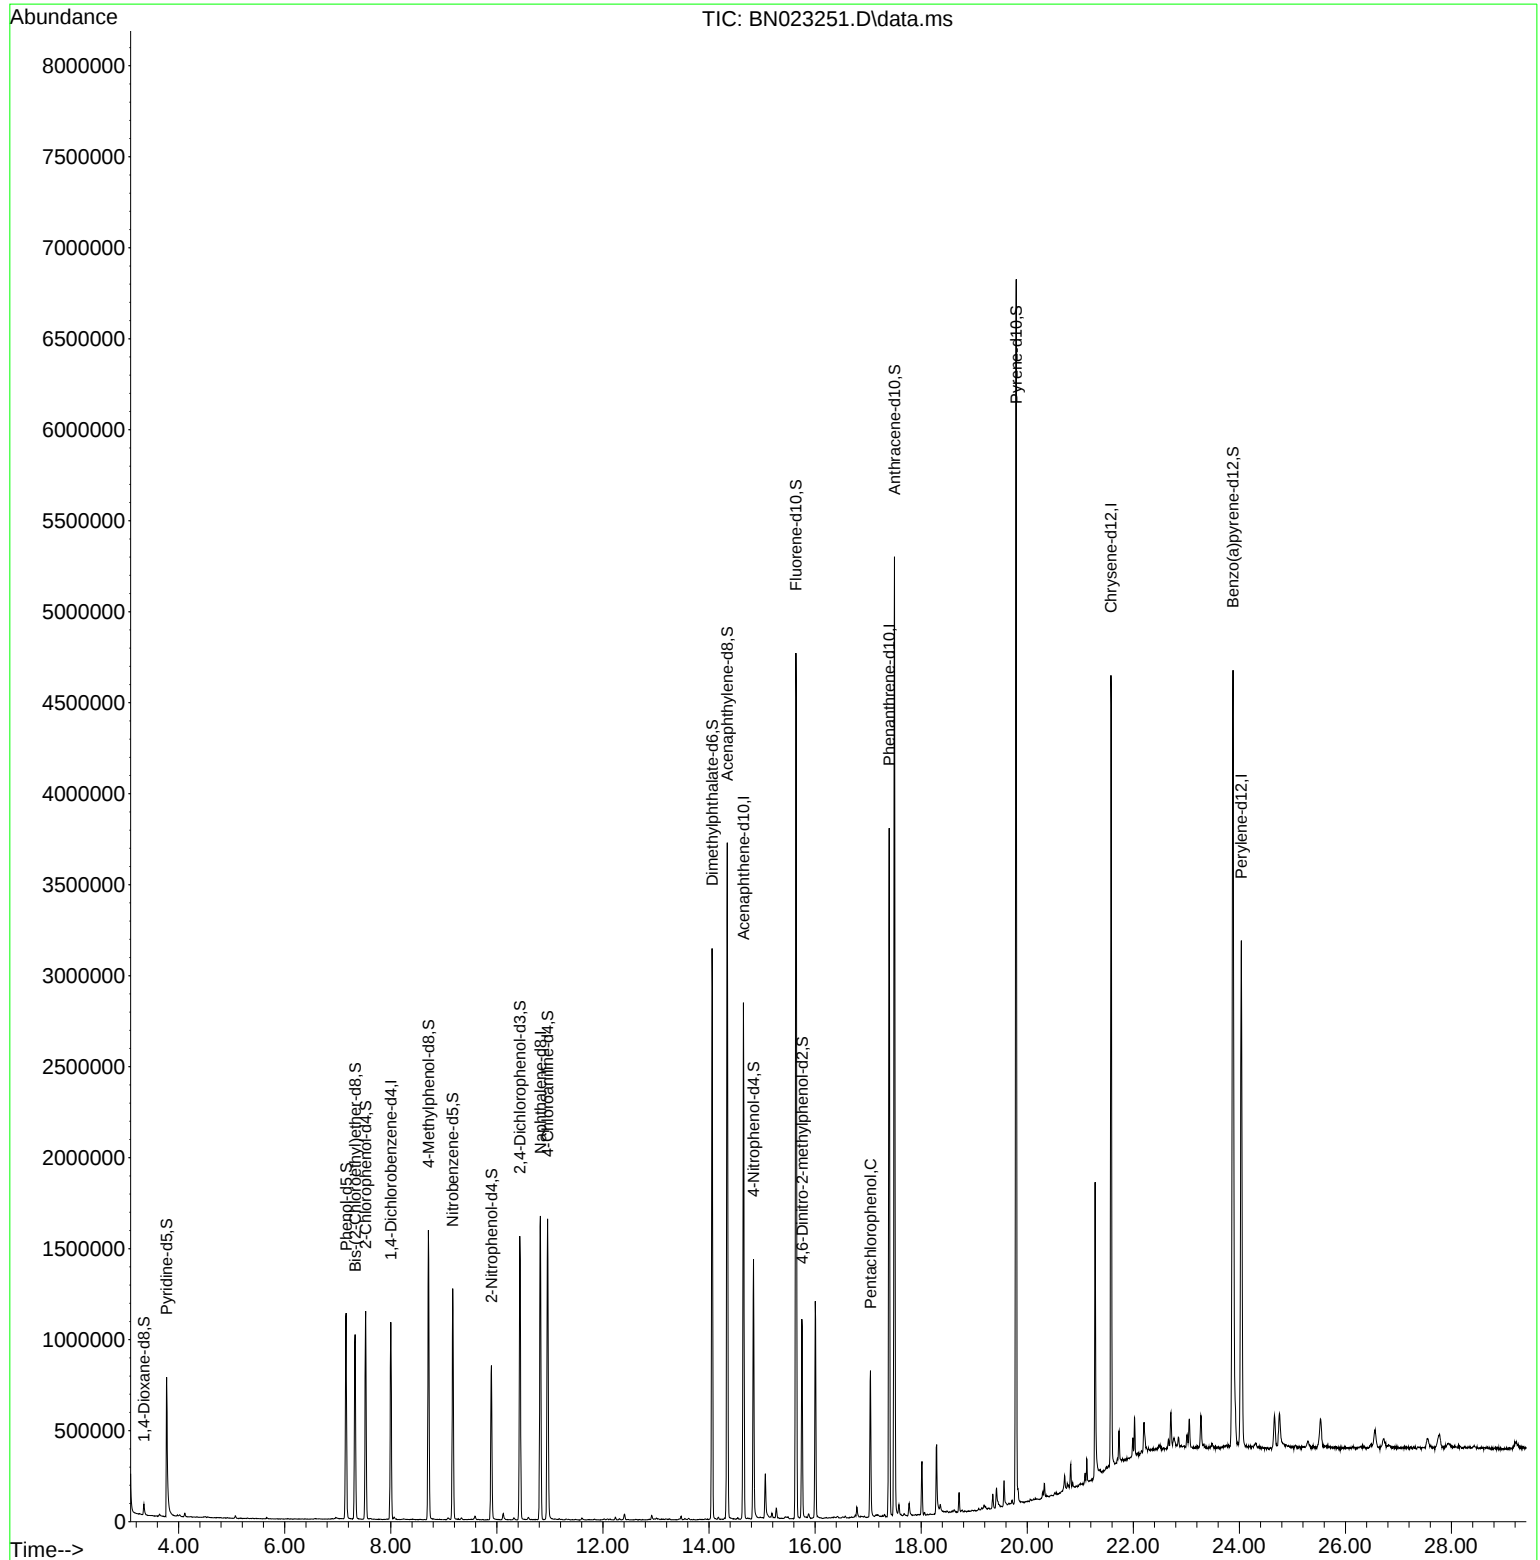

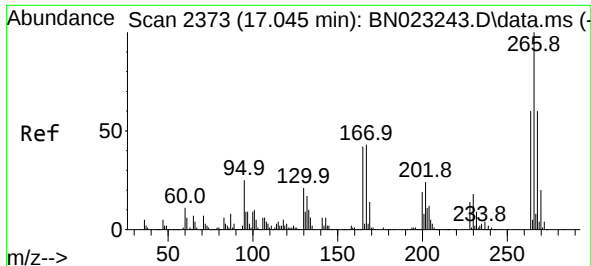

#71
 Pentachlorophenol
 Concen: 7.890 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023251.D
 Acq: 16 Dec 2022 22:01

Instrument :
 BNA_N
 ClientSampleId :
 COLB9

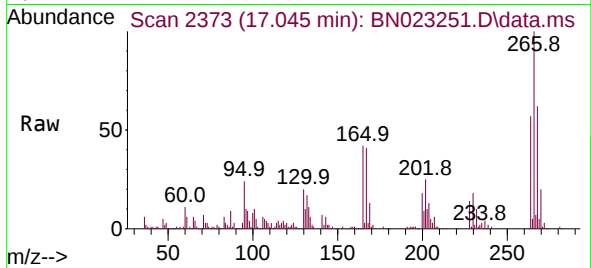

Tgt Ion:266 Resp: 125344
 Ion Ratio Lower Upper
 266 100
 264 56.9 50.5 75.7
 268 61.8 52.6 78.8

