

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023252.D
 Acq On : 16 Dec 2022 22:39
 Operator : CG/JU
 Sample : N5983-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLE1

Quant Time: Dec 17 00:21:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 15 23:22:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.999	152	290564	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1340969	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	891057	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.398	188	2032636	20.000	ng/u1	0.00
79) Chrysene-d12	21.580	240	1975408	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	1949494	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.346	96	50389	7.175	ng/uL	0.00
4) Pyridine-d5	3.770	84	759867	36.653	ng/u1	0.00
7) Phenol-d5	7.158	99	1060933	39.259	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	641746	40.807	ng/u1	0.00
11) 2-Chlorophenol-d4	7.528	132	834651	40.988	ng/u1	0.00
15) 4-Methylphenol-d8	8.711	113	901106	41.530	ng/u1	0.00
21) Nitrobenzene-d5	9.175	128	462720	44.661	ng/u1	0.00
24) 2-Nitrophenol-d4	9.899	143	514586	47.156	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	889076	43.158	ng/u1	0.00
31) 4-Chloroaniline-d4	10.958	131	1288167	38.862	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	3026687	45.326	ng/u1	0.00
49) Acenaphthylene-d8	14.346	160	3439999	45.937	ng/u1	0.00
54) 4-Nitrophenol-d4	14.846	143	627949	42.105	ng/u1	0.00
60) Fluorene-d10	15.645	176	2606999	45.832	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.757	200	487230	40.720	ng/u1	0.00
73) Anthracene-d10	17.498	188	4080702	44.796	ng/u1	0.00
81) Pyrene-d10	19.792	212	4928579	45.865	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	4619916	48.348	ng/u1	0.00
Target Compounds						
71) Pentachlorophenol	17.045	266	64212	4.241	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023252.D
Acq On : 16 Dec 2022 22:39
Operator : CG/JU
Sample : N5983-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLE1


Quant Time: Dec 17 00:21:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 15 23:22:36 2022
Response via : Initial Calibration

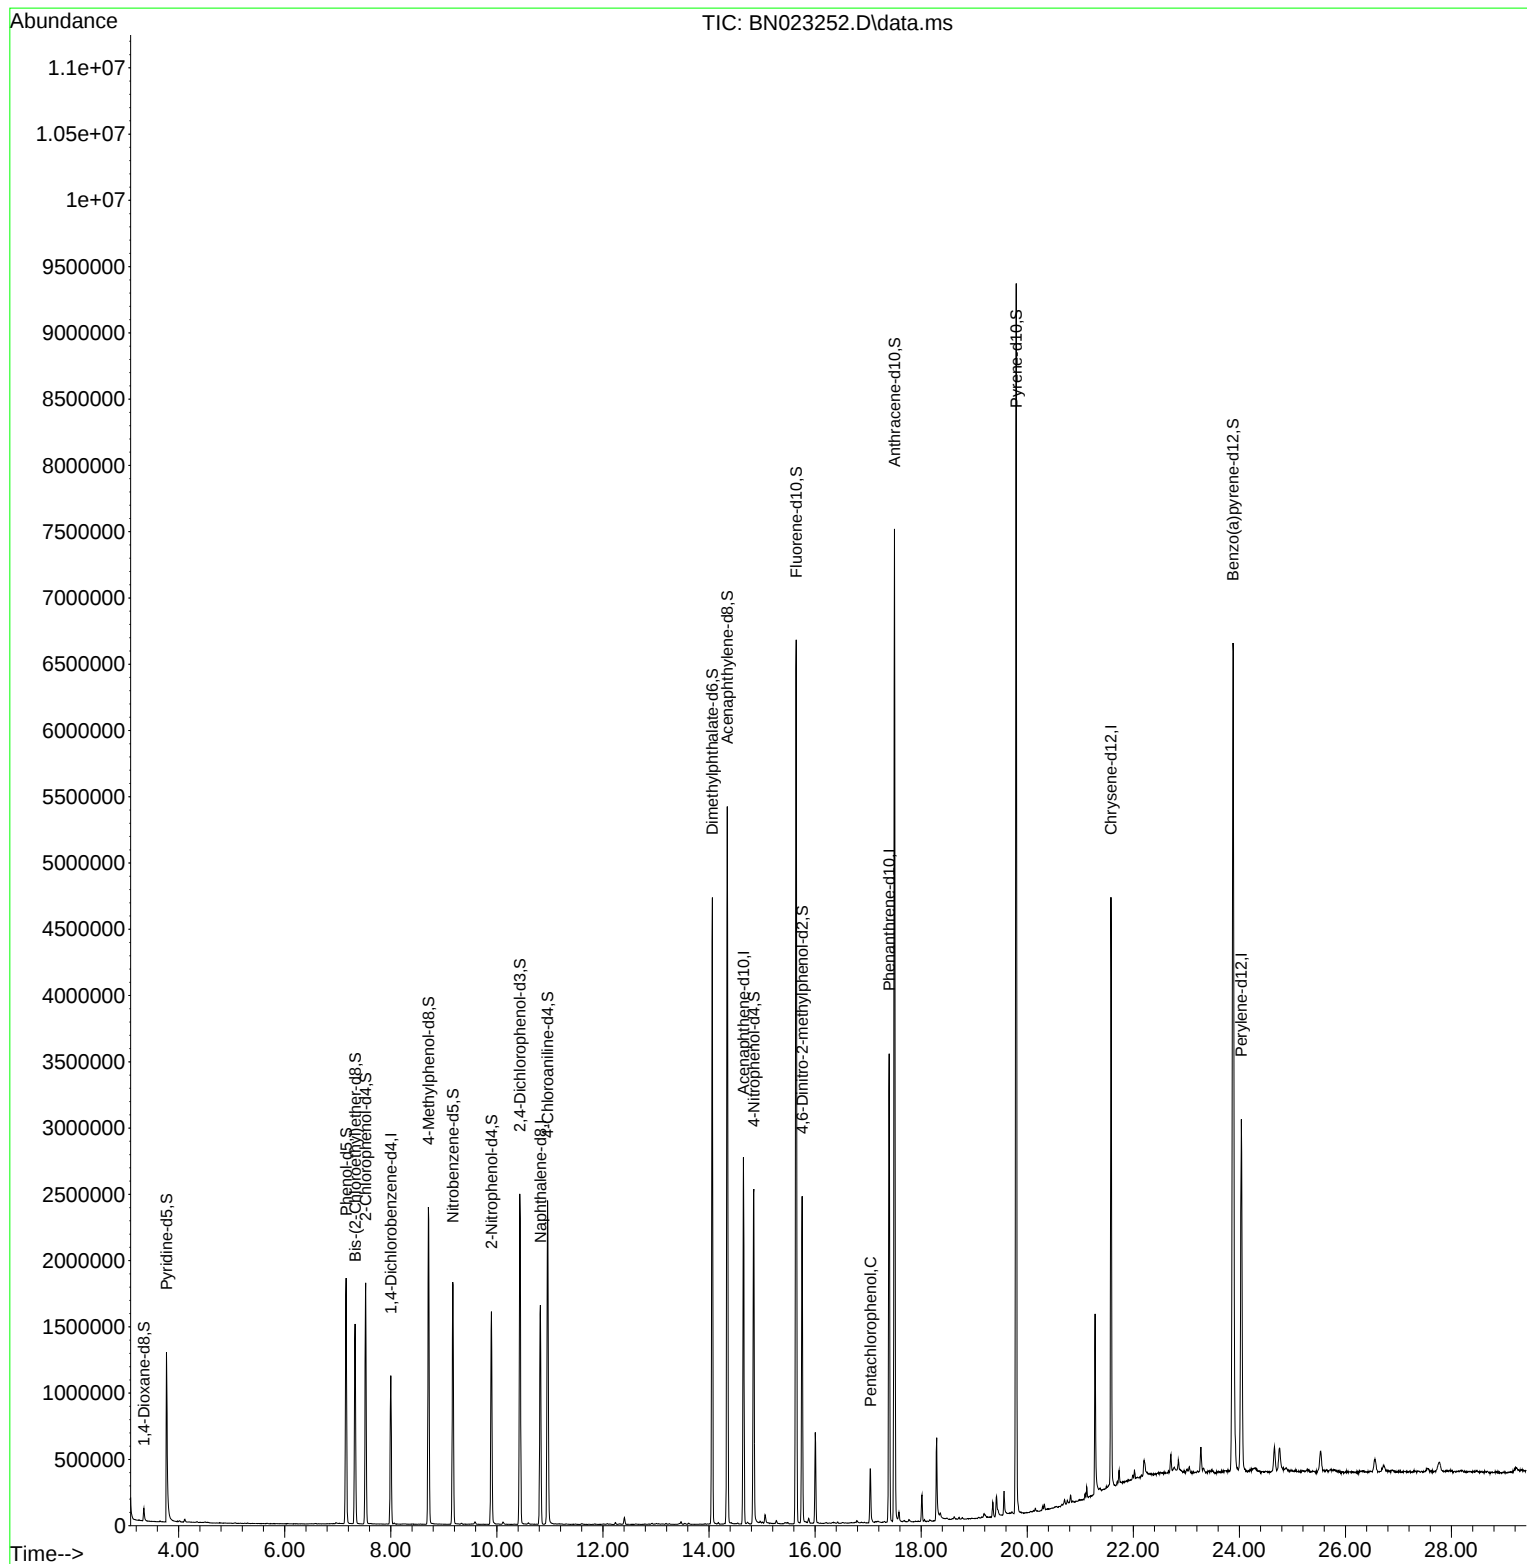

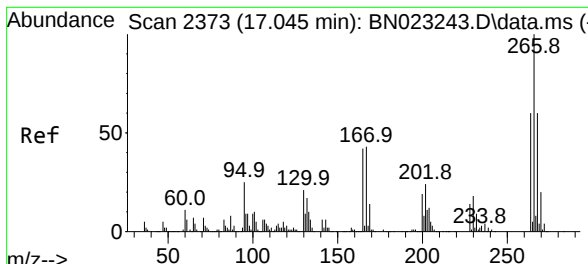

#71
 Pentachlorophenol
 Concen: 4.241 ng/ul
 RT: 17.045 min Scan# 2373
 Delta R.T. 0.000 min
 Lab File: BN023252.D
 Acq: 16 Dec 2022 22:39

Instrument :
 BNA_N
 ClientSampleId :
 COLE1

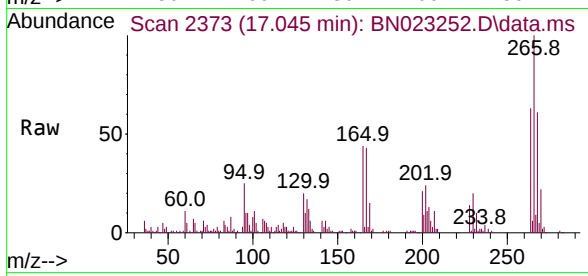

Tgt Ion:	266	Resp:	64212
Ion Ratio	Lower	Upper	
266	100		
264	63.2	50.5	75.7
268	60.7	52.6	78.8

