

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023244.D
 Acq On : 16 Dec 2022 17:40
 Operator : CG/JU
 Sample : PB149555BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK555

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023244.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	52	rVB	55957	80000	0.97%	0.102%
2	3.775	113	117	137	rBV	732063	1223319	14.83%	1.561%
3	4.116	170	175	183	rVB	45650	68779	0.83%	0.088%
4	7.157	685	692	703	rVB	1080871	1651387	20.02%	2.108%
5	7.328	714	721	732	rVB	874332	1345427	16.31%	1.717%
6	7.528	747	755	769	rBV	1082168	1681623	20.39%	2.146%
7	7.999	827	835	845	rBV	906529	1442172	17.49%	1.841%
8	8.710	949	956	972	rBV	1366033	2140988	25.96%	2.732%
9	9.169	1027	1034	1047	rBV	1057806	1714475	20.79%	2.188%
10	9.898	1150	1158	1167	rBV	894219	1431623	17.36%	1.827%
11	10.434	1241	1249	1263	rBV	1364637	2250718	27.29%	2.873%
12	10.822	1308	1315	1323	rBV	1415235	2291358	27.78%	2.924%
13	10.957	1329	1338	1358	rBV	1427948	2397663	29.07%	3.060%
14	12.404	1579	1584	1589	rBV	26053	40561	0.49%	0.052%
15	14.057	1859	1865	1876	rBV	2730933	3758930	45.58%	4.797%
16	14.345	1907	1914	1925	rBV	3085754	4436959	53.80%	5.663%
17	14.651	1959	1966	1975	rBV	2353077	3400076	41.23%	4.339%
18	14.733	1975	1980	1985	rVB6	5029	9184	0.11%	0.012%
19	14.839	1991	1998	2010	rBV	1525269	2128523	25.81%	2.717%
20	15.433	2094	2099	2104	rBV7	5929	9486	0.12%	0.012%
21	15.639	2127	2134	2147	rBV	3889430	5636638	68.35%	7.194%
22	15.757	2147	2154	2170	rVV	1359905	1830244	22.19%	2.336%
23	15.880	2171	2175	2181	rVB	20419	30721	0.37%	0.039%
24	17.186	2392	2397	2401	rBV3	5486	9027	0.11%	0.012%
25	17.398	2426	2433	2443	rBV	3147282	4347166	52.71%	5.548%
26	17.498	2443	2450	2465	rVV2	4493142	6388860	77.47%	8.154%
27	17.774	2492	2497	2499	rBV4	6788	9703	0.12%	0.012%
28	18.063	2543	2546	2552	rBV7	6242	8988	0.11%	0.011%
29	18.716	2654	2657	2661	rBV5	6364	9905	0.12%	0.013%
30	19.357	2761	2766	2771	rBV2	59680	87850	1.07%	0.112%
31	19.421	2773	2777	2783	rVV	62907	90614	1.10%	0.116%
32	19.792	2834	2840	2851	rBV	5923189	7996863	96.96%	10.206%
33	21.586	3140	3145	3157	rVB	3942311	5096058	61.79%	6.504%
34	23.886	3528	3536	3550	rVB2	3948399	8247269	100.00%	10.526%
35	24.045	3555	3563	3576	rVB2	2542081	5060354	61.36%	6.458%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023244.D
Acq On : 16 Dec 2022 17:40
Operator : CG/JU
Sample : PB149555BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK555

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Title : SVOA CALIBRATION


Sum of corrected areas: 78353511

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023244.D
Acq On : 16 Dec 2022 17:40
Operator : CG/JU
Sample : PB149555BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK555

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

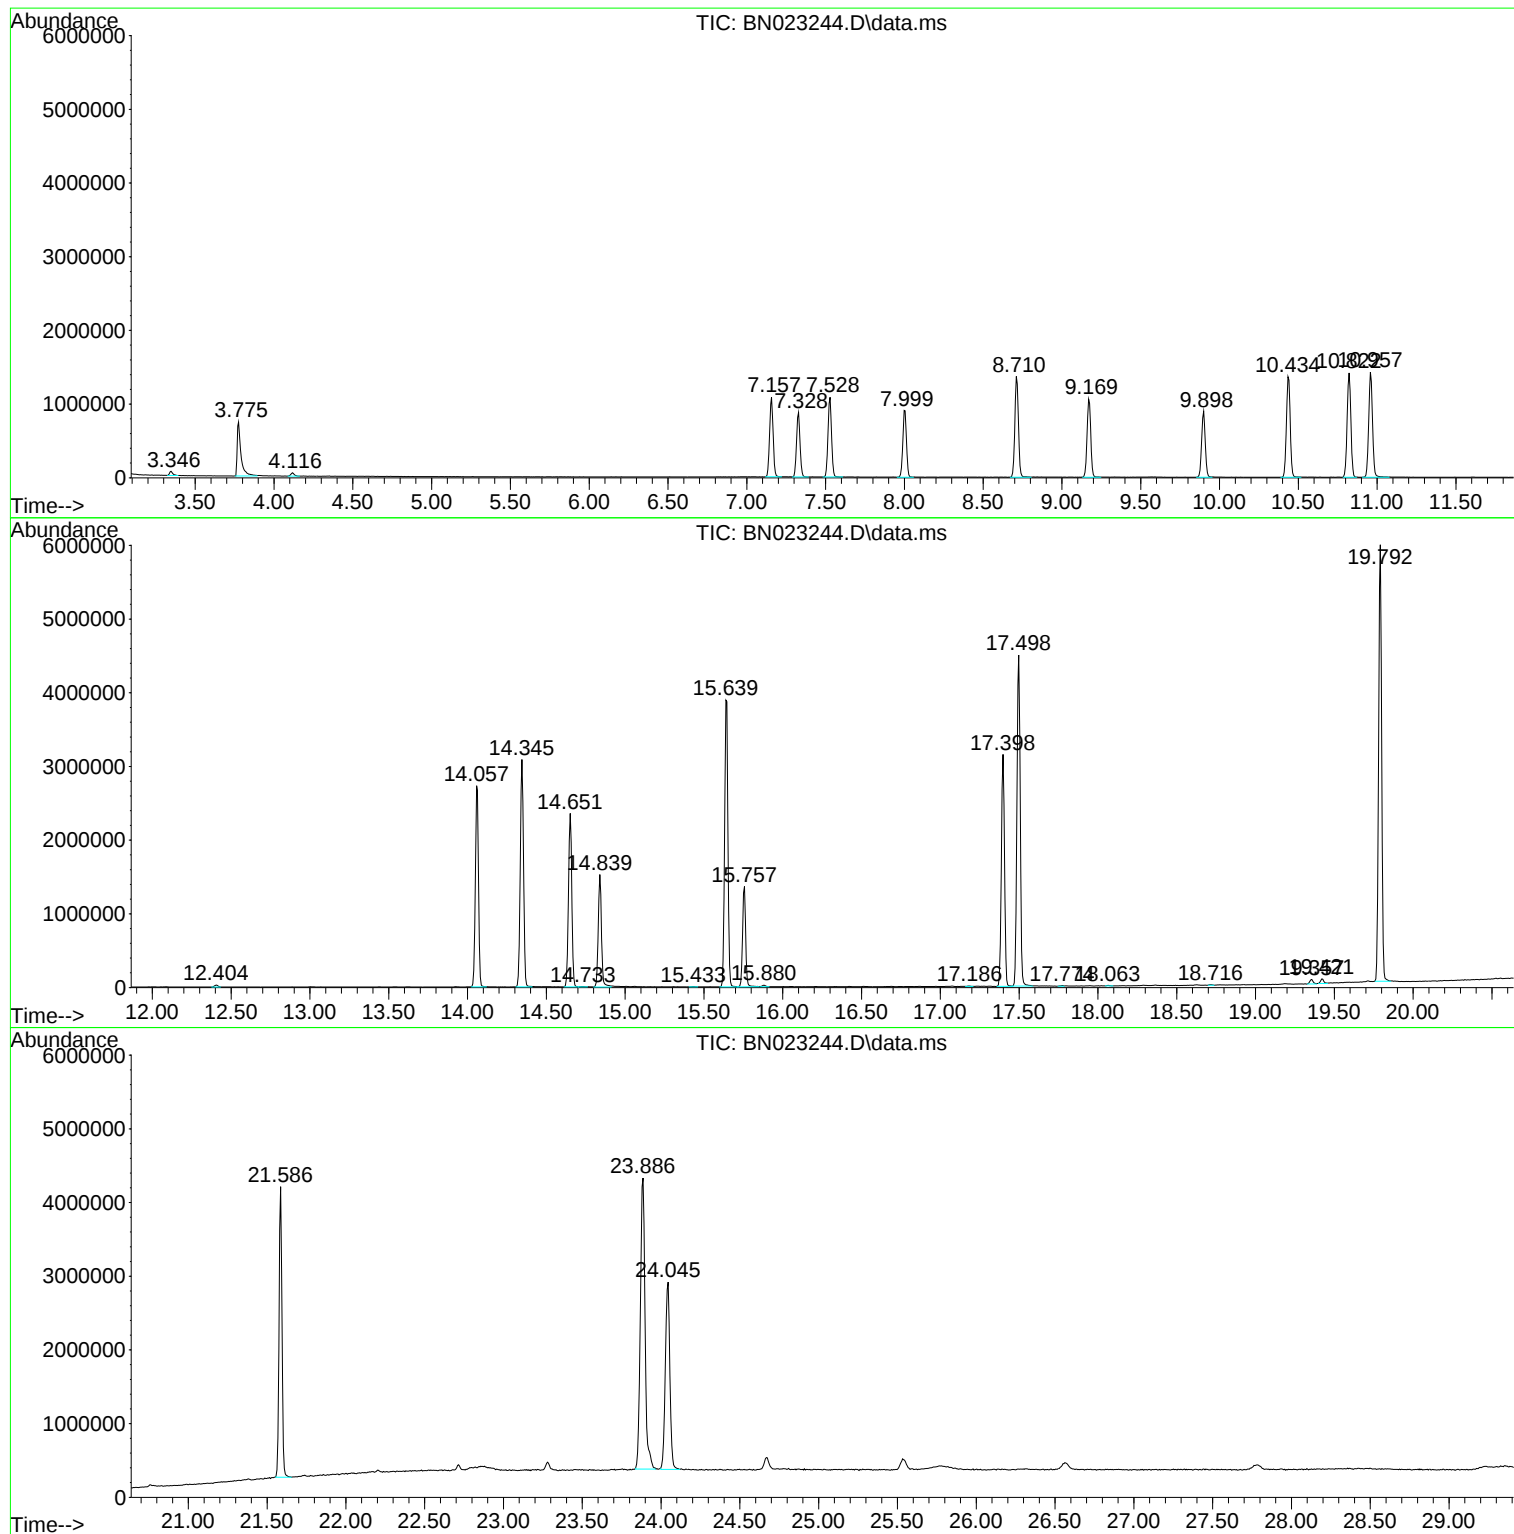

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023244.D
Acq On : 16 Dec 2022 17:40
Operator : CG/JU
Sample : PB149555BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK555

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023244.D
Acq On : 16 Dec 2022 17:40
Operator : CG/JU
Sample : PB149555BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK555

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc