

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
 Data File : BN023262.D
 Acq On : 17 Dec 2022 05:25
 Operator : CG/JU
 Sample : PB149588BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023262.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	55	rVB	66003	99140	1.19%	0.120%
2	3.769	114	116	137	rBV	791964	1342308	16.09%	1.622%
3	4.116	170	175	185	rVB	45517	69866	0.84%	0.084%
4	7.152	684	691	700	rBV	1145189	1757494	21.06%	2.123%
5	7.322	713	720	733	rVB	921241	1434570	17.19%	1.733%
6	7.522	746	754	764	rBV	1153012	1808170	21.67%	2.185%
7	7.999	827	835	843	rBV	1033433	1600670	19.18%	1.934%
8	8.710	949	956	964	rBV	1477993	2287898	27.42%	2.764%
9	9.169	1024	1034	1044	rBV	1158429	1830200	21.93%	2.211%
10	9.893	1149	1157	1174	rBV	930733	1549796	18.57%	1.872%
11	10.434	1241	1249	1264	rBV	1511614	2434658	29.18%	2.942%
12	10.816	1307	1314	1324	rVB	1521583	2564658	30.74%	3.099%
13	10.957	1330	1338	1354	rBV	1540298	2558376	30.66%	3.091%
14	11.598	1444	1447	1453	rBV7	5233	9352	0.11%	0.011%
15	12.404	1578	1584	1590	rVB	28670	47044	0.56%	0.057%
16	13.539	1774	1777	1782	rBV4	7380	9581	0.11%	0.012%
17	14.057	1858	1865	1875	rBV	3055640	3987069	47.78%	4.817%
18	14.345	1906	1914	1925	rBV	3235751	4783206	57.32%	5.779%
19	14.651	1958	1966	1975	rBV	2651240	3787357	45.39%	4.576%
20	14.728	1975	1979	1984	rVB6	5485	8846	0.11%	0.011%
21	14.839	1991	1998	2015	rBV	1602505	2231363	26.74%	2.696%
22	15.639	2126	2134	2146	rBV	4297816	6074185	72.80%	7.339%
23	15.751	2146	2153	2165	rVV	1453382	1912933	22.93%	2.311%
24	15.881	2171	2175	2181	rVB	21012	32368	0.39%	0.039%
25	16.422	2261	2267	2271	rBV7	4552	8641	0.10%	0.010%
26	17.180	2392	2396	2401	rVB	8052	11266	0.14%	0.014%
27	17.398	2426	2433	2443	rBV	3481415	4857042	58.21%	5.868%
28	17.492	2443	2449	2469	rVB2	4667851	6818950	81.72%	8.239%
29	17.769	2492	2496	2499	rBV4	7432	11014	0.13%	0.013%
30	18.716	2654	2657	2660	rBV5	6742	8536	0.10%	0.010%
31	19.351	2761	2765	2770	rBV2	63943	81948	0.98%	0.099%
32	19.422	2773	2777	2782	rBV	63494	83828	1.00%	0.101%
33	19.786	2833	2839	2852	rBV	6028177	8344164	100.00%	10.081%
34	21.580	3139	3144	3157	rVB	4366910	5460478	65.44%	6.597%
35	23.880	3527	3535	3547	rVB2	3757955	7812831	93.63%	9.440%
36	24.033	3554	3561	3573	rVB2	2530057	5047402	60.49%	6.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023262.D
Acq On : 17 Dec 2022 05:25
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK588

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 82767208

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023262.D
Acq On : 17 Dec 2022 05:25
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

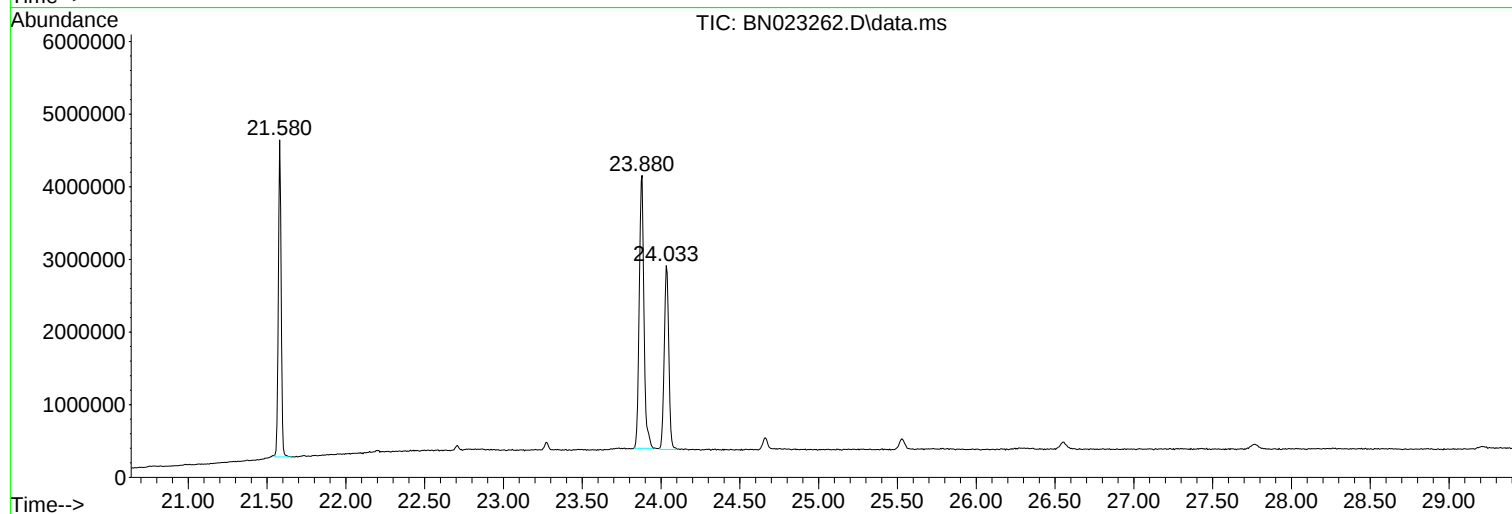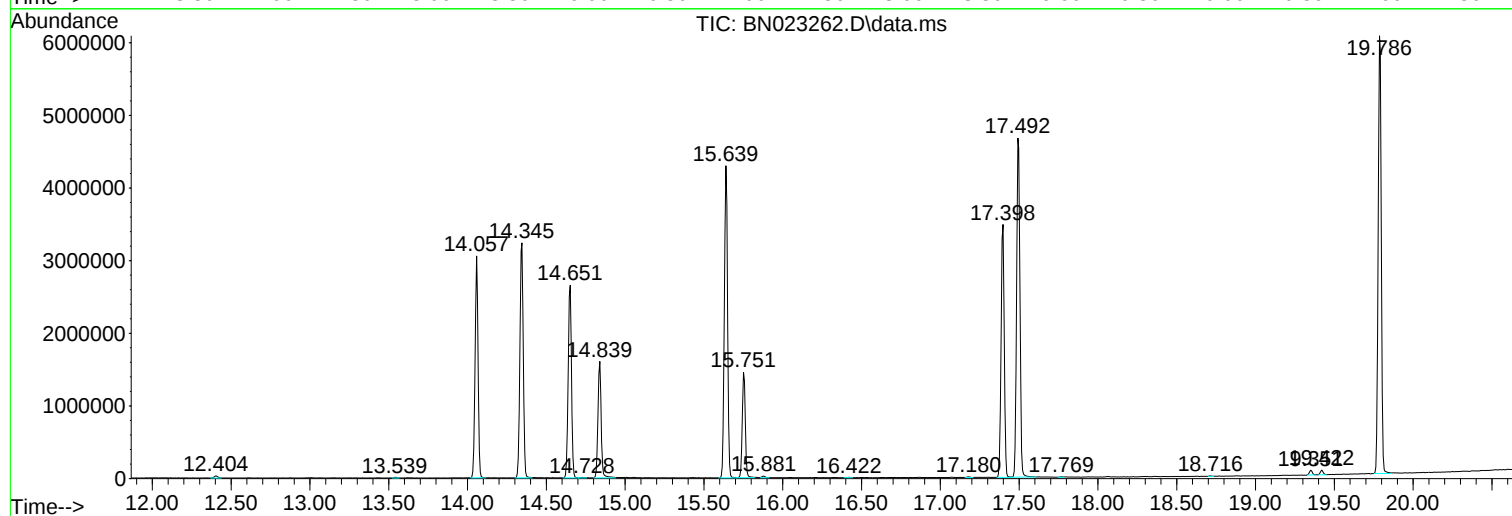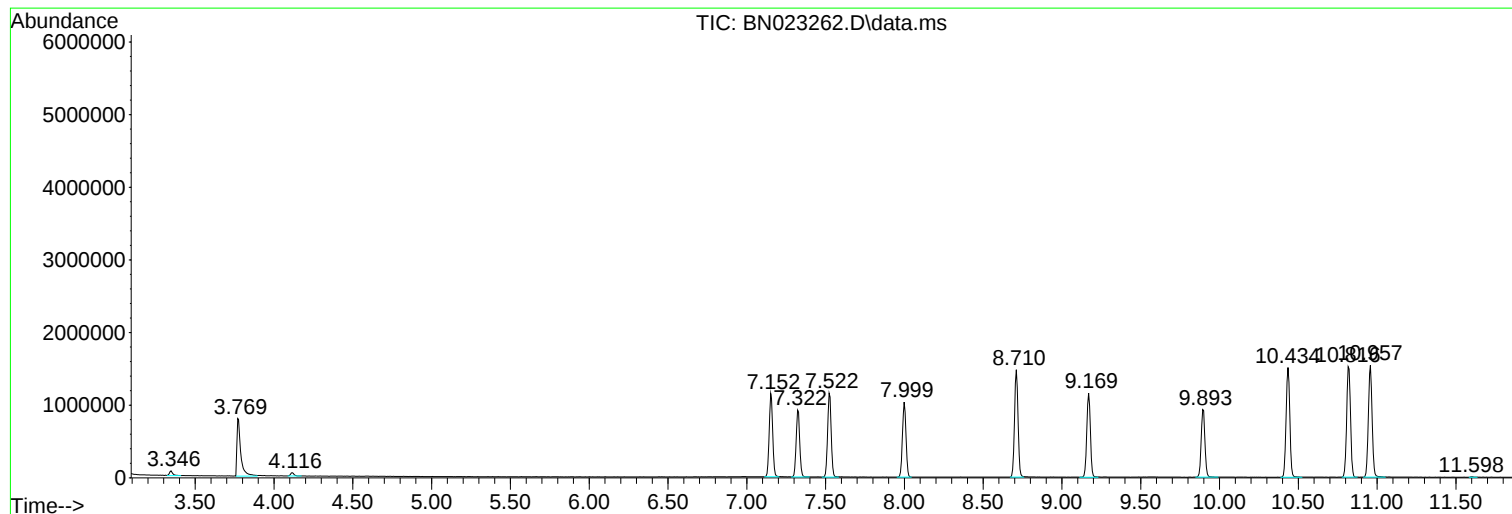

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023262.D
Acq On : 17 Dec 2022 05:25
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121622\
Data File : BN023262.D
Acq On : 17 Dec 2022 05:25
Operator : CG/JU
Sample : PB149588BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN121522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc