
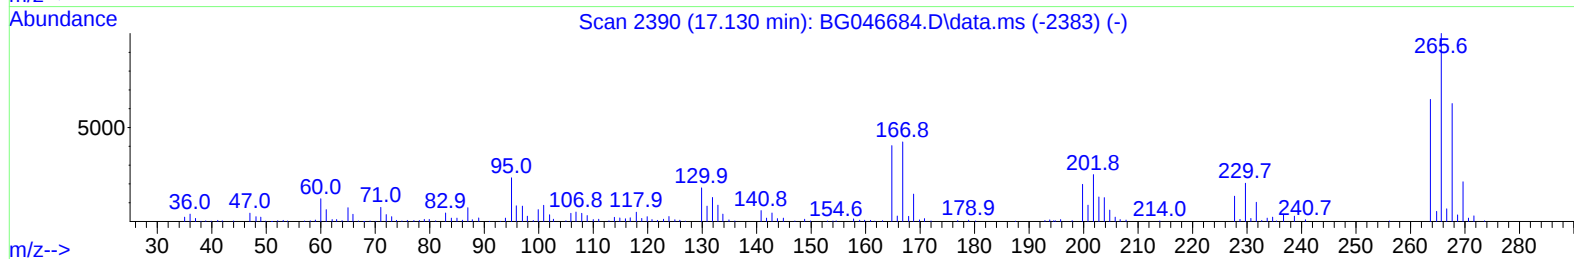
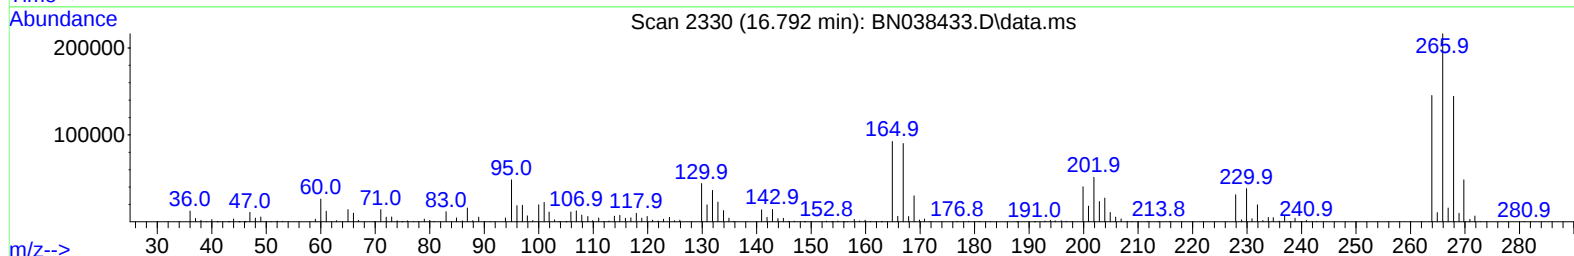


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038433.D
Acq On : 16 Dec 2025 09:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Dec 16 10:09:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

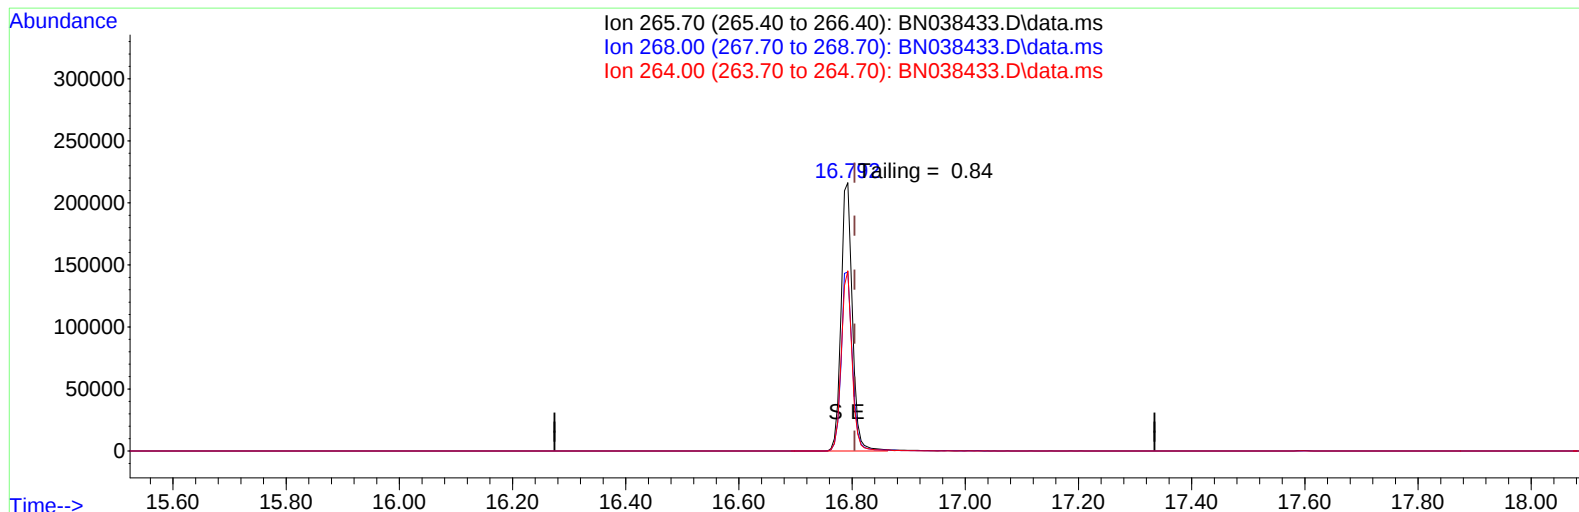

TIC: BN038433.D\data.ms

(70) Pentachlorophenol (C)




16.792min (-0.012) 712292.08 ng

response 301854

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.72
264.00	61.60	67.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038433.D
Acq On : 16 Dec 2025 09:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Dec 16 10:09:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

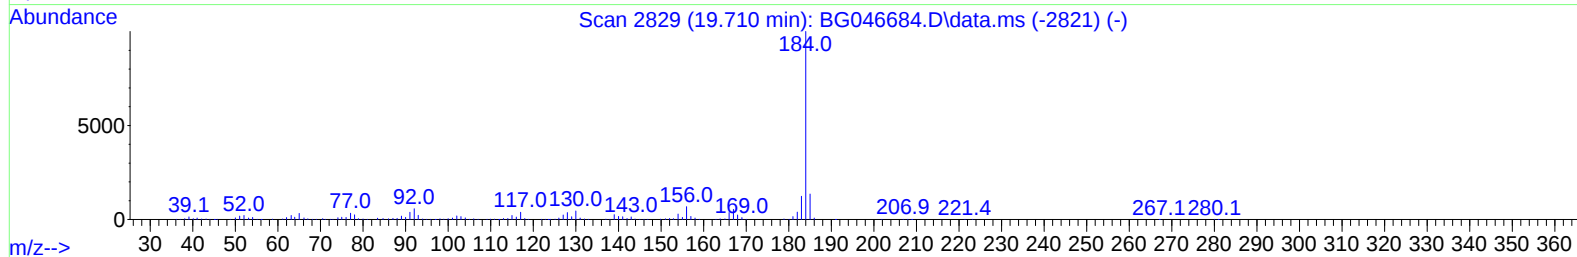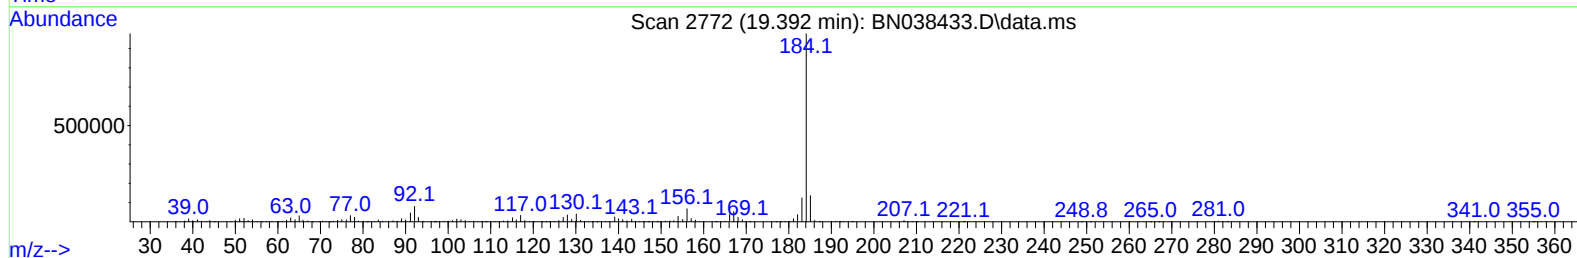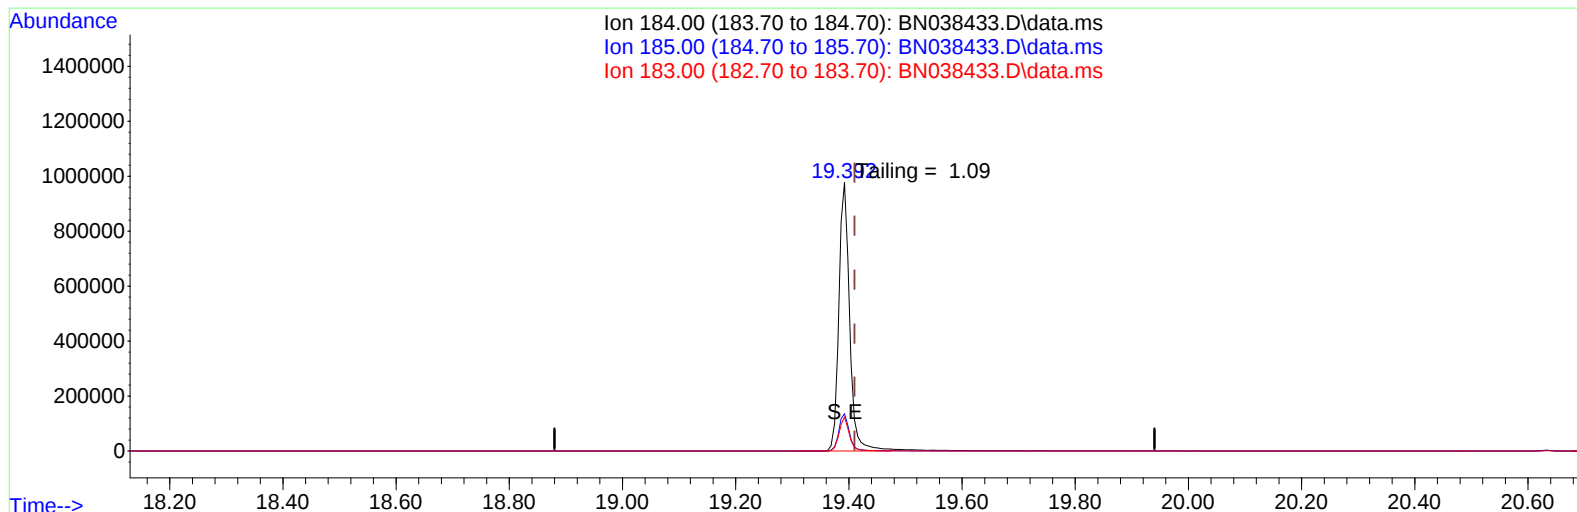

TIC: BN038433.D\data.ms

(77) Benzidine**19.392min (-0.018) 3870.32 ng****response 1302324**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.88
183.00	13.20	12.73
0.00	0.00	0.00