
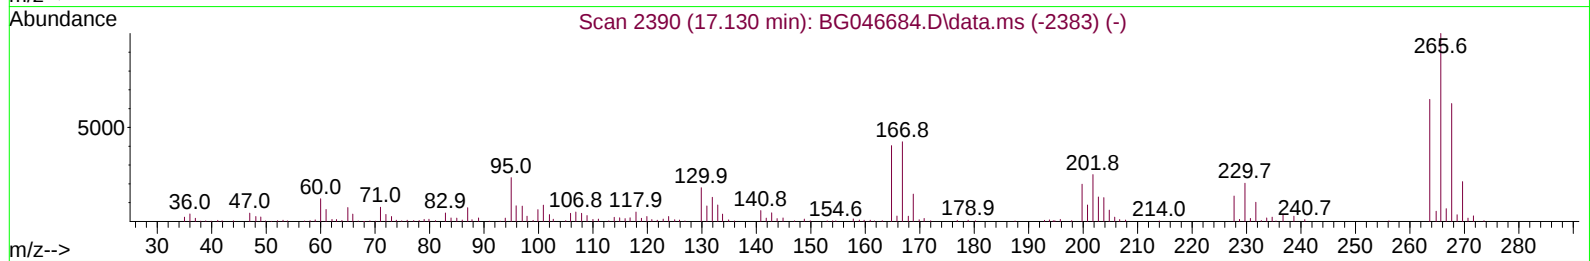
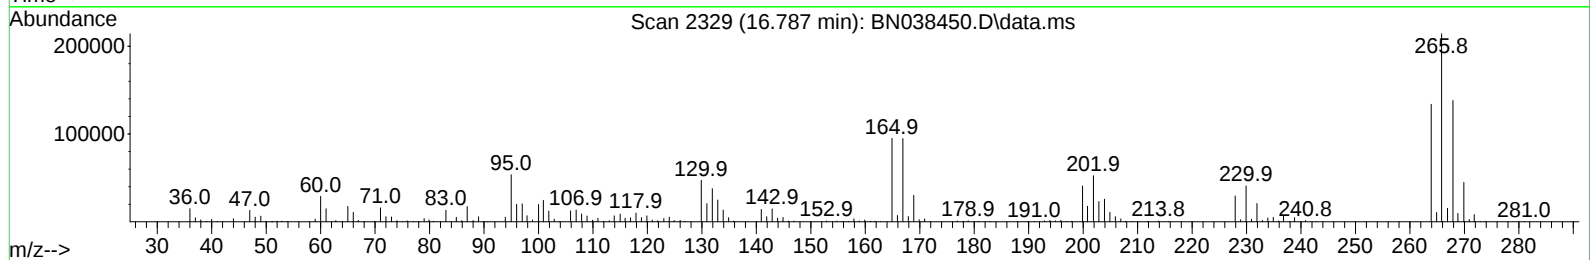


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038450.D
Acq On : 16 Dec 2025 20:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 07:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

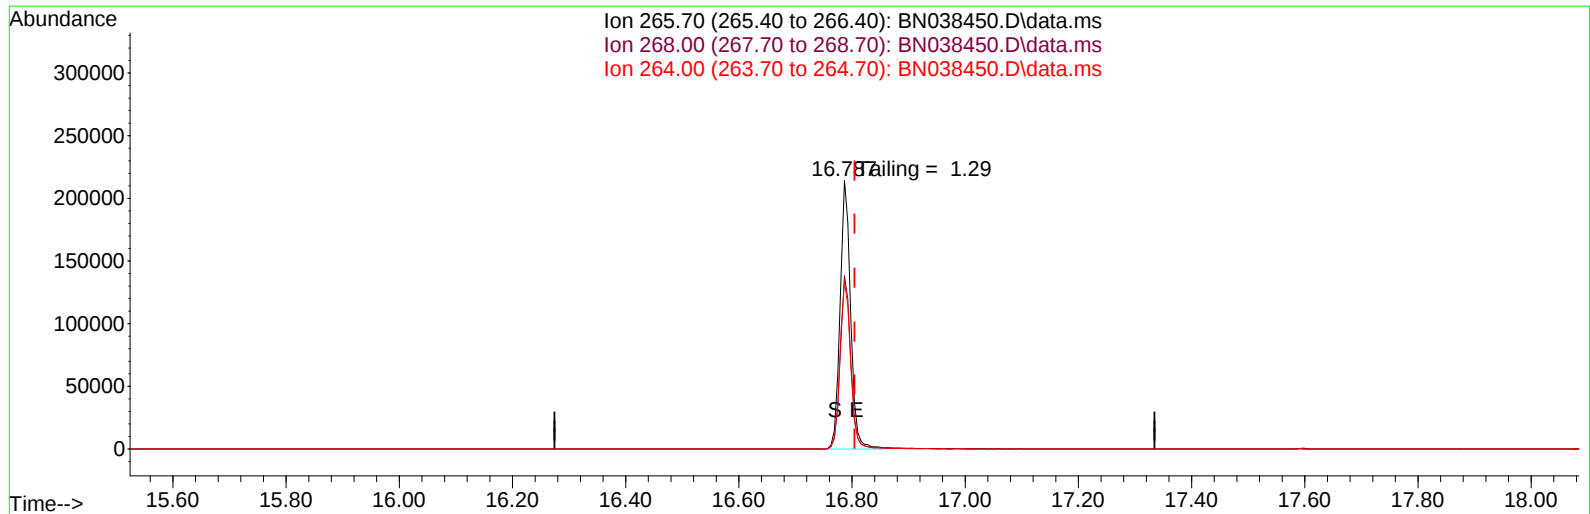

TIC: BN038450.D\data.ms

(70) Pentachlorophenol (C)




16.787min (-0.018) 522386.64 ng

response 278770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.54
264.00	61.60	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038450.D
Acq On : 16 Dec 2025 20:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 17 07:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

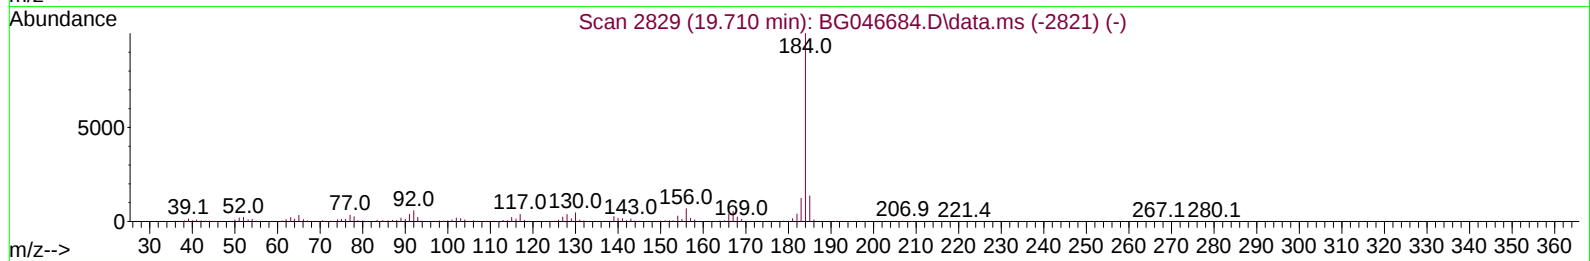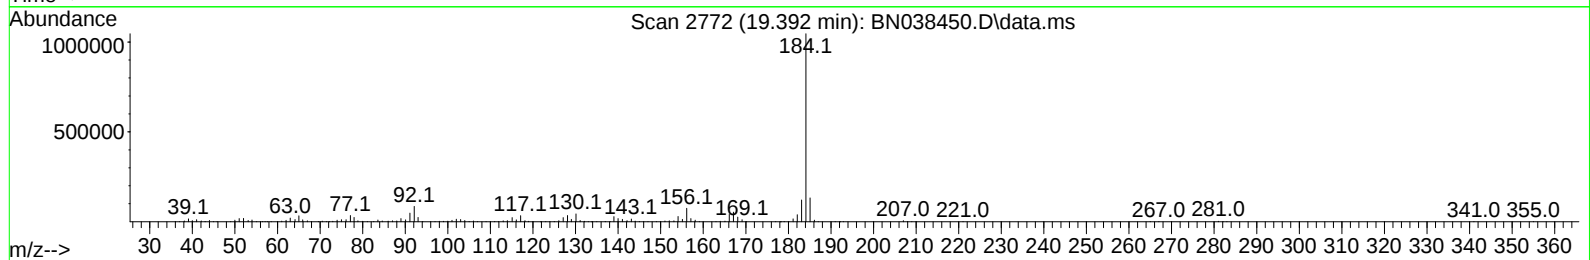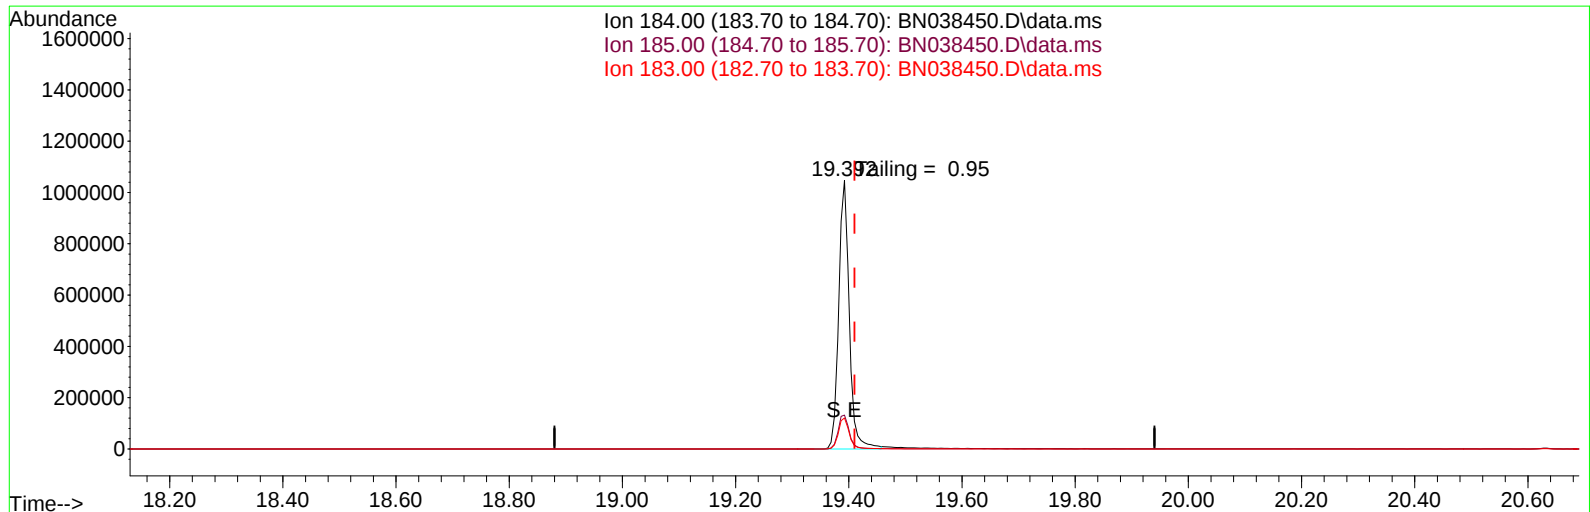

TIC: BN038450.D\data.ms

(77) Benzidine

19.392min (-0.018) 4281.21 ng

response 1372884

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.62
183.00	13.20	11.54
0.00	0.00	0.00