


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038450.D
Acq On : 16 Dec 2025 20:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 10 13:56:50 2025

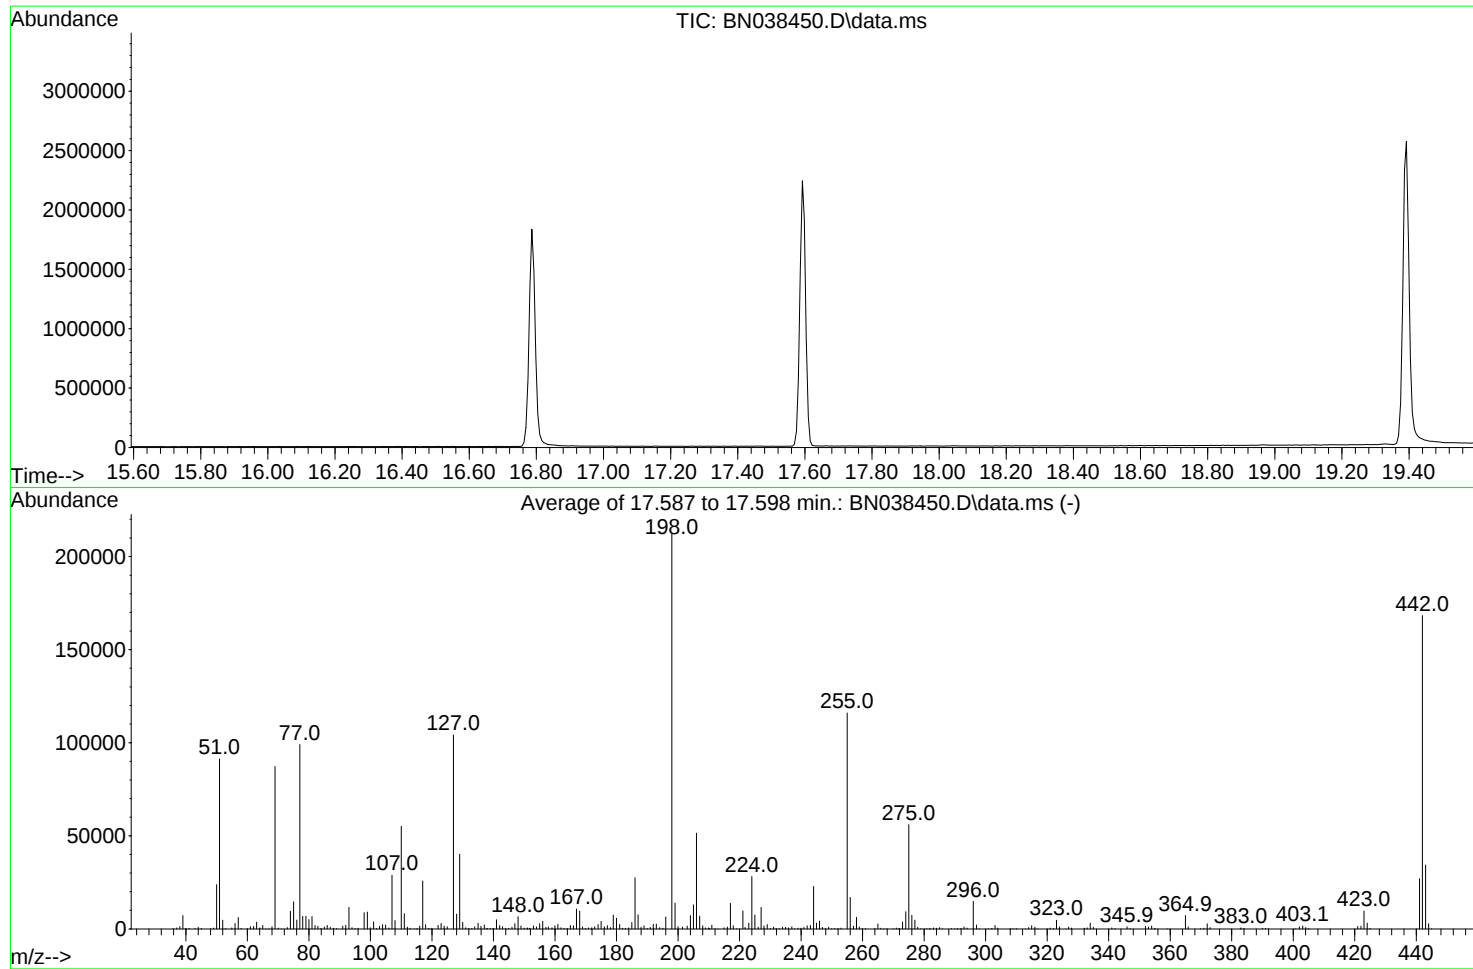




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.3	1160	PASS
69	69	100	100	100.0	87235	PASS
70	69	0.00	2	0.6	503	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	212053	PASS
199	198	5	9	6.6	13915	PASS
365	198	1	100	3.4	7212	PASS
441	443	0.01	150	78.3	26923	PASS
442	442	100	100	100.0	168307	PASS
443	442	15	24	20.4	34381	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038450.D
Acq On : 16 Dec 2025 20:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 17 07:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

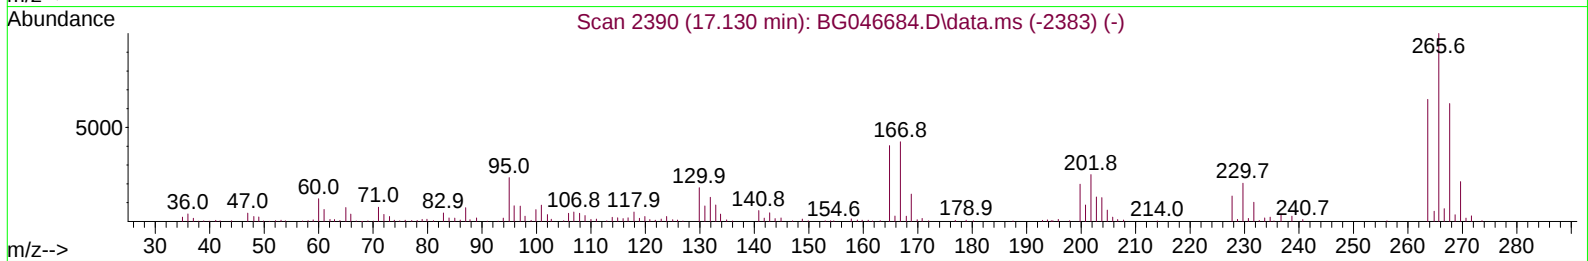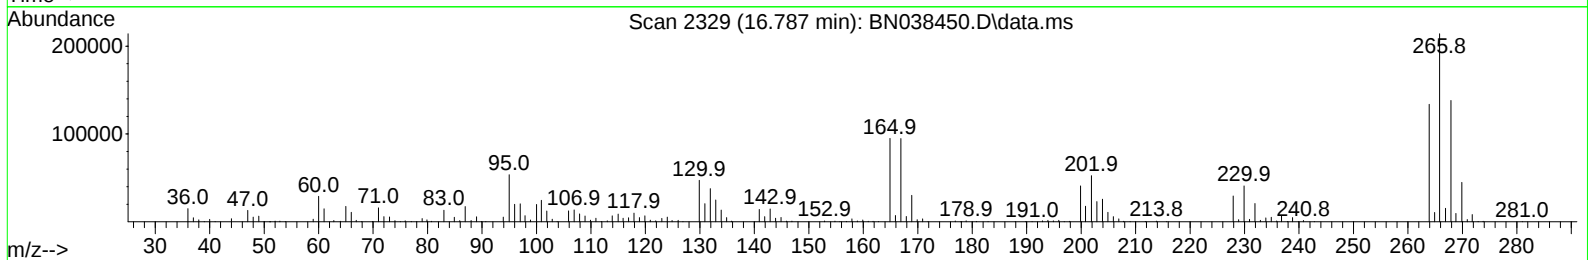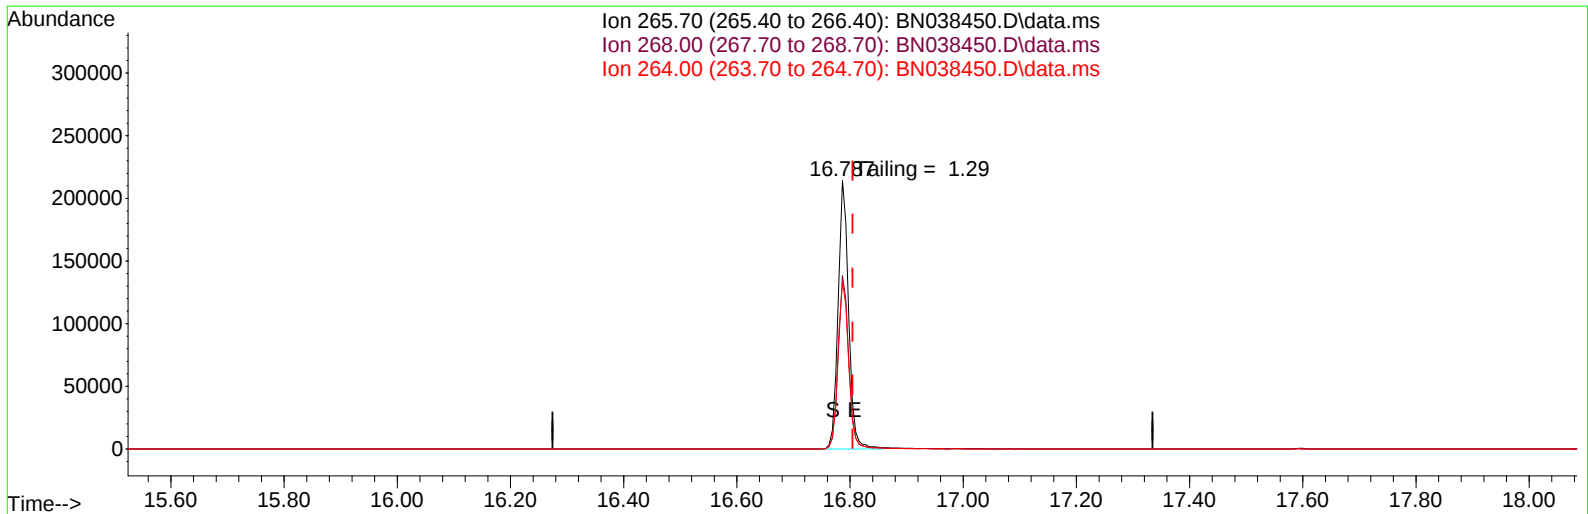

TIC: BN038450.D\data.ms

(70) Pentachlorophenol (C)

16.787min (-0.018) 522386.64 ng




response 278770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.54
264.00	61.60	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121625\
Data File : BN038450.D
Acq On : 16 Dec 2025 20:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 17 07:49:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 03:10:04 2025
Response via : Initial Calibration

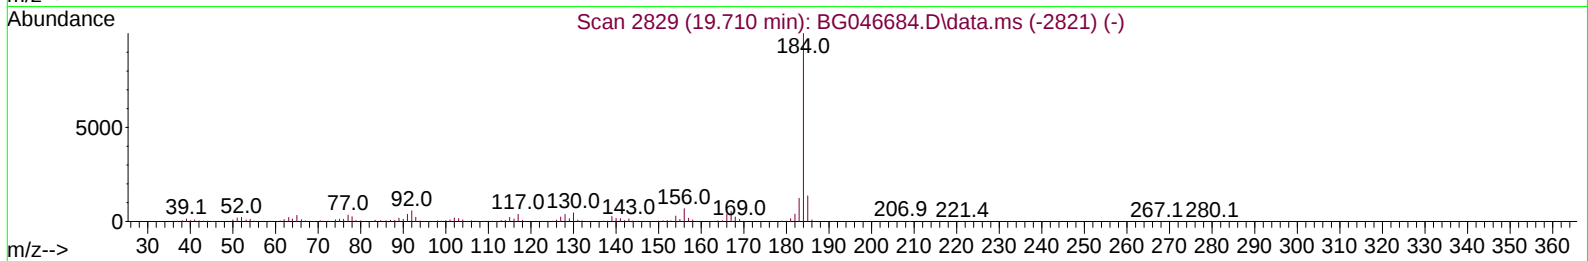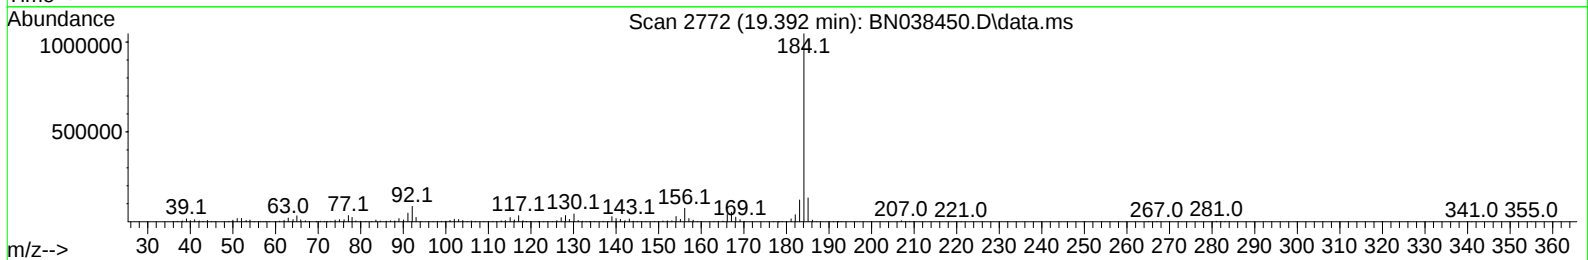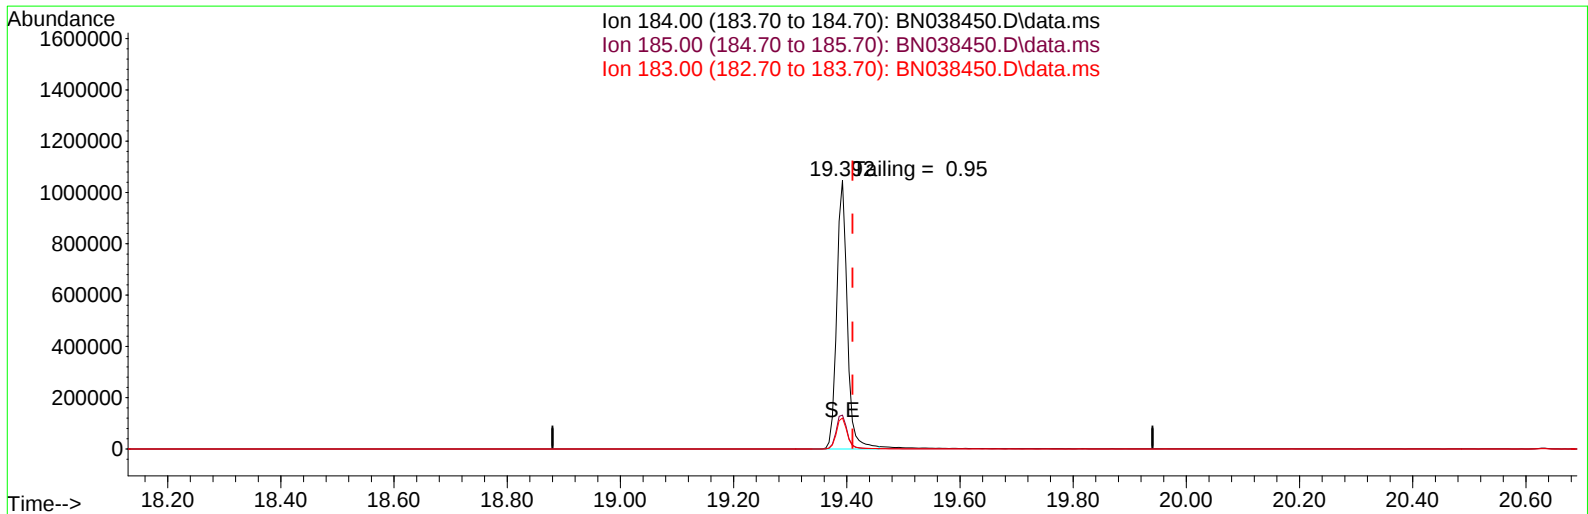

TIC: BN038450.D\data.ms

(77) Benzidine

19.392min (-0.018) 4281.21 ng

response 1372884

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.62
183.00	13.20	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/16/2025	BNA_N	<u>BN038450.D</u>
Compound Name	Response	Retention Time
DDT	734771	20.633
DDD	37892	20.192
DDE	1461	19.681
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39353	774124	5.08

S

Instrument :
BNA_N
ClientSampleId :
DFTPP