

Data File : BN004050.D
Acq On : 17 Dec 2018 23:42
Operator : JU/SJ
Sample : J6236-20
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F44

Quant Time: Dec 18 04:34:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 04:29:07 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1516	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7959	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5088	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	801943	0.40	ng/ul	0.10
16) Chrysene-d12	21.51	240	22	0.40	ng/ul	0.11
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.73
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3474	0.28	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
17) Pyrene	19.61	202	1863	23.611	ng/ul#	1
18) Benzo(a)anthracene	21.43	228	483	6.951	ng/ul#	53
19) Chrysene	21.54	228	4	0.050	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\

Quantitation Report (Not Reviewed)

Data File : BN004050.D

Acq On : 17 Dec 2018 23:42

Operator : JU/SJ

Sample : J6236-20

Misc :

ALS Vial : 18 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

F9F44


Quant Time: Dec 18 04:34:32 2018


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 18 04:29:07 2018

Response via : Initial Calibration




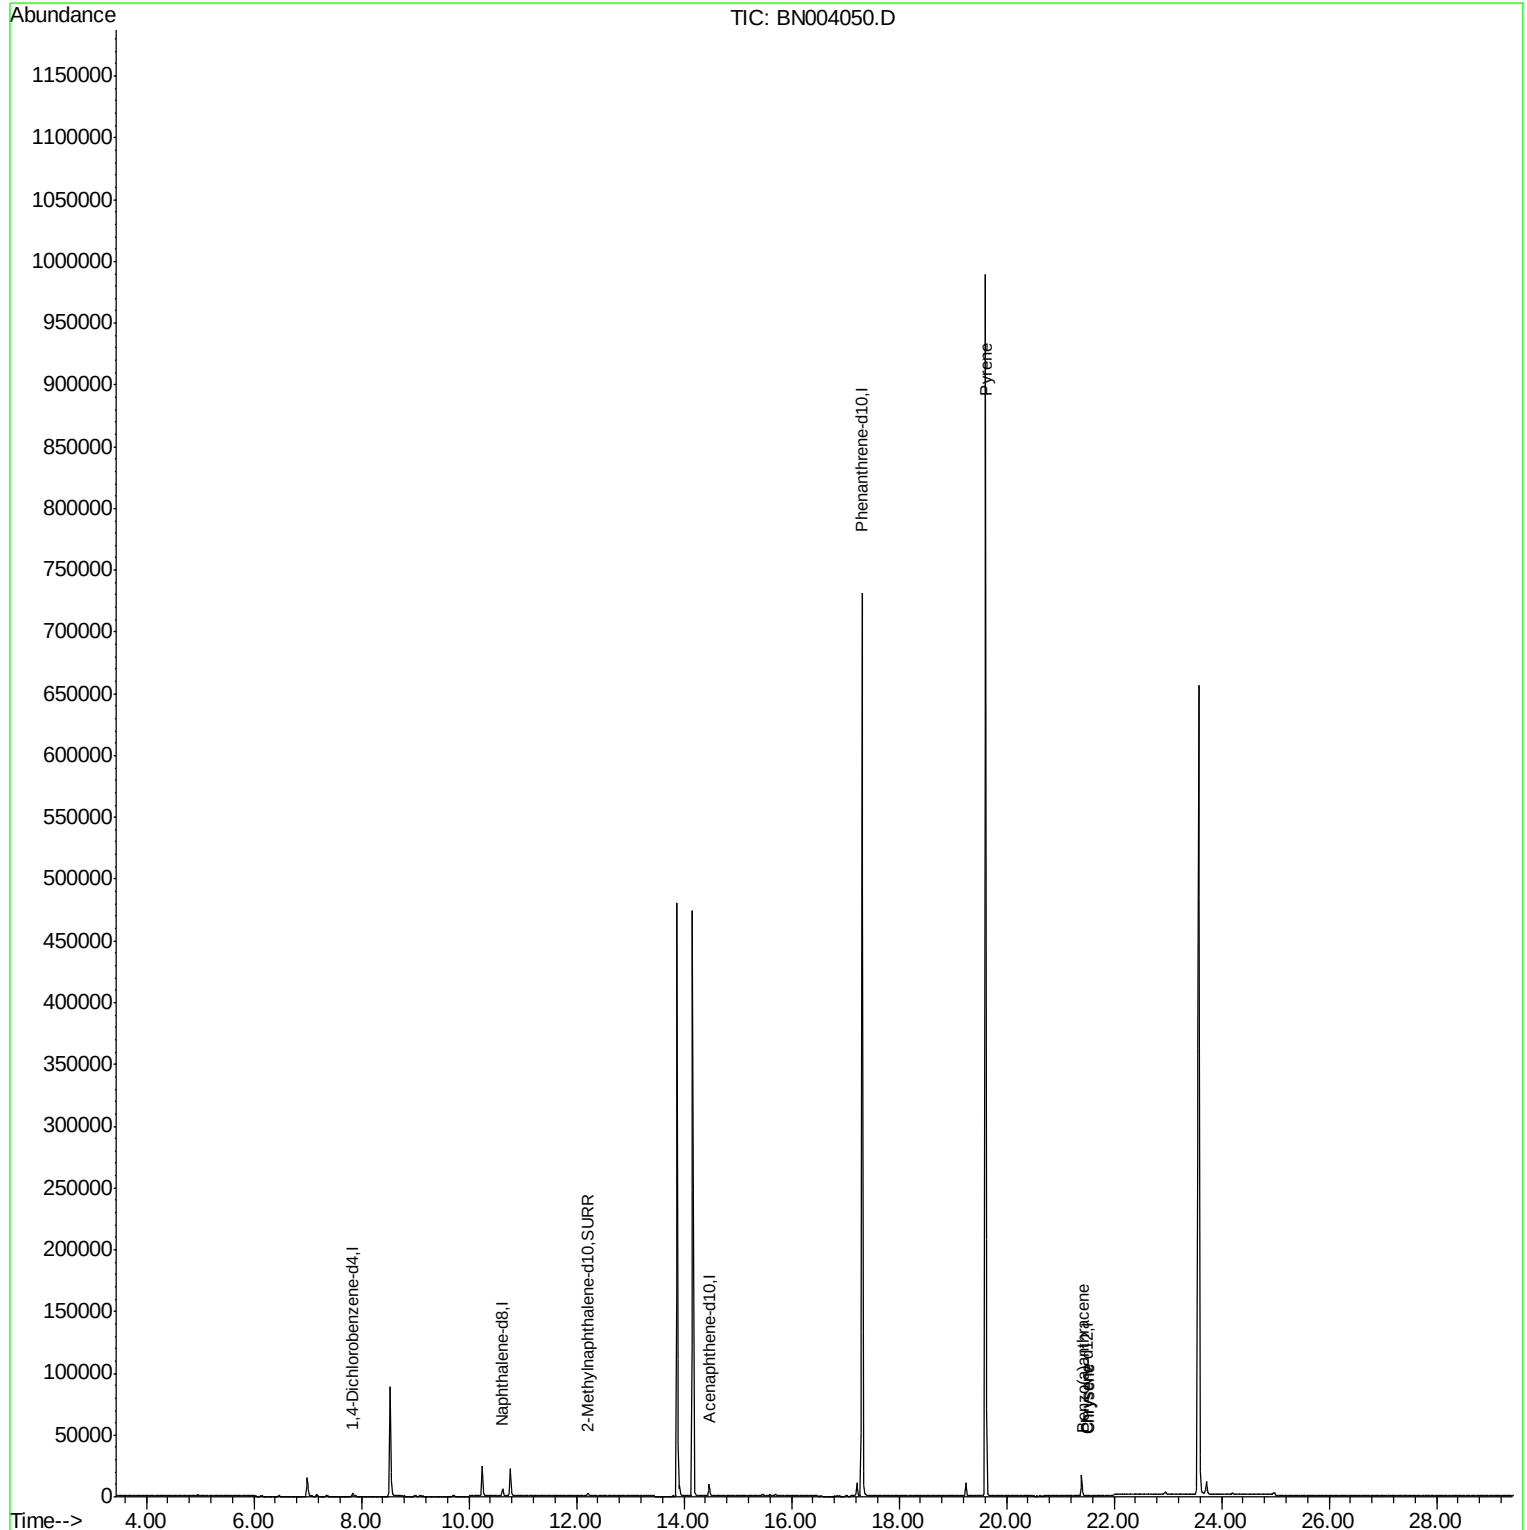


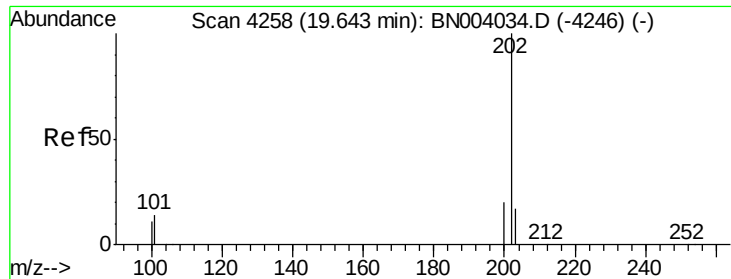

#17
Pyrene
 Concen: 23.611 ng/ul
 RT: 19.61 min Scan# 4251
 Delta R.T. -0.03 min
 Lab File: BN004050.D
 Acq: 17 Dec 2018 23:42




Instrument :
 BNA_N
 ClientSampleId :
 F9F44


Tgt Ion:202 Resp: 1863
 Ion Ratio Lower Upper
 202 100
 101 133.1 10.3 15.5#
 100 830.2 8.5 12.7#

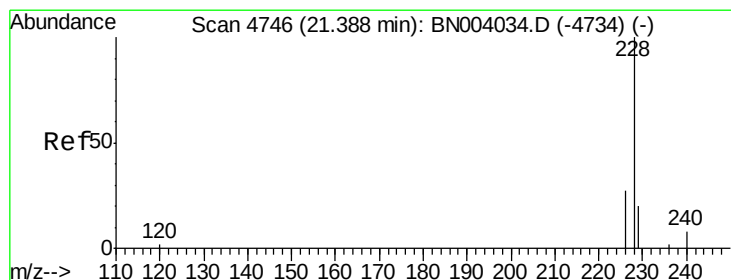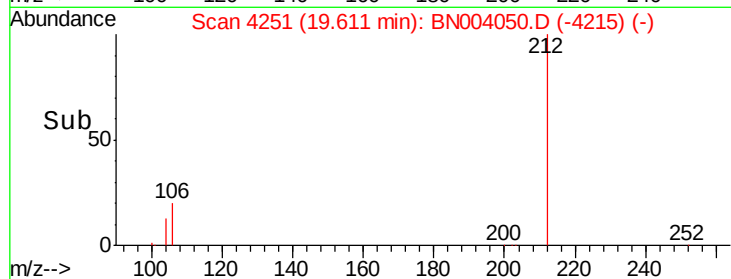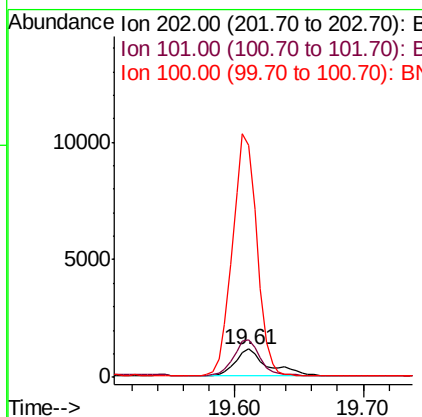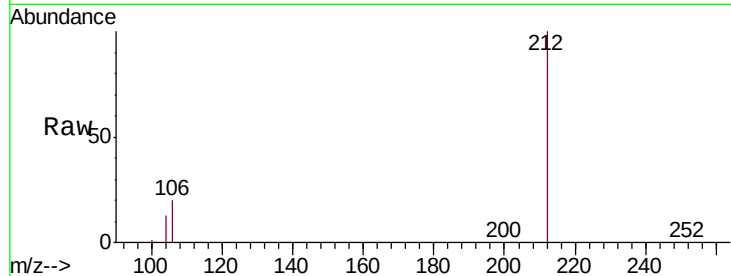

#18
Benzo(a)anthracene
 Concen: 6.951 ng/ul
 RT: 21.43 min Scan# 4762
 Delta R.T. 0.05 min
 Lab File: BN004050.D
 Acq: 17 Dec 2018 23:42

Tgt Ion:228 Resp: 483
 Ion Ratio Lower Upper
 228 100
 229 43.8 15.6 23.4#
 226 48.1 21.1 31.7#

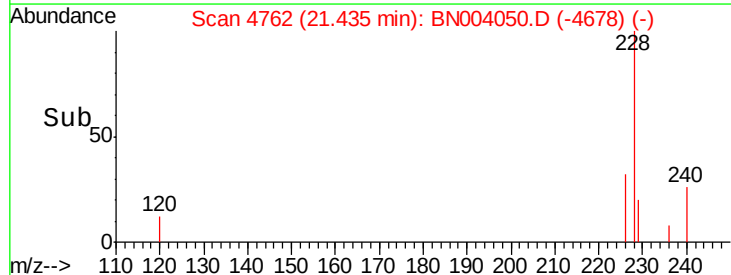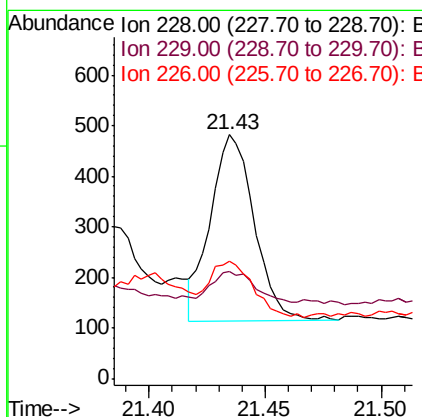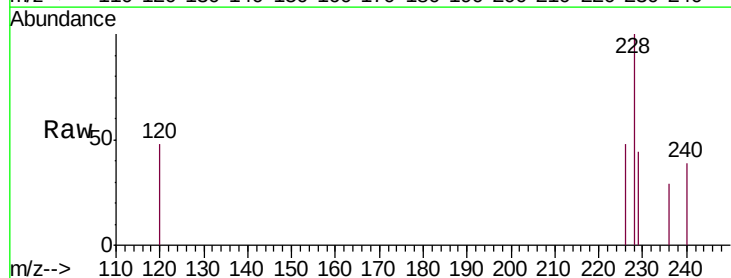

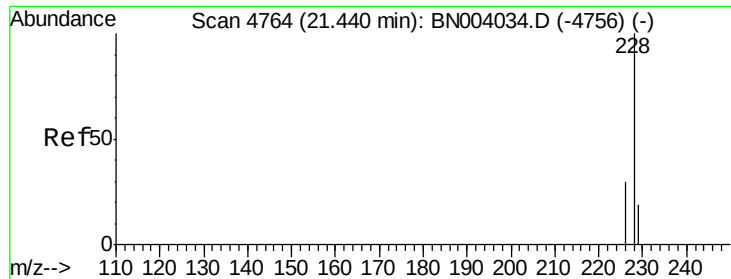

#19

Chrysene

Concen: 0.050 ng/ul

RT: 21.54 min Scan# 4798

Delta R.T. 0.10 min

Lab File: BN004050.D


Acq: 17 Dec 2018 23:42

Instrument :

BNA_N

ClientSampleId :

F9F44

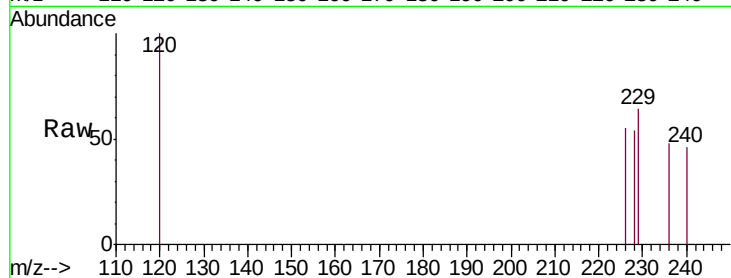

Tgt Ion:	228	Resp:	4
Ion	Ratio	Lower	Upper
228	100		
226	101.6	24.0	36.0#
229	119.4	15.7	23.5#

