

Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Quant Time: Dec 18 06:37:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1486	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7632	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4912	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	927117	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.72	264	13121	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3630	0.31	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	1470	0.065	ng/ul#	15
23) Benzo(a)pyrene	23.57	252	3789	0.081	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Quant Time: Dec 18 06:37:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

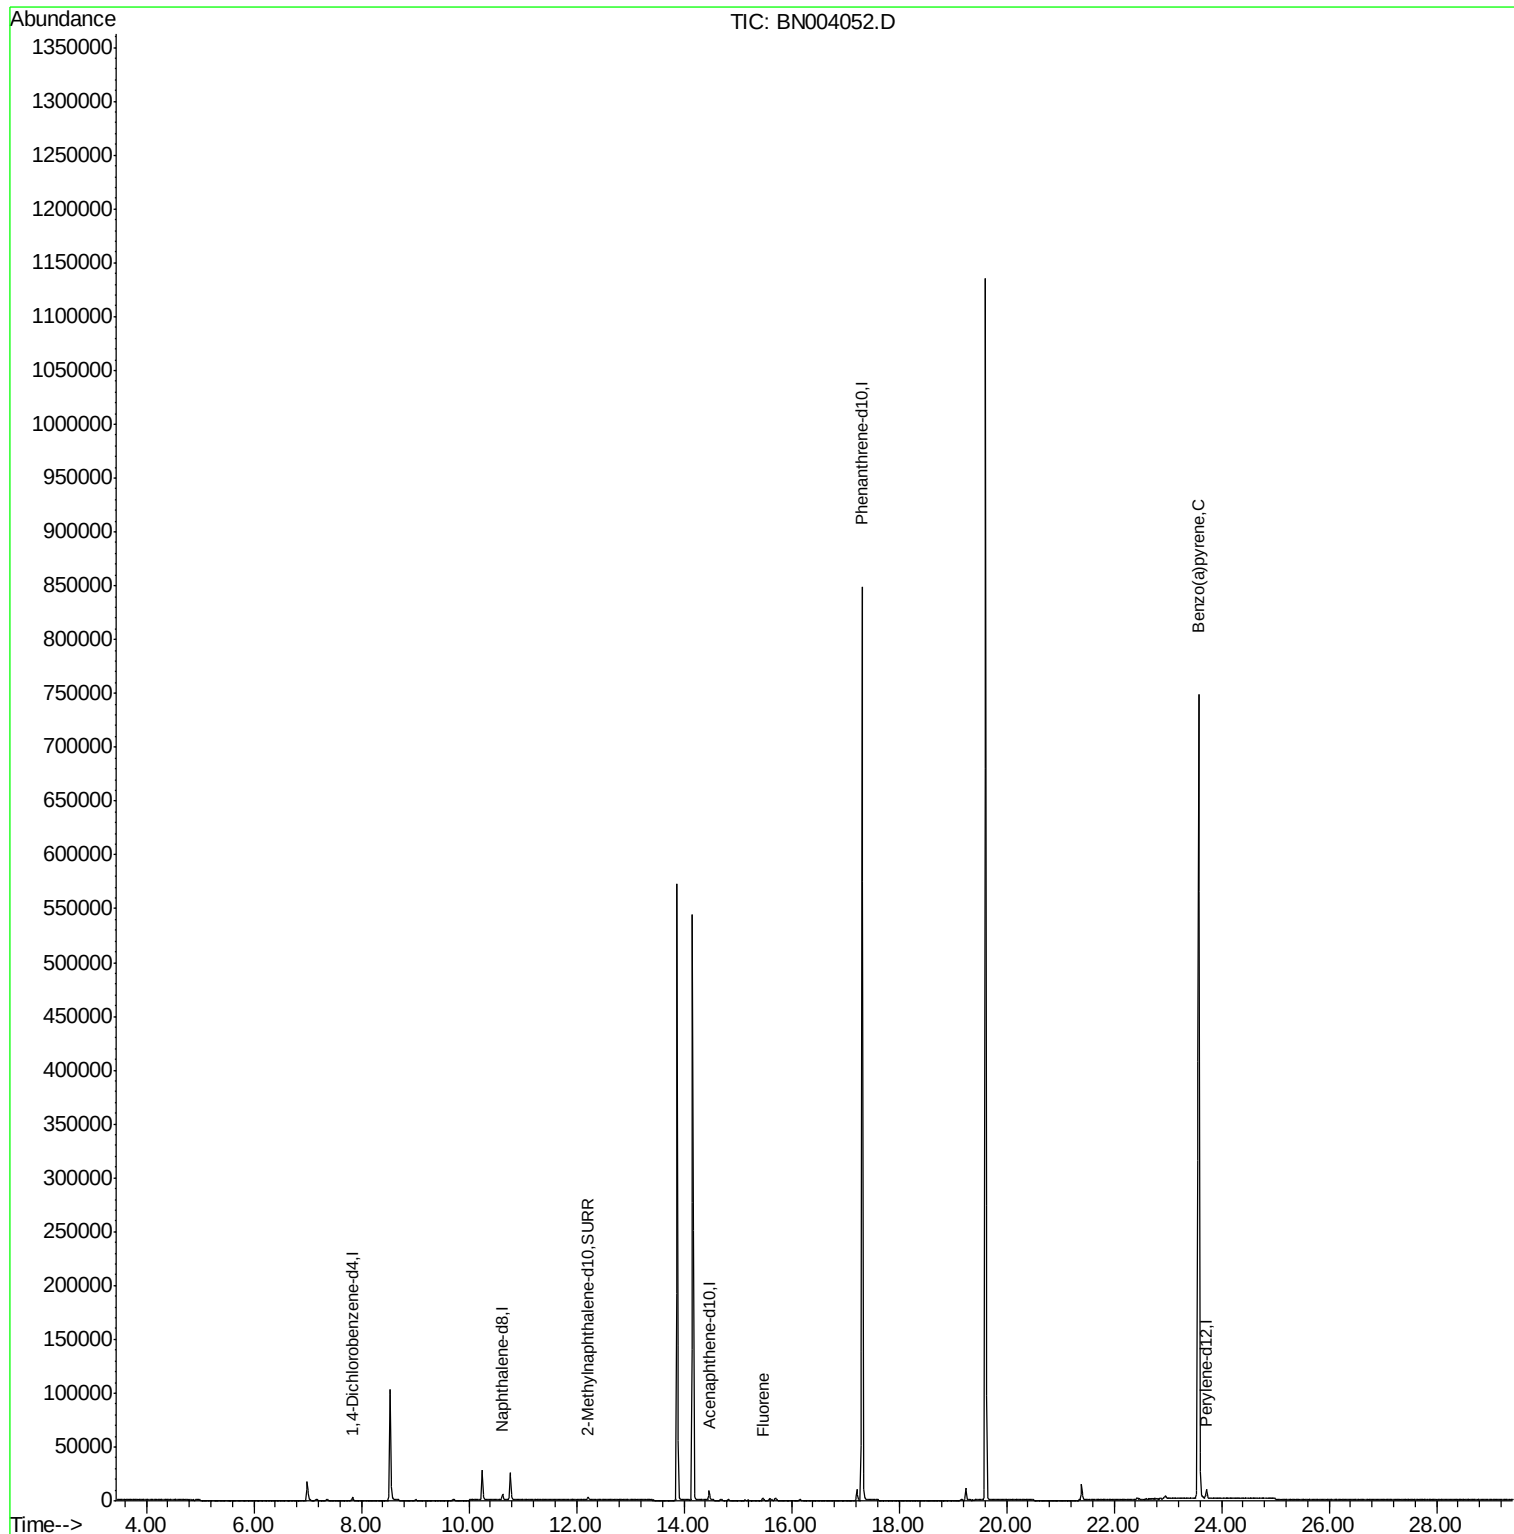


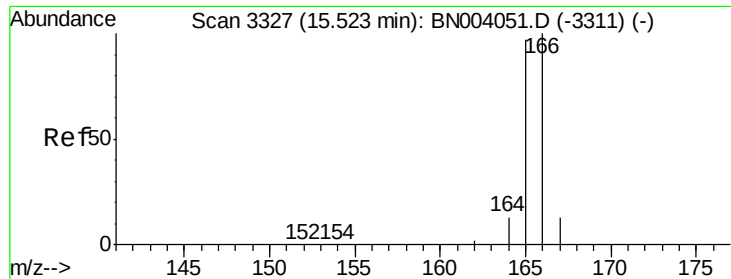




#9
Fluorene
 Concen: 0.065 ng/ul
 RT: 15.46 min Scan# 3314
 Delta R.T. -0.06 min
 Lab File: BN004052.D
 Acq: 18 Dec 2018 00:53

Instrument :
 BNA_N
 ClientSampleId :
 SBLK78

Tgt Ion:166 Resp: 1470
 Ion Ratio Lower Upper
 166 100
 165 9.5 78.3 117.5#
 167 34.5 11.3 16.9#

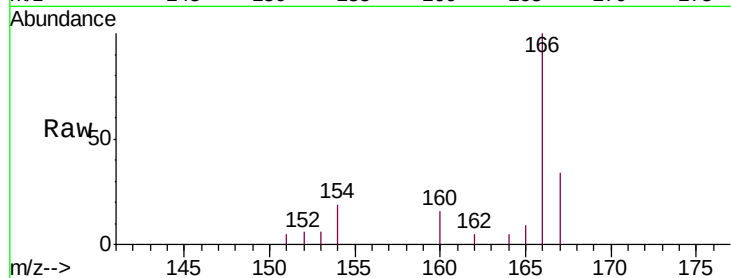


Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E

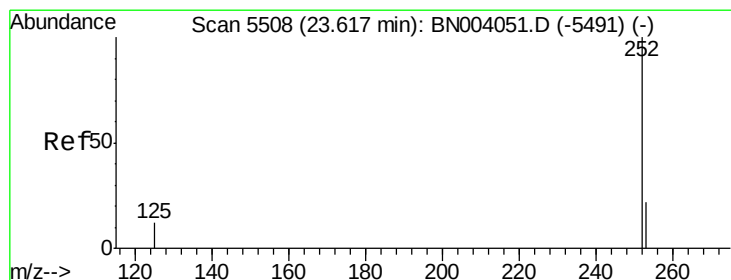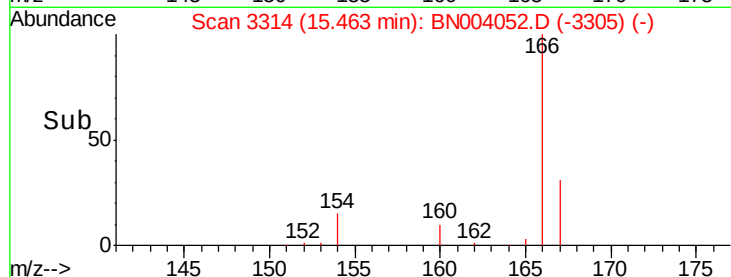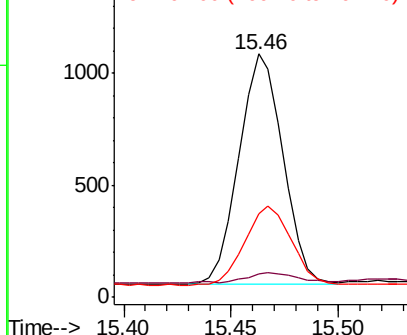

#23
Benzo(a)pyrene
 Concen: 0.081 ng/ul
 RT: 23.57 min Scan# 5494
 Delta R.T. -0.04 min
 Lab File: BN004052.D
 Acq: 18 Dec 2018 00:53

Tgt Ion:252 Resp: 3789
 Ion Ratio Lower Upper
 252 100
 253 38.4 19.0 28.4#
 125 30.9 10.2 15.4#

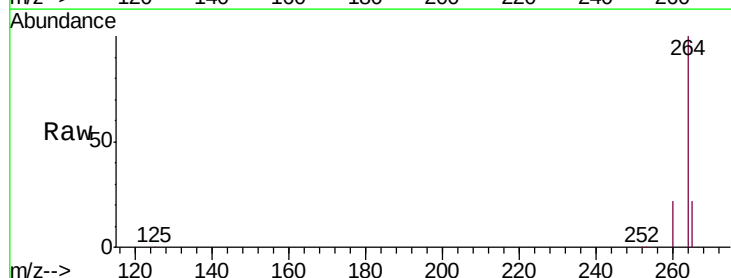

Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 253.00 (252.70 to 253.70): E
 Ion 125.00 (124.70 to 125.70): E

