

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)


Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:46:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

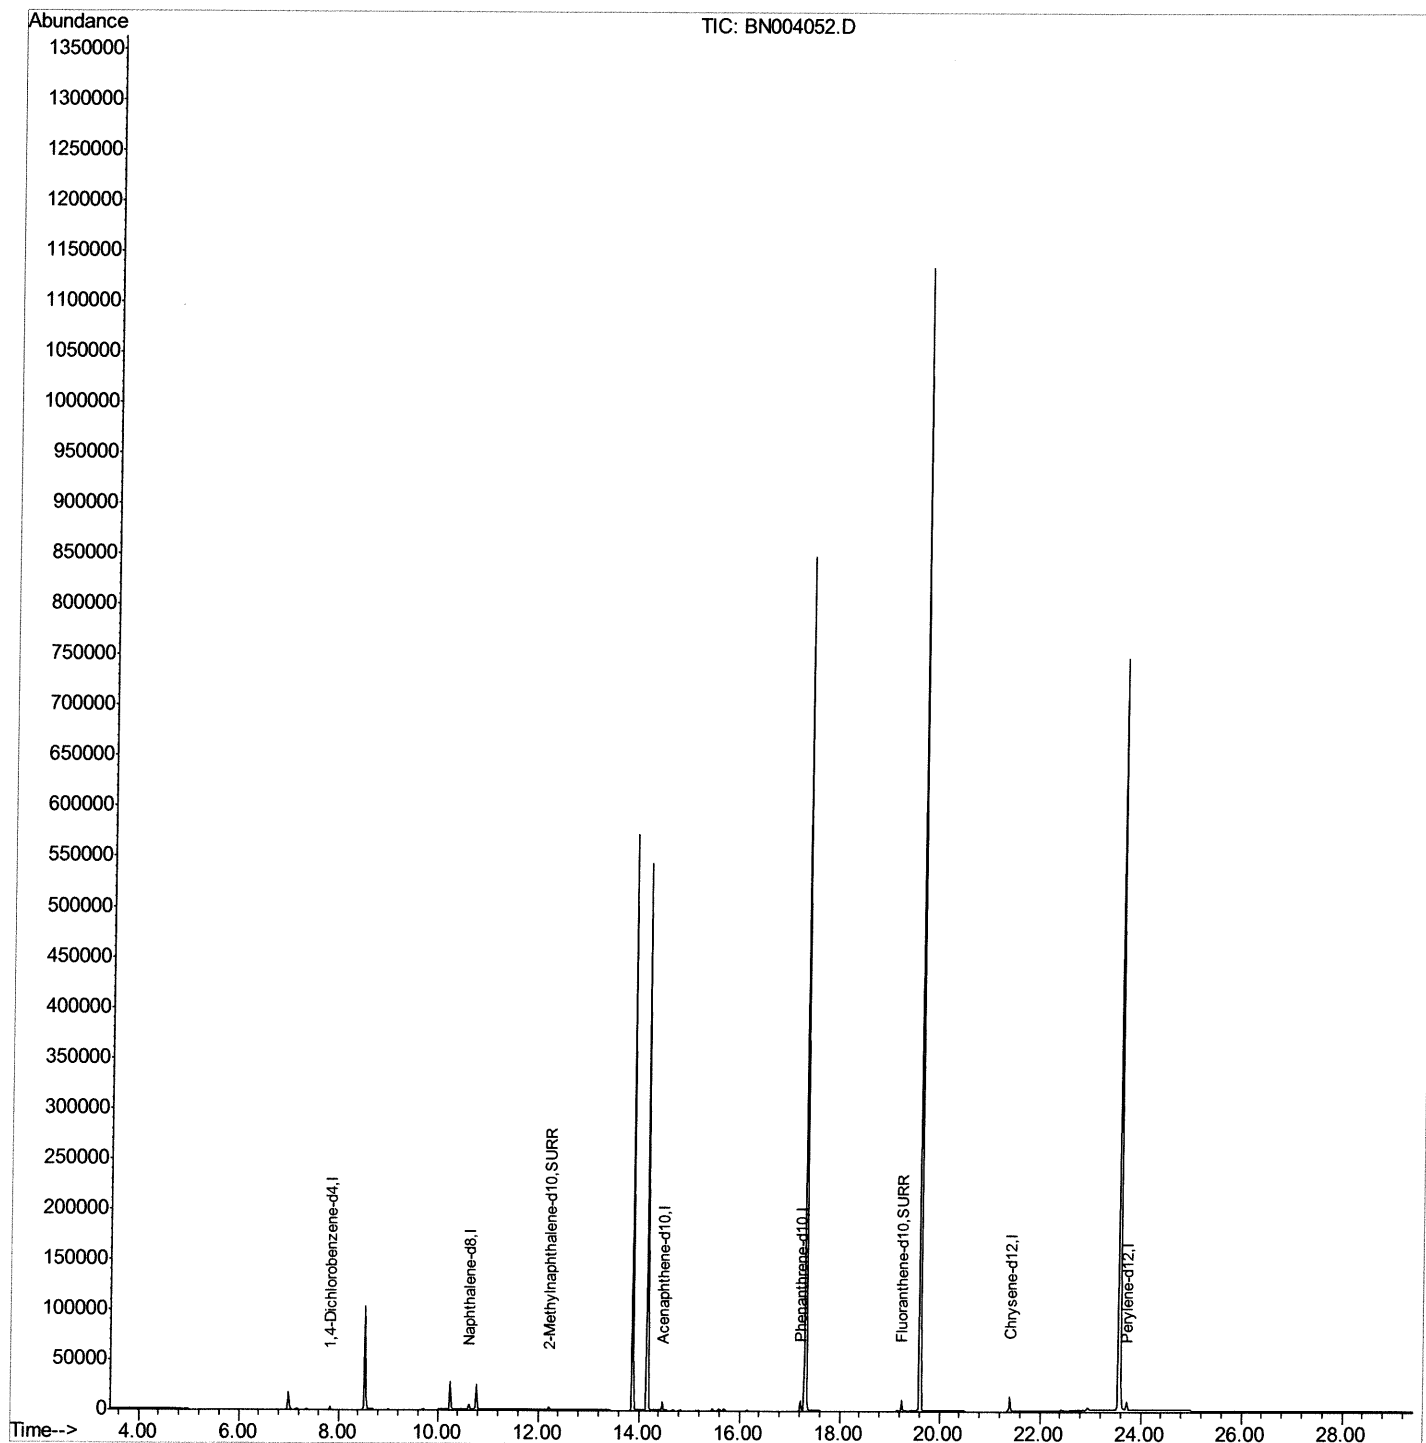

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:37:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

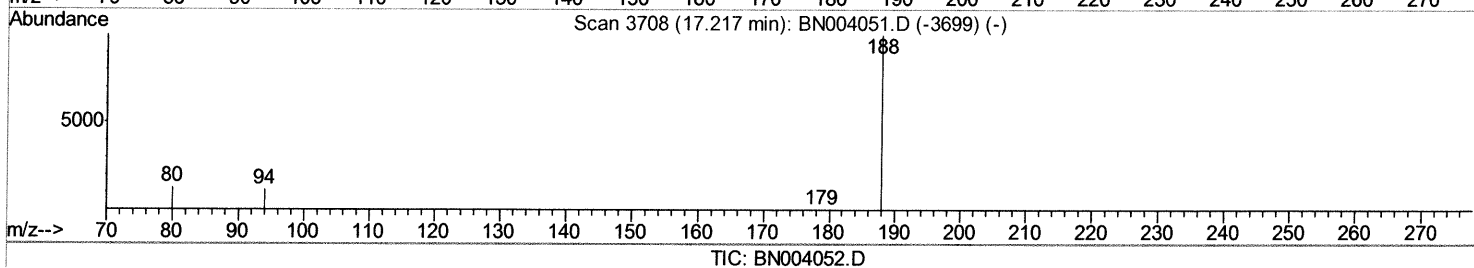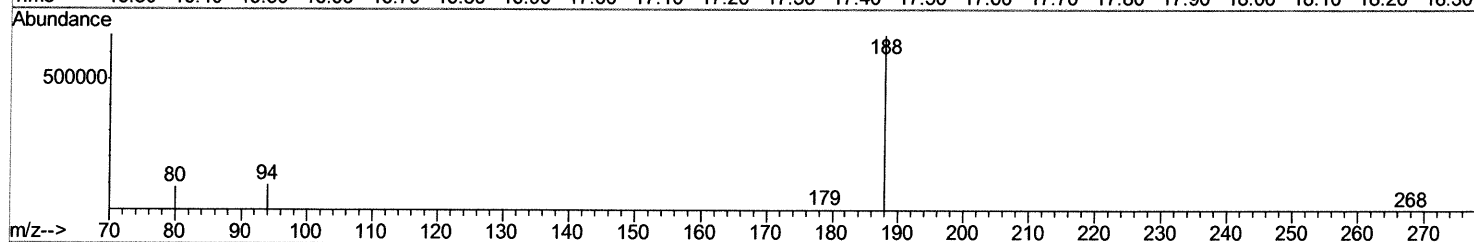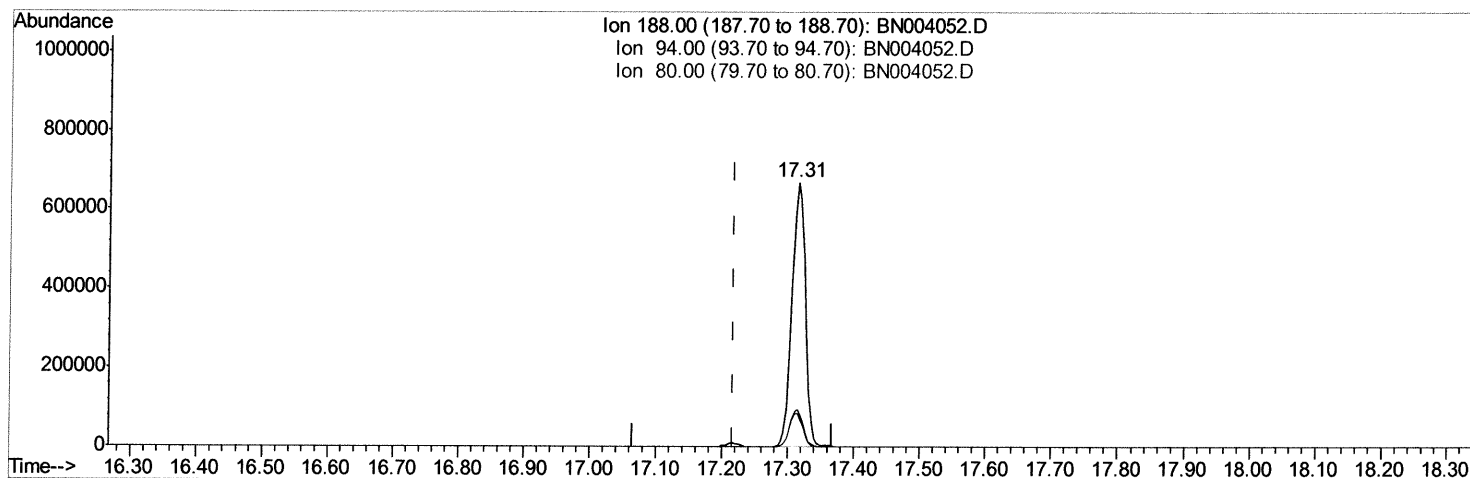

(10) Phenanthrene-d10 (I)
17.314min (+0.097) 0.40ng/ul
response 927117

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.12#
80.00	11.60	12.73
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:37:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

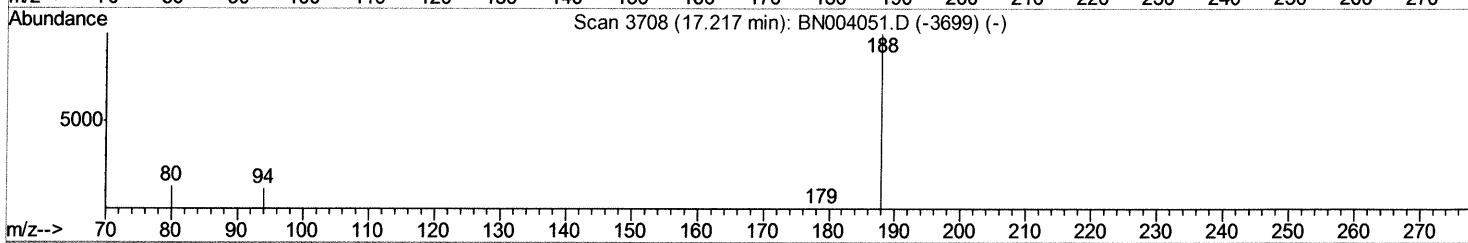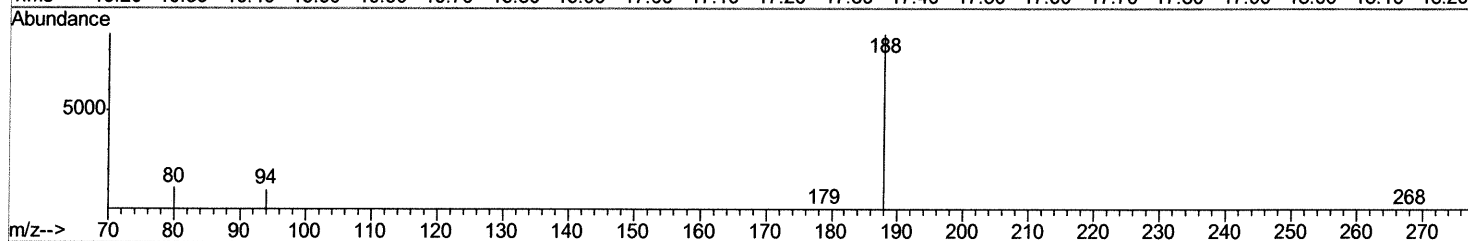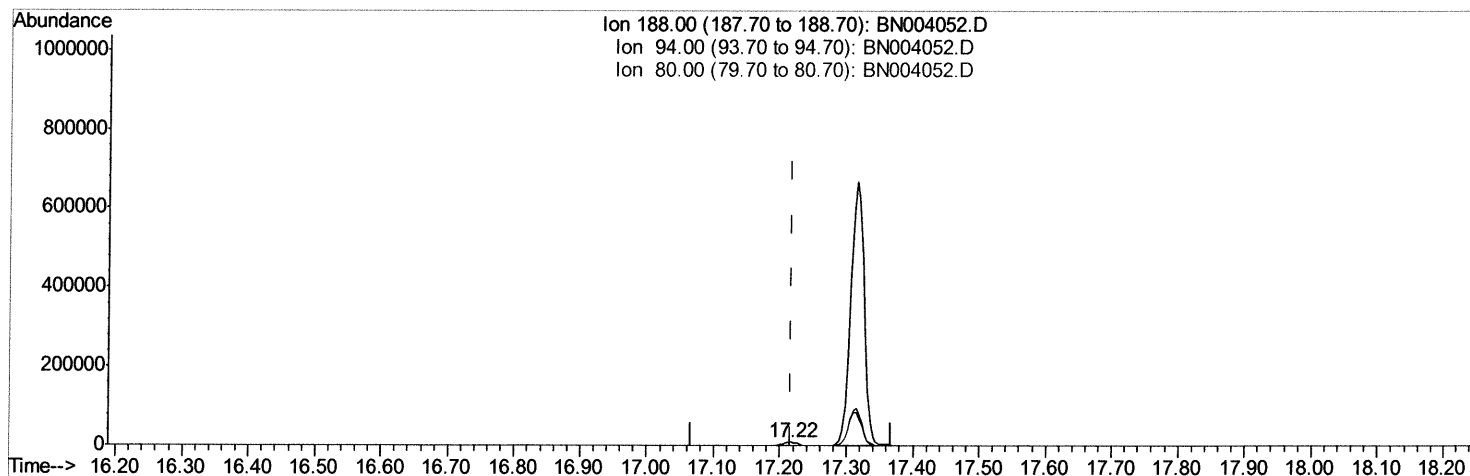

TIC: BN004052.D

(10) Phenanthrene-d10 (I)

17.217min (+0.000) 0.40ng/ul m

response 12219

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.63
80.00	11.60	12.53
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:45:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

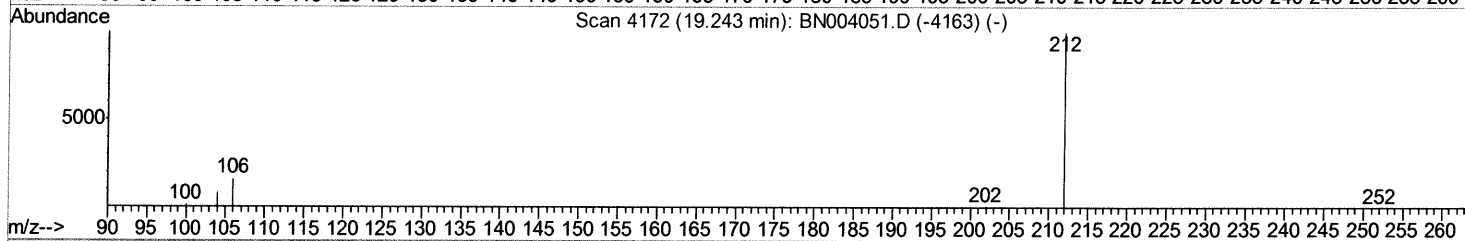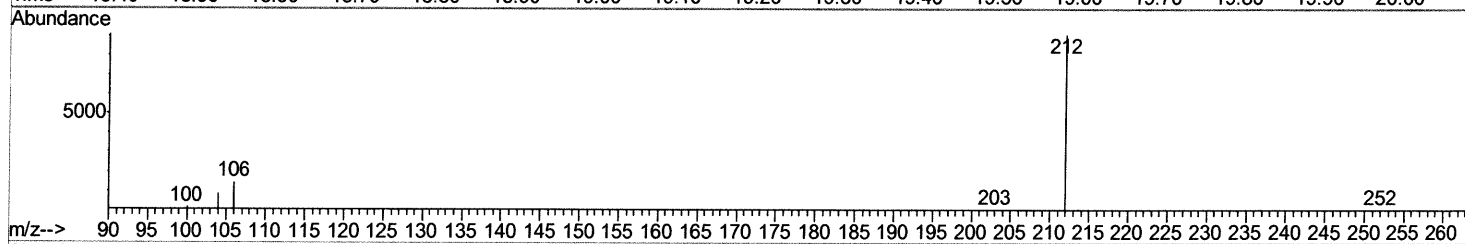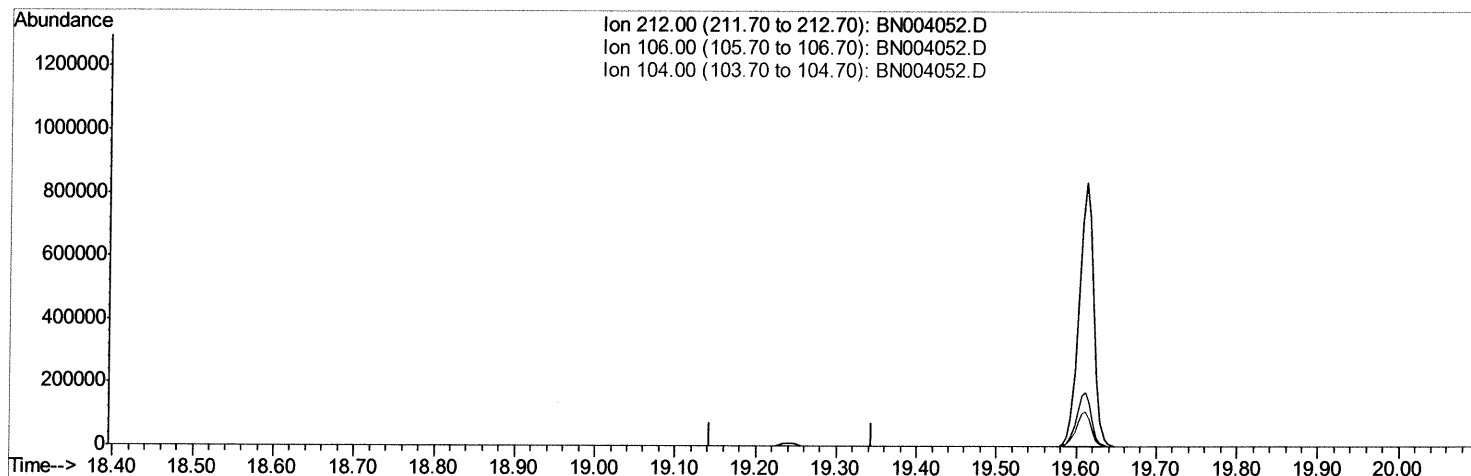

TIC: BN004052.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:45:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

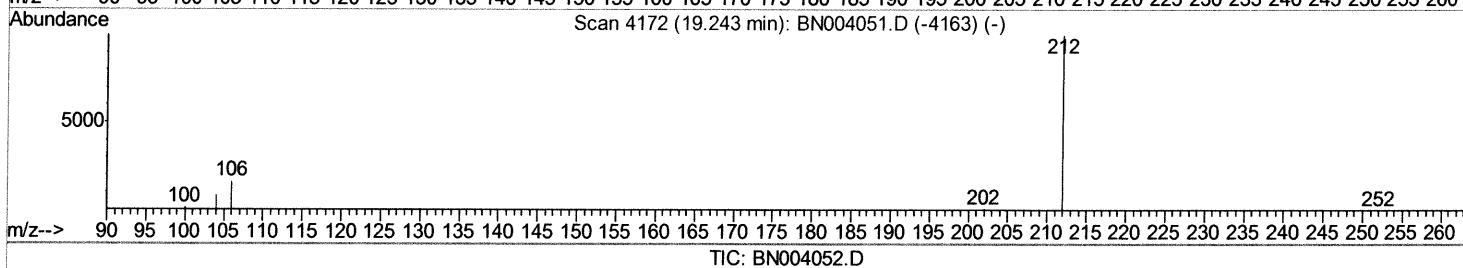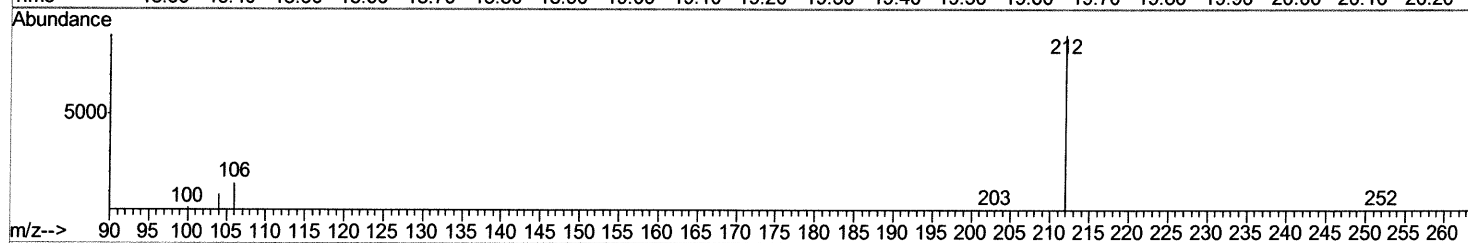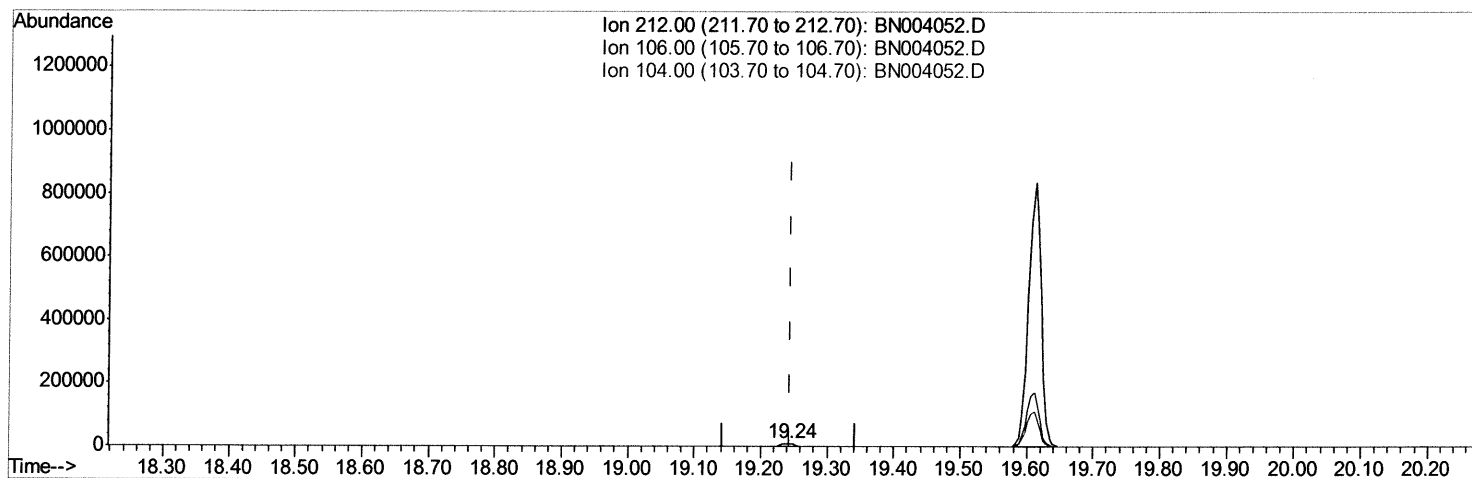

(14) Fluoranthene-d10 (SURR)

19.244min (+0.000) 0.34ng/ul m

response 11977

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:45:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

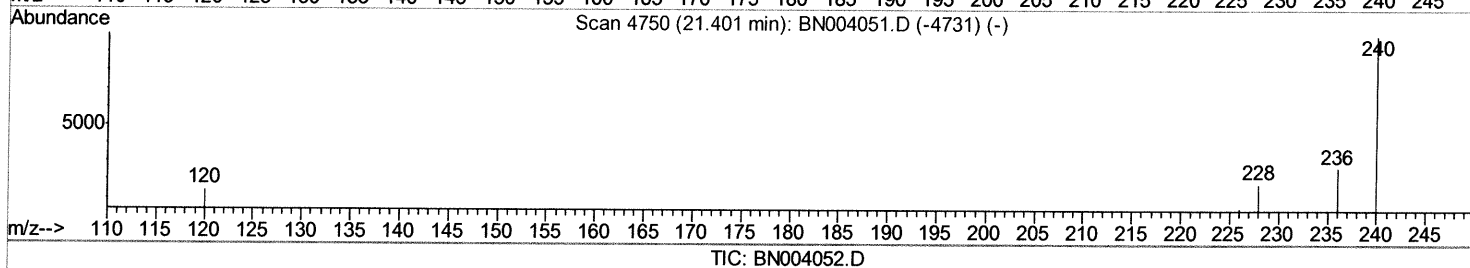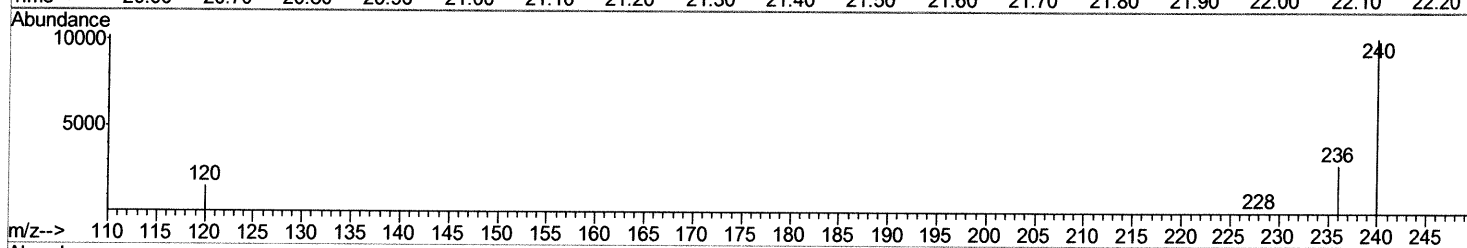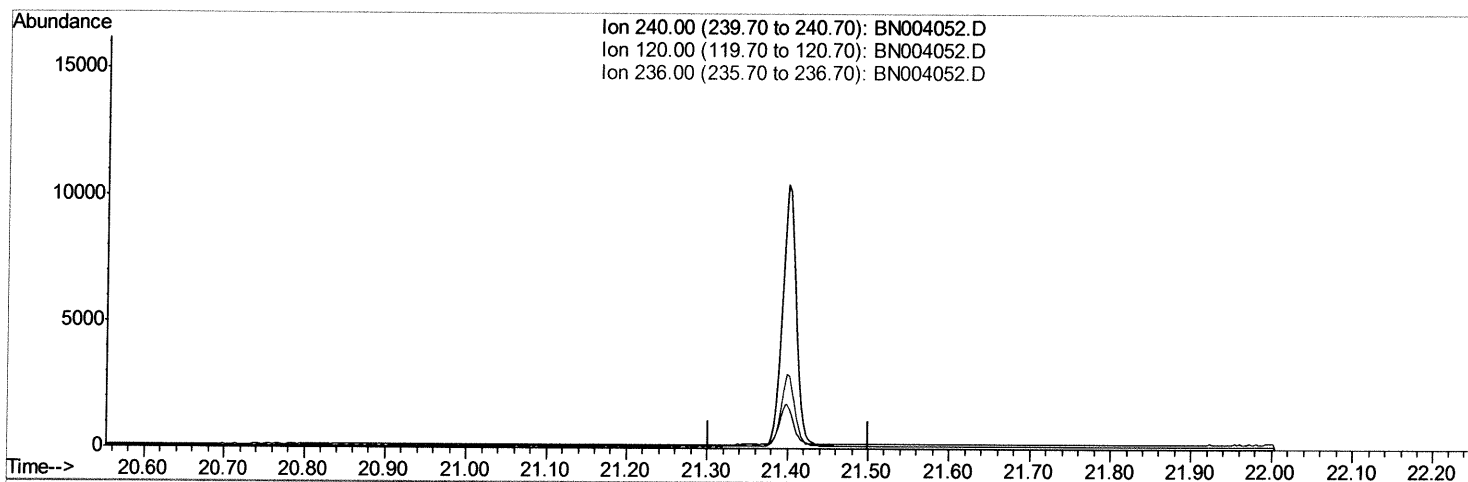

(16) Chrysene-d12 (I)

21.401min (-21.401) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:45:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

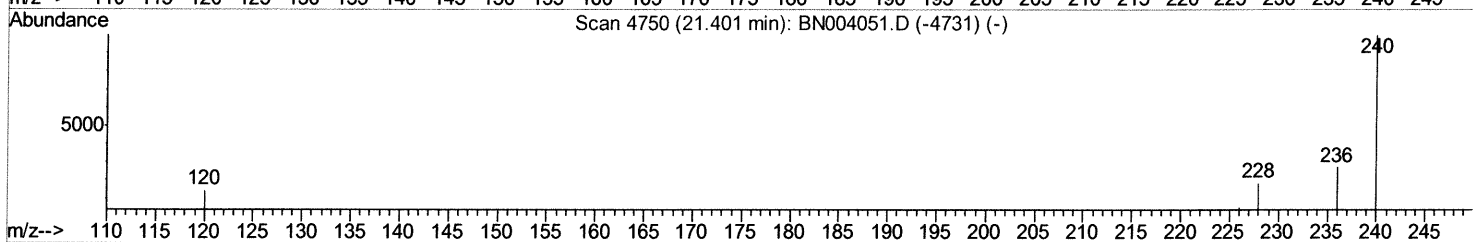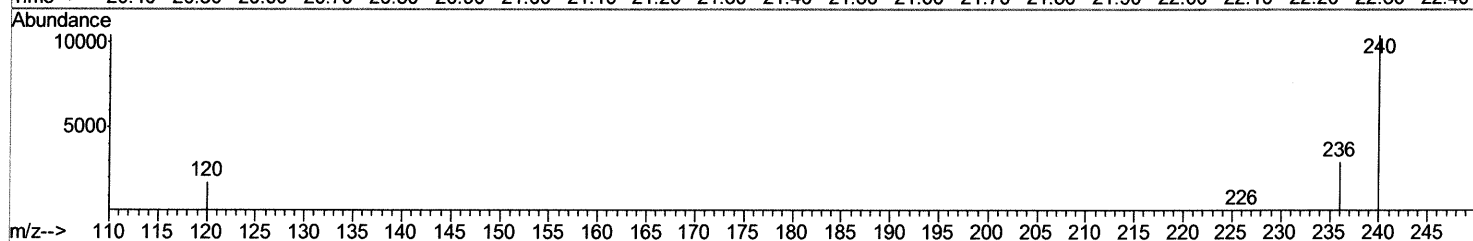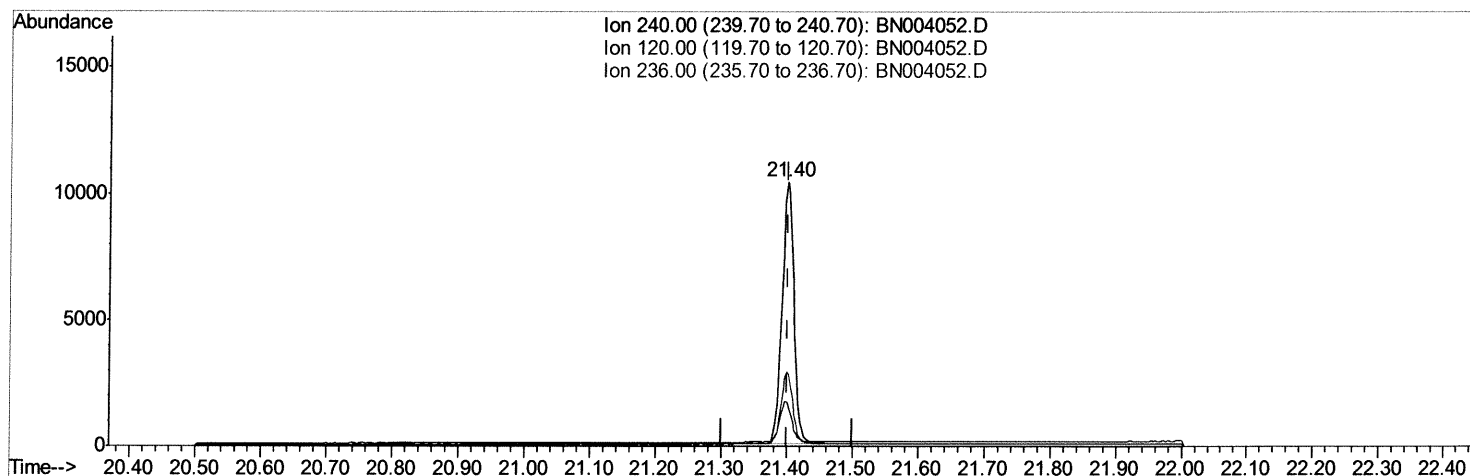

TIC: BN004052.D

(16) Chrysene-d12 (I)

21.400min (-0.002) 0.40ng/ul m

response 13098

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.78
236.00	27.60	28.30
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:46:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

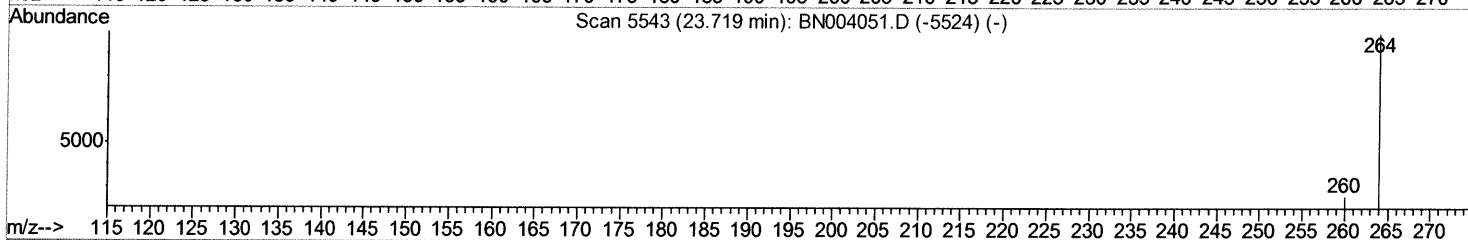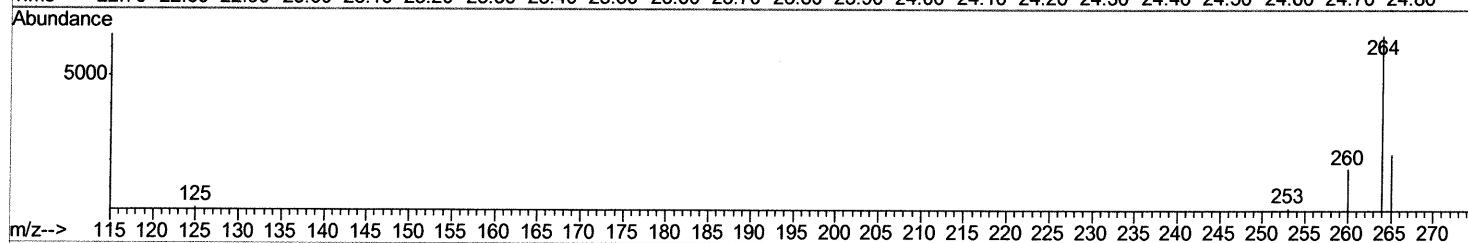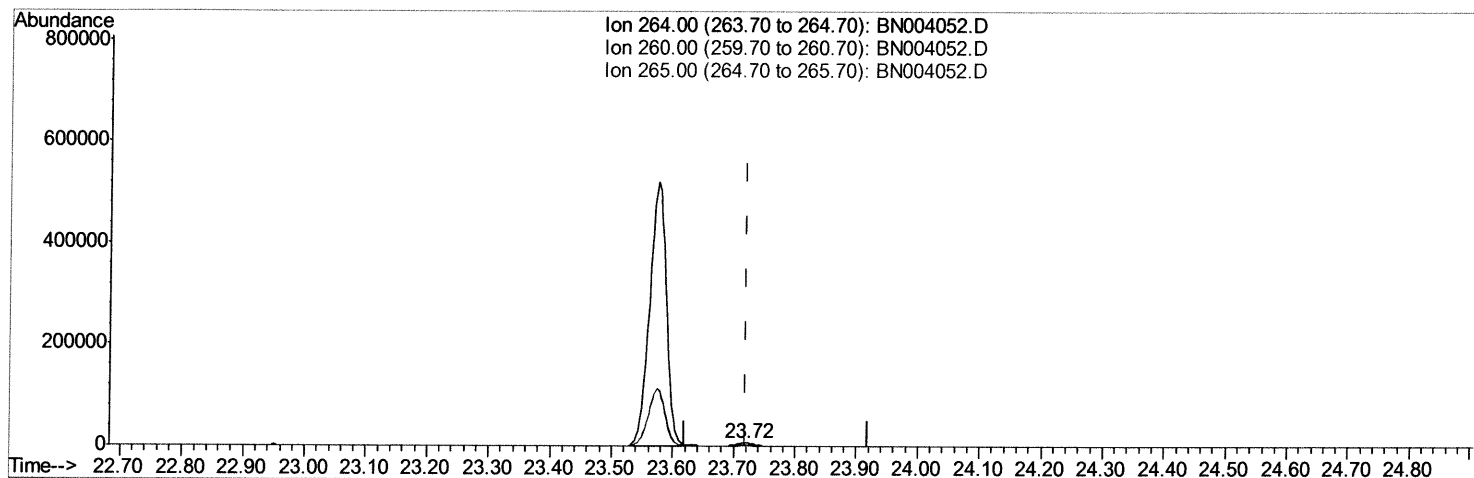

TIC: BN004052.D

(20) Perylene-d12 (I)

23.721min (+0.001) 0.40ng/ul

response 13121

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.57
265.00	33.50	34.79
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:46:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

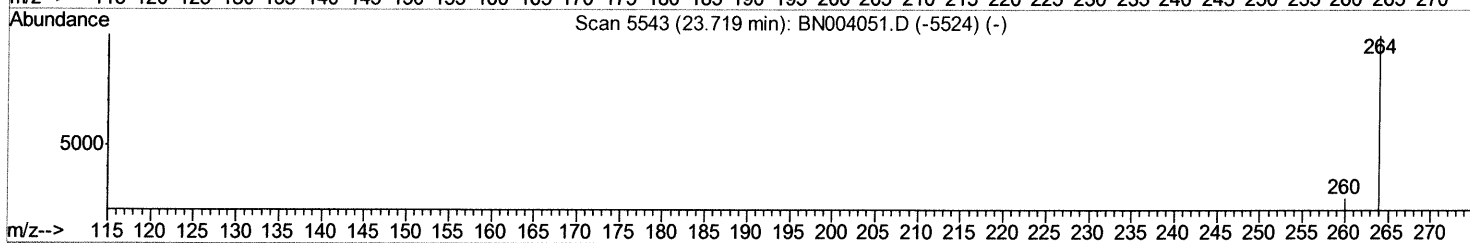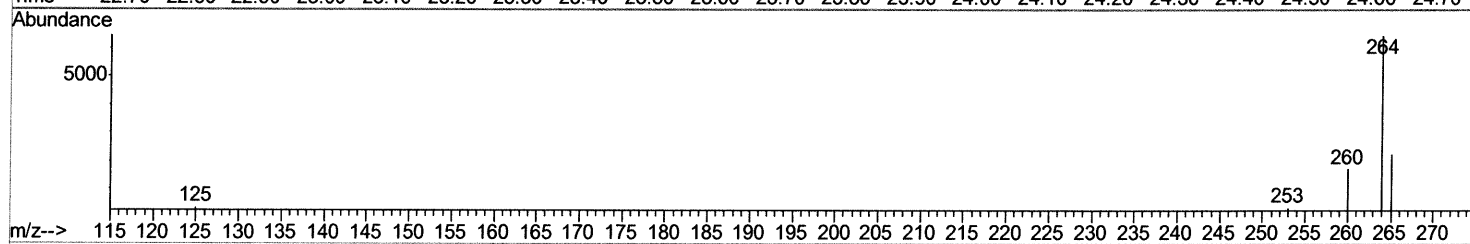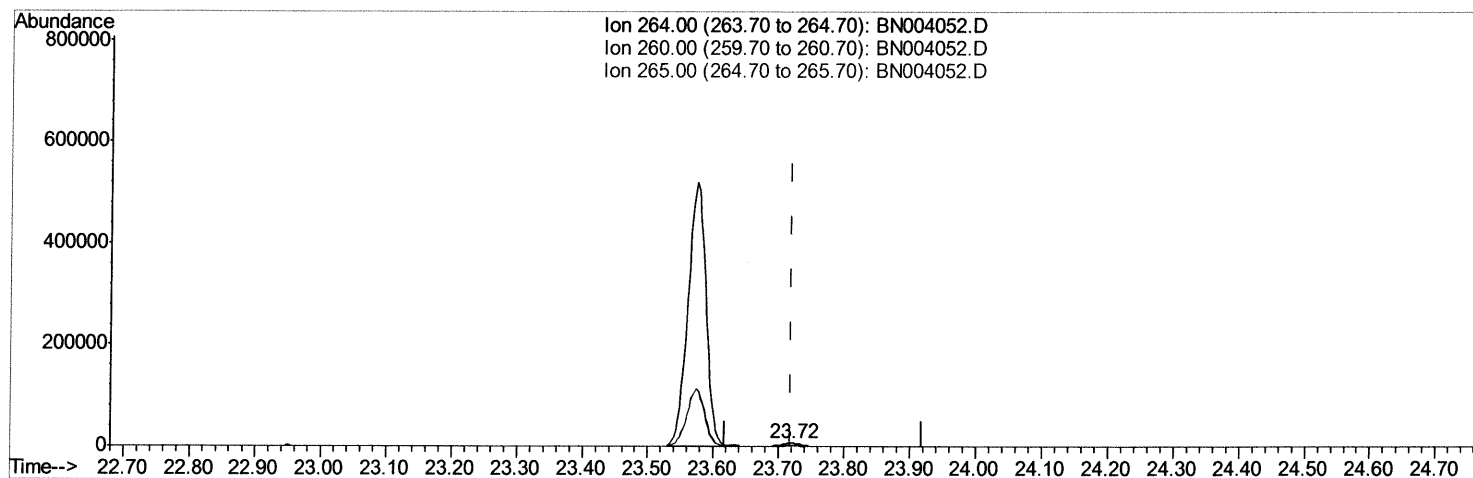

TIC: BN004052.D

(20) Perylene-d12 (I)

23.721min (+0.001) 0.40ng/ul m

response 11351

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	26.57
265.00	33.50	34.79
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)

Data File : BN004052.D
Acq On : 18 Dec 2018 00:53
Operator : JU/SJ
Sample : PB115478BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK78

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:36 PM

Quant Time: Dec 18 06:46:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1486	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	7632	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4912	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	12219m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	13098m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	11351m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3630	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	11977m	0.34	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/18/18