

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)


Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:30:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

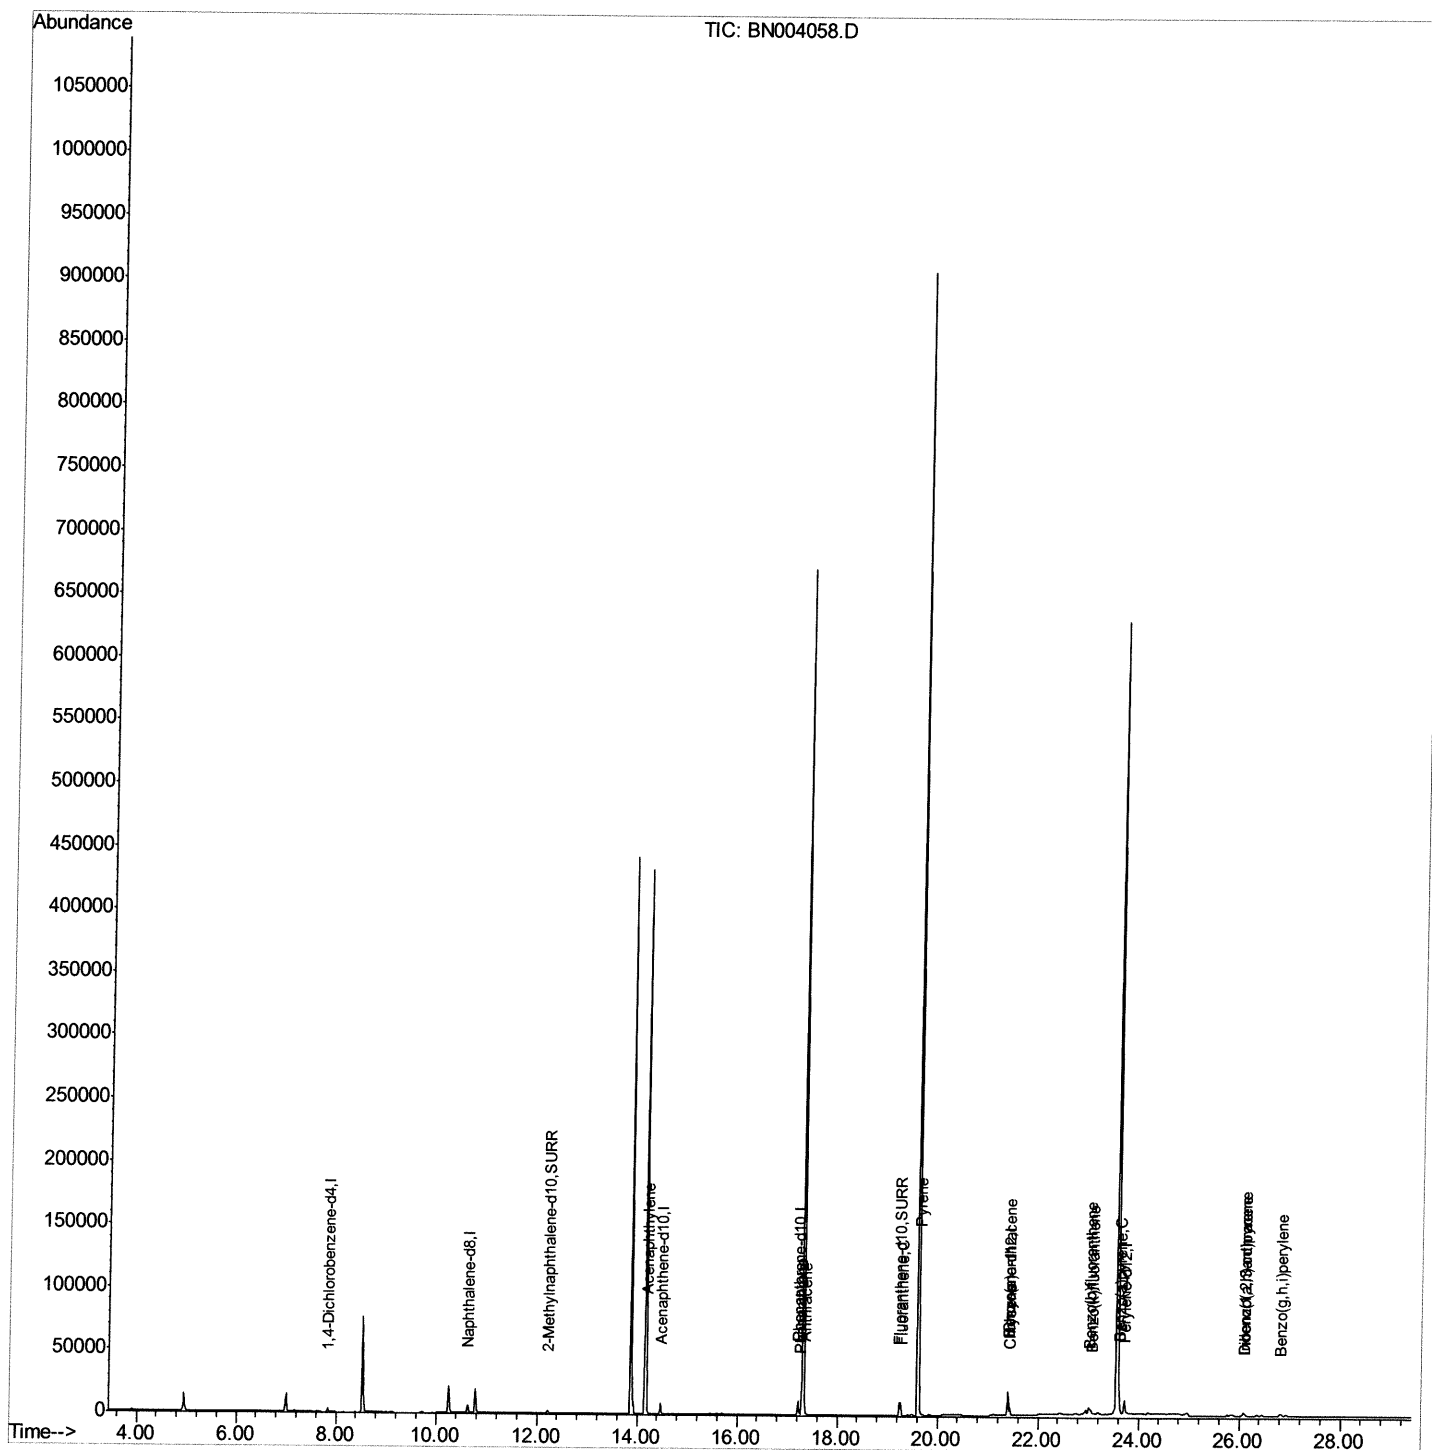

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 06:38:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

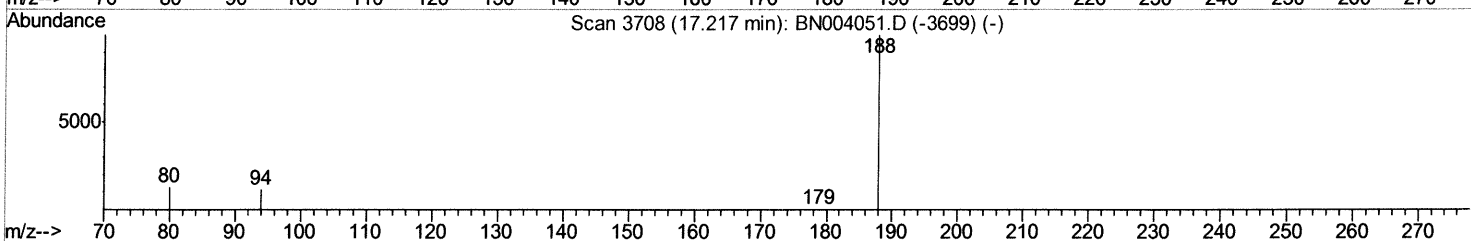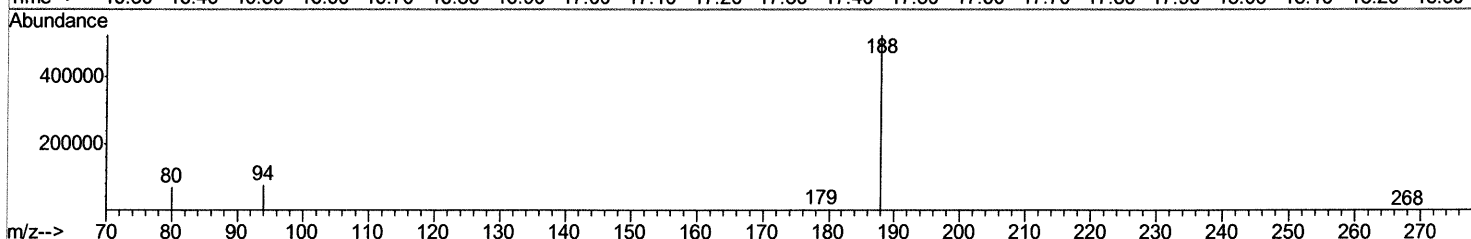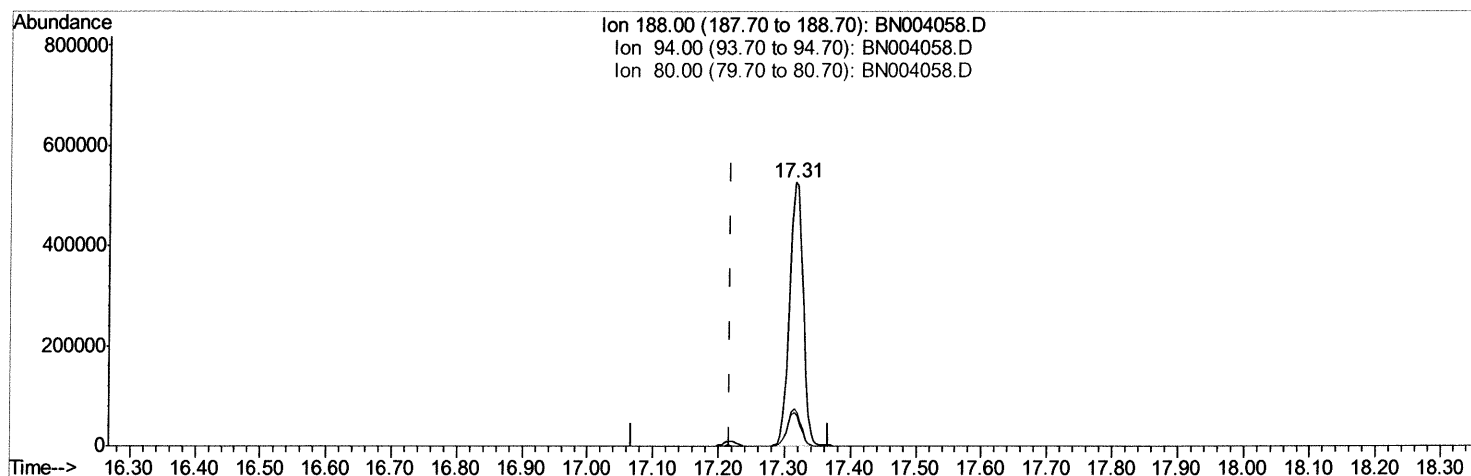

TIC: BN004058.D

(10) Phenanthrene-d10 (I)

17.314min (+0.097) 0.40ng/ul

response 741481

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.26#
80.00	11.60	12.90
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 06:38:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

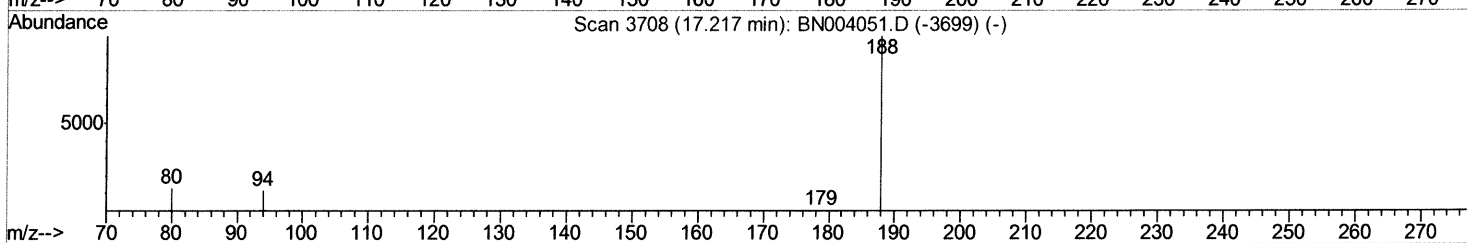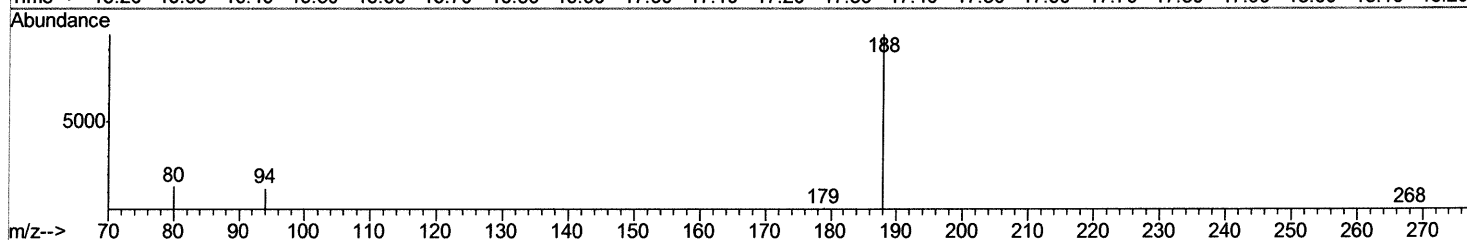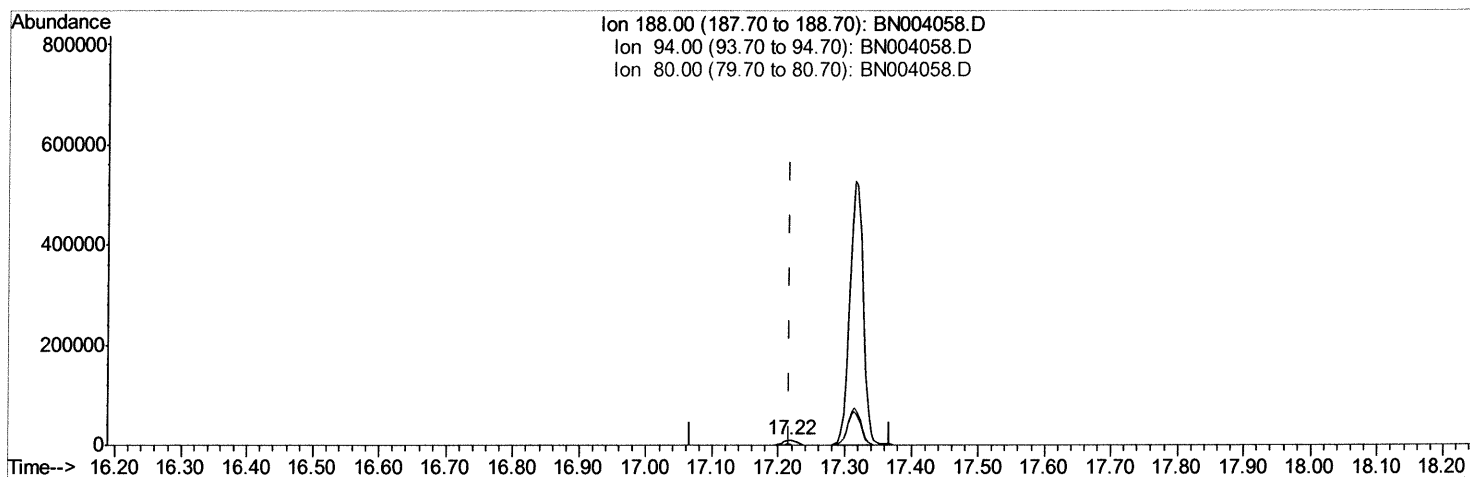

TIC: BN004058.D

(10) Phenanthrene-d10 (I)

17.217min (+0.000) 0.40ng/ul m

response 13443

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.30
80.00	11.60	13.37
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

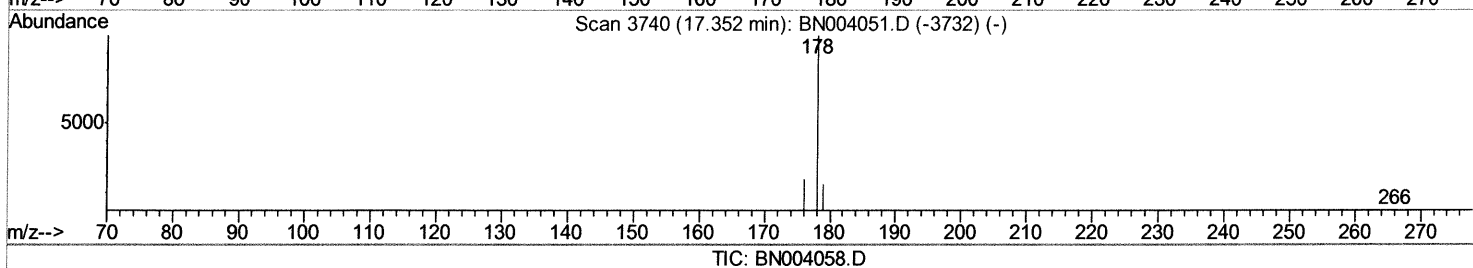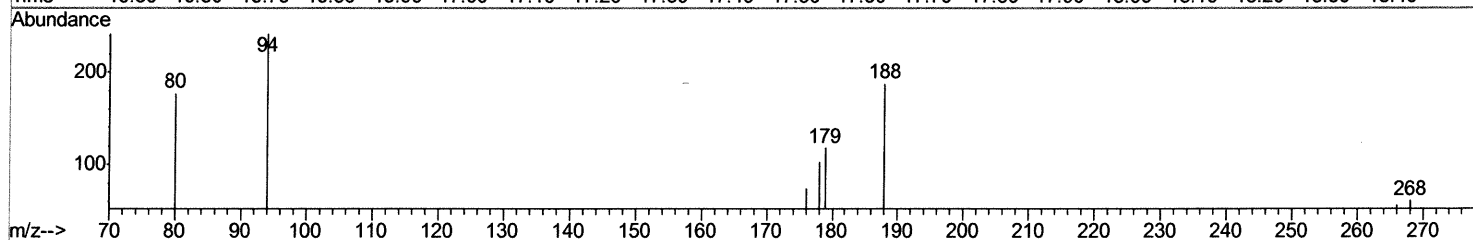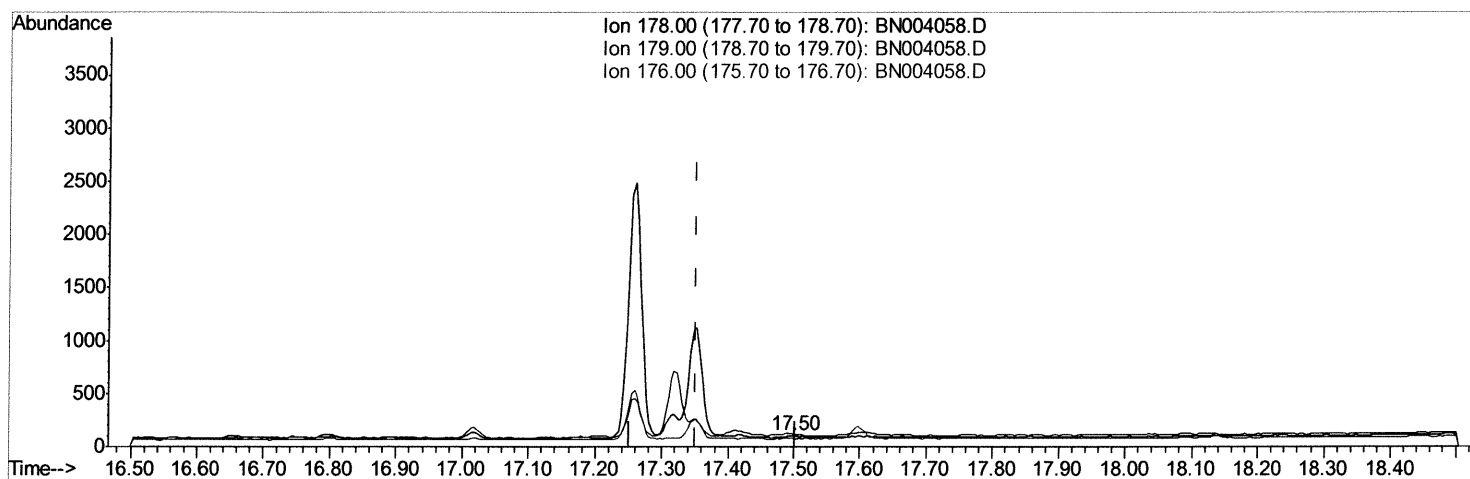

(13) Anthracene

17.500min (+0.148) 0.00ng/ul

response 35

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	114.56#
176.00	18.50	71.84#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

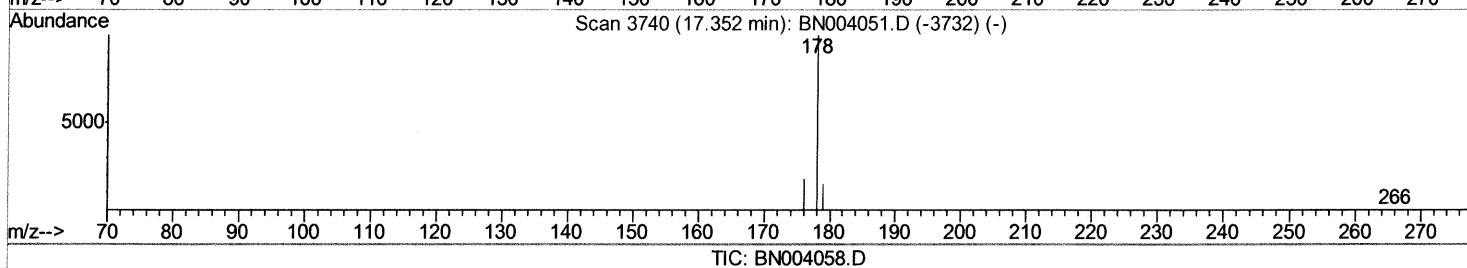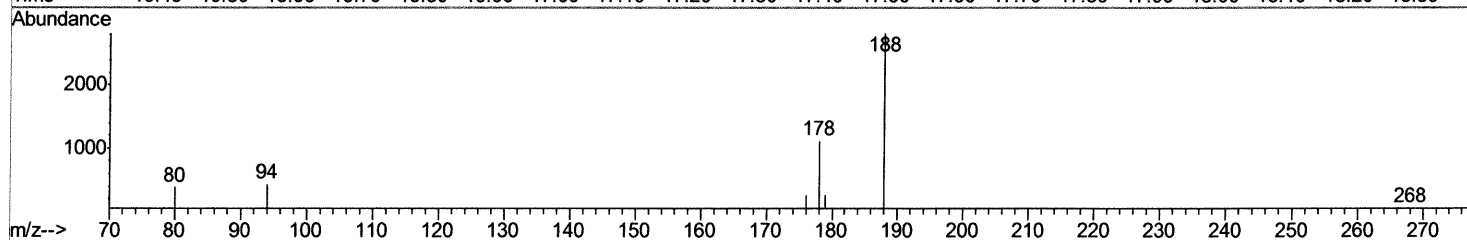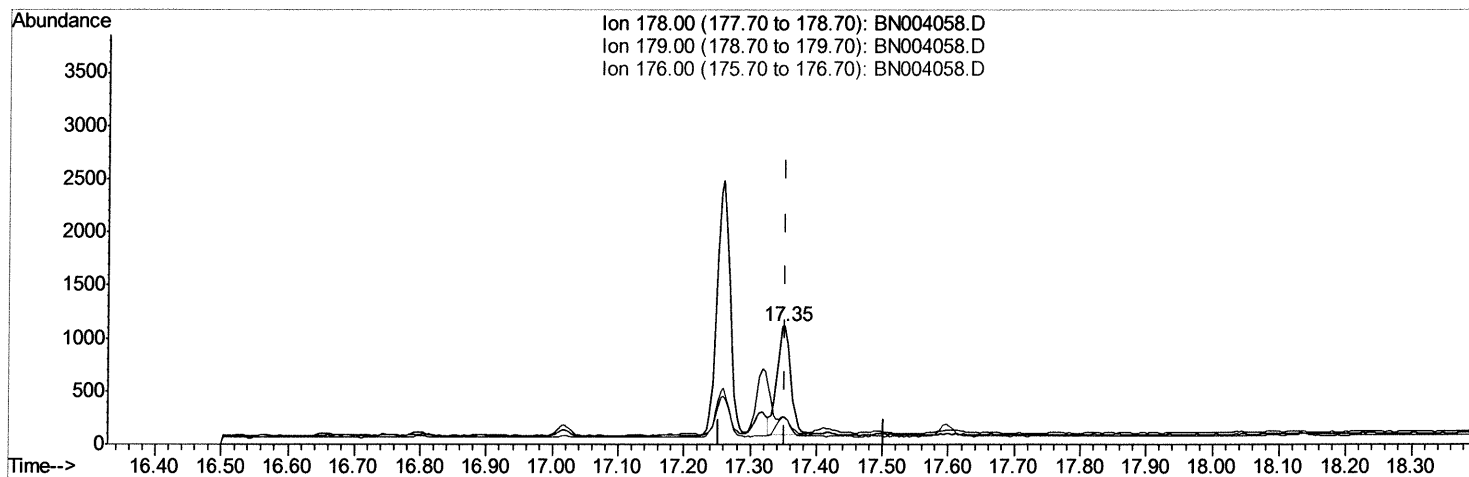

(13) Anthracene

17.352min (+0.000) 0.04ng/ul m

response 1488

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	22.69#
176.00	18.50	23.05#
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

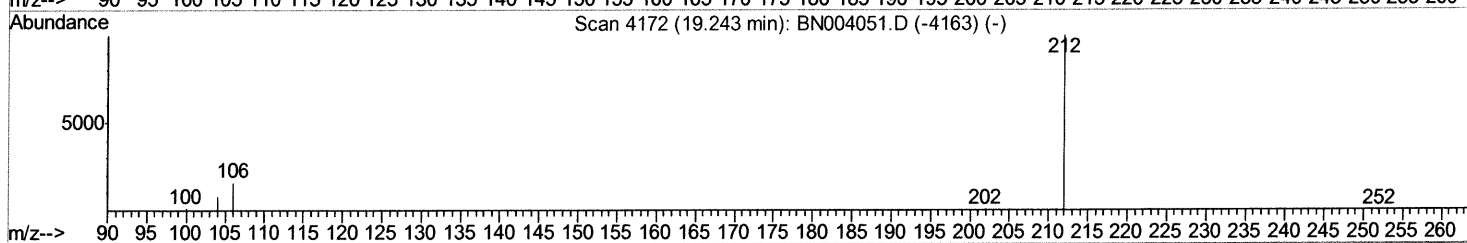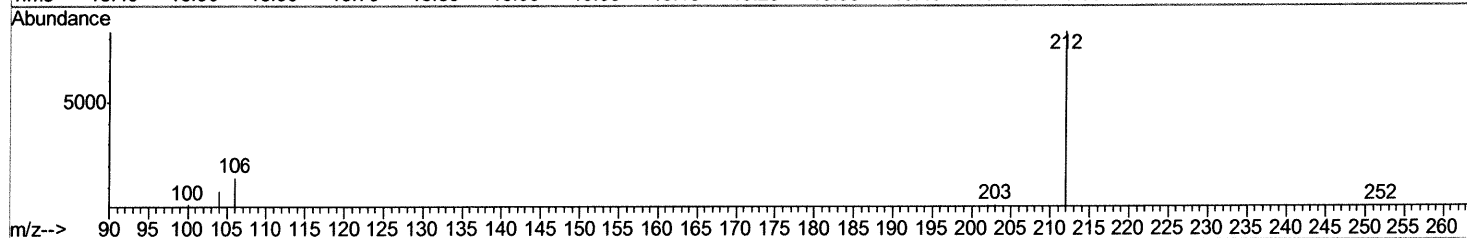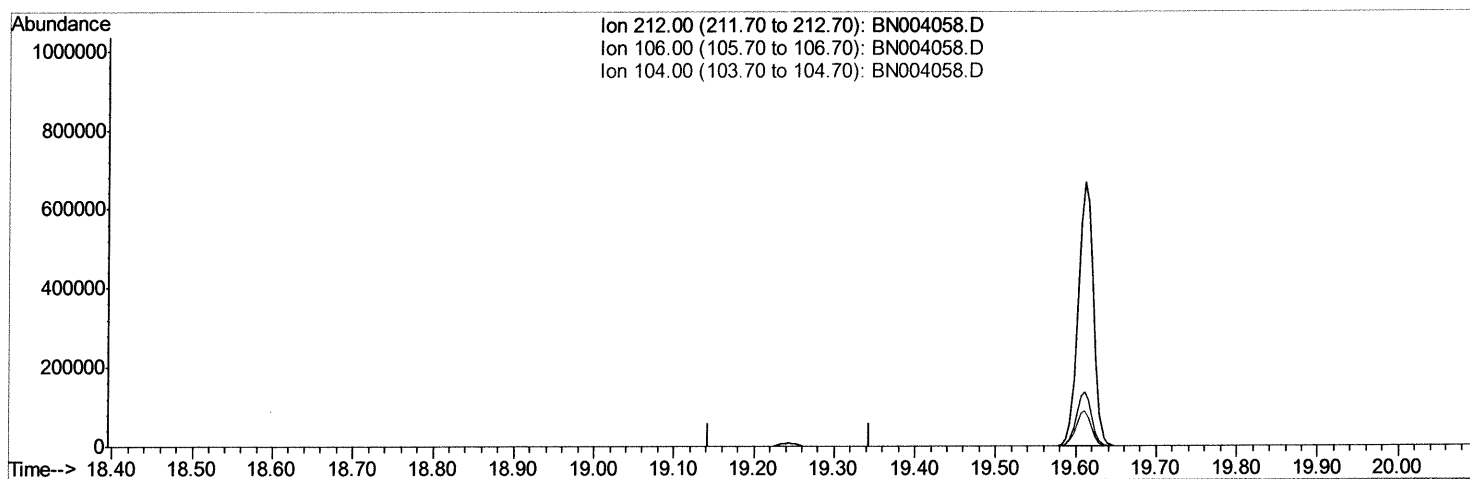

TIC: BN004058.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

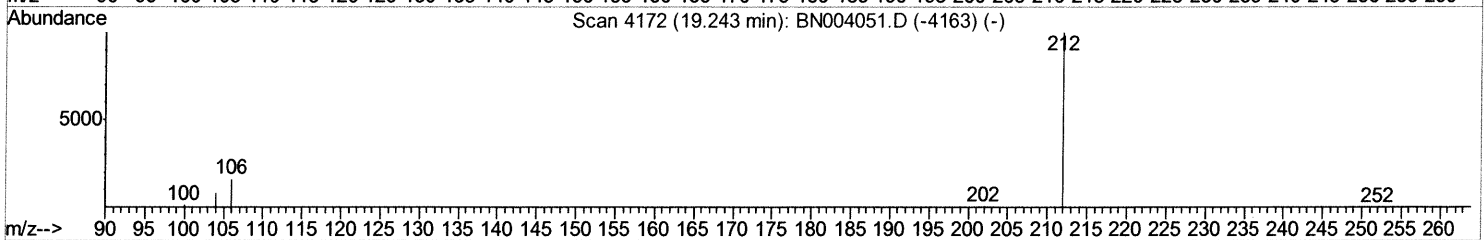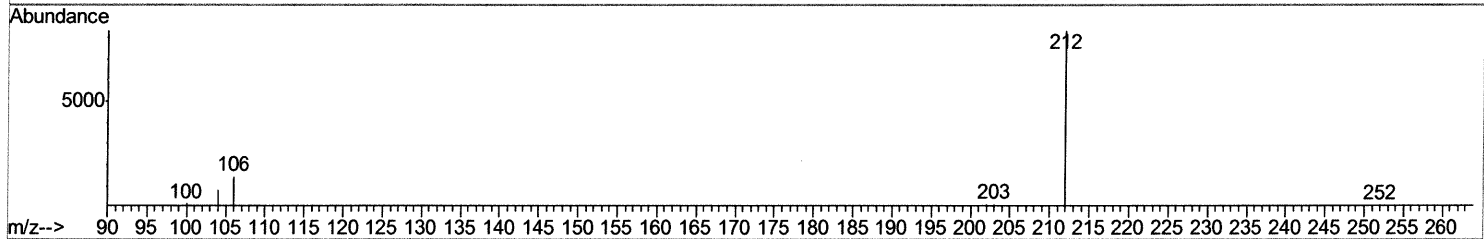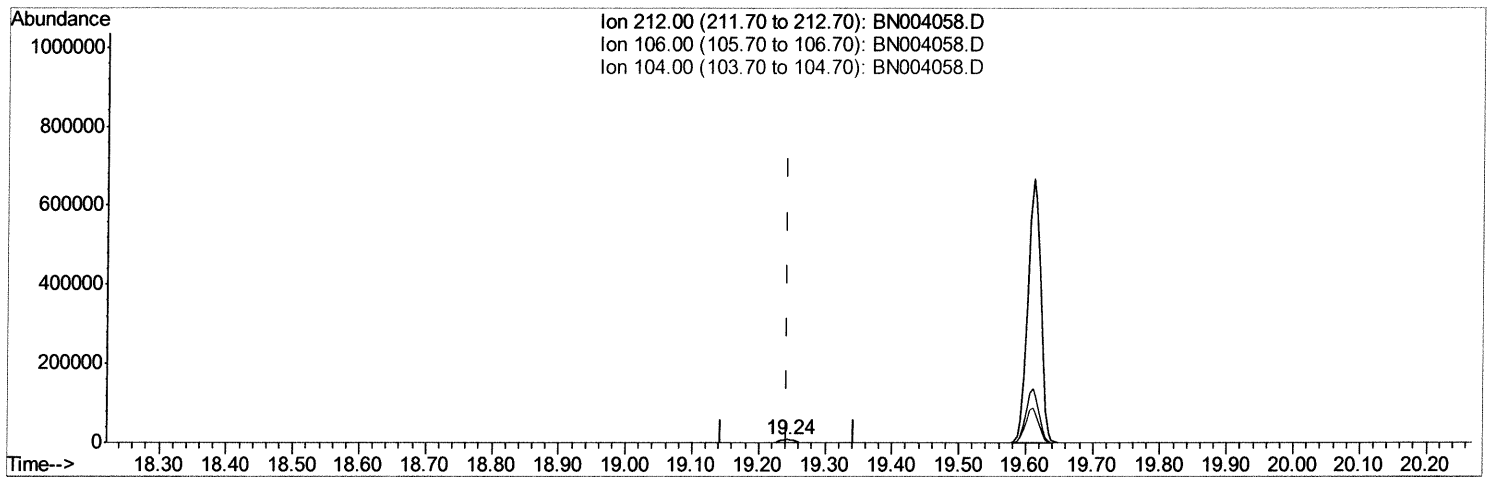

TIC: BN004058.D

(14) Fluoranthene-d10 (SURR)

19.244min (+0.000) 0.29ng/ul m

response 11281

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

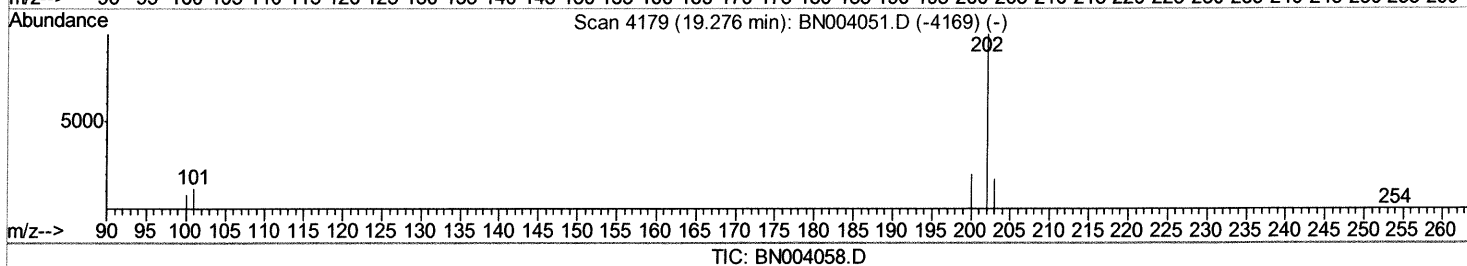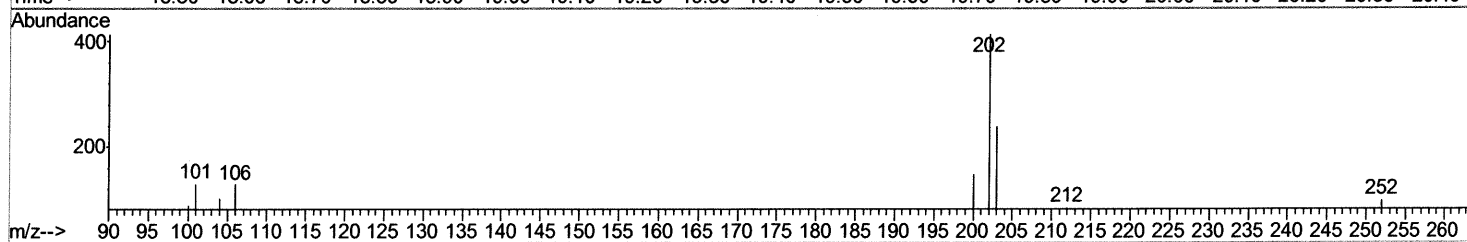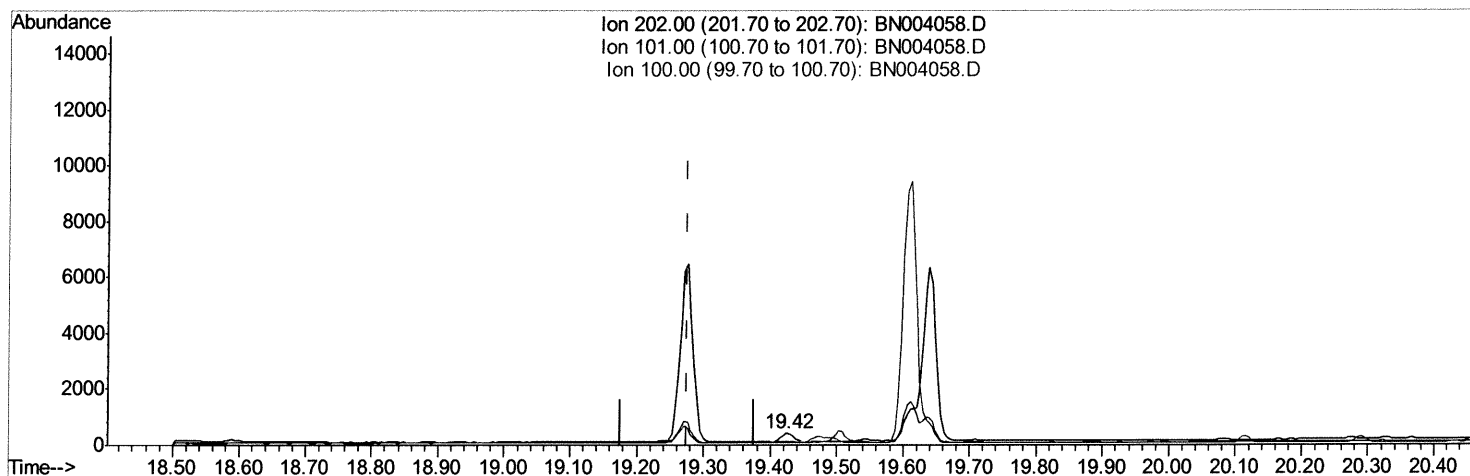

(15) Fluoranthene (C)

19.425min (+0.149) 0.01ng/ui

response 376

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	31.40#
100.00	8.10	21.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

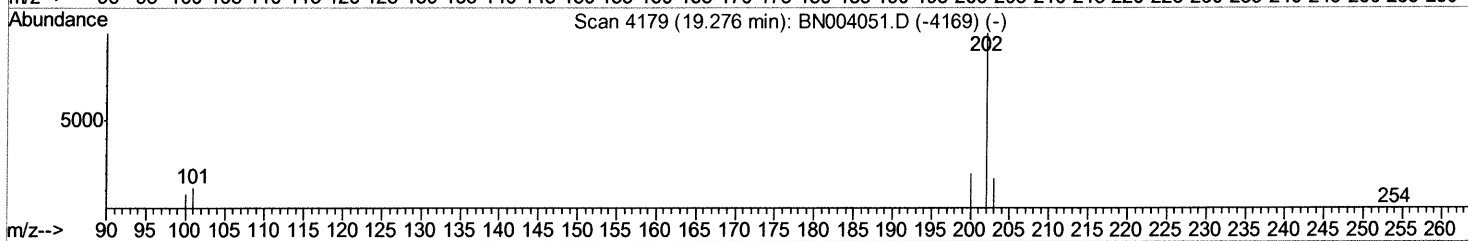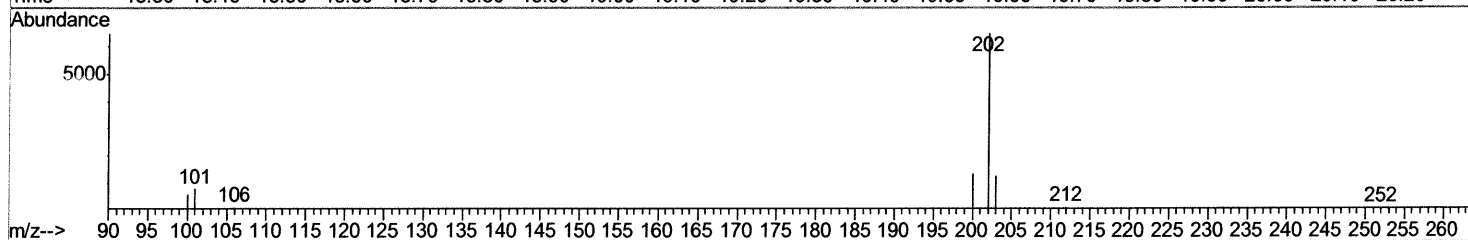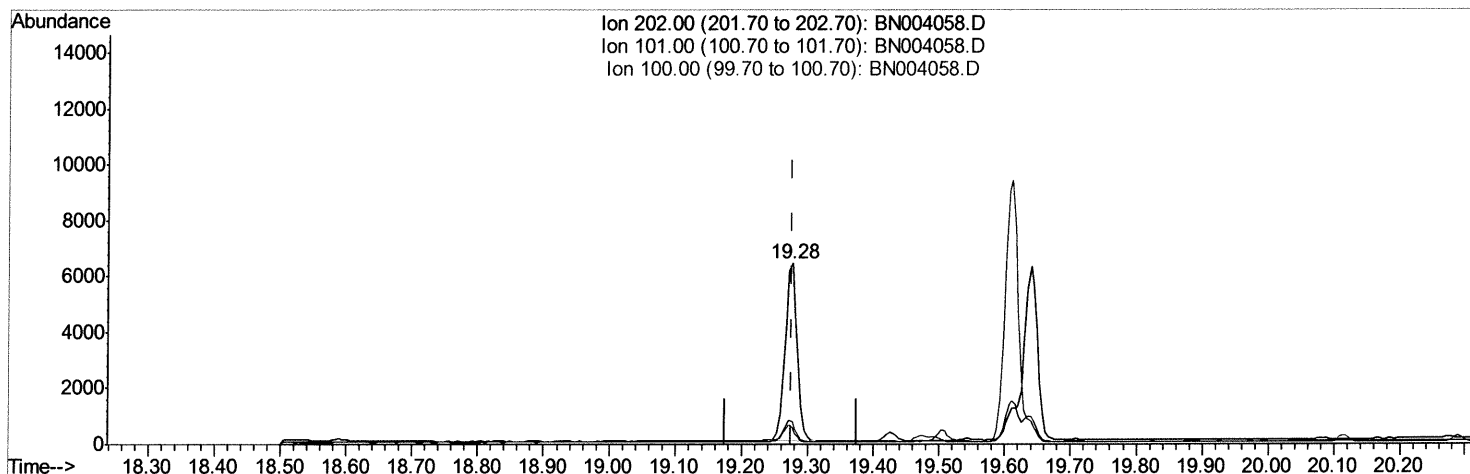

TIC: BN004058.D

(15) Fluoranthene (C)

19.276min (+0.000) 0.16ng/ul m

response 8216

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	12.43
100.00	8.10	9.18
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

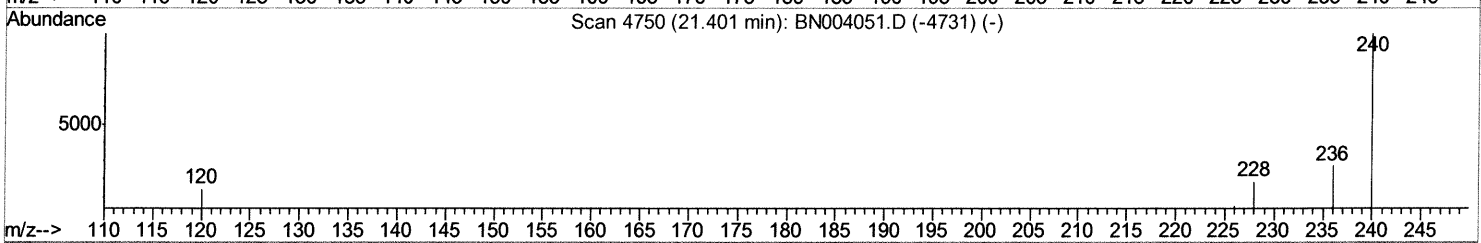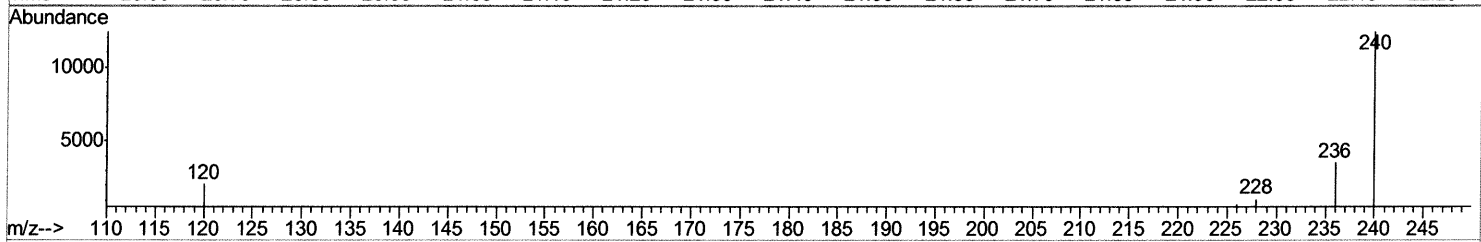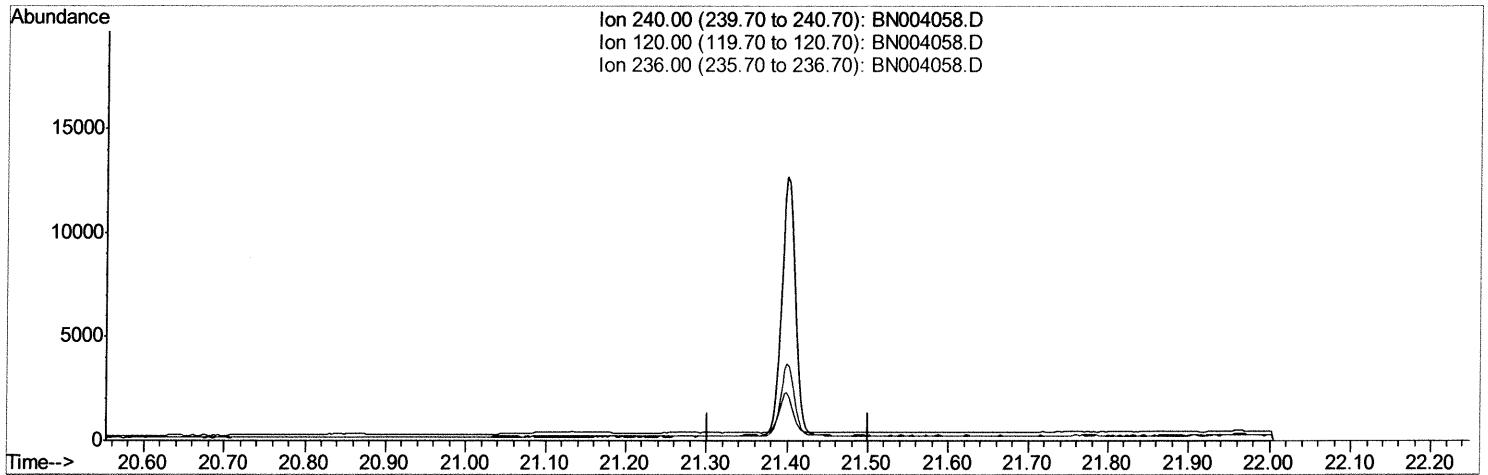

TIC: BN004058.D

(16) Chrysene-d12 (I)

21.401min (-21.401) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:27:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

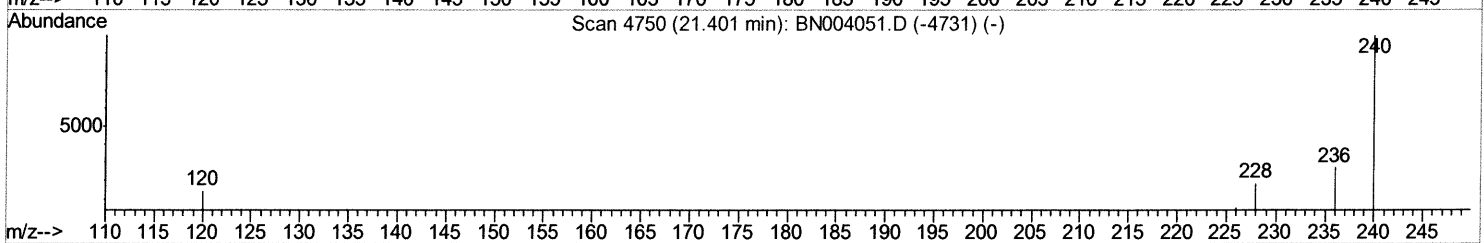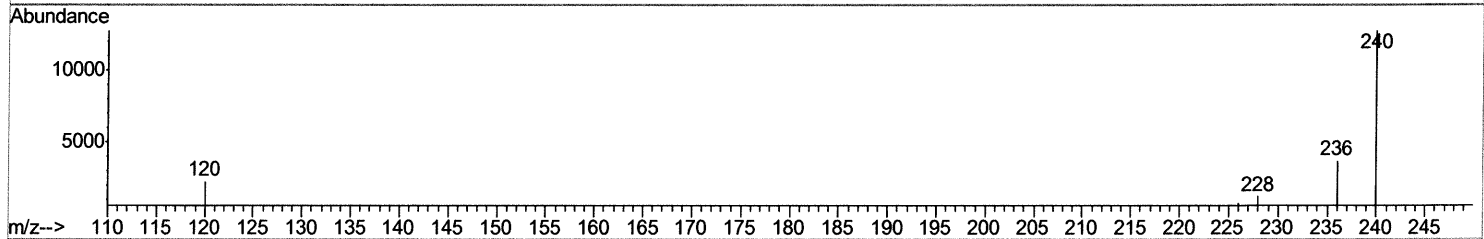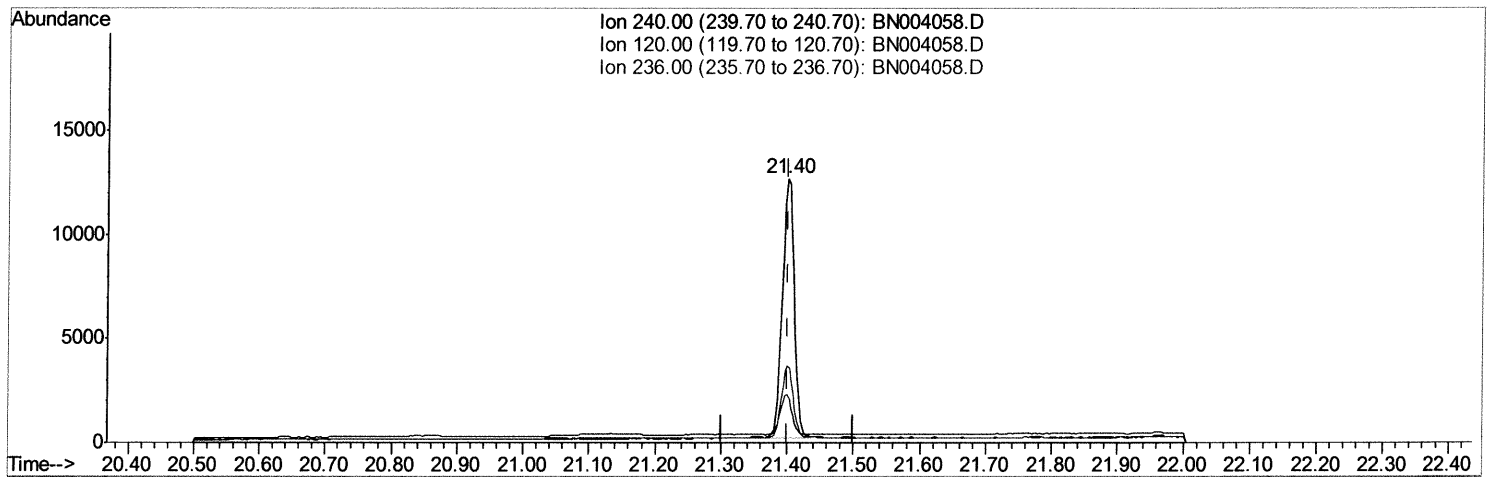

TIC: BN004058.D

(16) Chrysene-d12 (I)

21.400min (-0.002) 0.40ng/ul m

response 15396

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	18.00#
236.00	27.60	29.15
0.00	0.00	0.00

SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:28:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

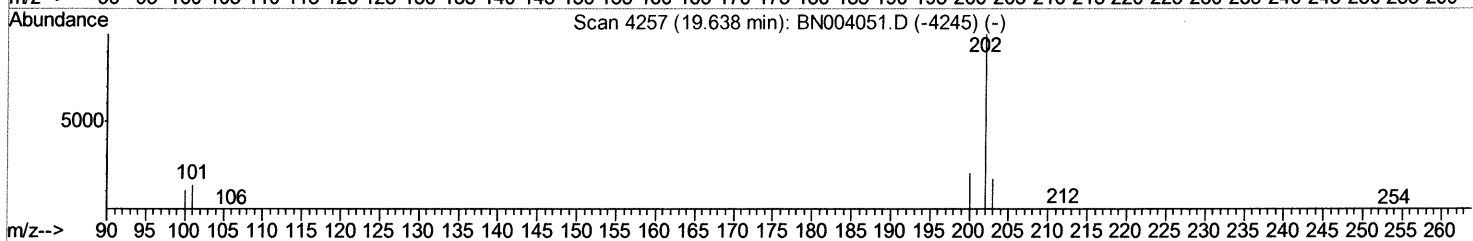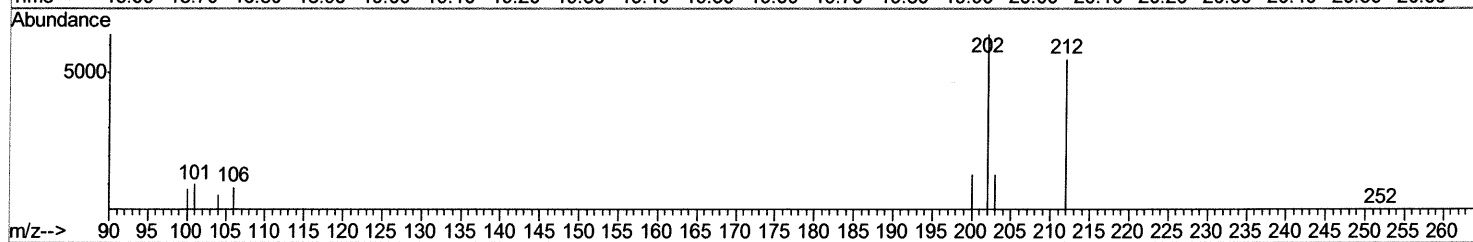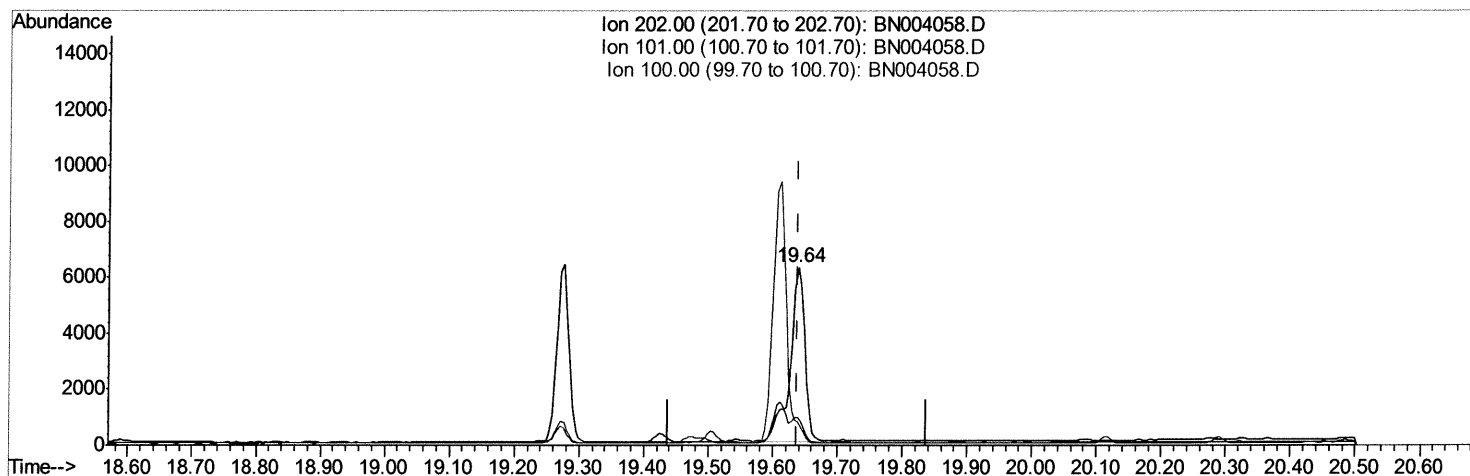

TIC: BN004058.D

(17) Pyrene

19.639min (+0.000) 0.18ng/ul

response 9816

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.56#
100.00	10.60	12.64
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:28:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

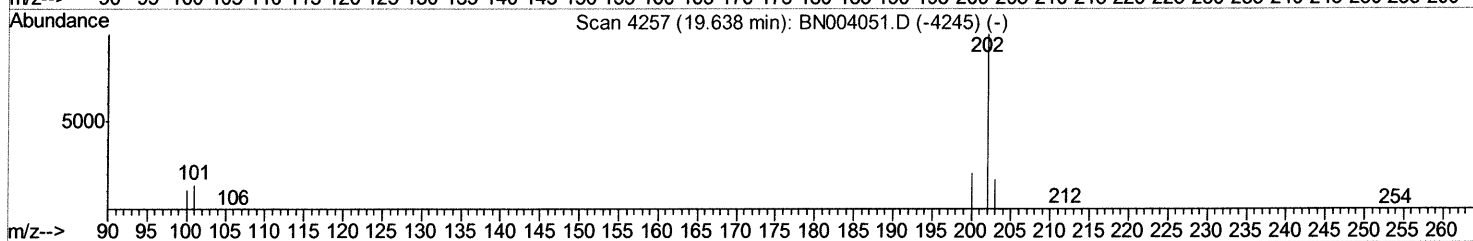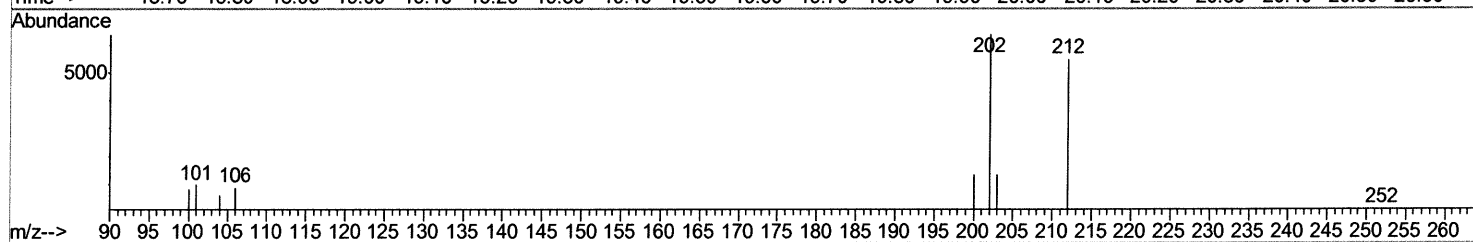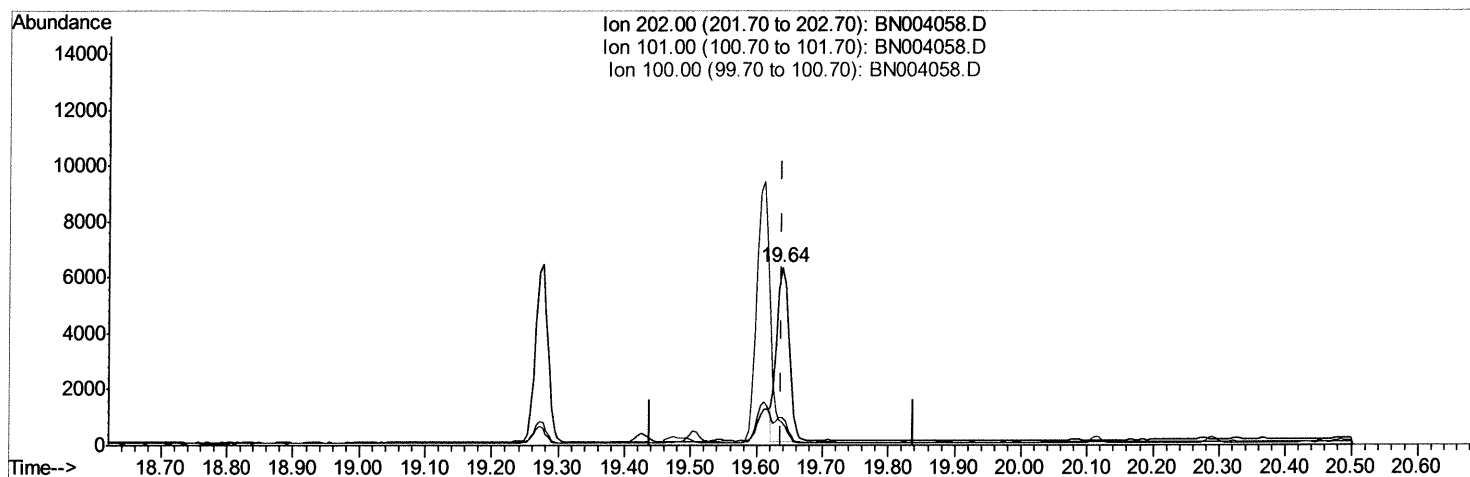

TIC: BN004058.D

(17) Pyrene

19.639min (+0.000) 0.15ng/ul m

response 8340

Ion	Exp%	Act%
202.00	100	100
101.00	12.90	15.56#
100.00	10.60	12.64
0.00	0.00	0.00

> 55
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:28:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

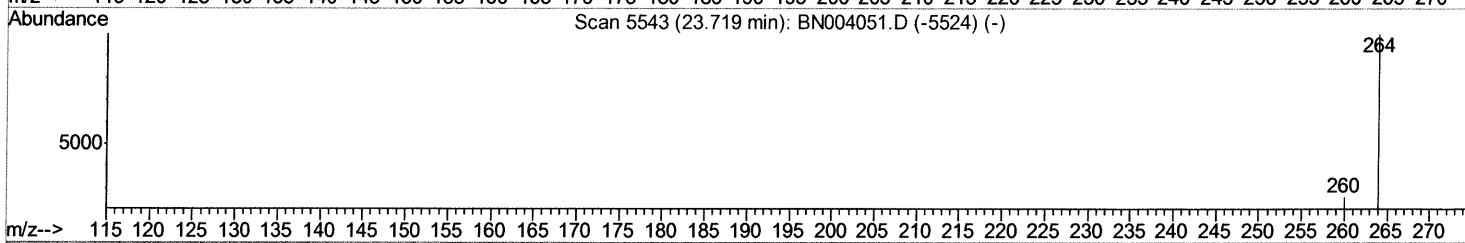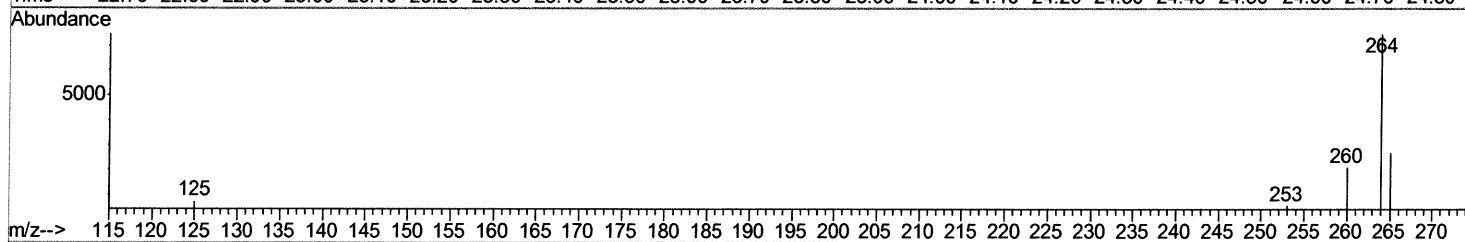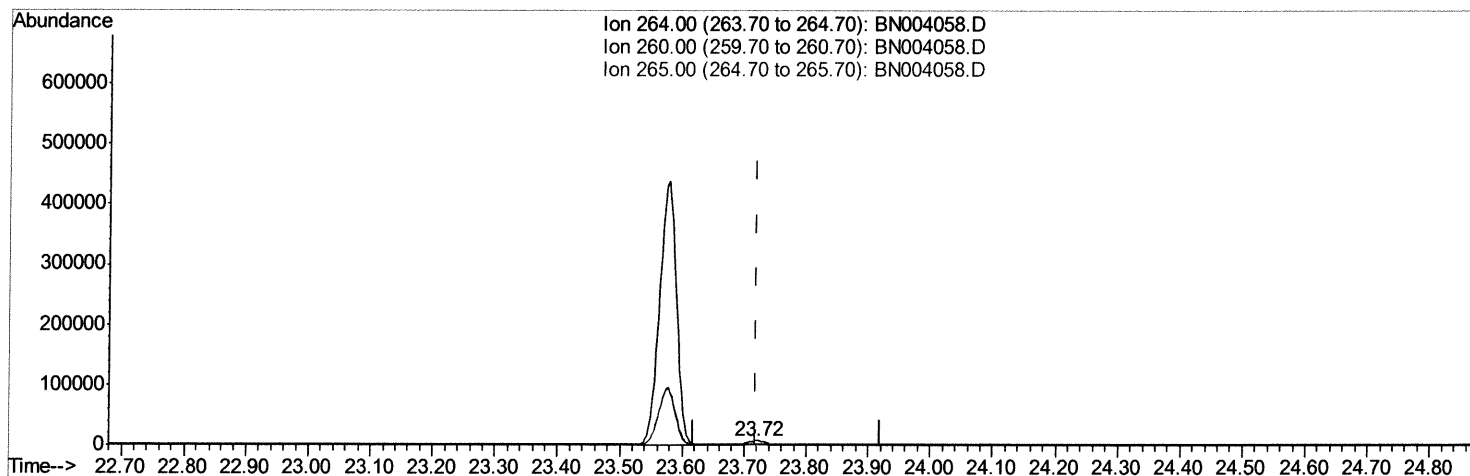

TIC: BN004058.D

(20) Perylene-d12 (I)

23.721min (+0.001) 0.40ng/ul

response 14946

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	28.04
265.00	33.50	35.87
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:28:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

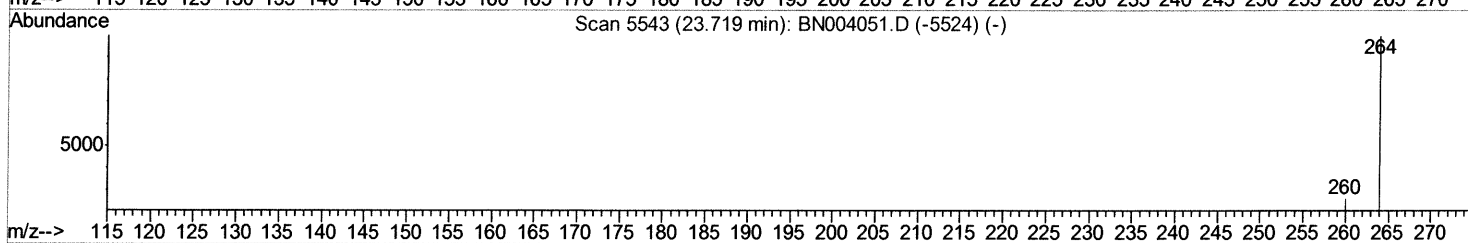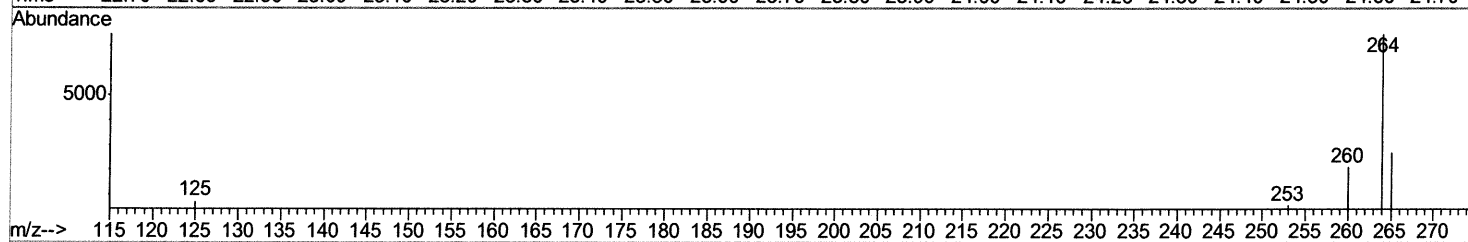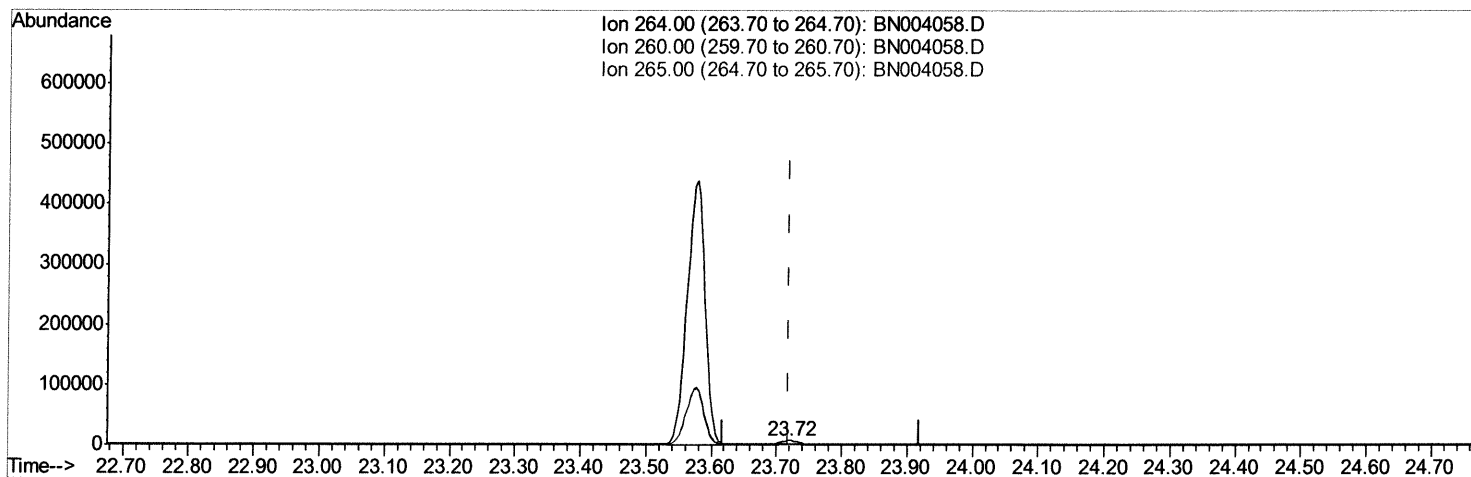

TIC: BN004058.D

(20) Perylene-d12 (I)

23.721min (+0.001) 0.40ng/ul m

response 13477

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	28.04
265.00	33.50	35.87
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

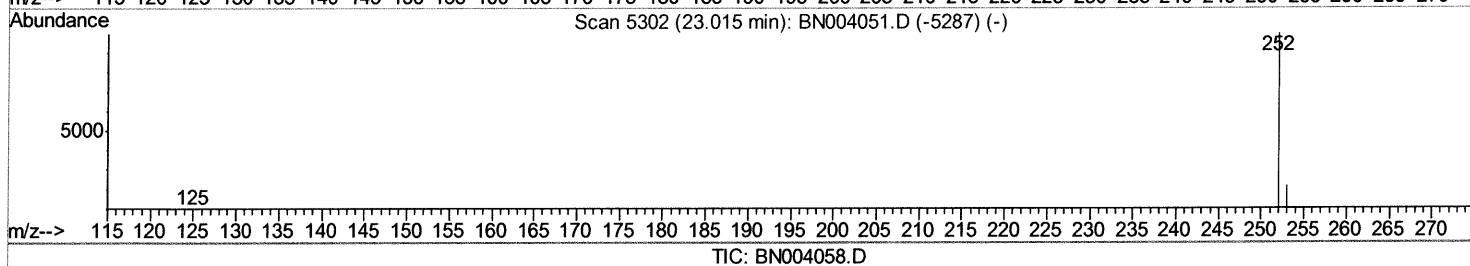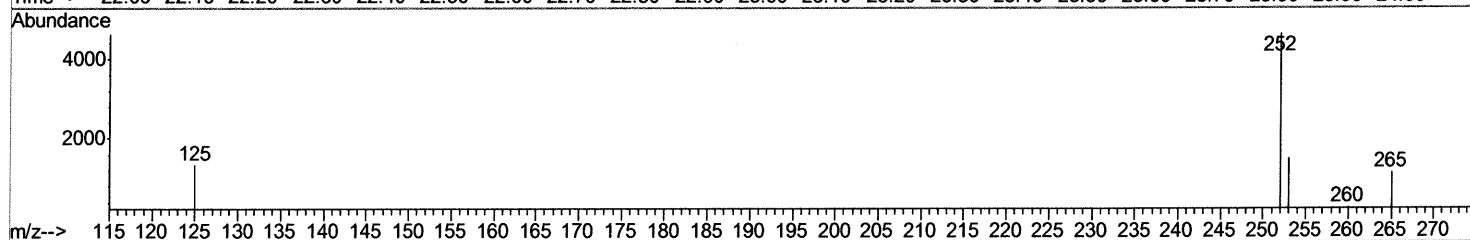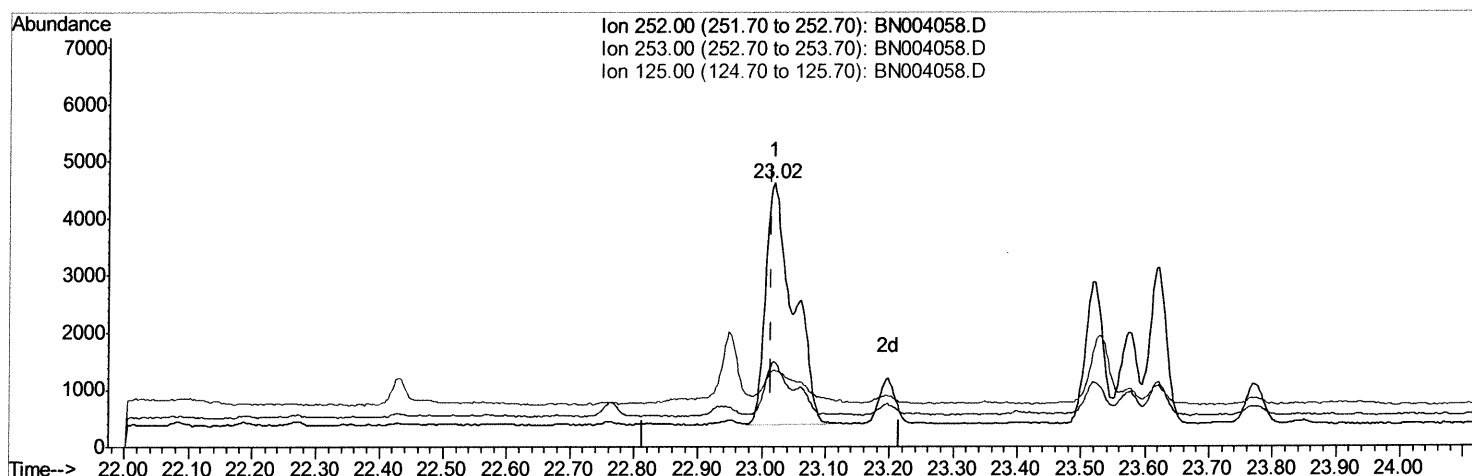

(21) Benzo(b)fluoranthene
23.019min (+0.004) 0.23ng/ul
response 12670

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	32.18
125.00	11.20	28.98#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

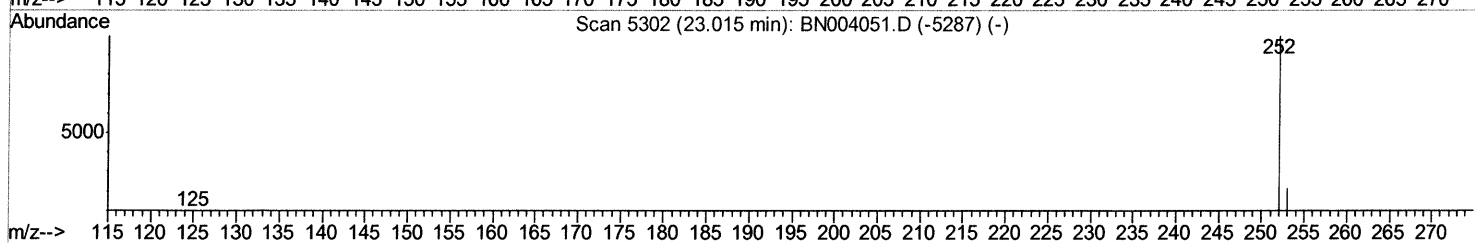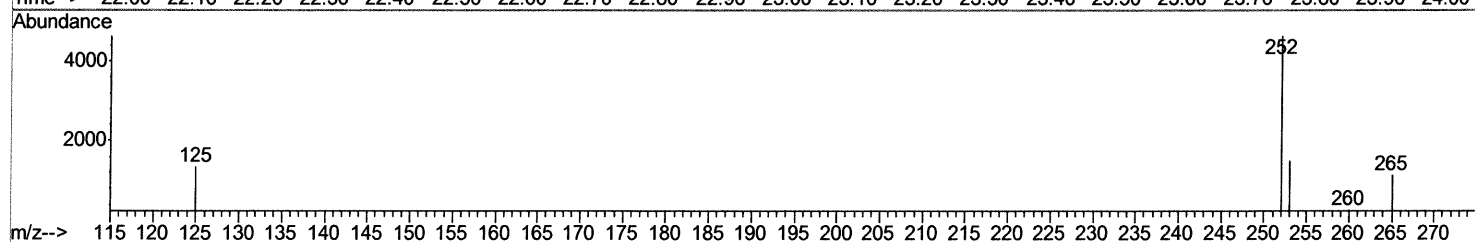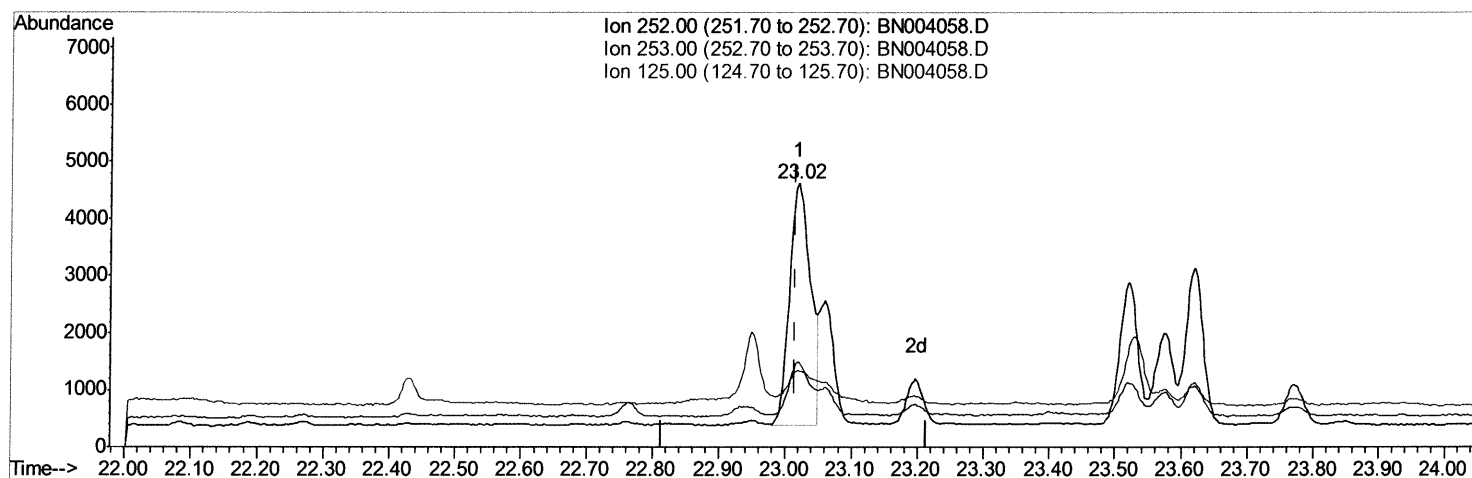

TIC: BN004058.D

(21) Benzo(b)fluoranthene

23.019min (+0.004) 0.17ng/ul m

response 9419

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	32.18
125.00	11.20	28.98#
0.00	0.00	0.00

> 53
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

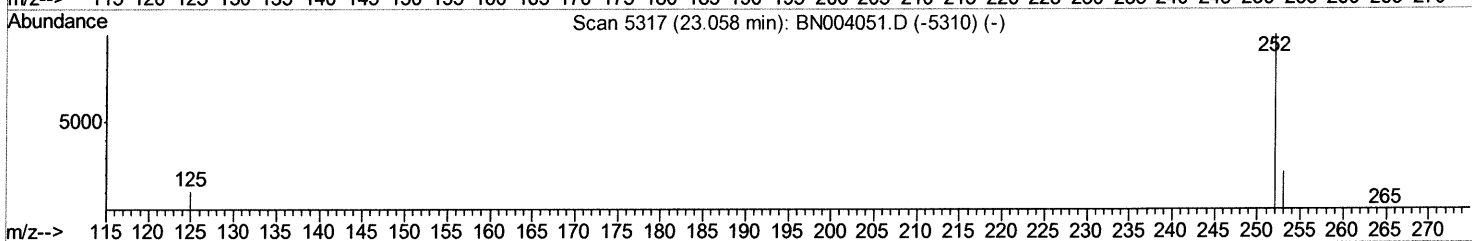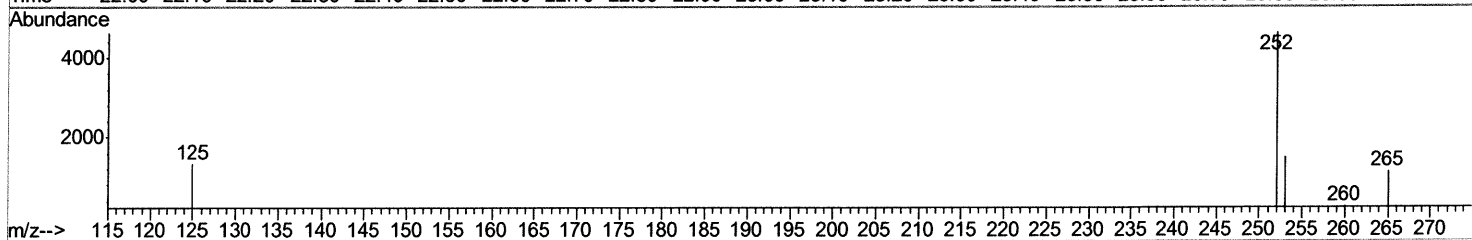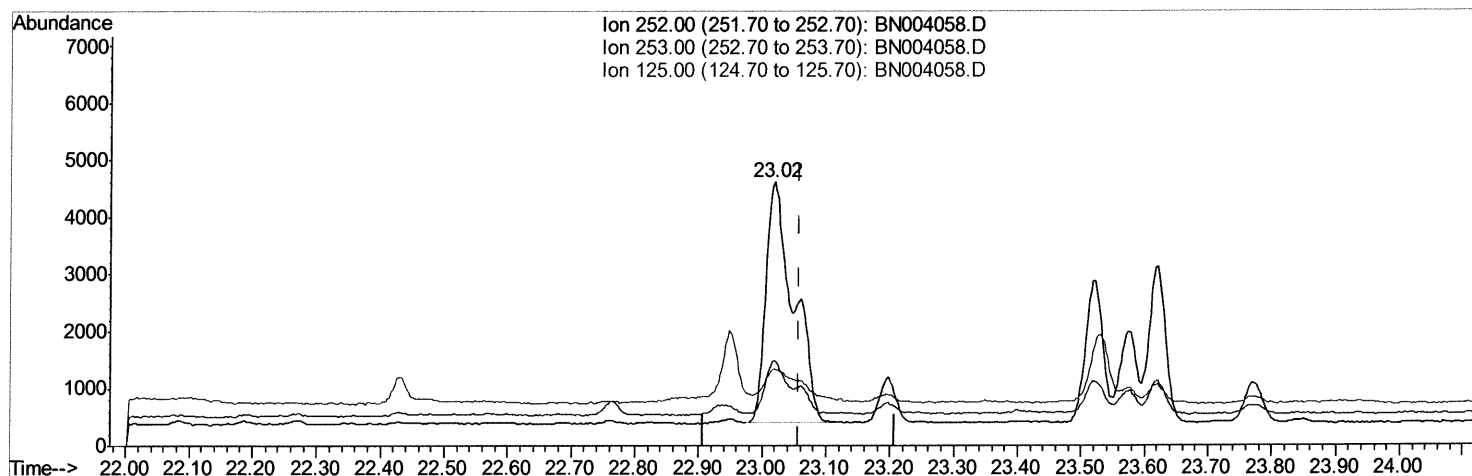

TIC: BN004058.D

(22) Benzo(k)fluoranthene
23.019min (-0.040) 0.23ng/ul
response 12649

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	32.18#
125.00	11.30	28.98#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:29:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

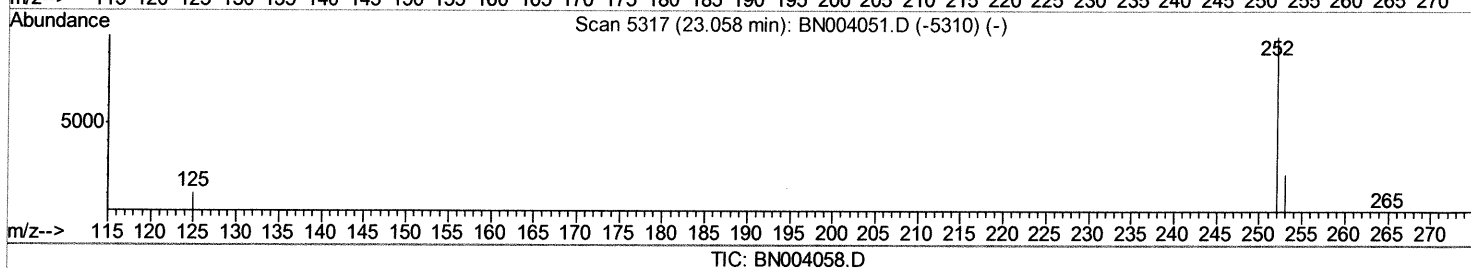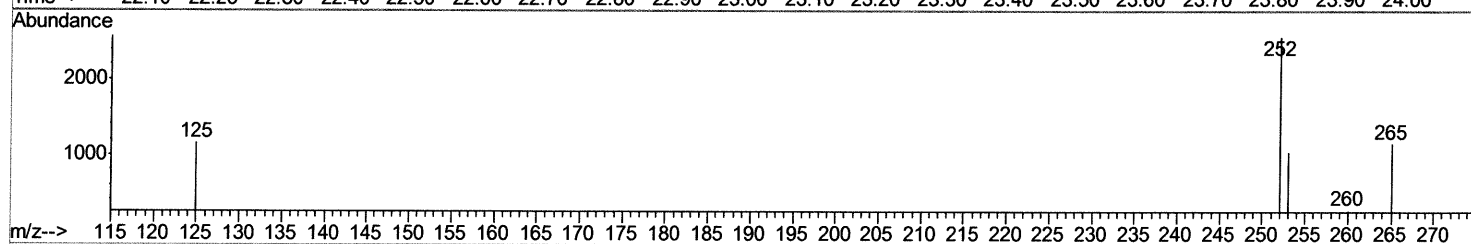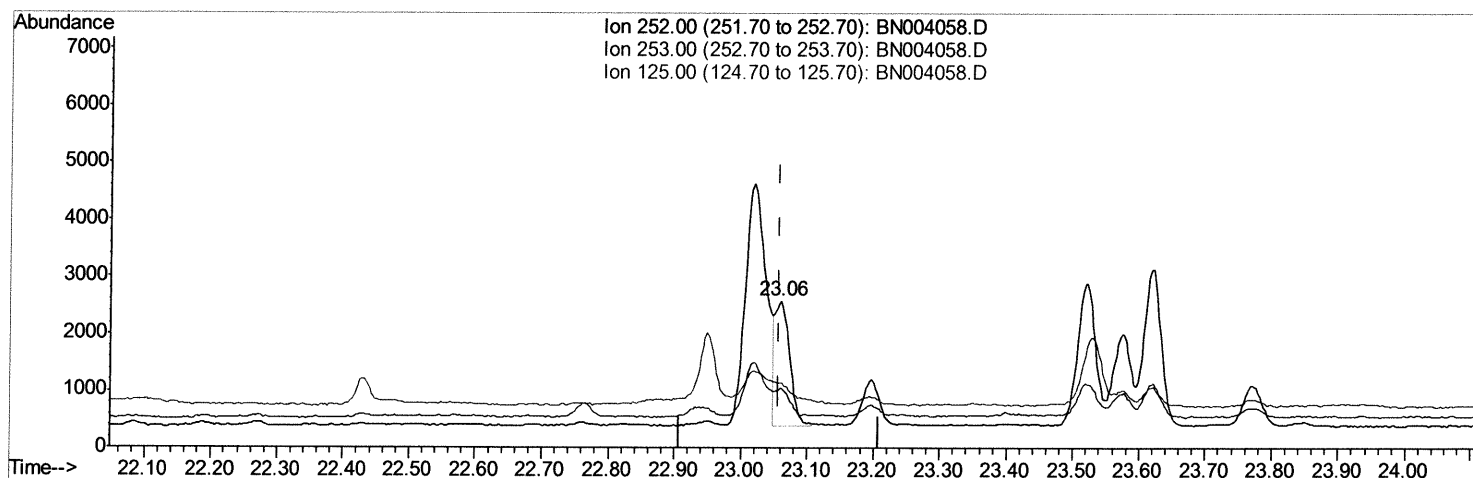

(22) Benzo(k)fluoranthene

23.060min (+0.001) 0.06ng/ul m

response 3321

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	40.73#
125.00	11.30	44.59#
0.00	0.00	0.00

> 55
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)

Data File : BN004058.D
Acq On : 18 Dec 2018 04:24
Operator : JU/SJ
Sample : J6270-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E05

Manual Integrations
APPROVED

Sohil
12/18/2018 5:56:56 PM

Quant Time: Dec 18 07:30:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1611	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8246	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5163	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	13443m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	15396m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	13477m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	3236	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	11281m	0.29	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
7) Acenaphthylene	14.20	152	1083	0.047	ng/ul#	83
12) Phenanthrene	17.26	178	3310	0.075	ng/ul	94
13) Anthracene	17.35	178	1488m	0.041	ng/ul	
15) Fluoranthene	19.28	202	8216m	0.158	ng/ul	
17) Pyrene	19.64	202	8340m	0.151	ng/ul	
18) Benzo(a)anthracene	21.39	228	5745	0.118	ng/ul#	87
19) Chrysene	21.43	228	6562	0.118	ng/ul#	87
21) Benzo(b)fluoranthene	23.02	252	9419m	0.169	ng/ul	
22) Benzo(k)fluoranthene	23.06	252	3321m	0.061	ng/ul	
23) Benzo(a)pyrene	23.62	252	4996	0.103	ng/ul#	64
24) Indeno(1,2,3-cd)pyrene	26.08	276	4109	0.074	ng/ul#	95
25) Dibenzo(a,h)anthracene	26.09	278	1122	0.025	ng/ul#	1
26) Benzo(g,h,i)perylene	26.82	276	2929	0.061	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/18/18