

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)


Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:55:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

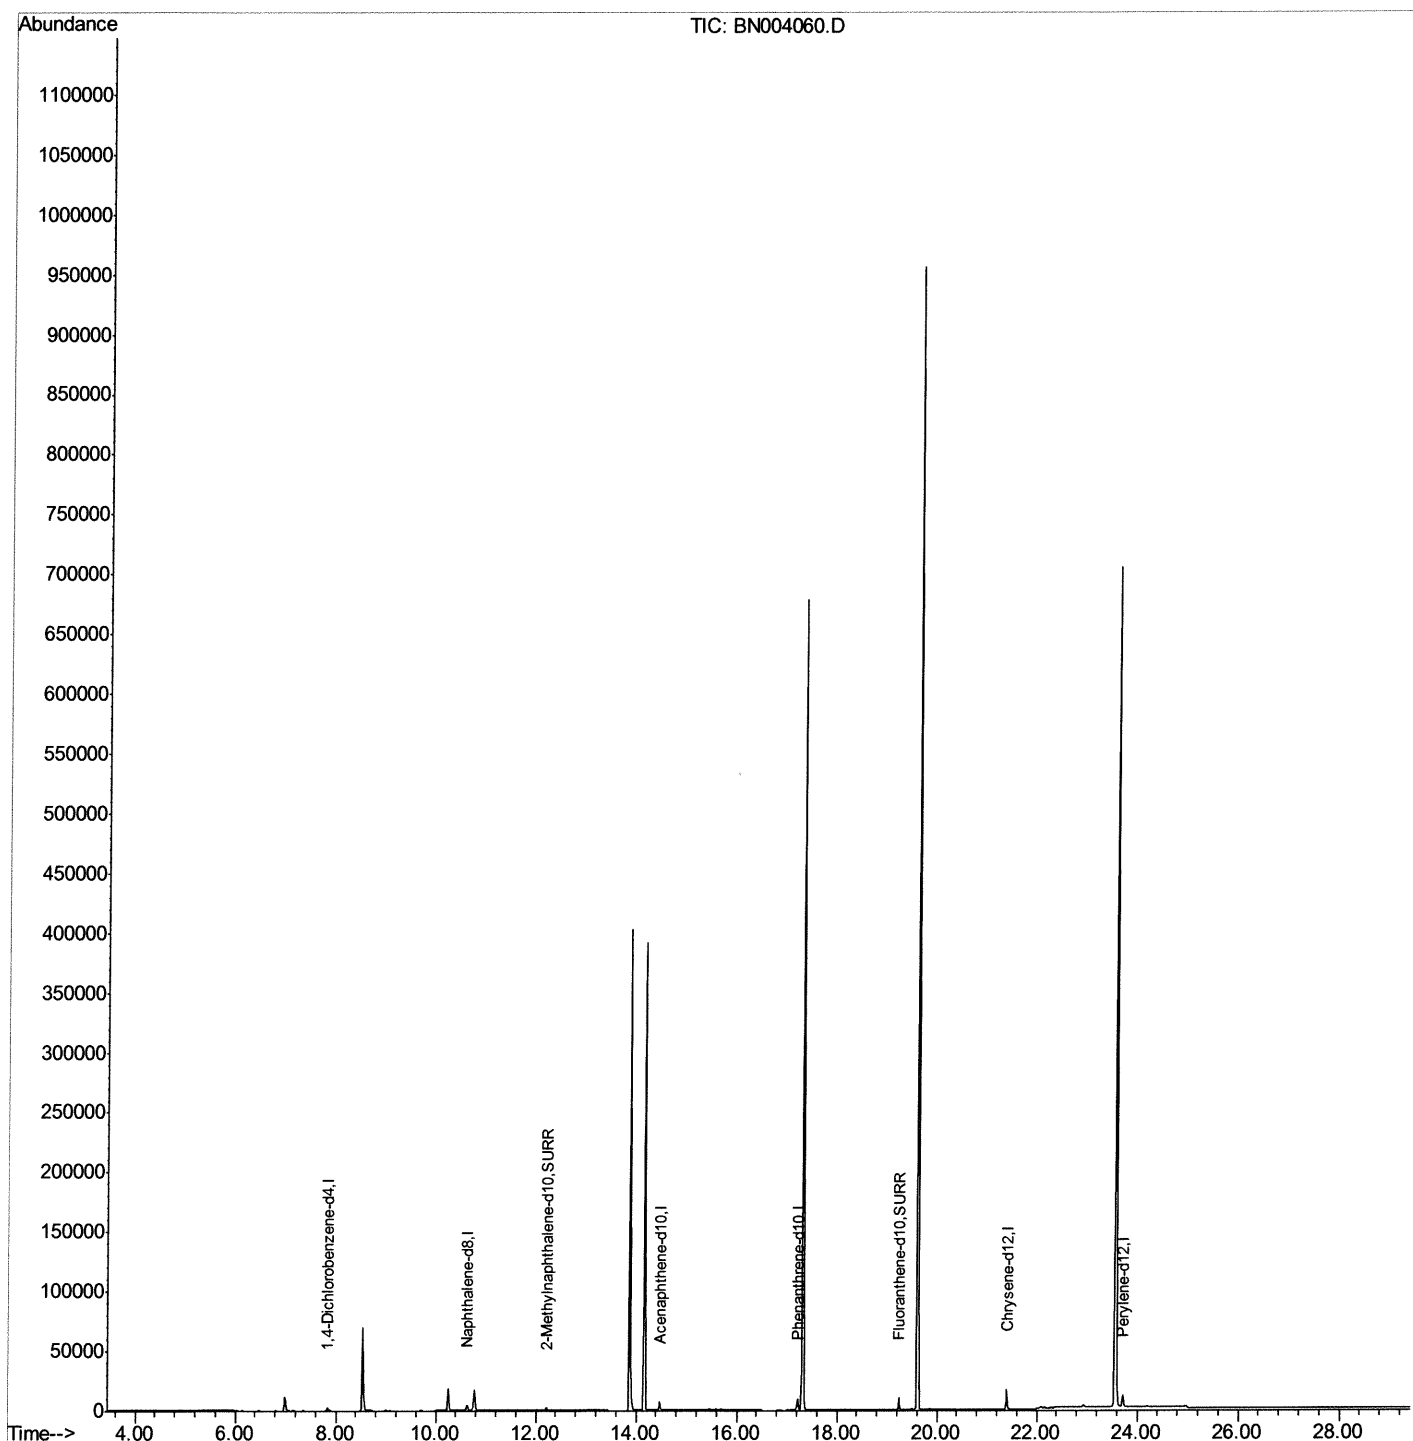

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 06:39:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

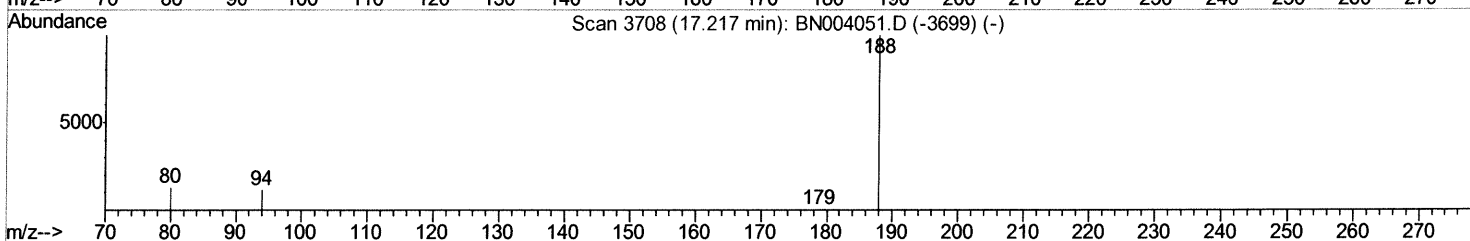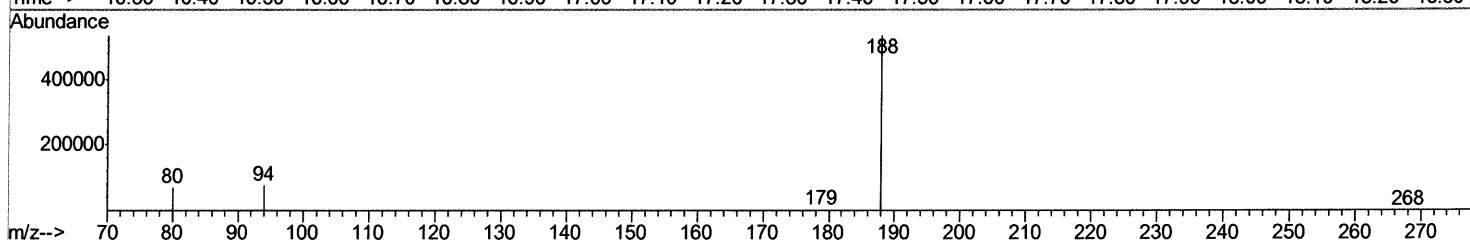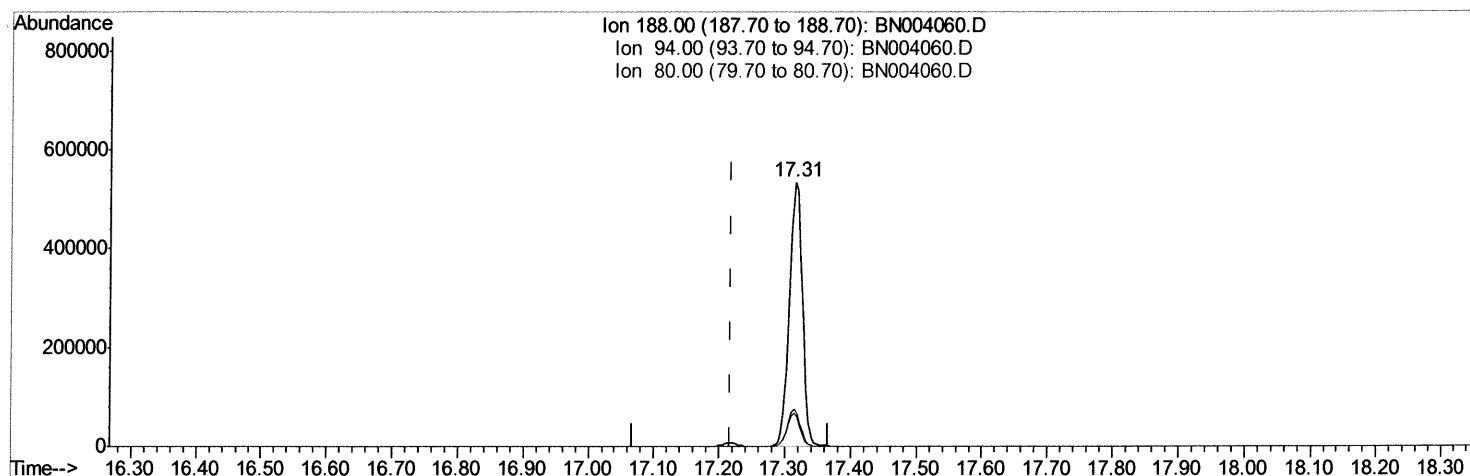

TIC: BN004060.D

(10) Phenanthrene-d10 (I)
17.314min (+0.097) 0.40ng/ul
response 727474

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.11#
80.00	11.60	12.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 06:39:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

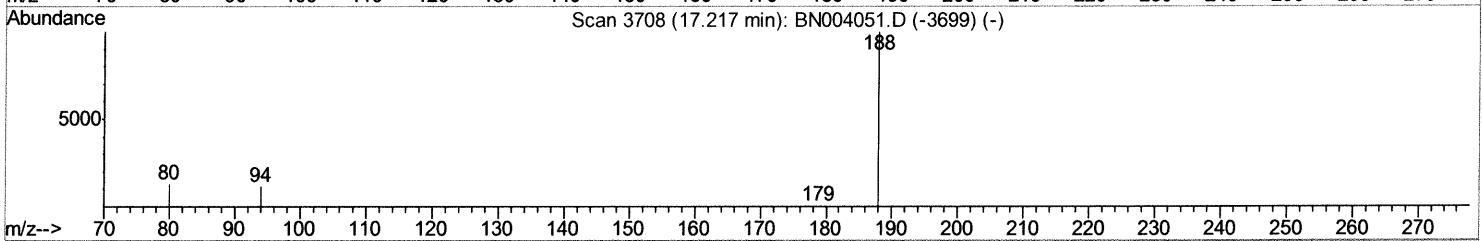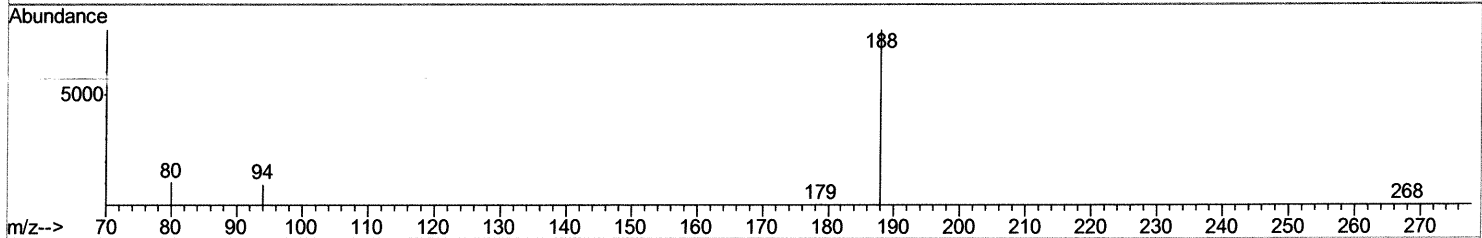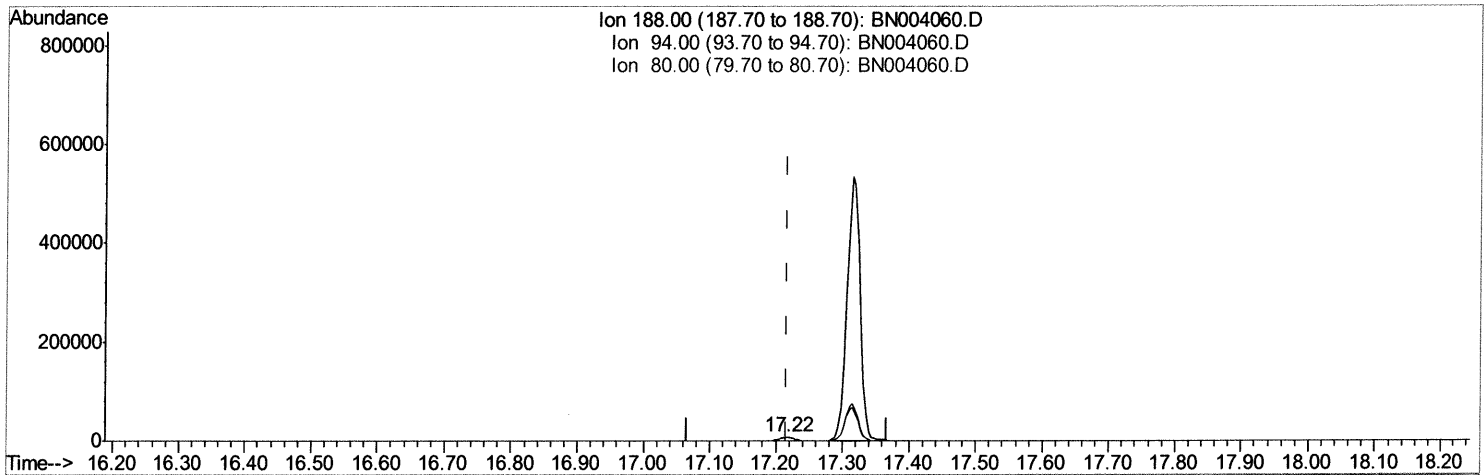

TIC: BN004060.D

(10) Phenanthrene-d10 (I)

17.217min (+0.000) 0.40ng/ul m

response 11113

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.49#
80.00	11.60	13.39
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

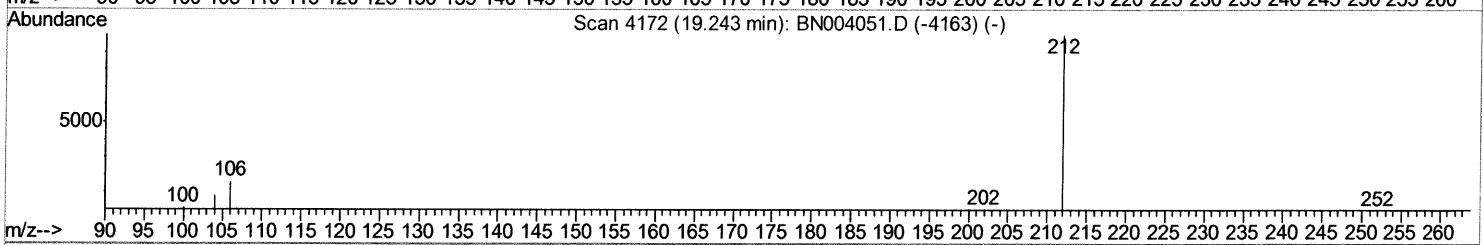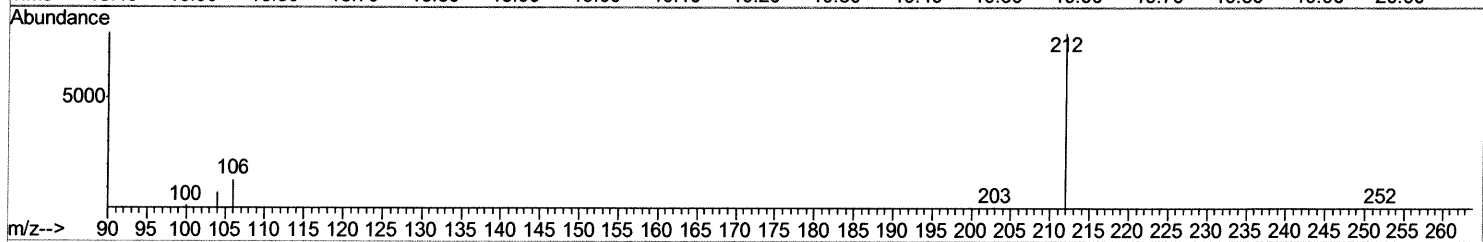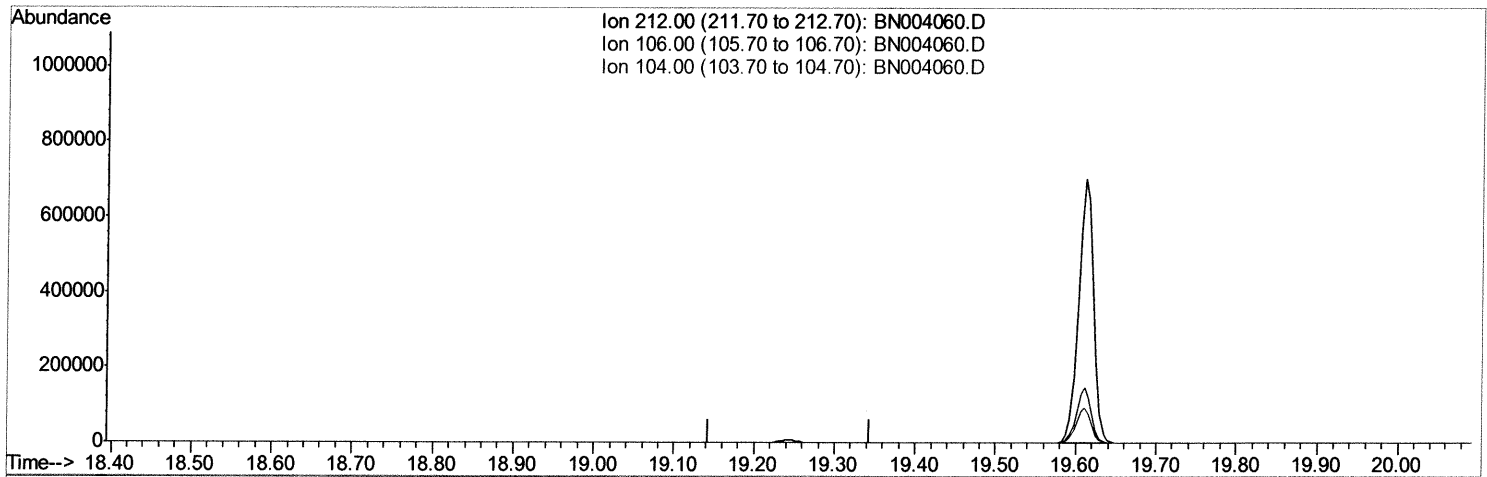

TIC: BN004060.D

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

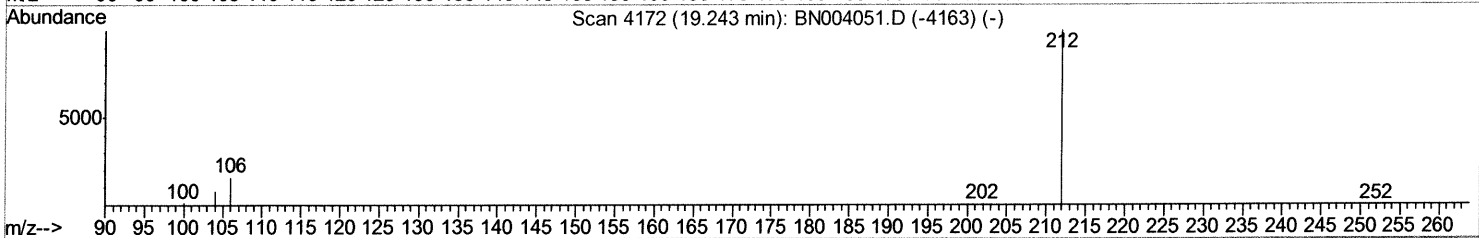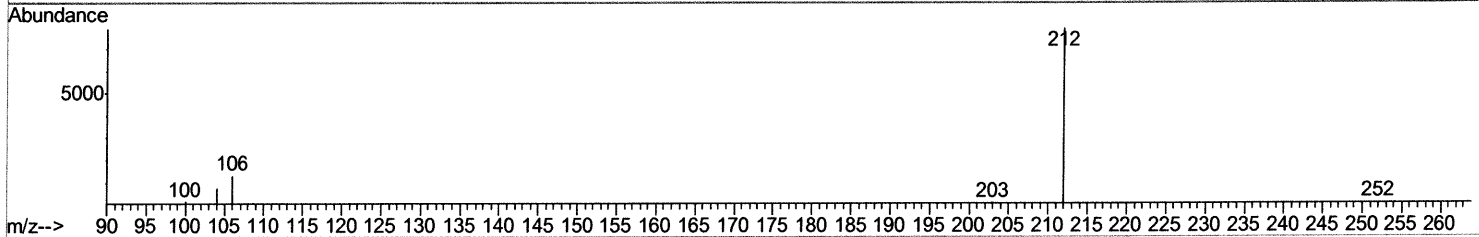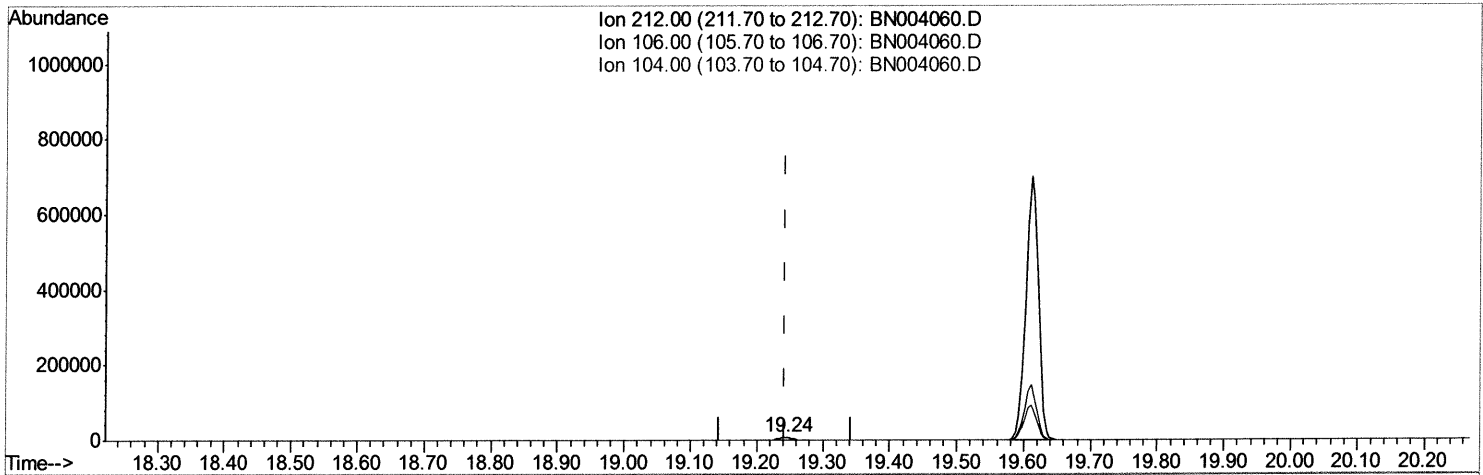

TIC: BN004060.D

(14) Fluoranthene-d10 (SURR)

19.243min (+0.000) 0.32ng/ul m

response 10340

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

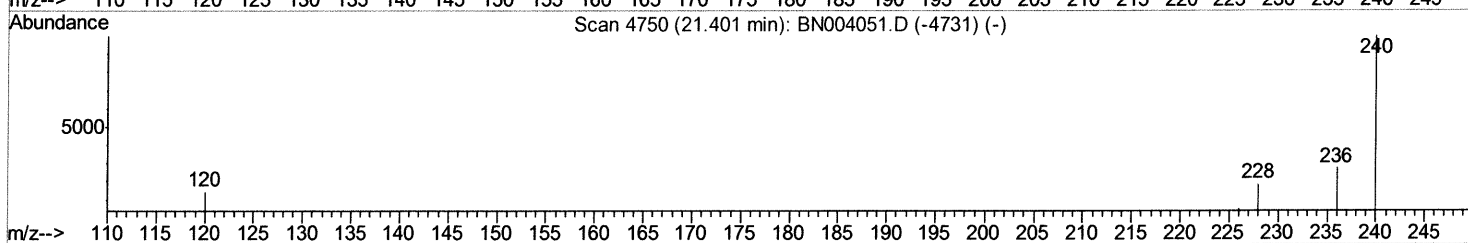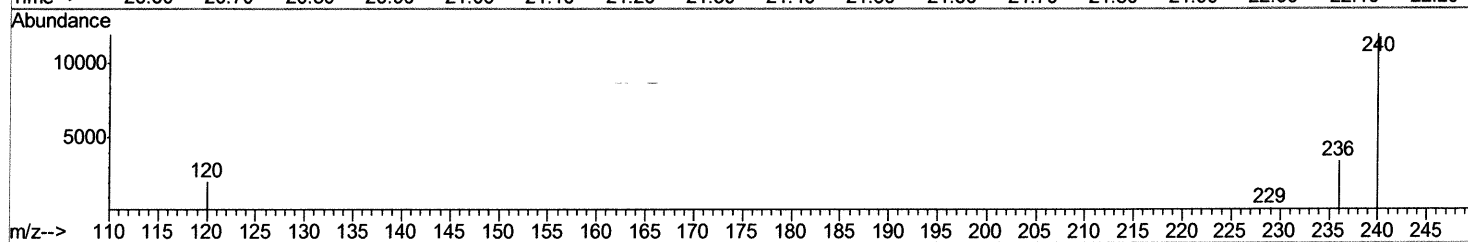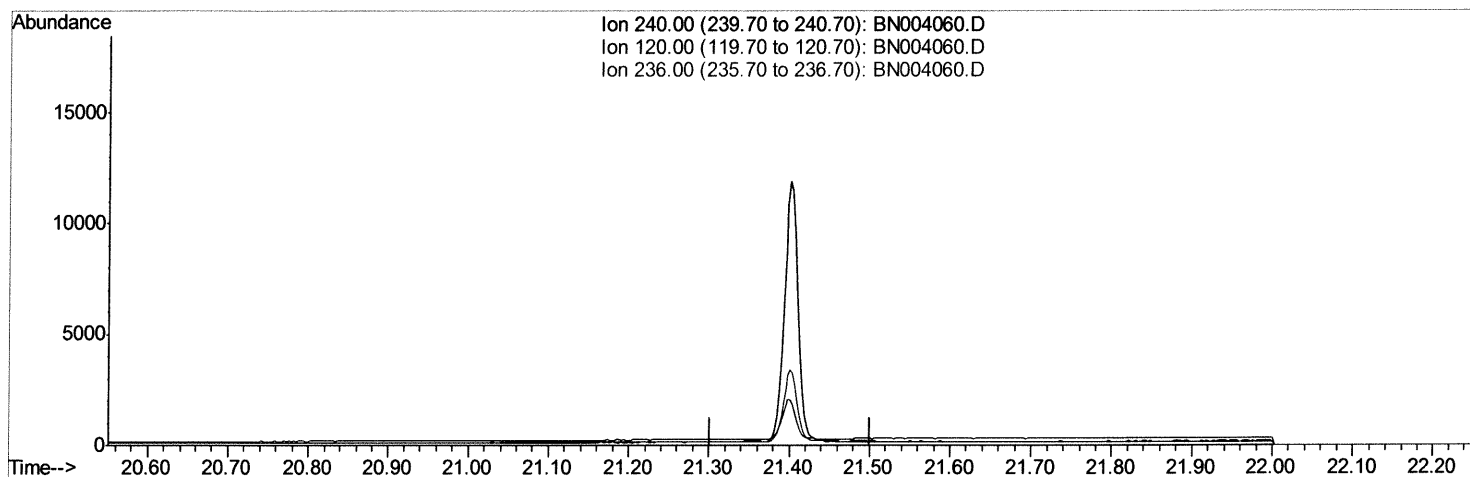

TIC: BN004060.D

(16) Chrysene-d12 (I)

21.401min (-21.401) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.00	0.00#
236.00	27.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

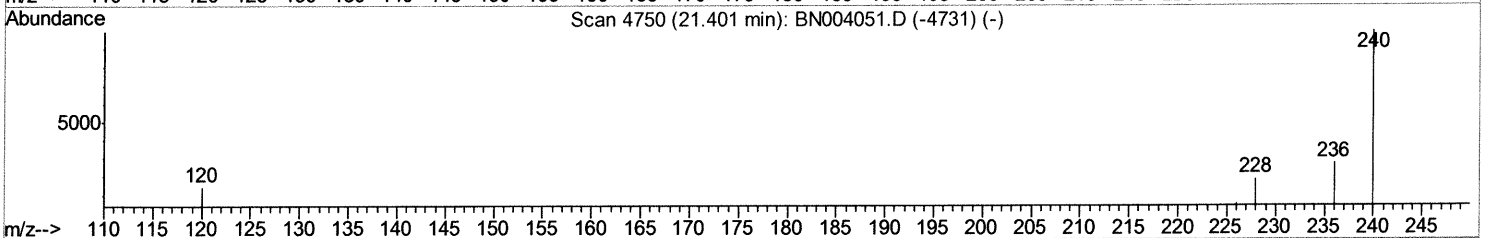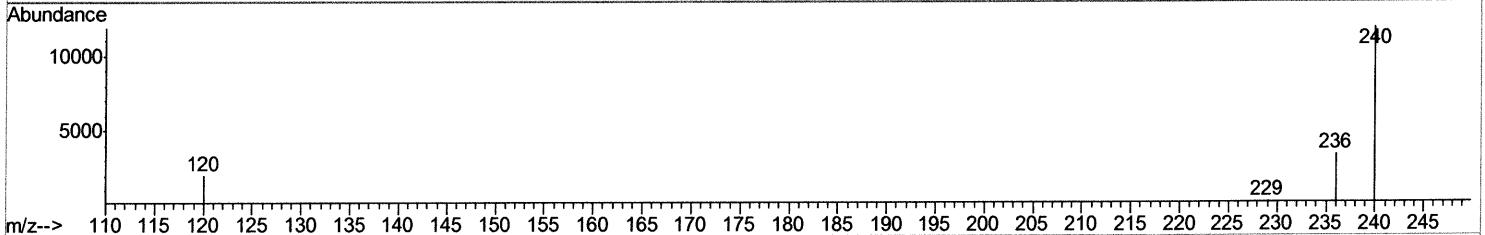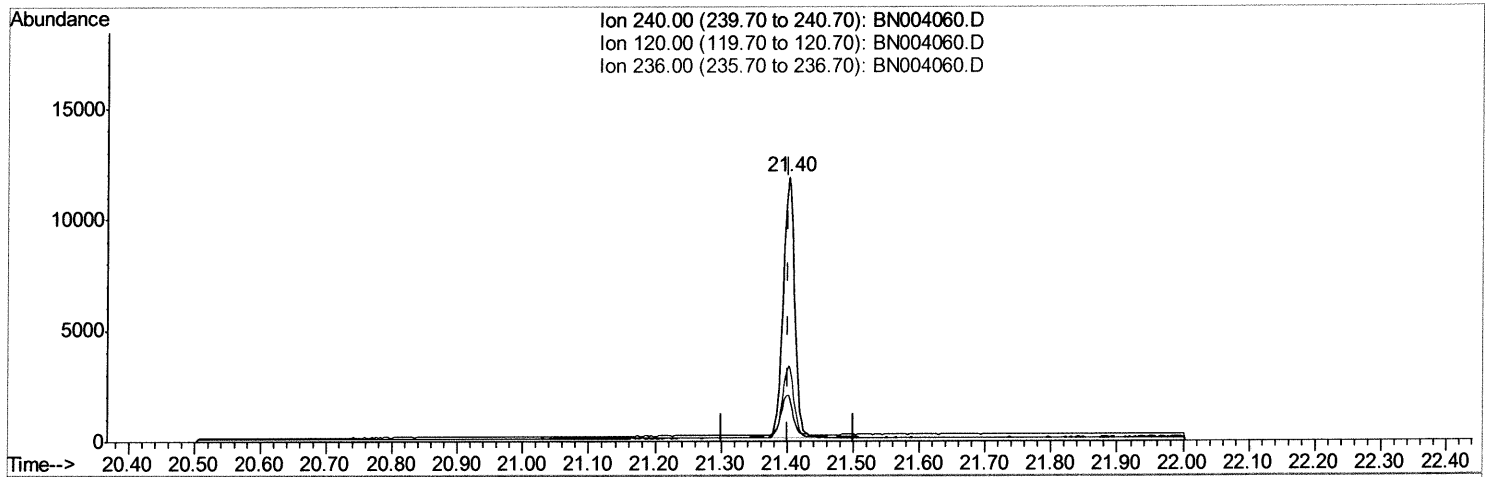

TIC: BN004060.D

(16) Chrysene-d12 (I)

21.401min (+0.000) 0.40ng/ul m

response 14260

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	17.25#
236.00	27.60	28.74
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

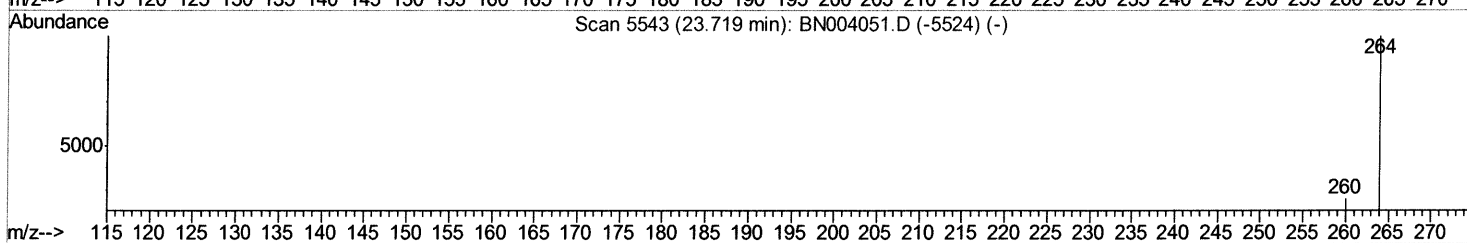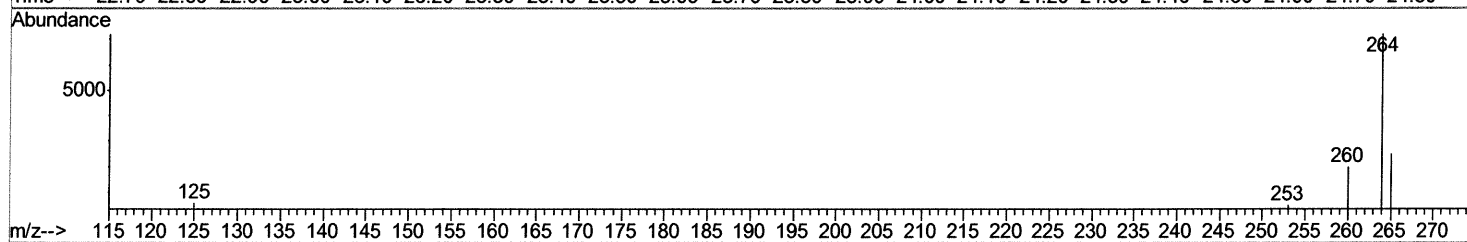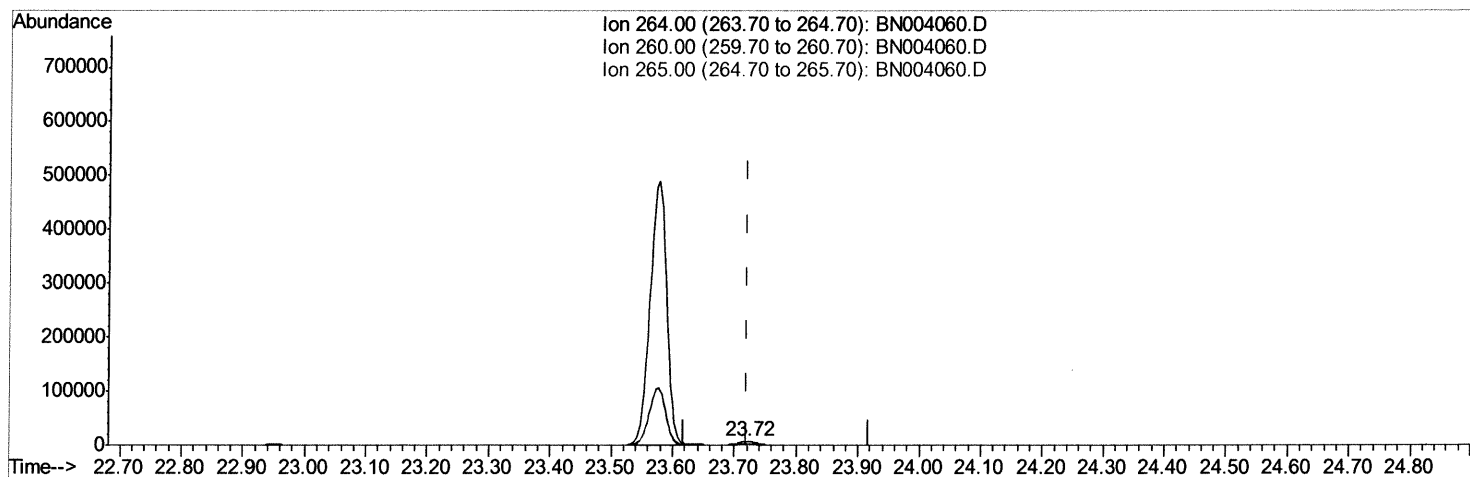

TIC: BN004060.D

(20) Perylene-d12 (I)

23.722min (+0.003) 0.40ng/ul

response 14322

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.22
265.00	33.50	34.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (Qedit)




Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:53:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

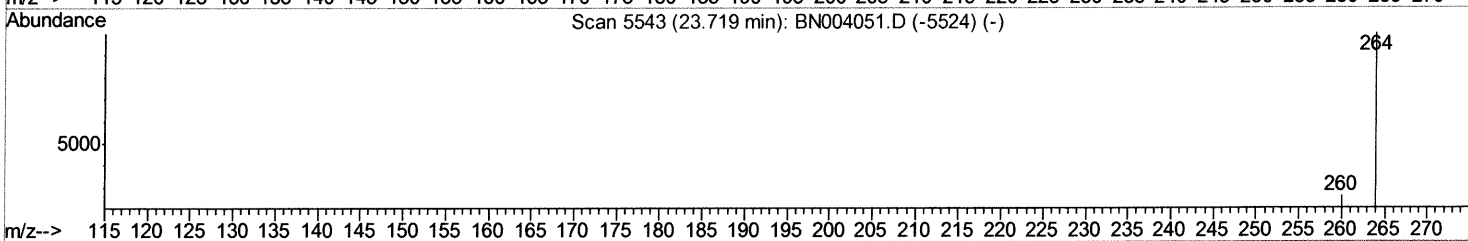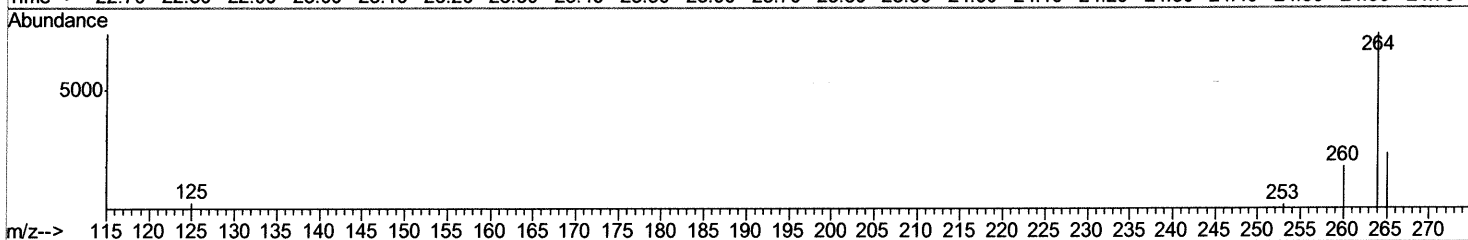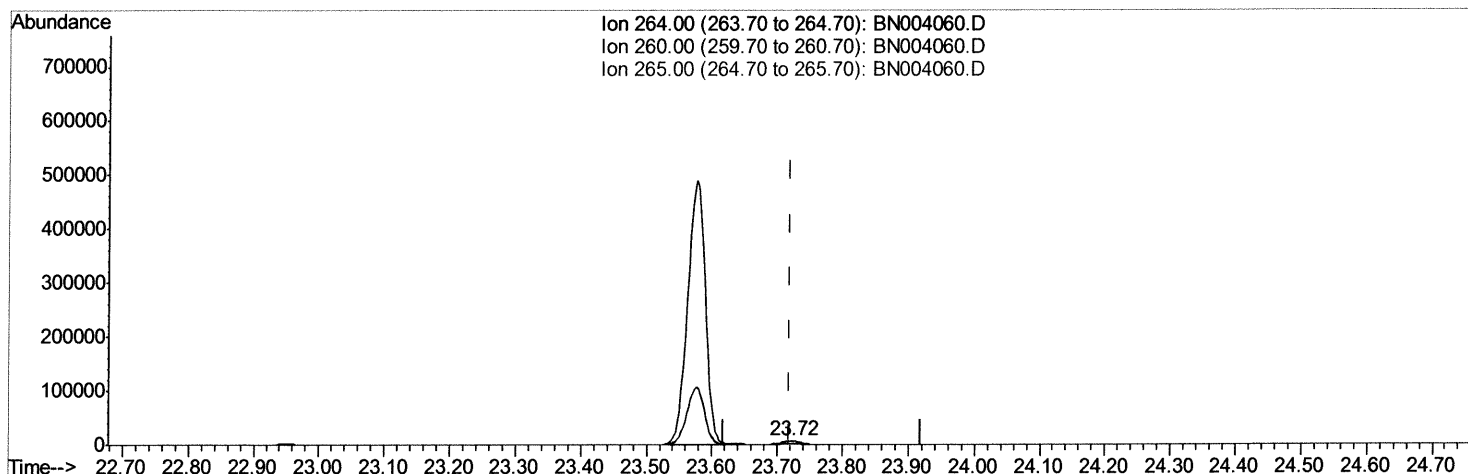

TIC: BN004060.D

(20) Perylene-d12 (I)

23.722min (+0.003) 0.40ng/ul m

response 12754

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.22
265.00	33.50	34.98
0.00	0.00	0.00

> SJ
12/18/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121718\
Quantitation Report (QT Reviewed)

Data File : BN004060.D
Acq On : 18 Dec 2018 05:34
Operator : JU/SJ
Sample : J6270-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9E07

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:00 PM

Quant Time: Dec 18 07:55:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1110	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	6161	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	4098	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	11113m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	14260m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	12754m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.22	152	2615	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	10340m	0.32	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
12/18/18