

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:33:56 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 18 06:35:27 2018

Response via : Initial Calibration

Instrument :

BNA_N

Client Sampled :


F9E13

Manual Integrations

APPROVED

Sohil

12/18/2018 5:57:23 PM

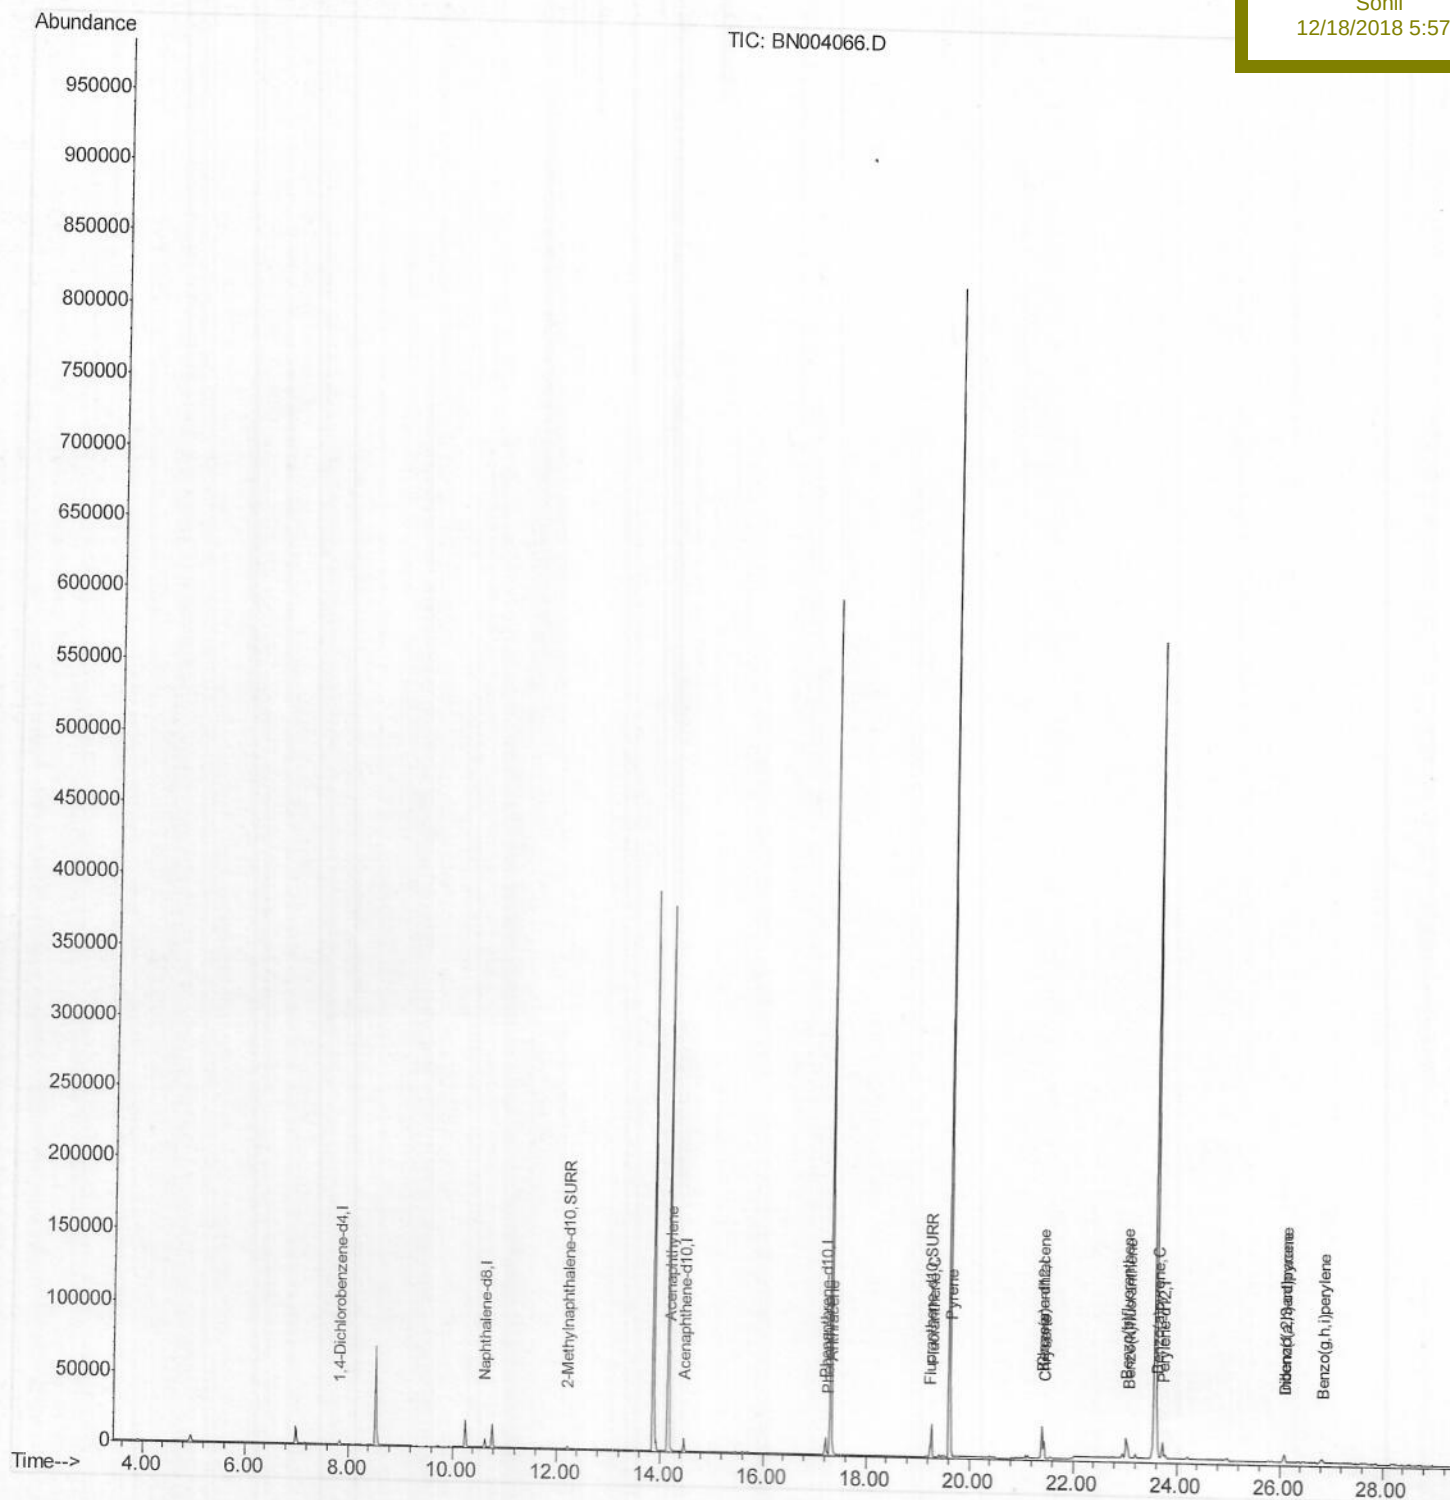

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Quant Time: Dec 18 11:27:42 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

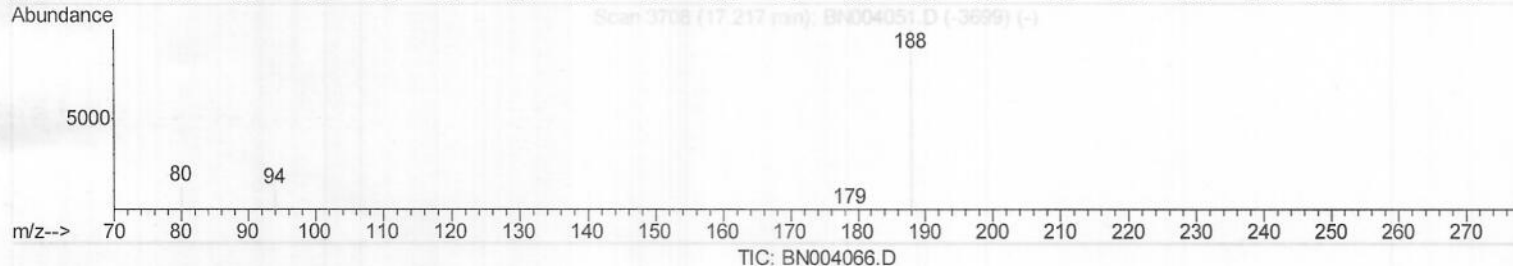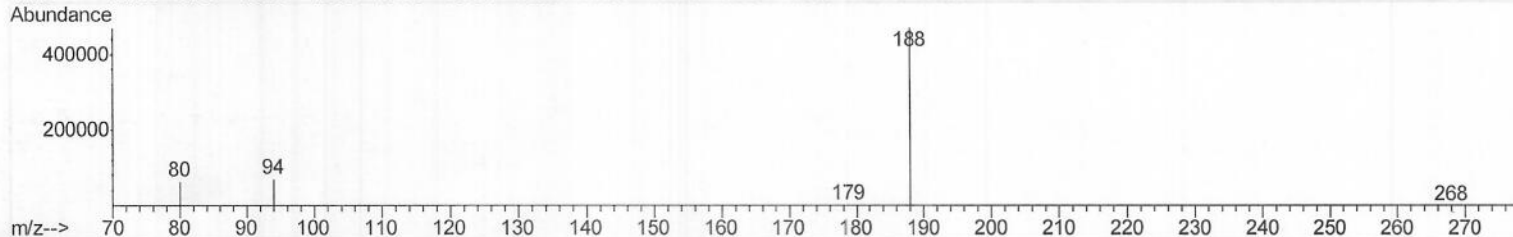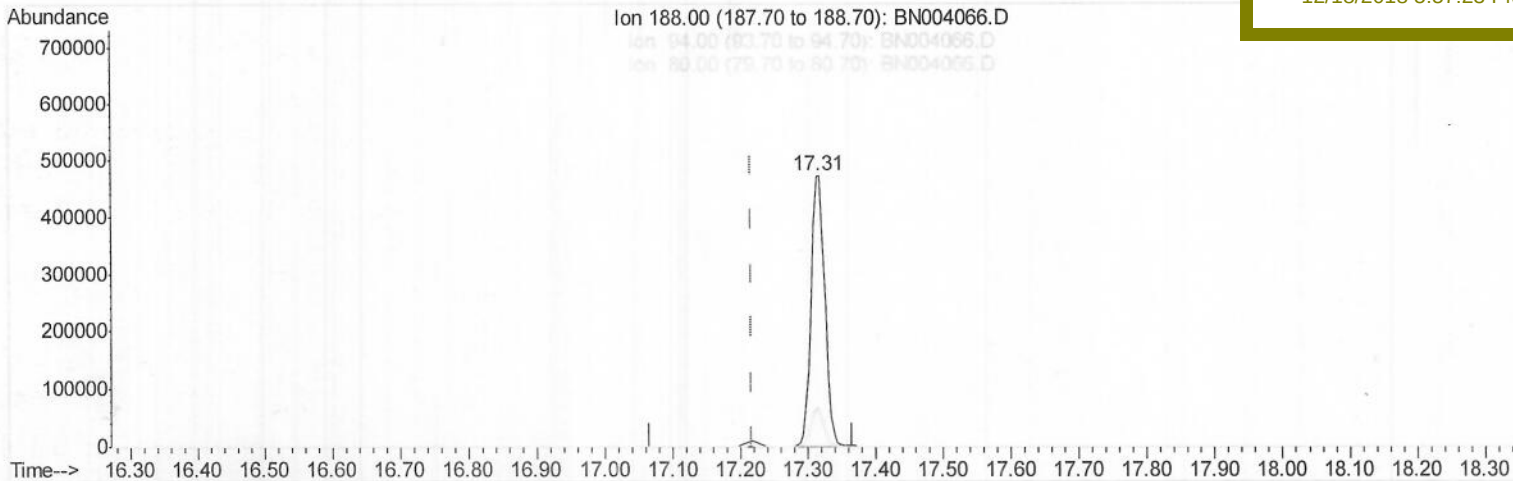

(10) Phenanthrene-d10 (I)
 17.314min (+0.097) 0.40ng/ul
 response 658541

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.40#
80.00	11.60	13.09
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:33:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
ClientSampleId :
 F9E13

Manual Integrations
APPROVED

Sohil
 12/18/2018 5:57:23 PM

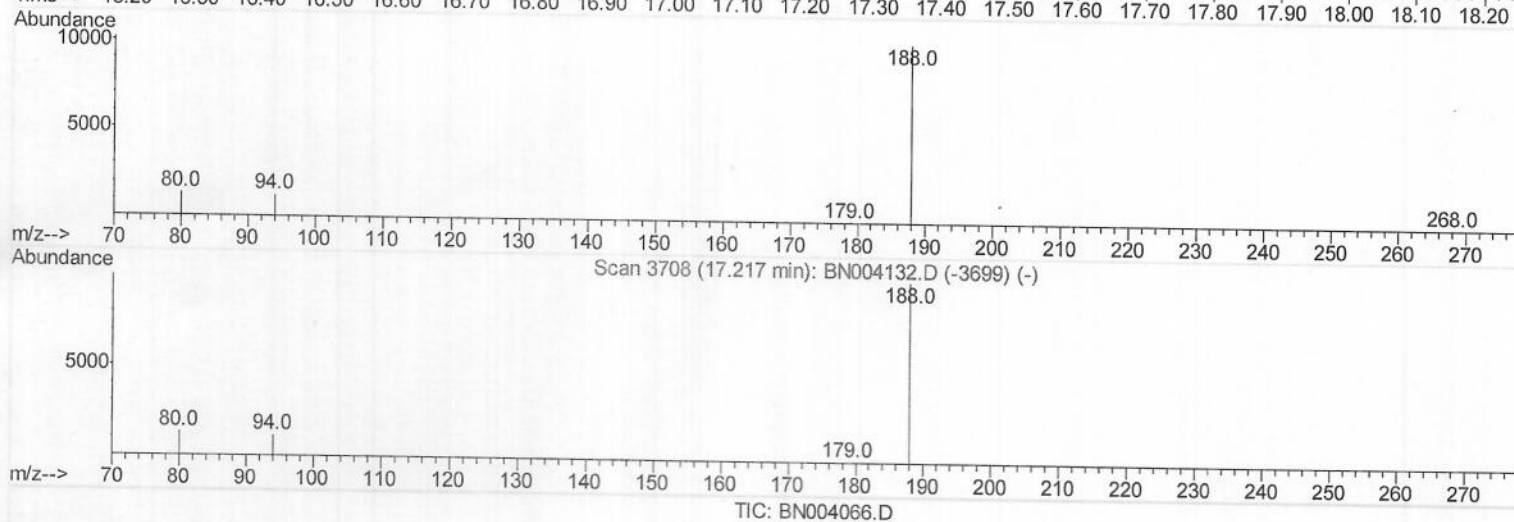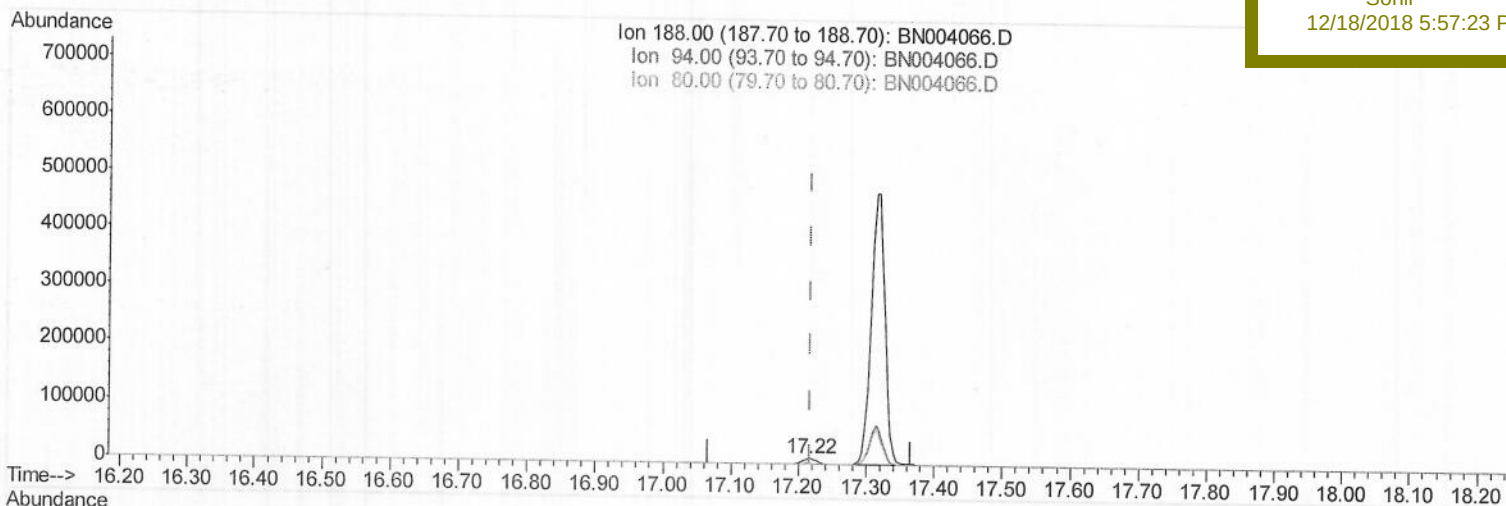

(10) Phenanthrene-d10 (I)

17.217min (-0.000) 0.40ng/ul m

response 14054

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	12.24
80.00	11.60	13.27
0.00	0.00	0.00

SJ
12/18/18


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
F9E13

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

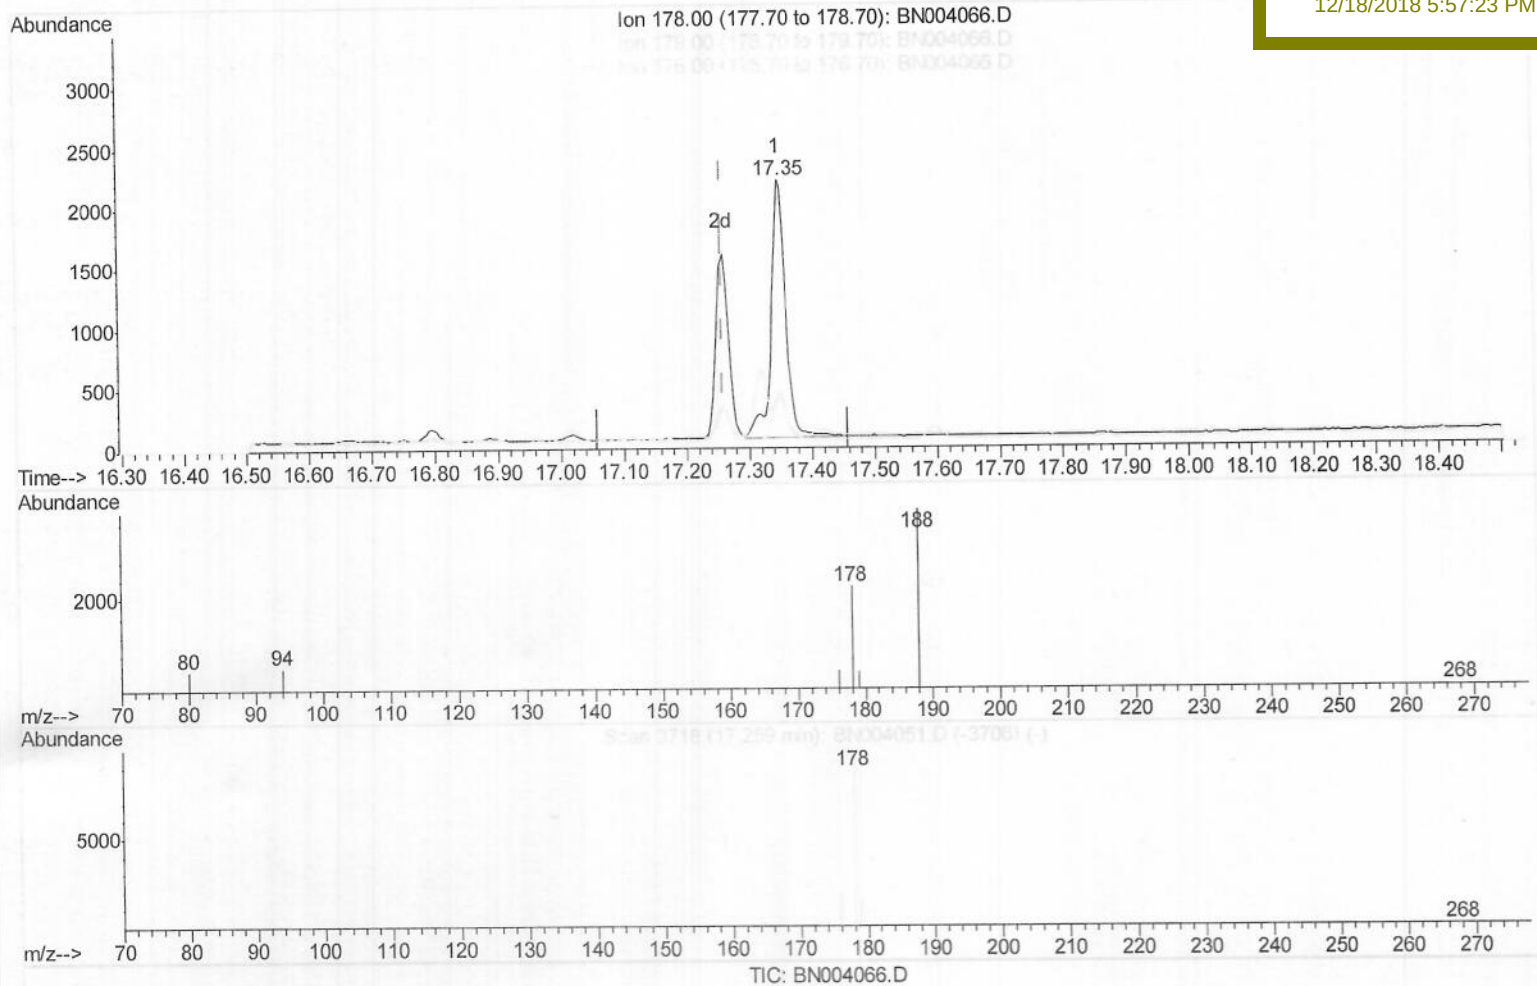

(12) Phenanthrene

17.347min (+0.088) 0.08ng/ul

response 3468

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	18.65
176.00	18.70	20.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :

BNA_N


ClientSampleId :

F9E13

Quant Time: Dec 18 11:28:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

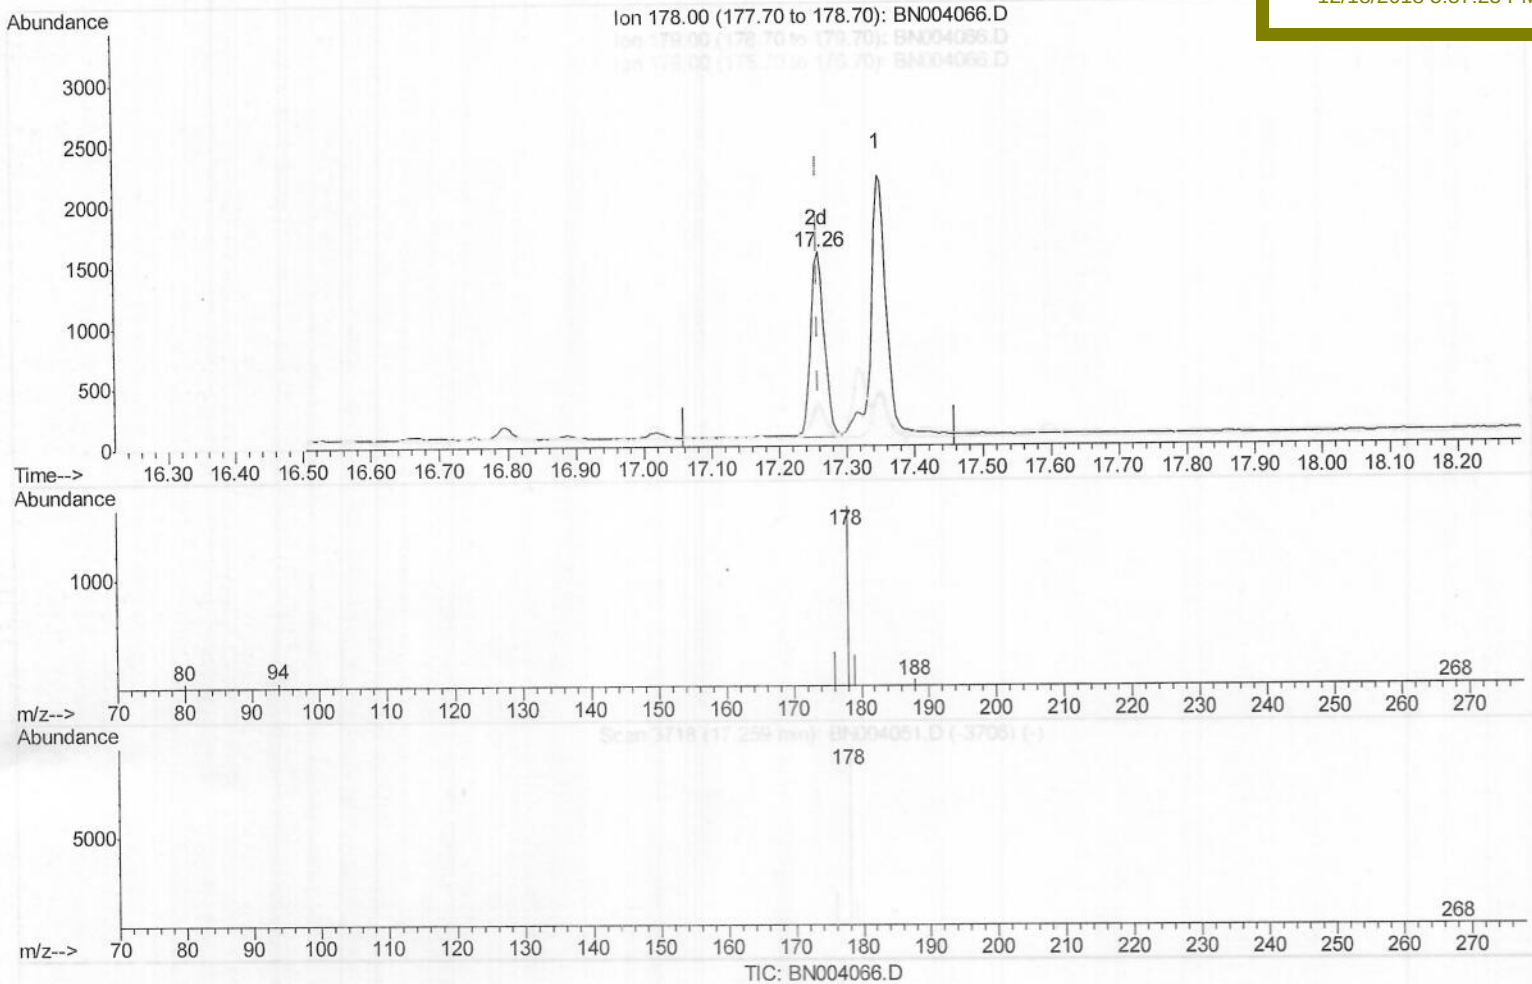

(12) Phenanthrene

17.259min (-0.000) 0.05ng/ul m

response 2161

Ion	Exp%	Act%
178.00	100	100
179.00	15.60	19.88#
176.00	18.70	21.81
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 Client Sampled :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

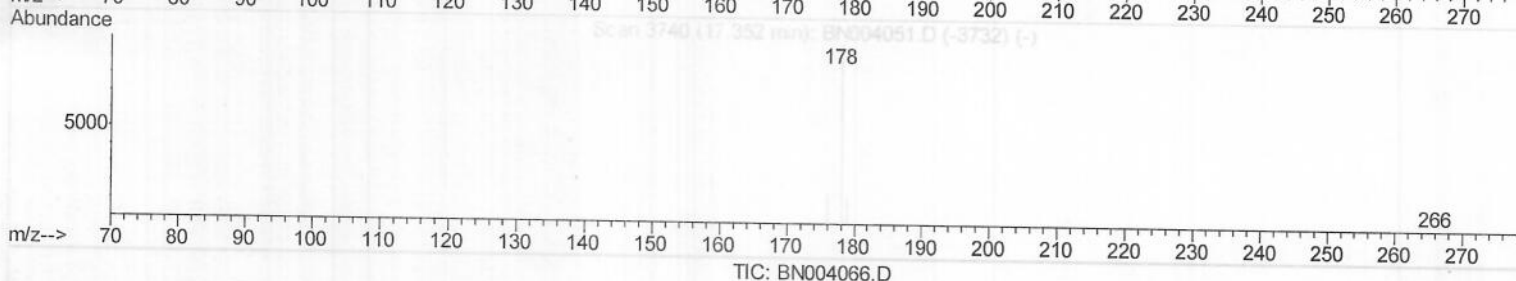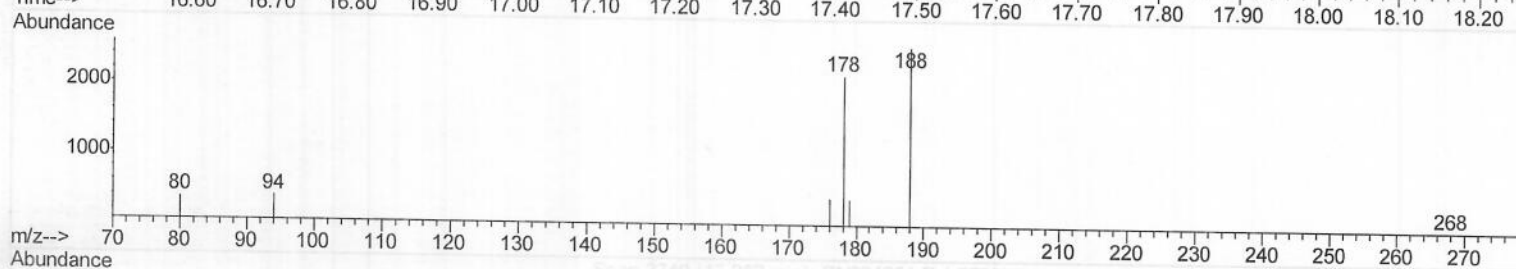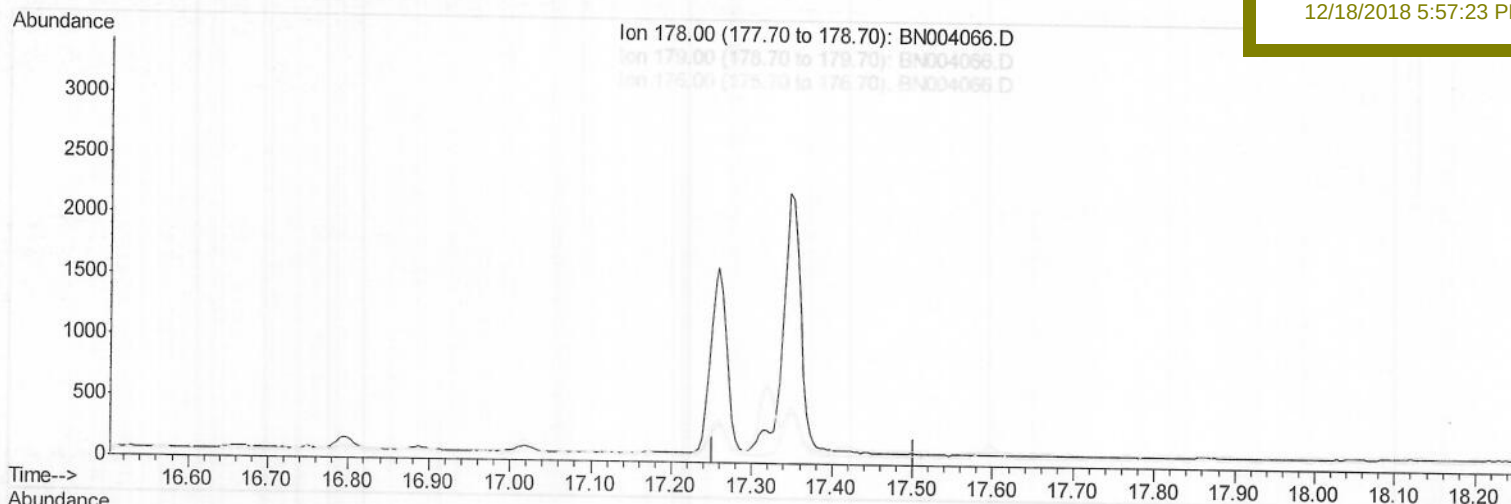

(13) Anthracene

17.352min (-17.352) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	15.40	0.00#
176.00	18.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
ClientSampleId :
 F9E13

Manual Integrations
APPROVED

Sohil
 12/18/2018 5:57:23 PM

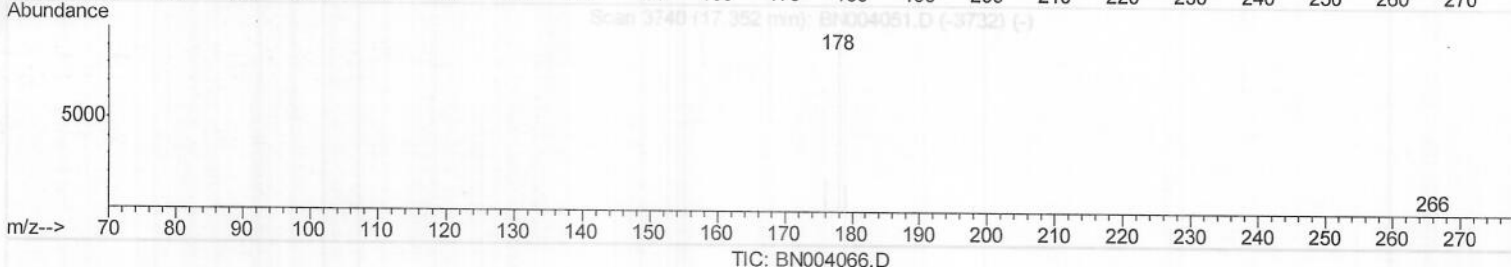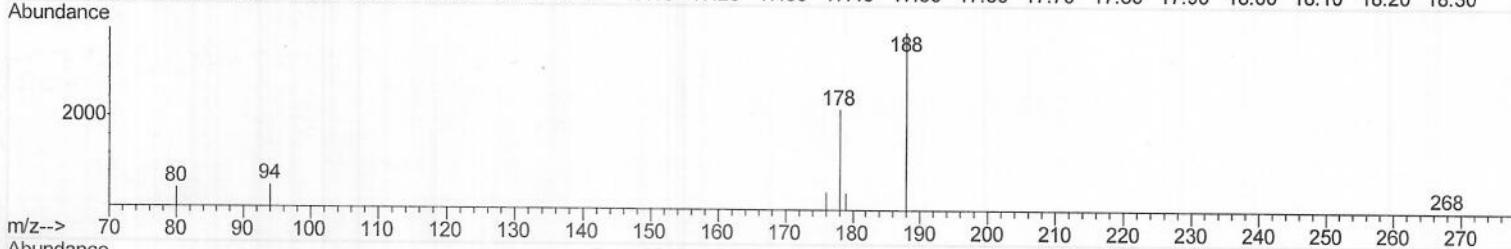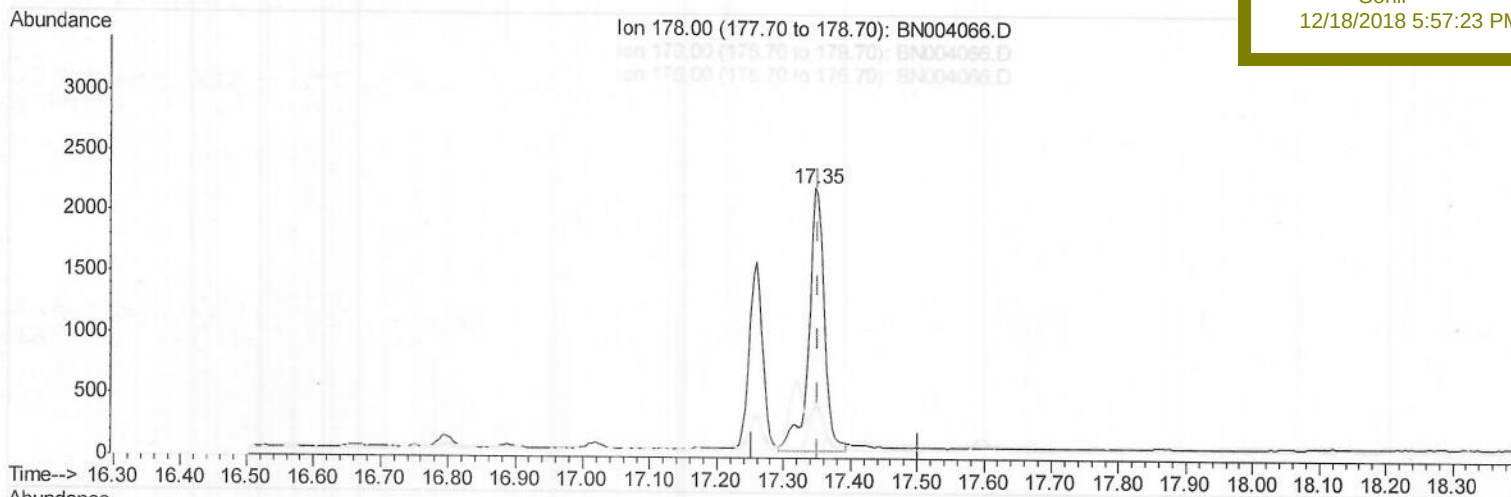

(13) Anthracene

17.347min (-0.005) 0.09ng/ul m

response 3482

Ion	Exp%	Act%
178.00	100	100
179.00	15.40	18.65#
176.00	18.50	20.60
0.00	0.00	0.00

SJ
 12/18/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

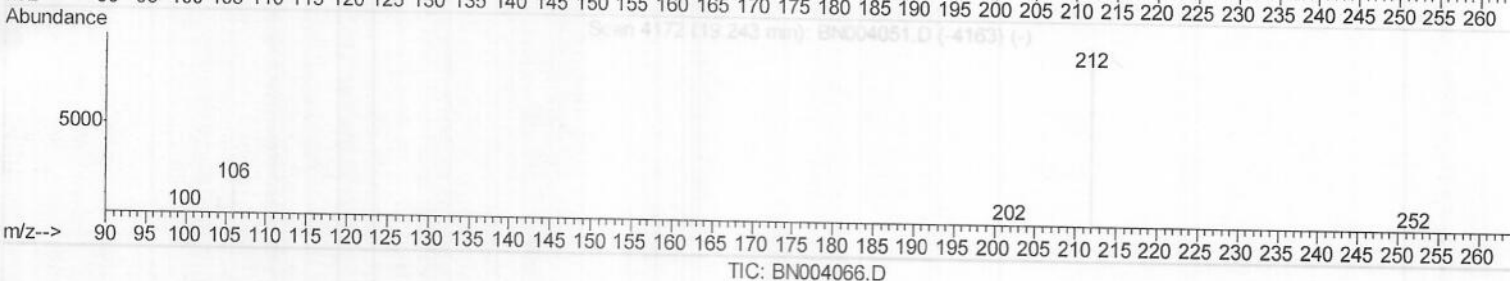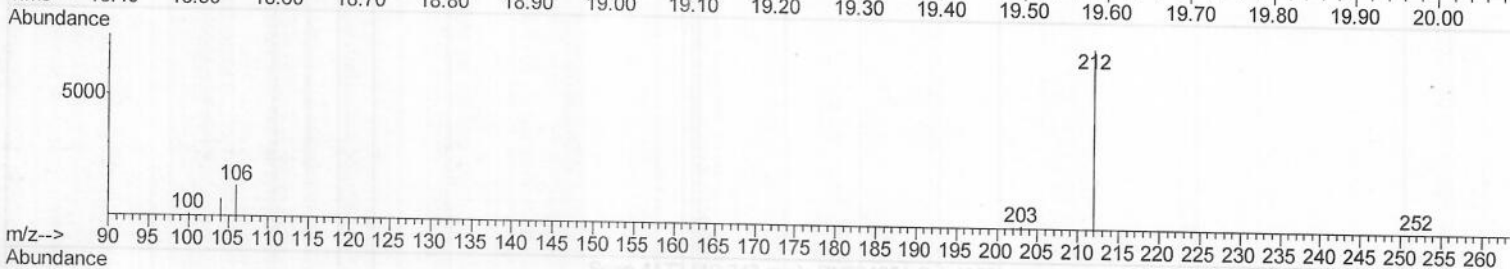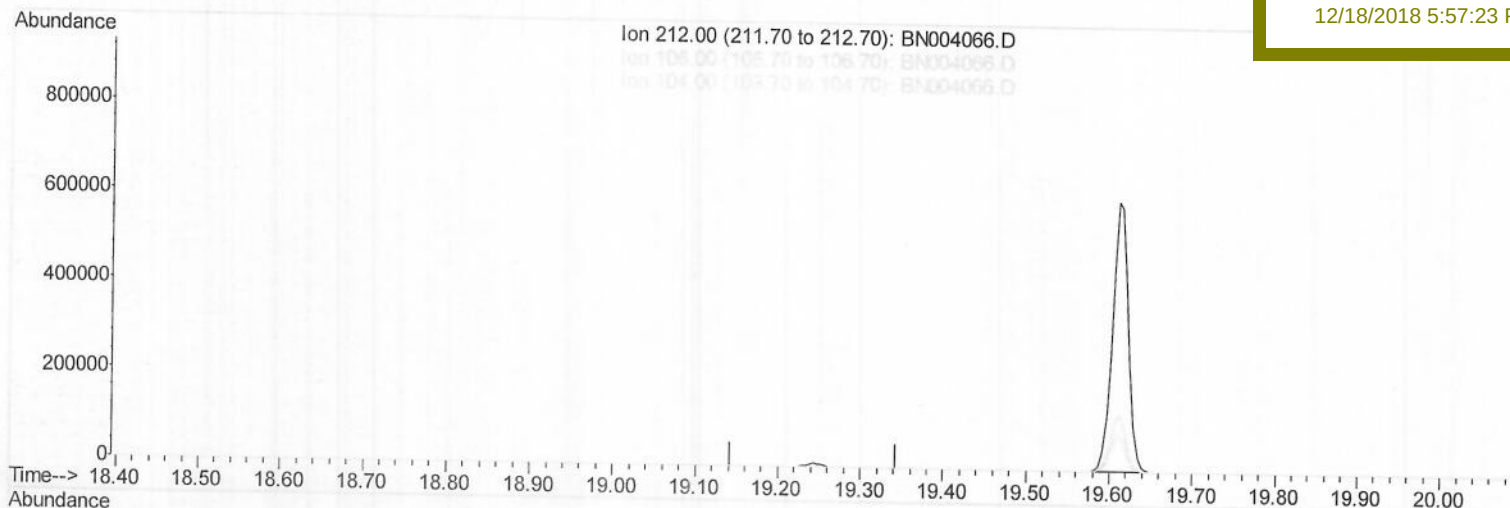

(14) Fluoranthene-d10 (SURR)

19.243min (-19.243) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

F9E13

Manual Integrations
APPROVED

Sohil

12/18/2018 5:57:23 PM

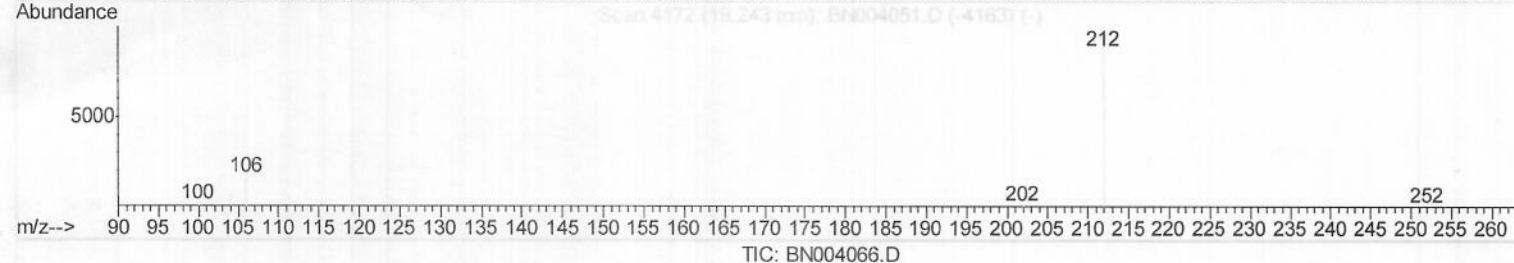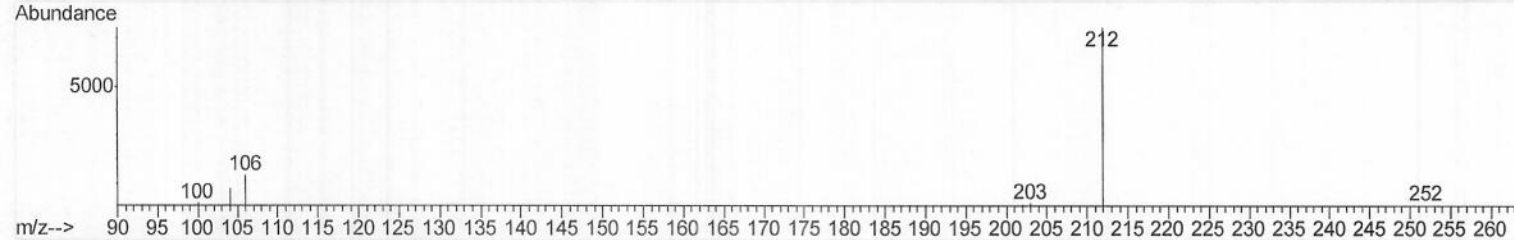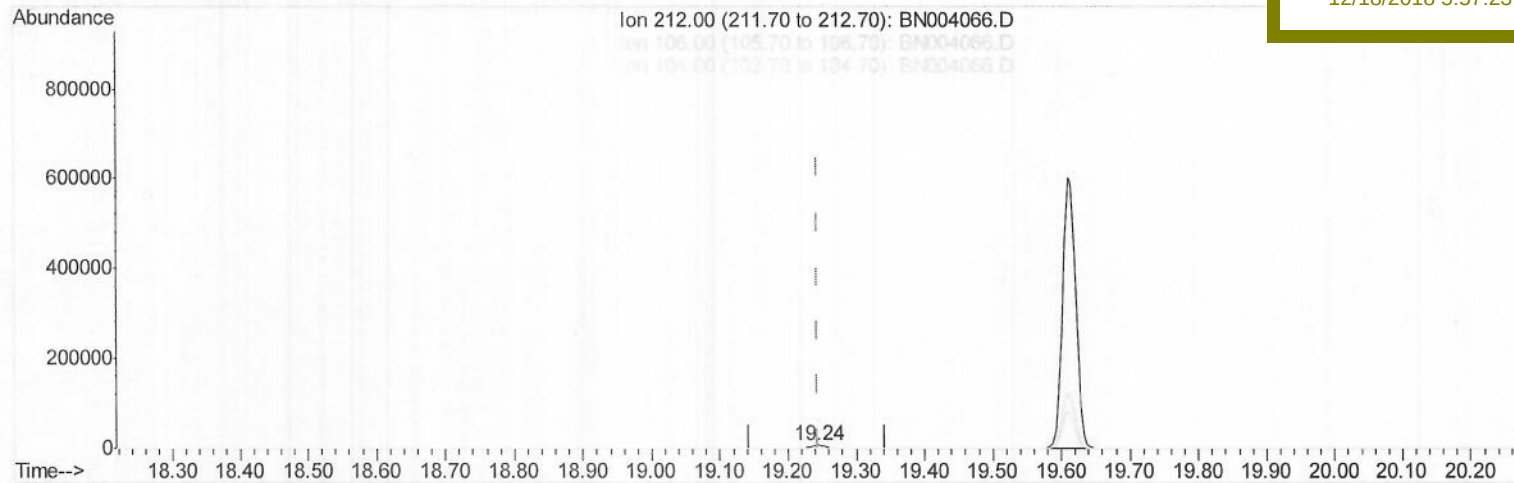

(14) Fluoranthene-d10 (SURR)

19.243min (-0.000) 0.23ng/ul m

response 9624

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

SJ
12/18/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

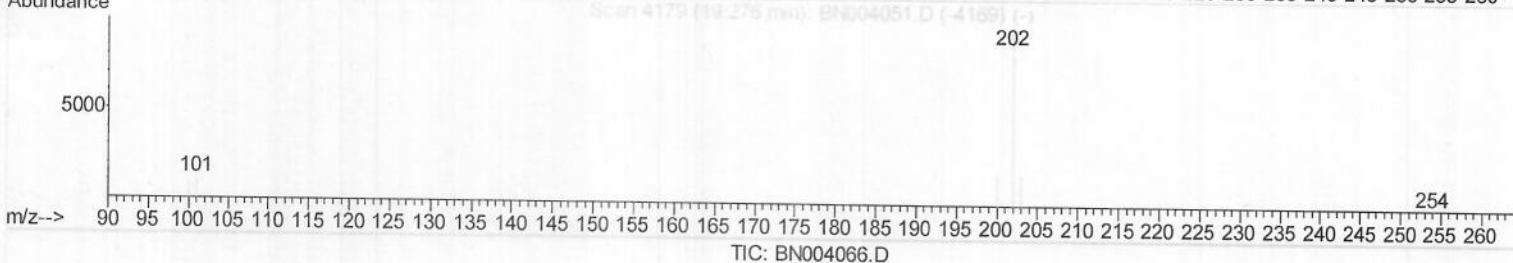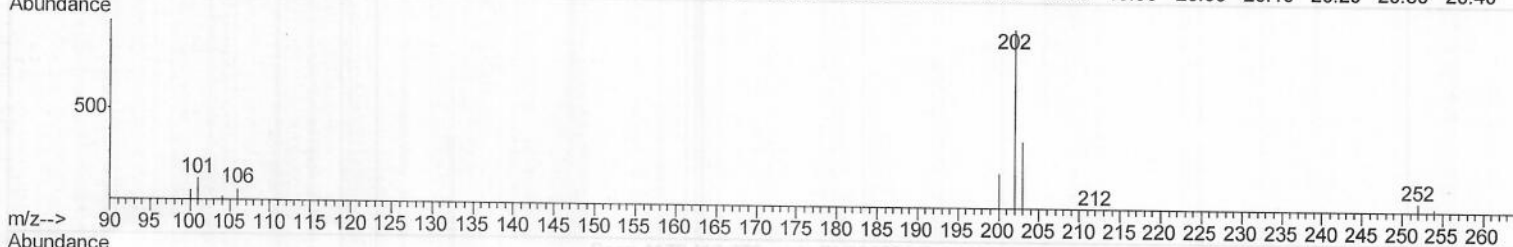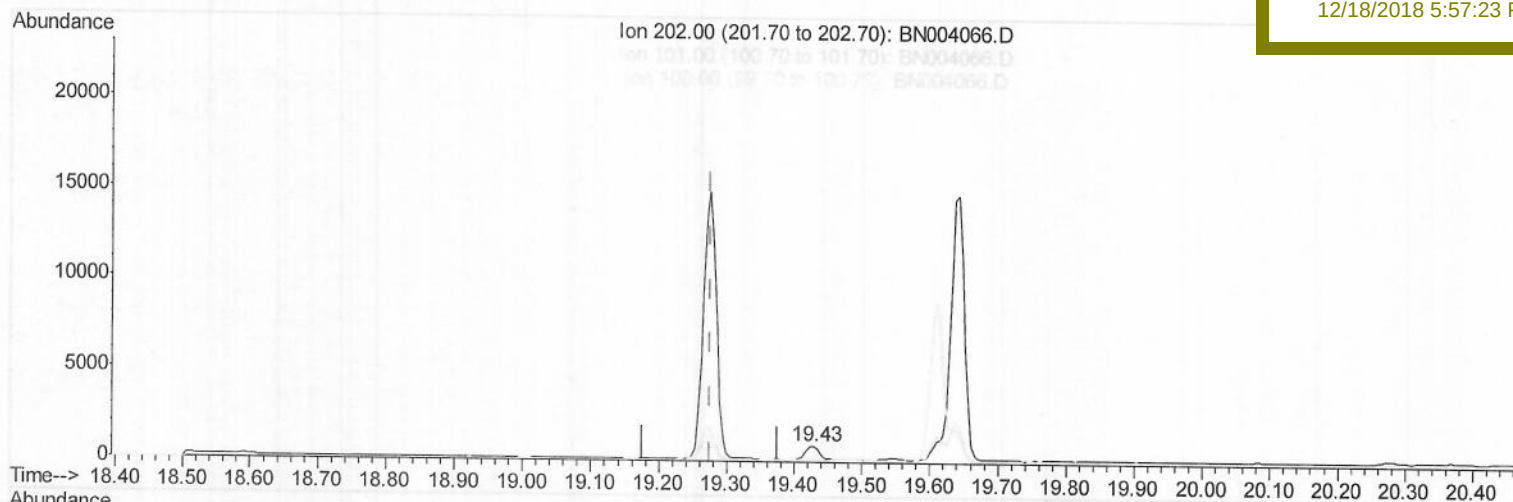

(15) Fluoranthene (C)

19.429min (+0.153) 0.02ng/ul

response 1068

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	20.56
100.00	8.10	14.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

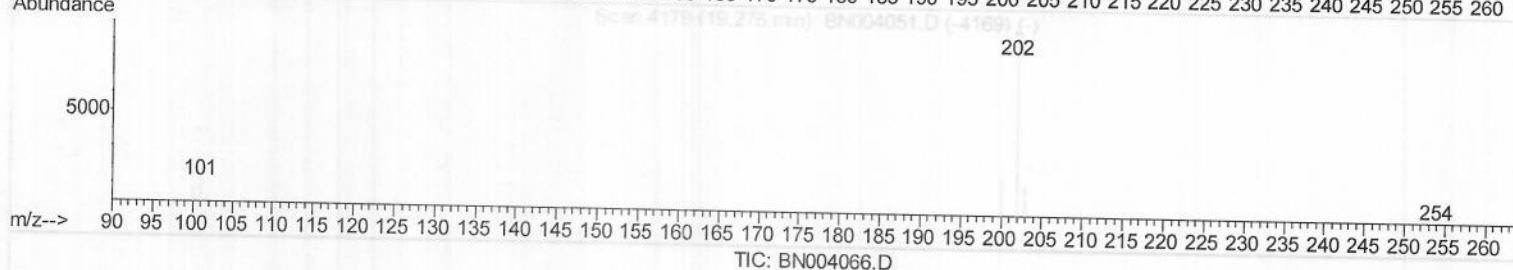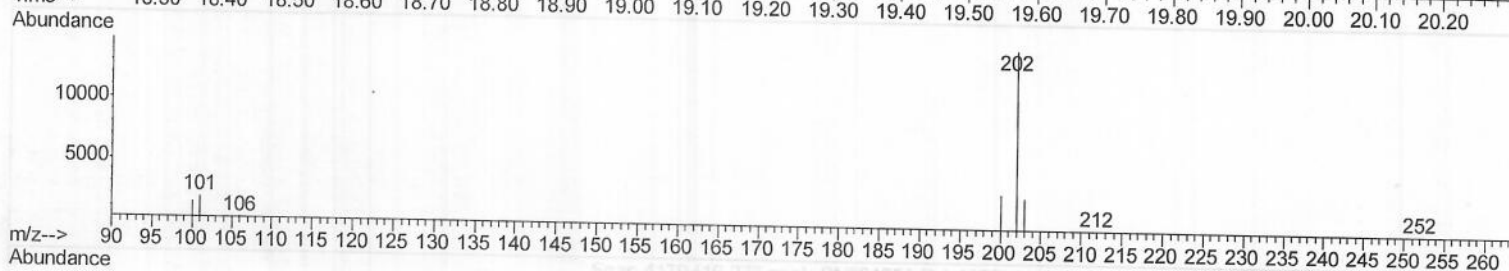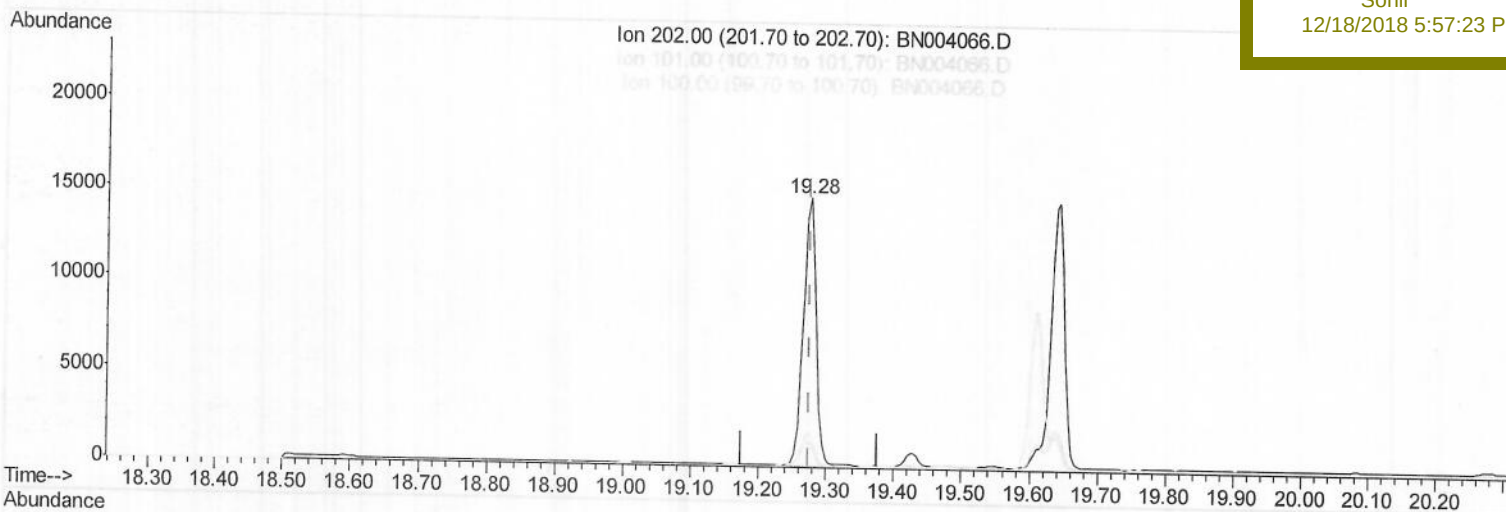

(15) Fluoranthene (C)

19.276min (-0.000) 0.36ng/ul m

response 19551

Ion	Exp%	Act%
202.00	100	100
101.00	10.70	12.34
100.00	8.10	9.15
0.00	0.00	0.00

SJ
 12/18/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

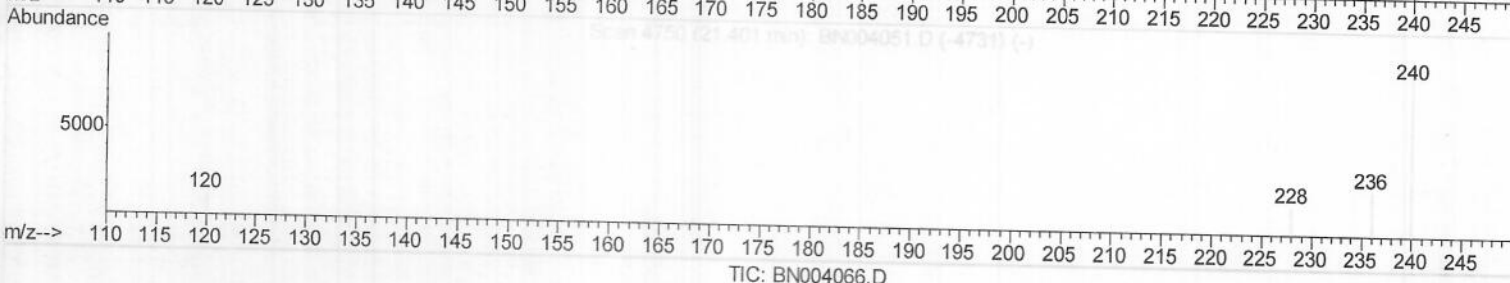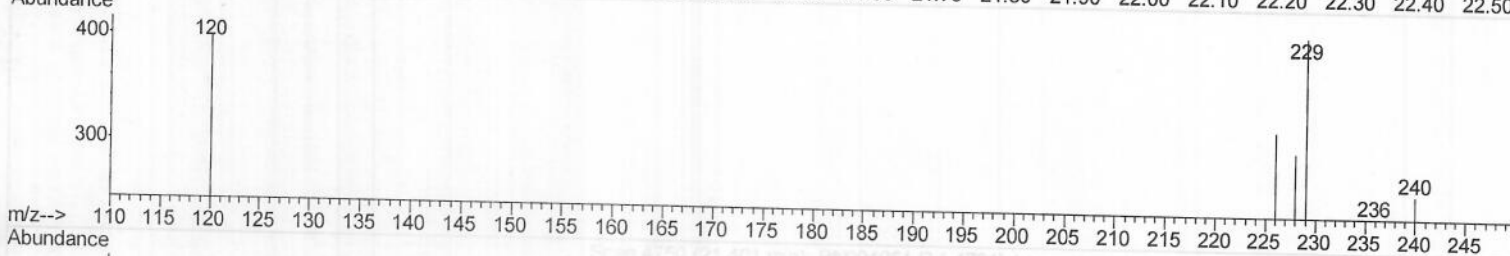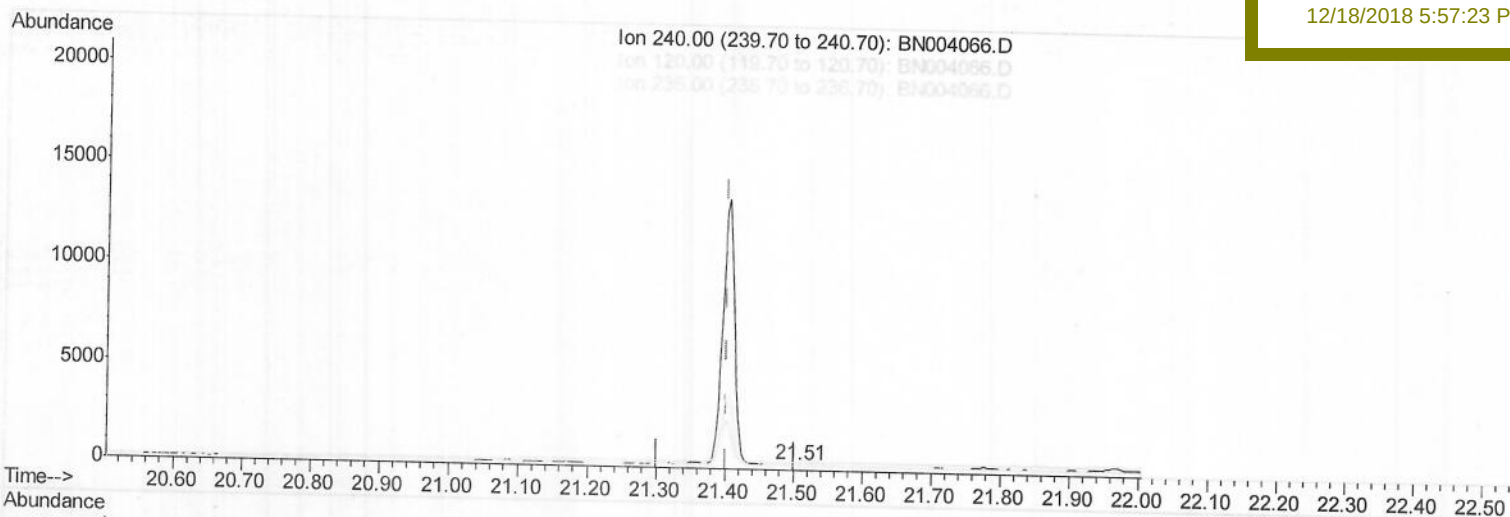

(16) Chrysene-d12 (I)
 21.506min (+0.105) 0.40ng/ul
 response 44

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	149.62#
236.00	27.60	91.73#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:28:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :

BNA_N




ClientSampleId :

F9E13

Manual Integrations
APPROVED

Sohil

12/18/2018 5:57:23 PM

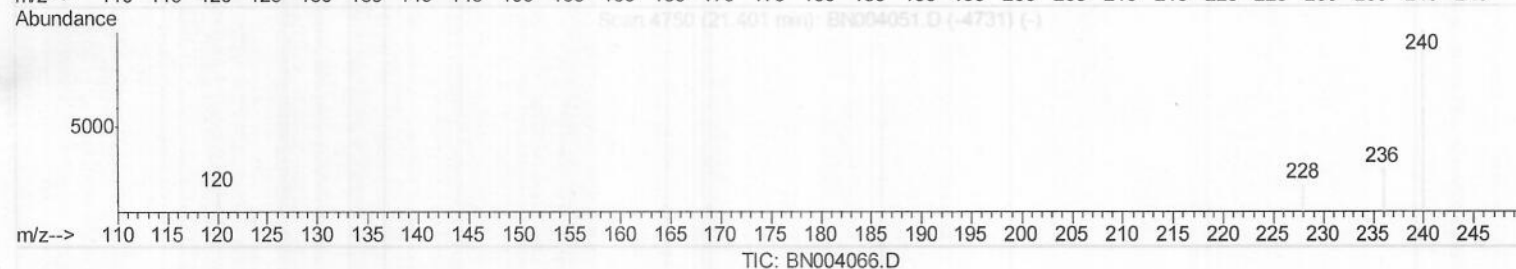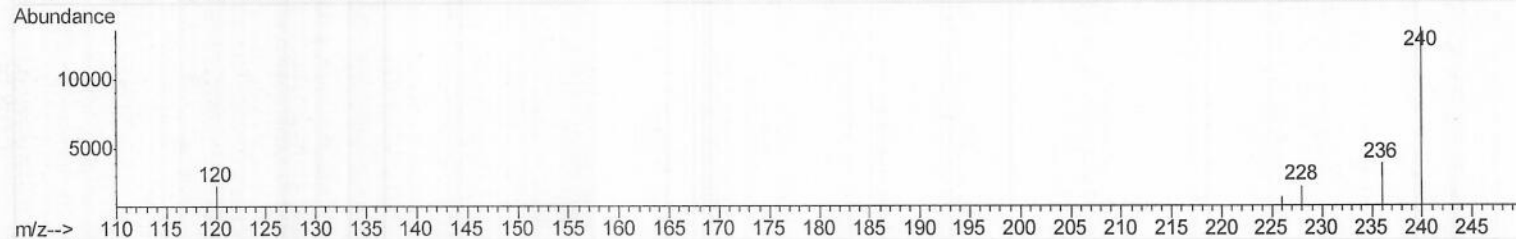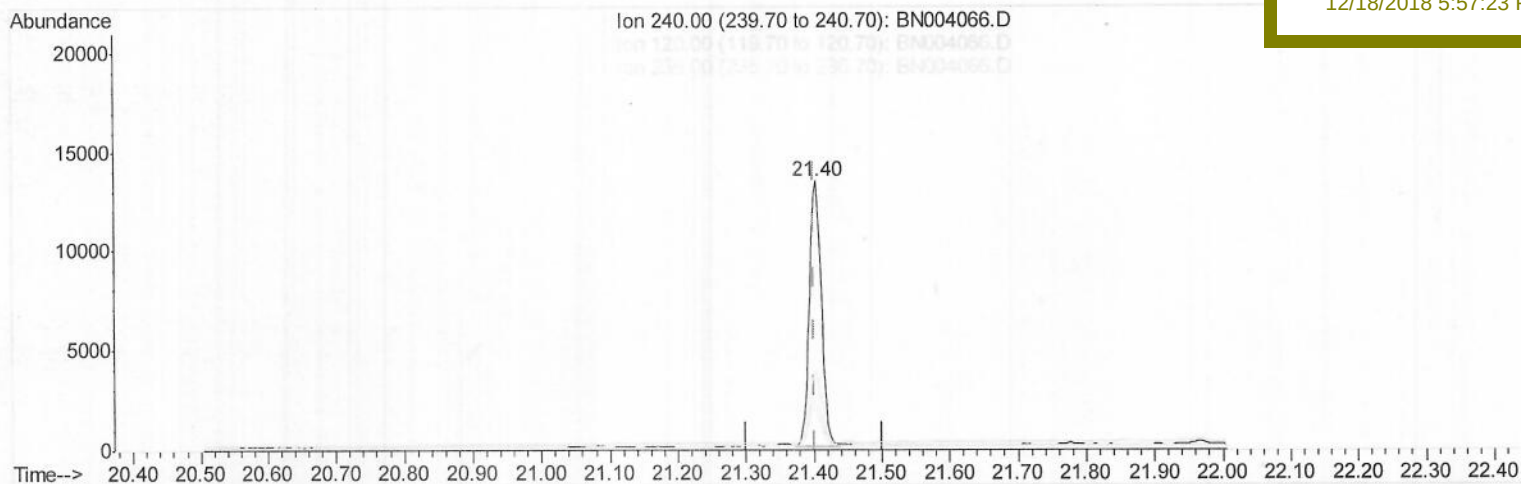

(16) Chrysene-d12 (I)

21.404min (+0.003) 0.40ng/ul m

response 16033

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	16.94#
236.00	27.60	28.44
0.00	0.00	0.00

SJ
12/18/18




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:31:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
F9E13

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

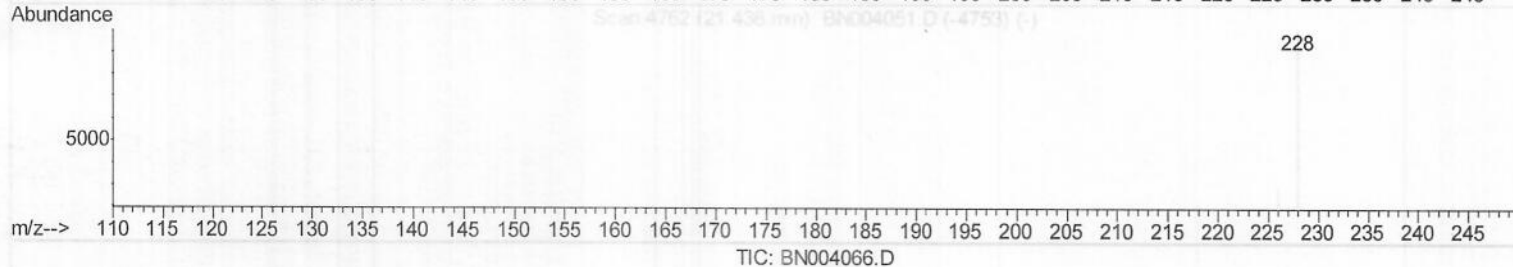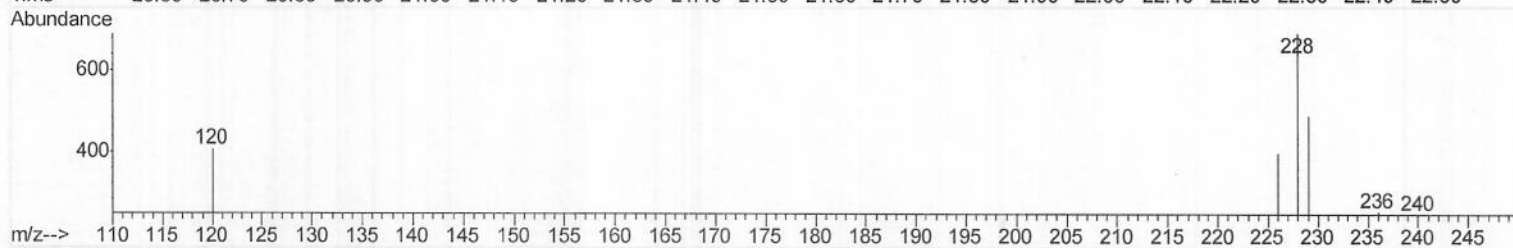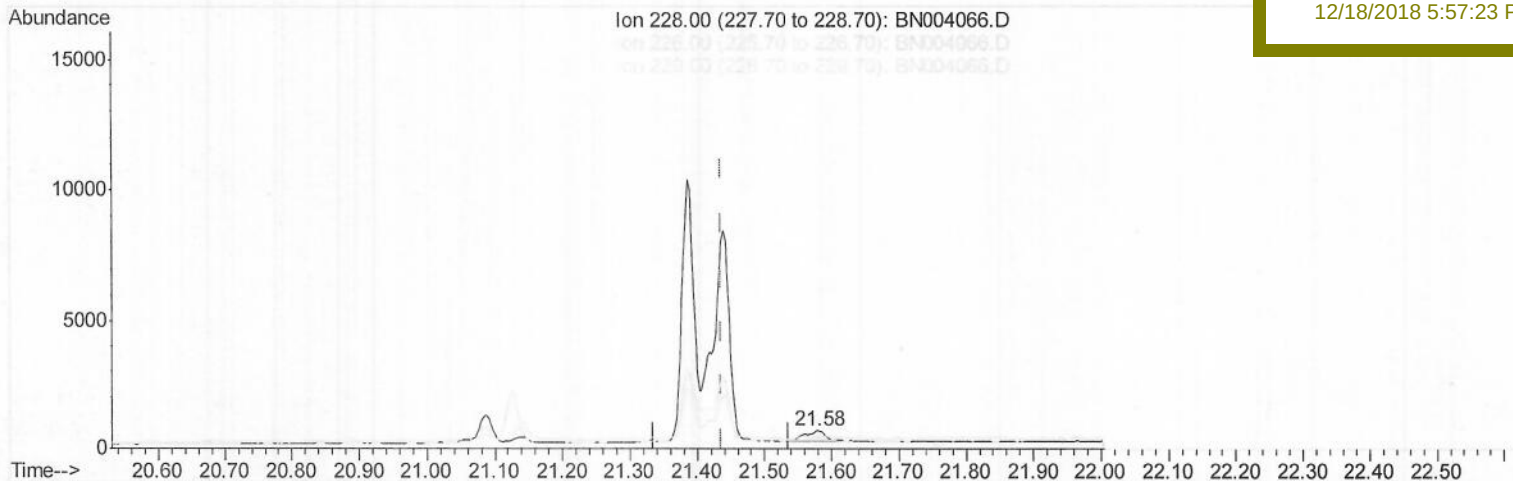

(19) Chrysene

21.579min (+0.143) 0.02ng/ul

response 898

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	57.41#
229.00	19.60	70.93#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1


Quant Time: Dec 18 11:31:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :

F9E13

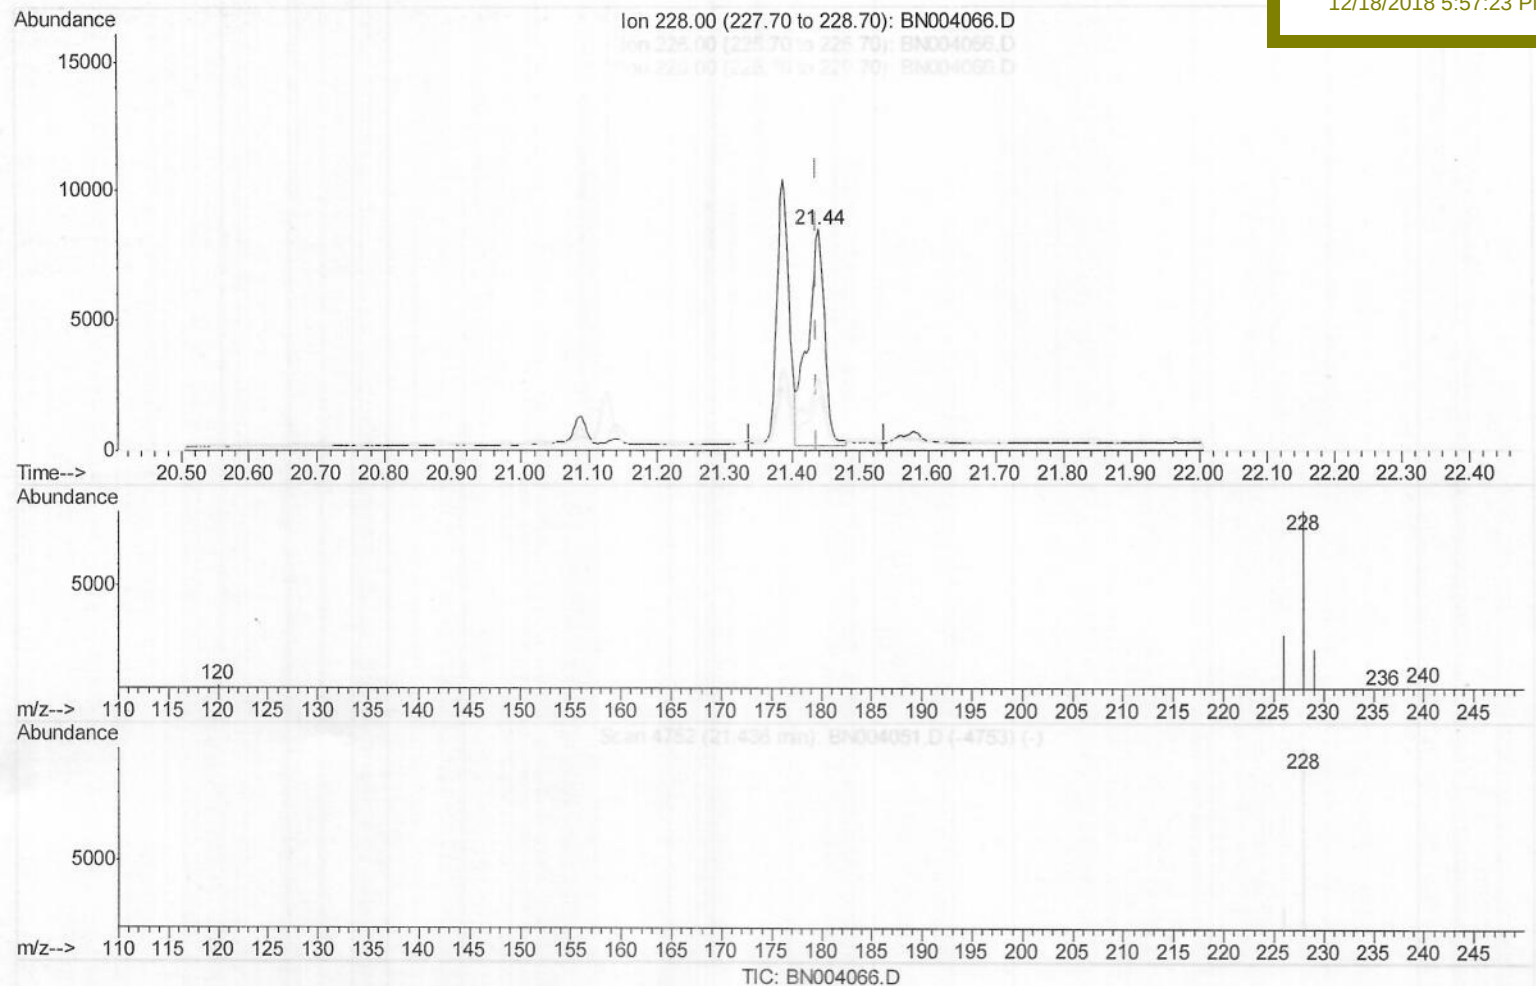Manual Integrations
APPROVEDSohil
12/18/2018 5:57:23 PM

(19) Chrysene

21.439min (+0.003) 0.25ng/ul m

response 14294

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	32.26
229.00	19.60	24.42#
0.00	0.00	0.00

SJ
12/18/18

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:31:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Instrument :
 BNA_N
 ClientSampleId :
 F9E13

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

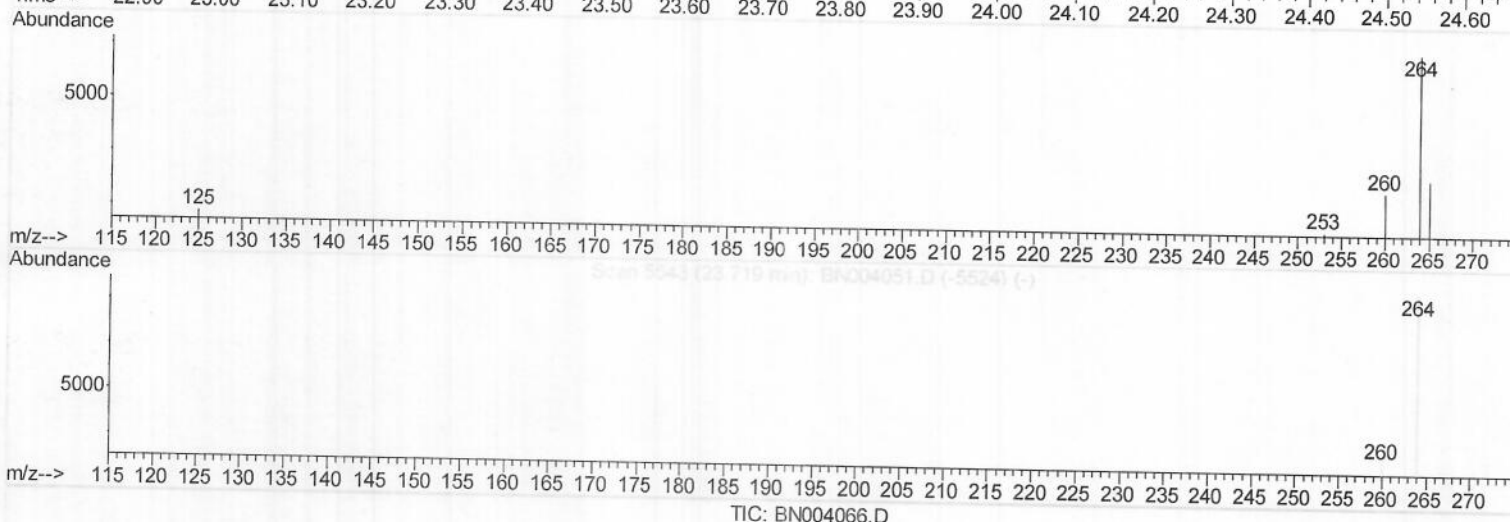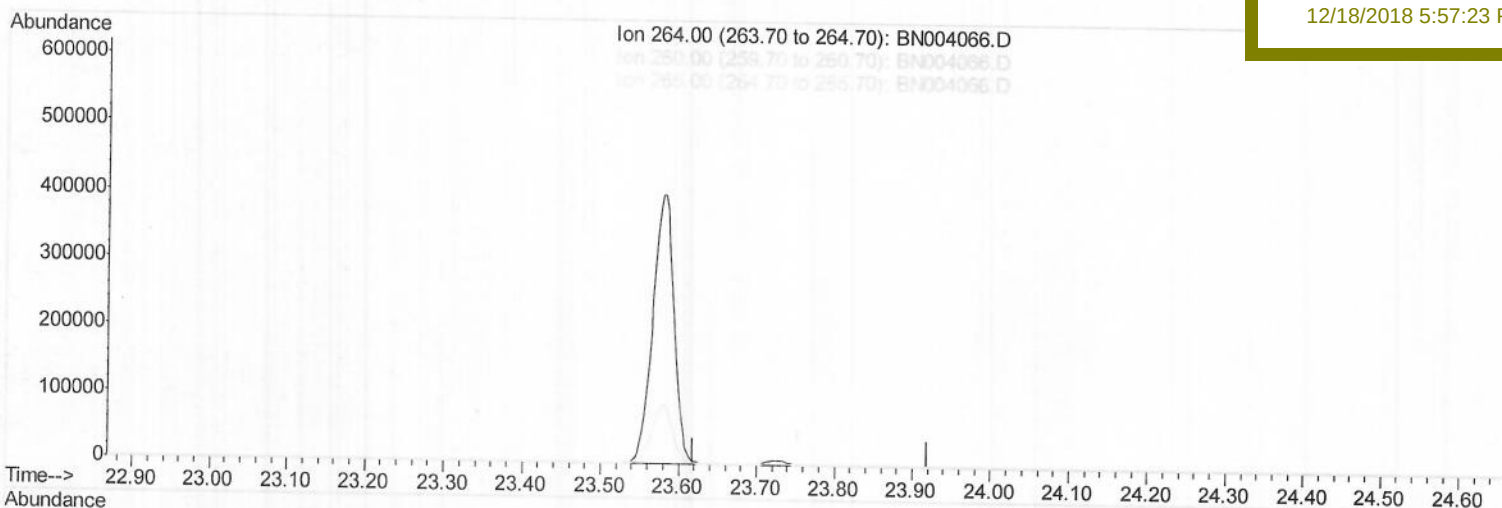

TIC: BN004066.D

(20) Perylene-d12 (I)

23.719min (-23.719) 0.00ng/ul

response 0

Ion	Exp%	Act%
264.00	100	0.00
260.00	26.20	0.00#
265.00	33.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\

Data File : BN004066.D

Acq On : 18 Dec 2018 09:04

Operator : JU/SJ

Sample : J6270-14

Misc :

ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:31:17 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 18 06:35:27 2018

Response via : Initial Calibration

Instrument :

BNA_N

ClientSampleId :




F9E13

Manual Integrations

APPROVED

Sohil

12/18/2018 5:57:23 PM

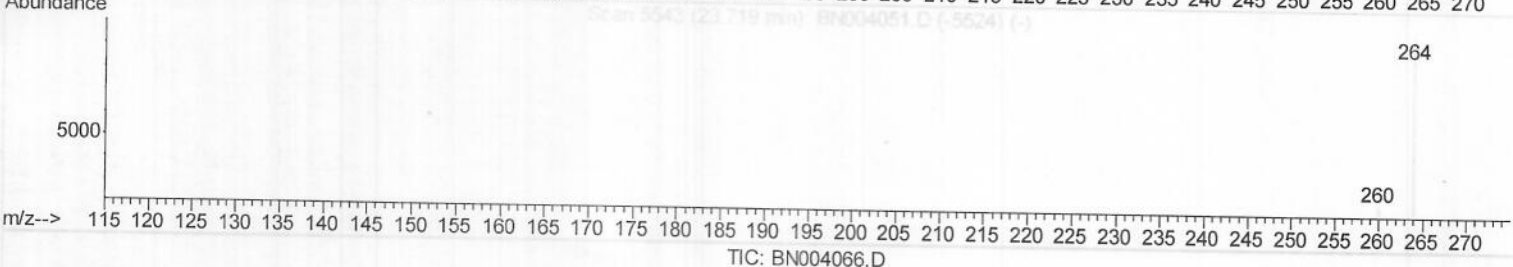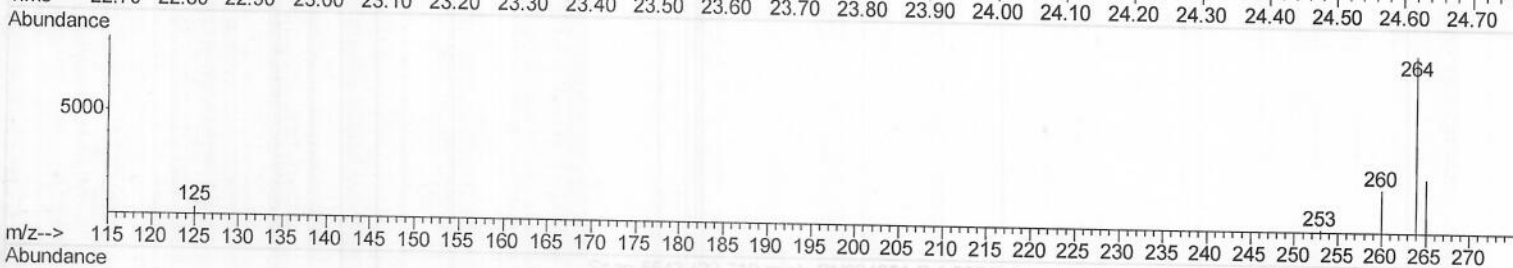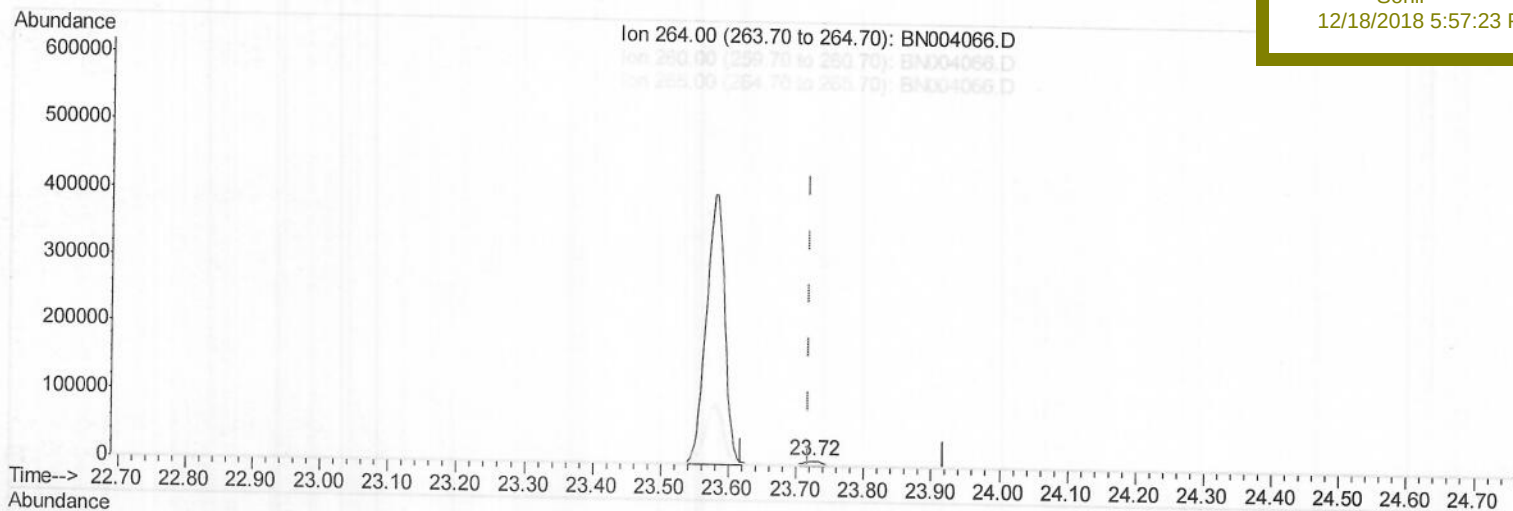

(20) Perylene-d12 (I)

23.725min (+0.006) 0.40ng/ul m

response 13788

Ion	Exp%	Act%
264.00	100	100
260.00	26.20	27.98
265.00	33.50	34.04
0.00	0.00	0.00

53

12/18/18

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 F9E13

Manual Integrations
APPROVED

Sohil
 12/18/2018 5:57:23 PM

Quant Time: Dec 18 11:32:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

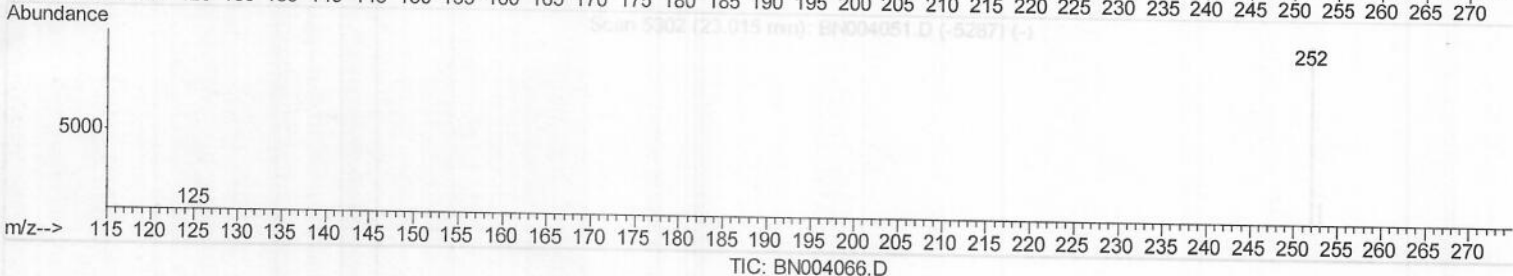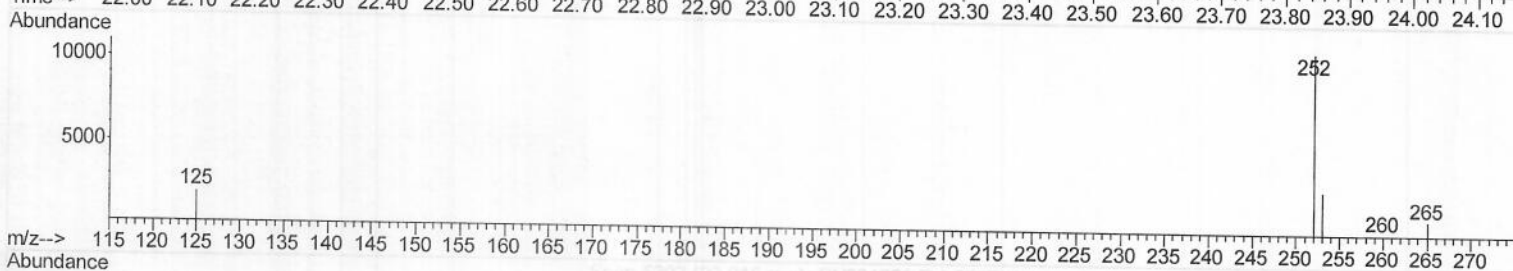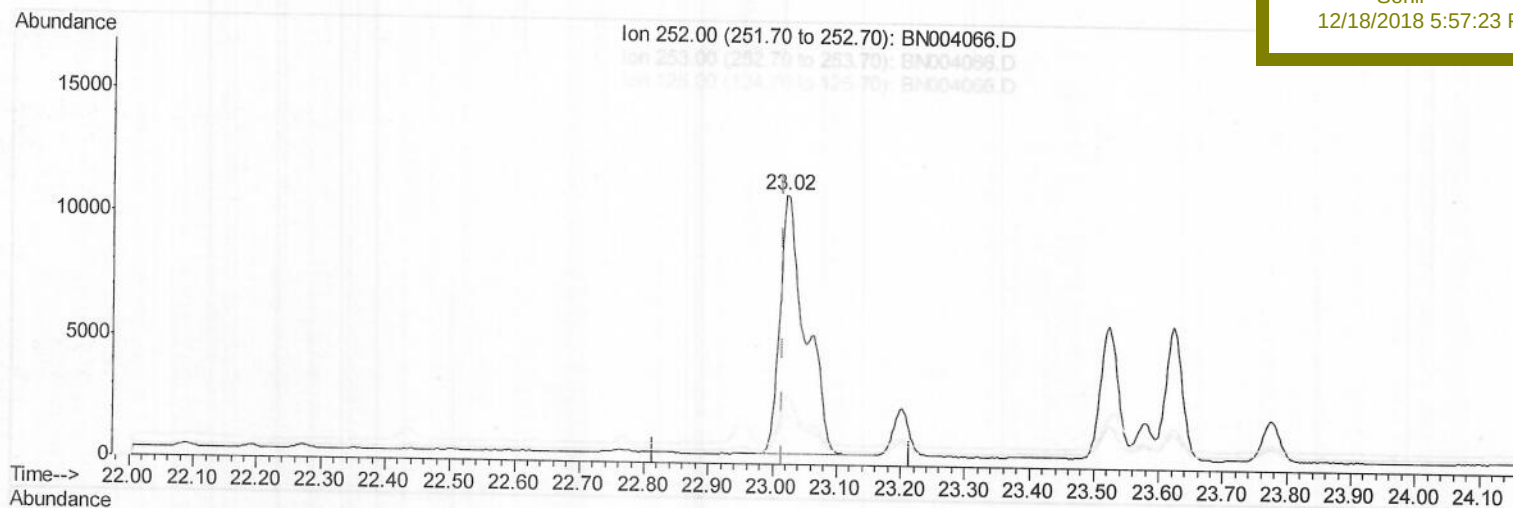

(21) Benzo(b)fluoranthene
 23.020min (+0.006) 0.52ng/ul
 response 29666

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	25.86
125.00	11.20	18.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:32:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :
BNA_N
Client Sampled :
F9E13

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

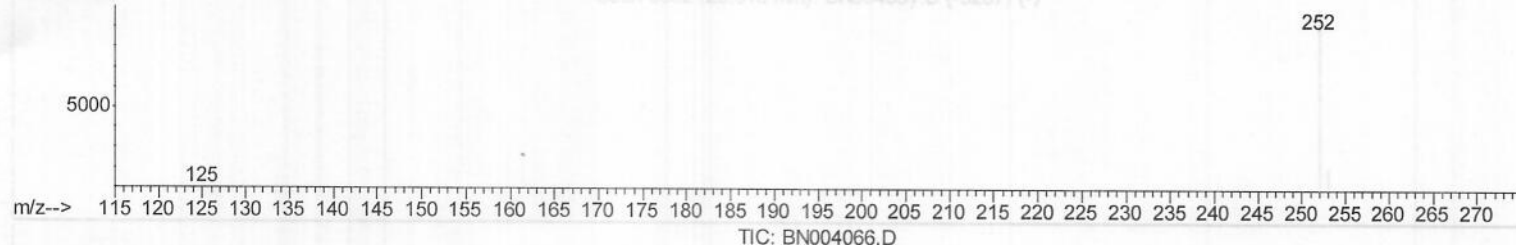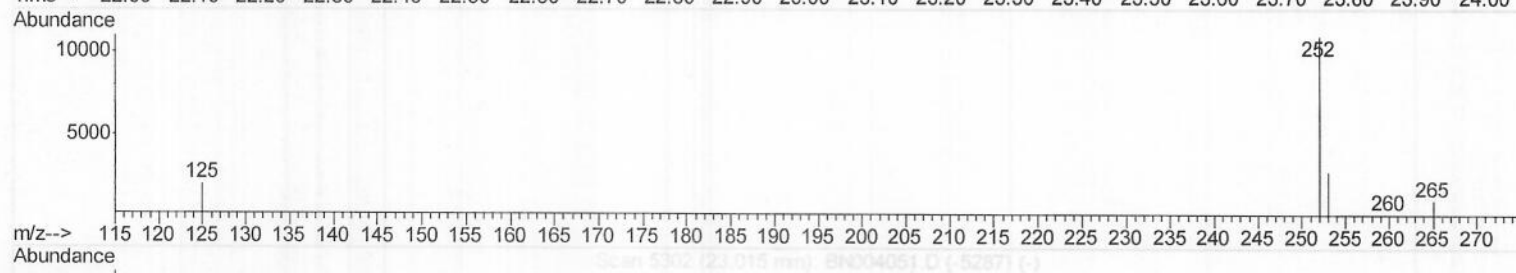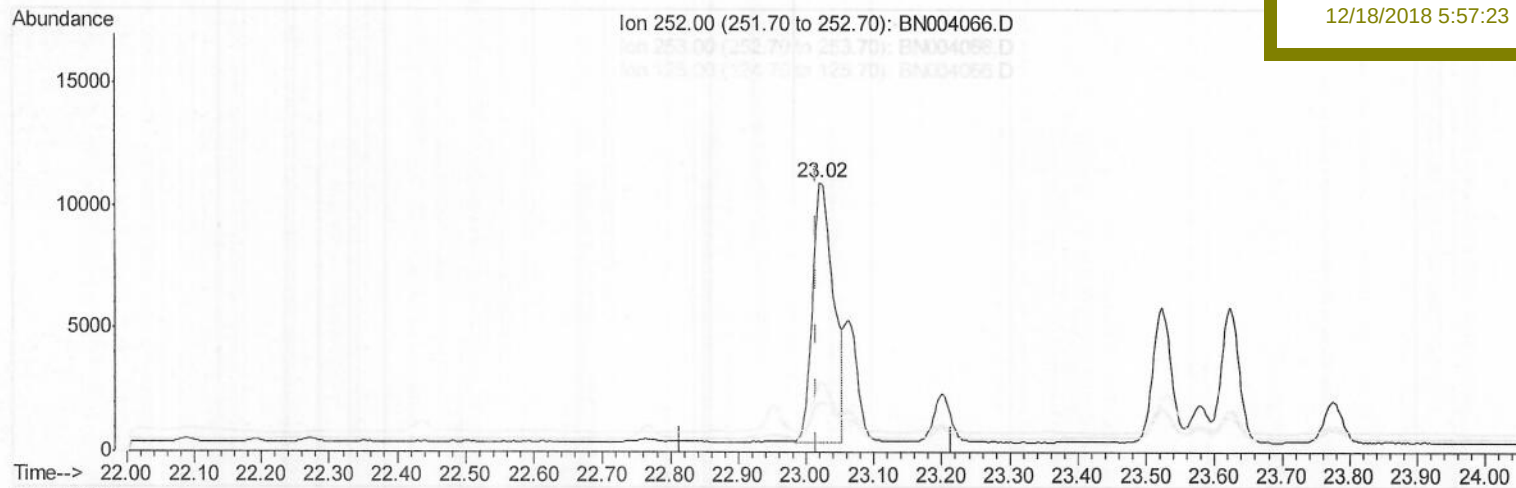

(21) Benzo(b)fluoranthene

23.020min (+0.006) 0.40ng/ul m

response 22539

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	25.86
125.00	11.20	18.45
0.00	0.00	0.00

SJ
12/18/18




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:32:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
F9E13

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

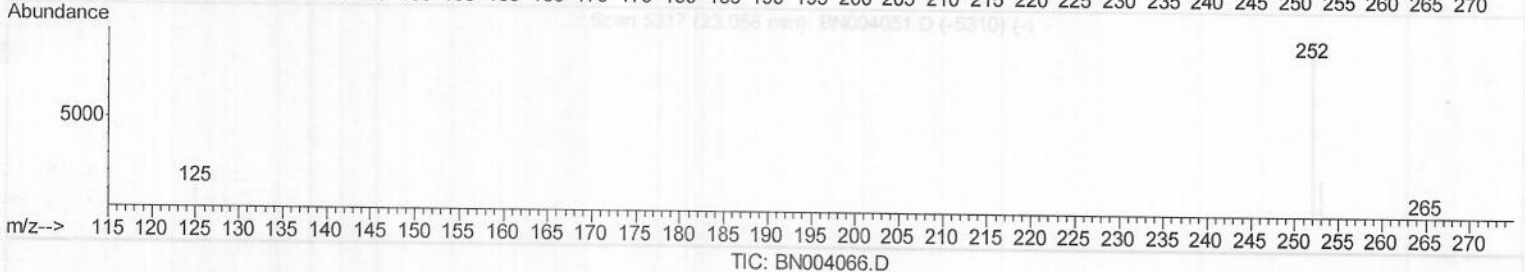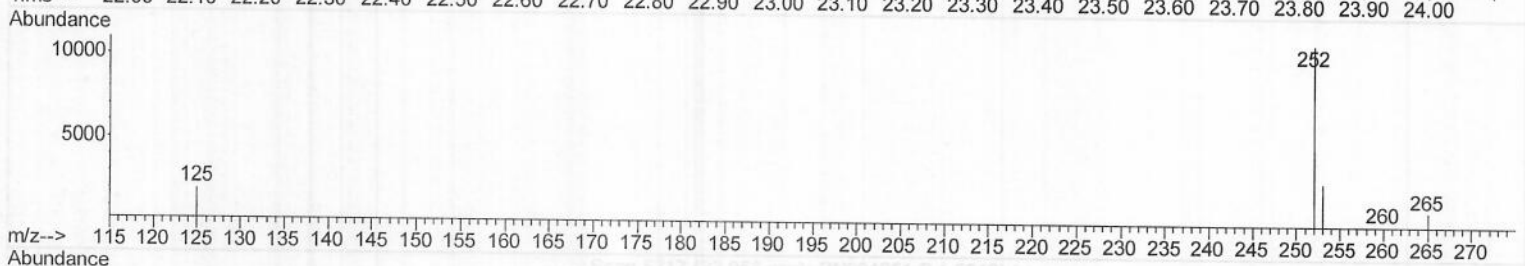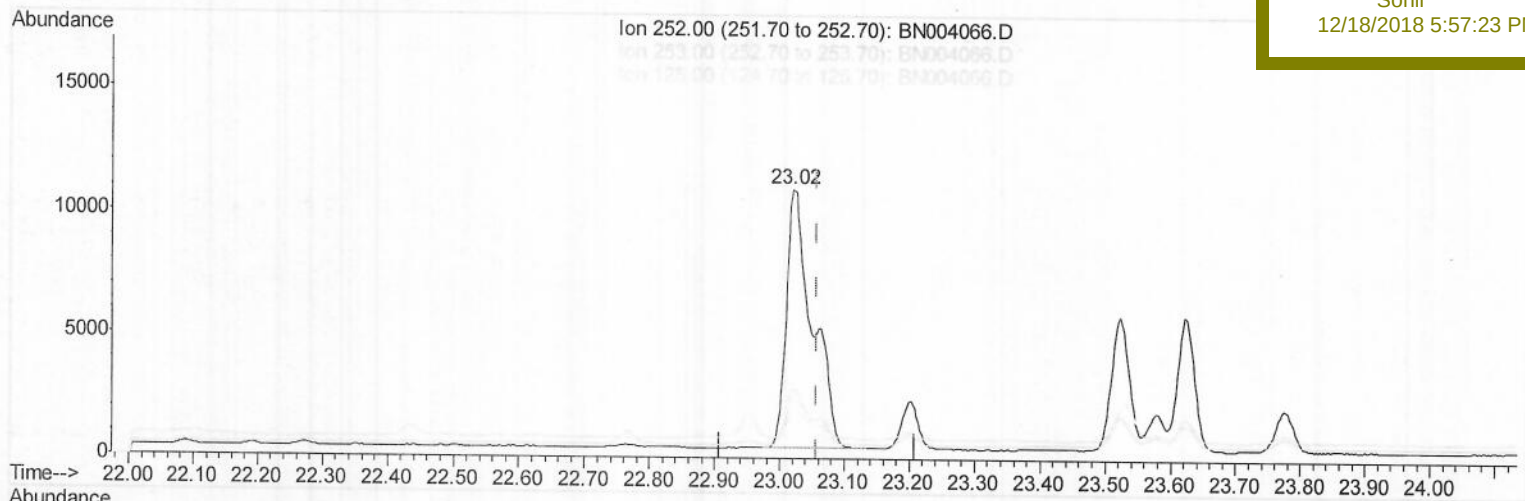

(22) Benzo(k)fluoranthene

23.020min (-0.038) 0.53ng/ui

response 29636

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	25.86
125.00	11.30	18.45#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
Data File : BN004066.D
Acq On : 18 Dec 2018 09:04
Operator : JU/SJ
Sample : J6270-14
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Dec 18 11:32:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 18 06:35:27 2018
Response via : Initial Calibration

Instrument :
BNA_N
ClientSampleId :
F9E13

Manual Integrations
APPROVED

Sohil
12/18/2018 5:57:23 PM

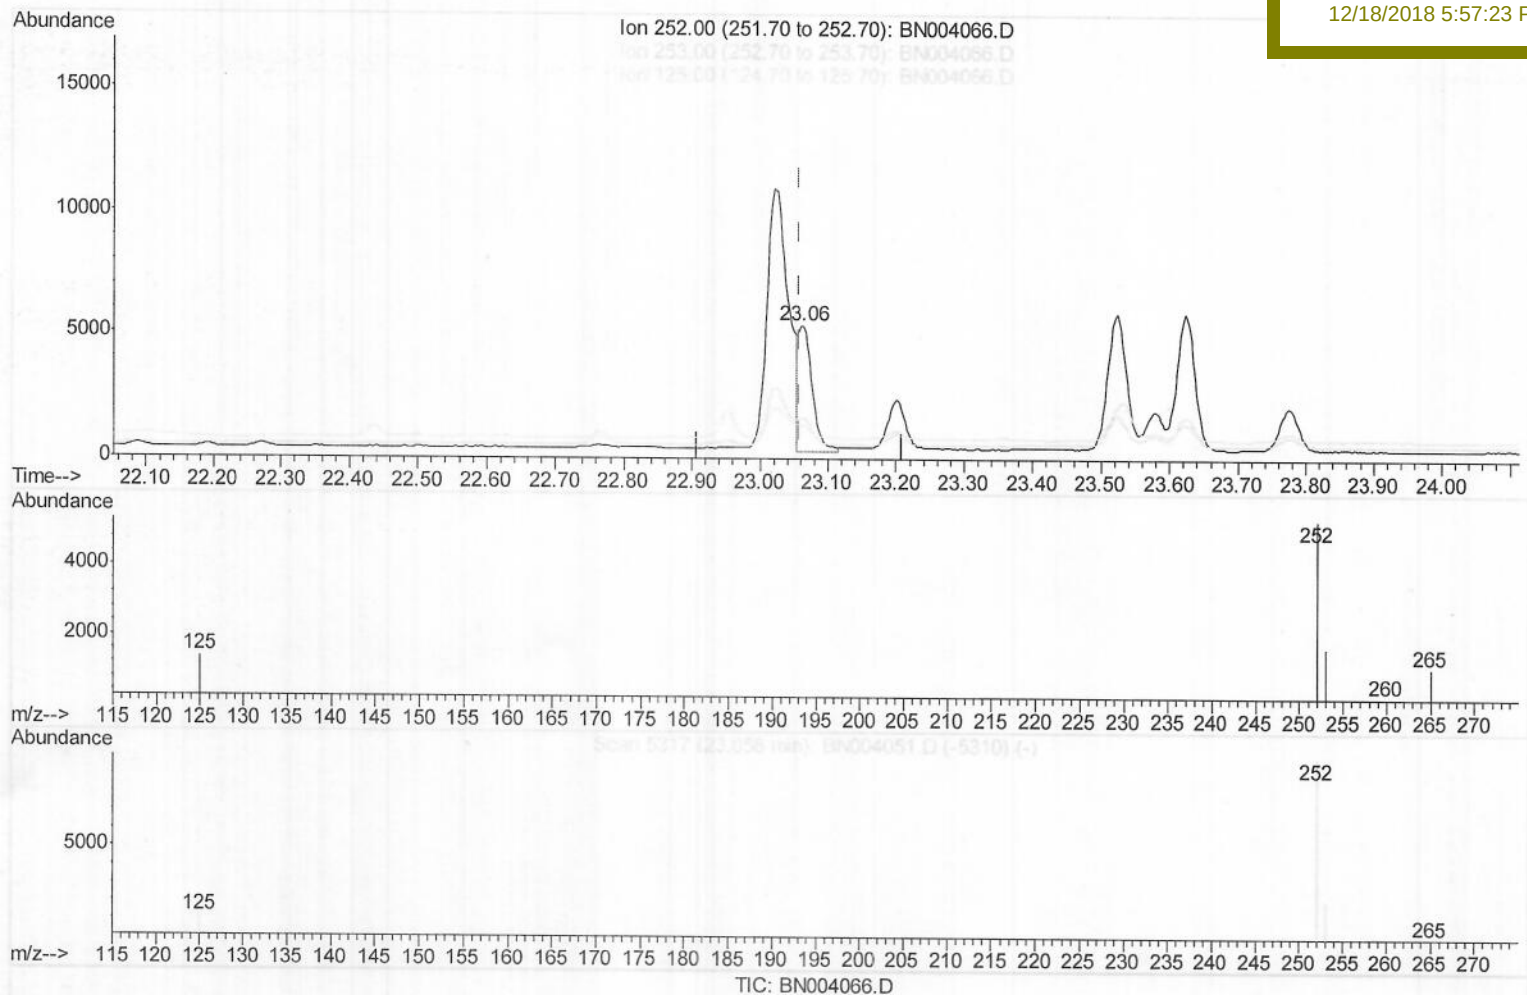

(22) Benzo(k)fluoranthene
23.061min (+0.003) 0.14ng/ul m
response 7635

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	31.16#
125.00	11.30	25.60#
0.00	0.00	0.00

SJ
12/18/18

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121718\
 Data File : BN004066.D
 Acq On : 18 Dec 2018 09:04
 Operator : JU/SJ
 Sample : J6270-14
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 Client Sample ID :
 F9E13

Quant Time: Dec 18 11:33:56 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 18 06:35:27 2018
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 12/18/2018 5:57:23 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1614	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	8250	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	5257	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	14054m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	16033m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	13788m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	2632	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	9624m	0.23	ng/ul	0.00
Target Compounds						
7) Acenaphthylene	14.19	152	3427	0.145	ng/ul	Qvalue 96
12) Phenanthrene	17.26	178	2161m	0.047	ng/ul	
13) Anthracene	17.35	178	3482m	0.092	ng/ul	
15) Fluoranthene	19.28	202	19551m	0.359	ng/ul	
17) Pyrene	19.64	202	20683	0.360	ng/ul	98
18) Benzo(a)anthracene	21.39	228	12789	0.253	ng/ul	93
19) Chrysene	21.44	228	14294m	0.247	ng/ul	
21) Benzo(b)fluoranthene	23.02	252	22539m	0.395	ng/ul	
22) Benzo(k)fluoranthene	23.06	252	7635m	0.137	ng/ul	
23) Benzo(a)pyrene	23.62	252	9941	0.201	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	26.09	276	9376	0.166	ng/ul#	96
25) Dibenzo(a,h)anthracene	26.09	278	2387	0.052	ng/ul#	28
26) Benzo(g,h,i)perylene	26.82	276	7364	0.150	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
 12/18/18