
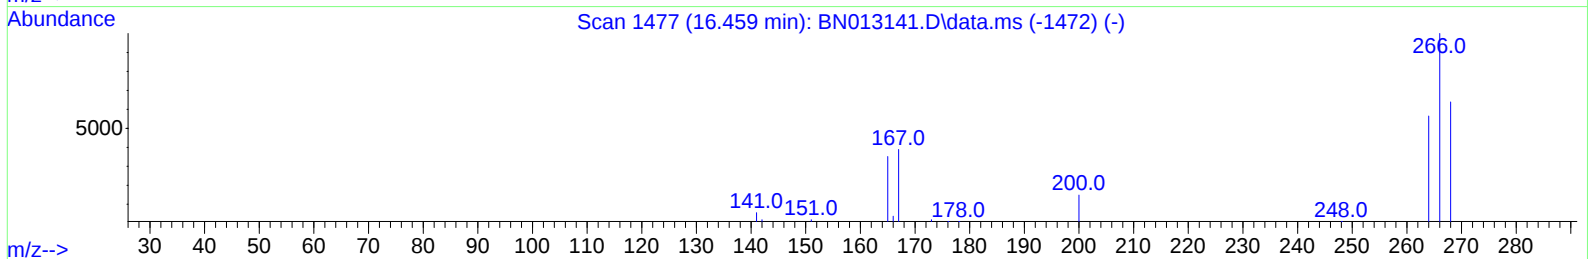
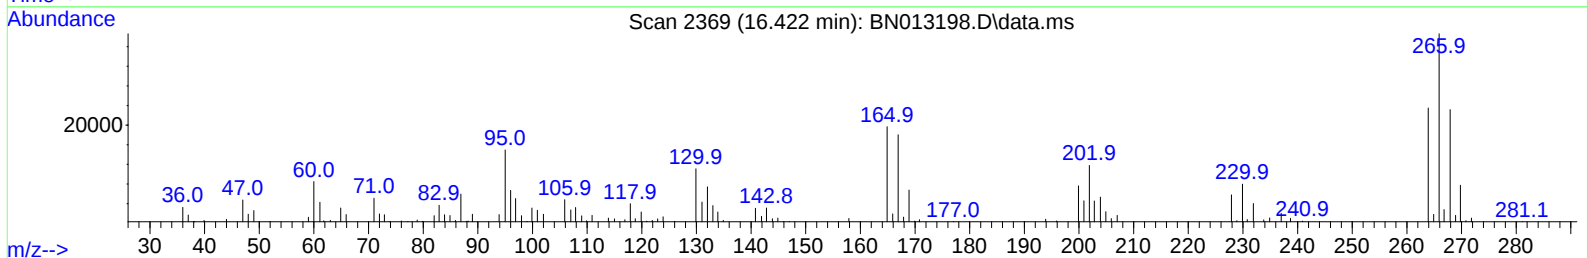


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121720\
Data File : BN013198.D
Acq On : 18 Dec 2020 00:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 04:22:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 17 12:34:52 2020
Response via : Initial Calibration

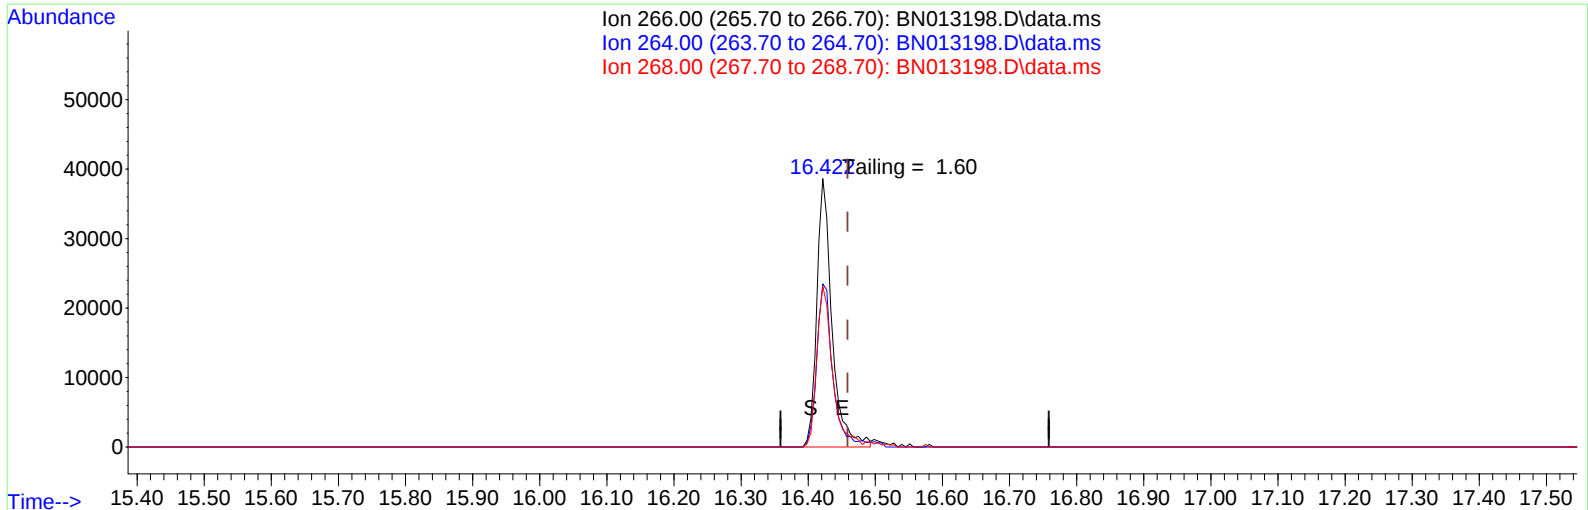

TIC: BN013198.D\data.ms

(24) Pentachlorophenol

16.422min (-0.037) 0.00 ng

response 62112

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	63.92
268.00	64.40	60.73
0.00	0.00	0.00