


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121720\
 Data File : BN013180.D
 Acq On : 17 Dec 2020 10:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 12:34:52 2020

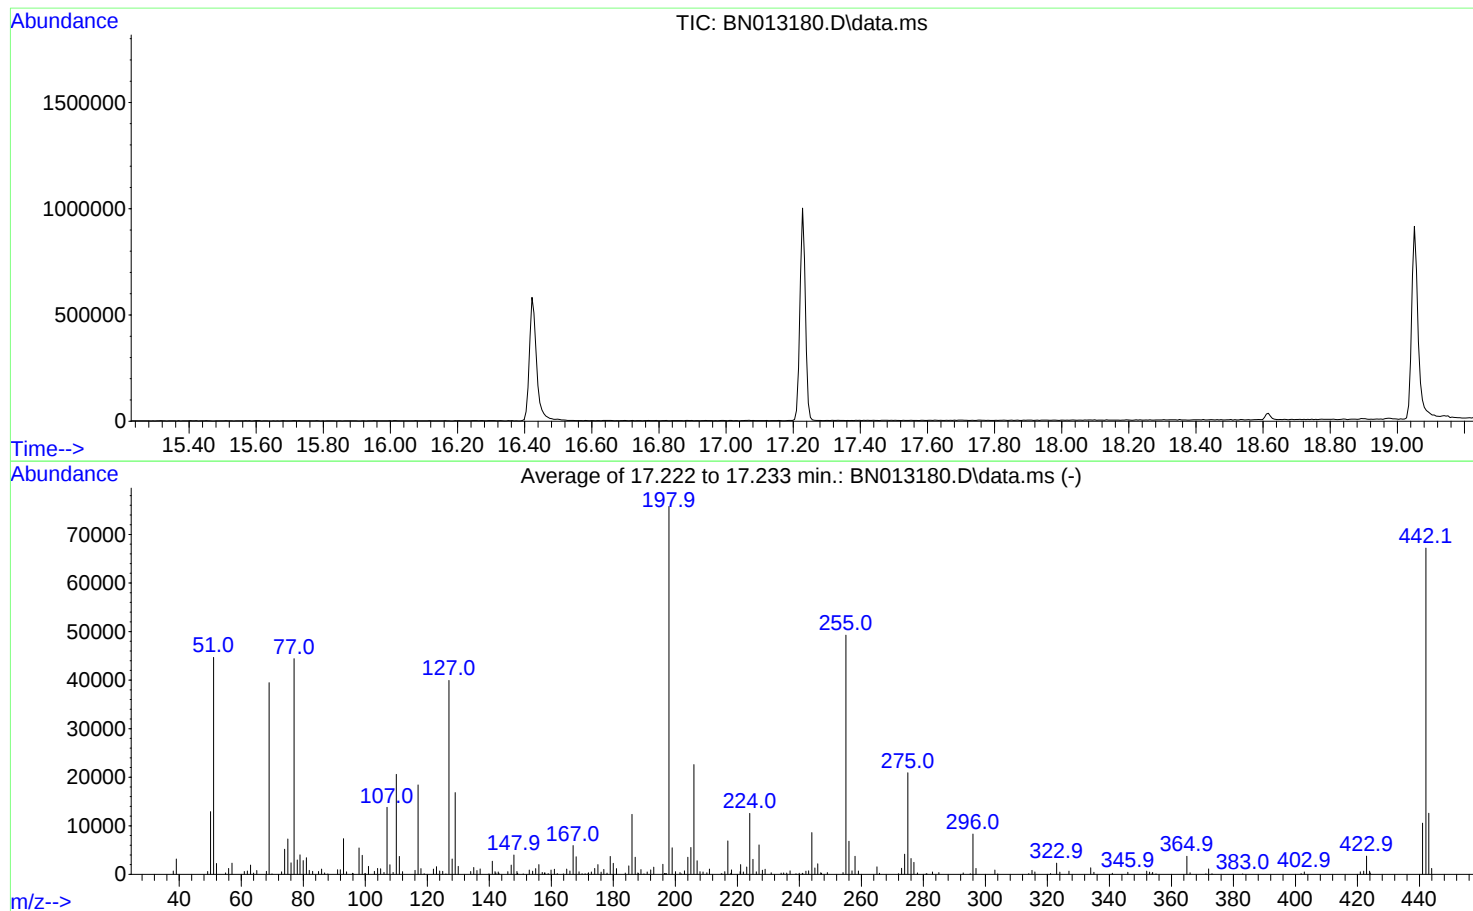

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	44685	PASS
68	69	0.00	2	1.6	632	PASS
69	198	0.00	100	52.1	39485	PASS
70	69	0.00	2	0.3	115	PASS
127	198	10	80	52.7	39939	PASS
197	198	0.00	2	0.2	173	PASS
198	198	100	100	100.0	75752	PASS
199	198	5	9	7.2	5478	PASS
275	198	10	60	27.6	20919	PASS
365	198	1	100	4.9	3714	PASS
441	198	0.01	100	13.9	10537	PASS
442	442	50	100	100.0	67192	PASS
443	442	15	24	18.7	12589	PASS