


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121720\
 Data File : BN013198.D
 Acq On : 18 Dec 2020 00:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 17 12:34:52 2020

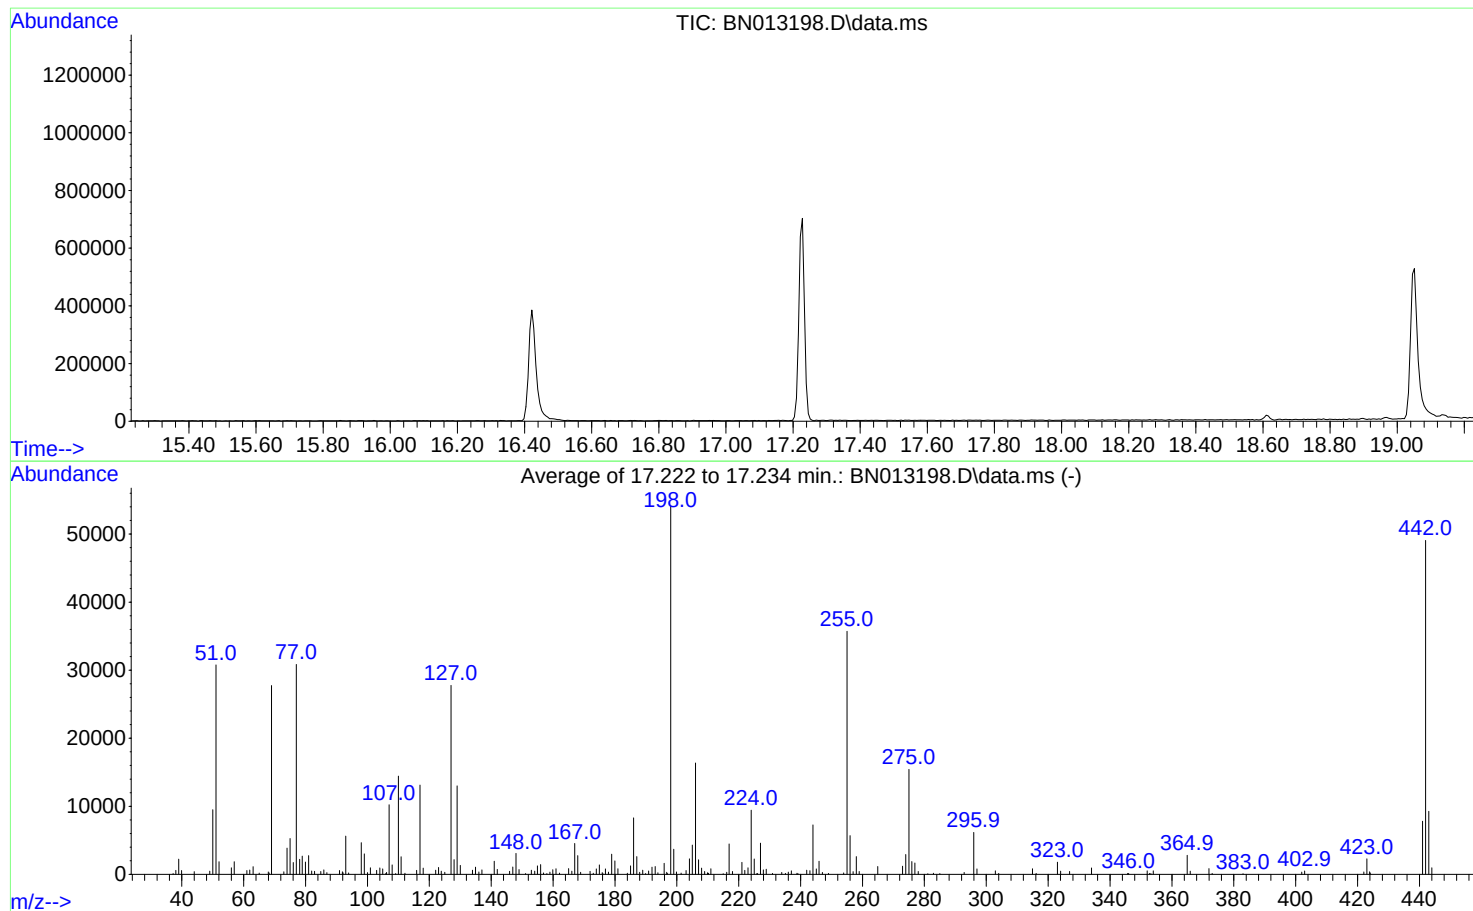

Spectrum Information: Average of 17.222 to 17.234 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.0	30784	PASS
68	69	0.00	2	1.3	357	PASS
69	198	0.00	100	51.3	27733	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	27776	PASS
197	198	0.00	2	0.5	296	PASS
198	198	100	100	100.0	54051	PASS
199	198	5	9	6.8	3694	PASS
275	198	10	60	28.6	15434	PASS
365	198	1	100	5.2	2798	PASS
441	198	0.01	100	14.5	7813	PASS
442	442	50	100	100.0	49069	PASS
443	442	15	24	18.9	9266	PASS